

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091222\
 Data File : PL077692.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2022 01:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 14:38:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.626	29921412	59655934	18.666	20.095
28)	SA Decachlor...	8.903	7.723	26573796	51697578	20.561	20.595
Target Compounds							
5)	MB Aldrin	0.000	4.063	0	886701	N.D.	0.234 #
6)	B beta-BHC	0.000	3.745	0	289721	N.D.	0.174 #
8)	B Heptachlo...	5.569	0.000	6522016	0	3.741	N.D. #
13)	MA Dieldrin	0.000	5.168	0	3992260	N.D.	1.204 #
14)	MA Endrin	0.000	5.471f	0	2656257	N.D.	0.932 #
15)	B Endosulfa...	6.707f	0.000	1024447	0	0.742	N.D. #
17)	MA 4,4'-DDT	0.000	5.853	0	98383	N.D.	0.037 #
21)	B Endrin ke...	7.569f	0.000	1026914	0	0.743	N.D. #
23)	Chlordane-1	0.000	3.604	0	604963	N.D.	5.567 #
24)	Chlordane-2	0.000	4.161	0	2193661	N.D.	18.313 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091222\
Data File : PL077692.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2022 01:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 14:38:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

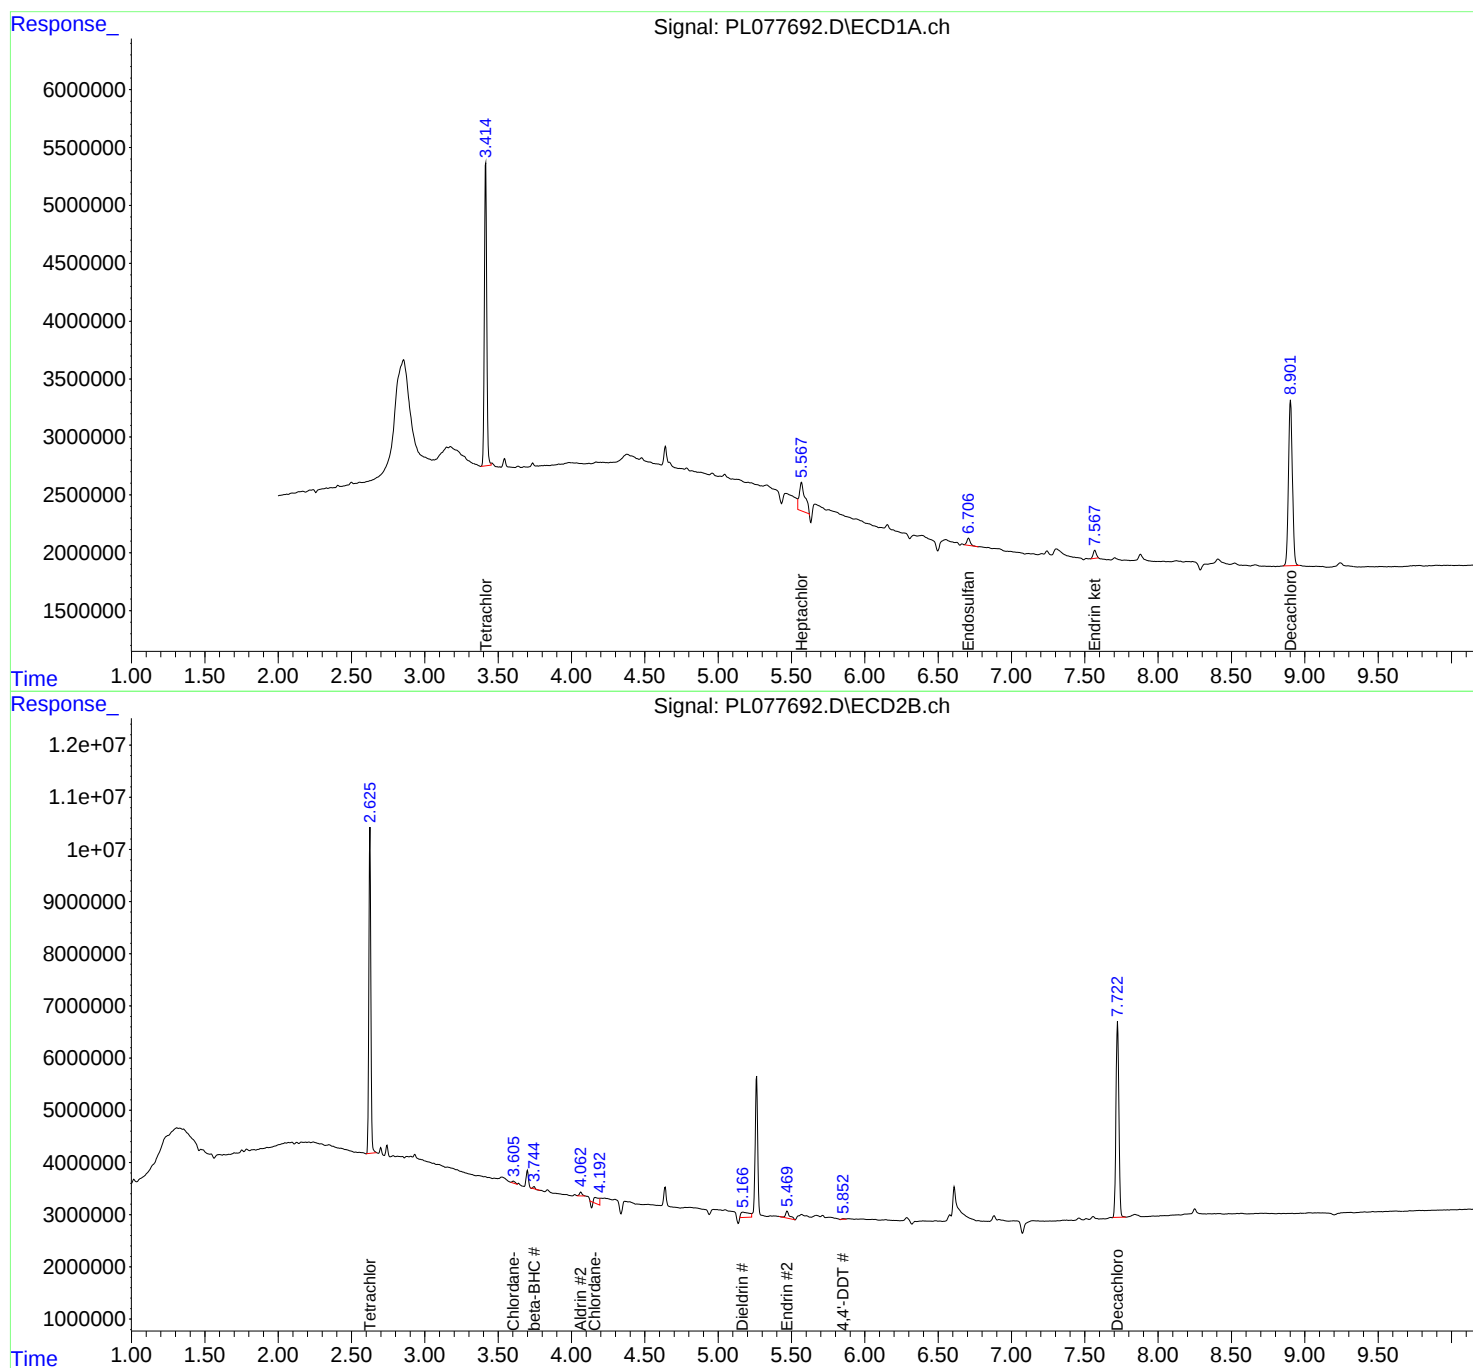


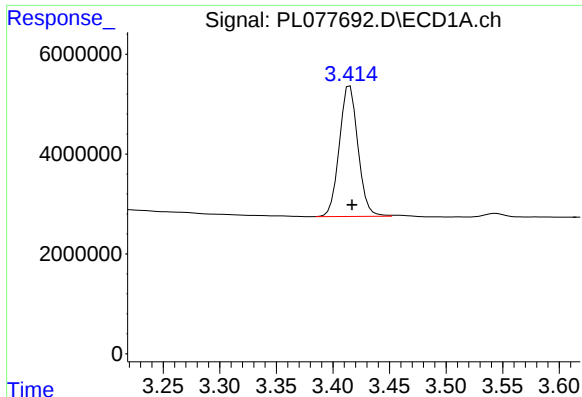

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: -0.002 min
Response: 29921412
Conc: 18.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

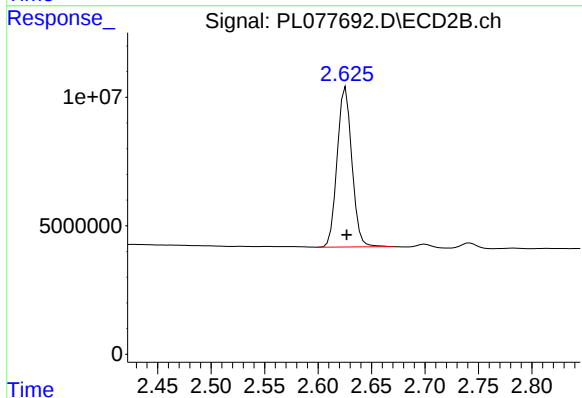


#1 Tetrachloro-m-xylene

R.T.: 2.626 min
Delta R.T.: 0.000 min
Response: 59655934
Conc: 20.09 ng/ml

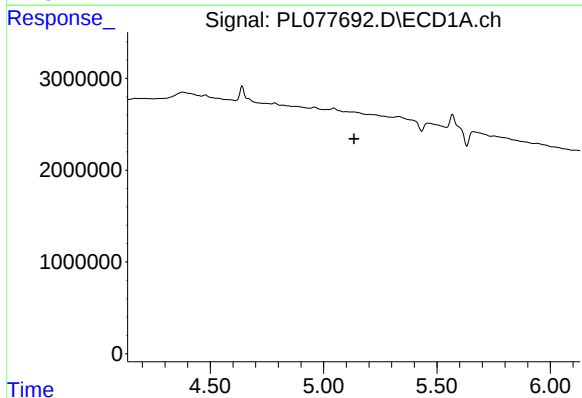


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.134 min
Response: 0
Conc: N.D.

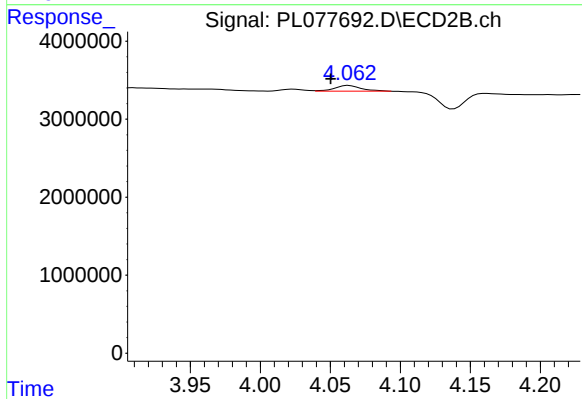

#5 Aldrin


R.T.: 4.063 min
Delta R.T.: 0.013 min
Response: 886701
Conc: 0.23 ng/ml

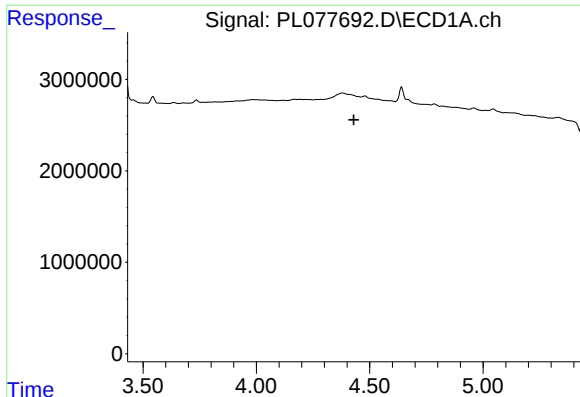

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

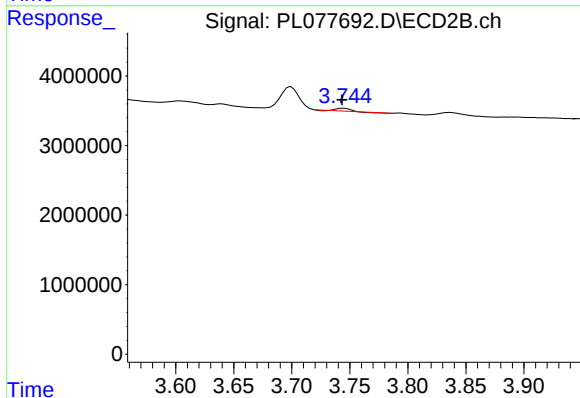


#6 beta-BHC

R.T.: 3.745 min
Delta R.T.: 0.002 min
Response: 289721
Conc: 0.17 ng/ml

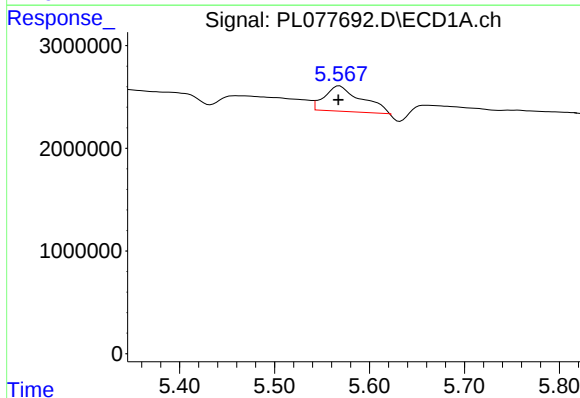


#8 Heptachlor epoxide

R.T.: 5.569 min
Delta R.T.: 0.001 min
Response: 6522016
Conc: 3.74 ng/ml

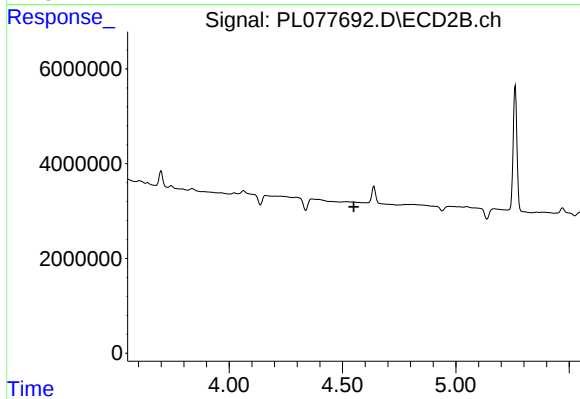

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.549 min
Response: 0
Conc: N.D.

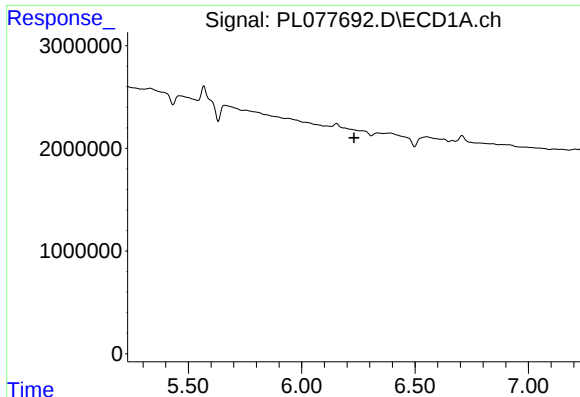

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

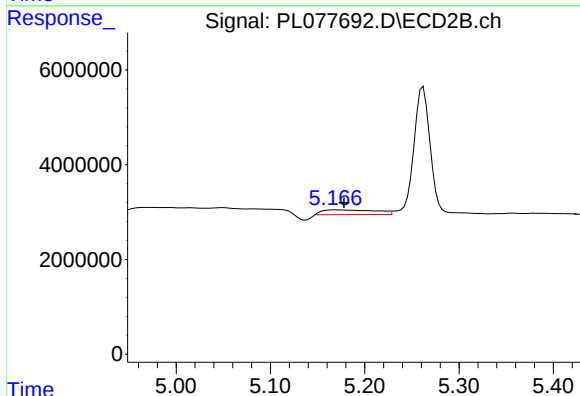


#13 Dieldrin

R.T.: 5.168 min
Delta R.T.: -0.010 min
Response: 3992260
Conc: 1.20 ng/ml

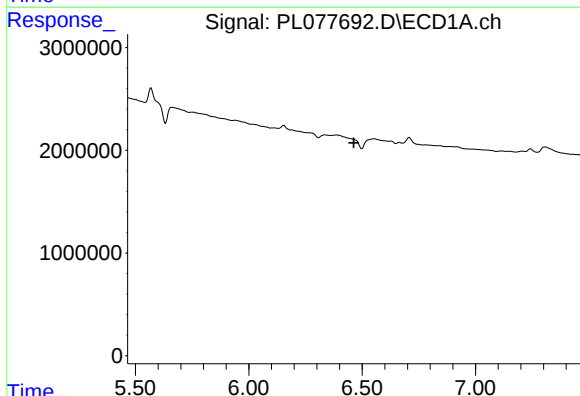


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

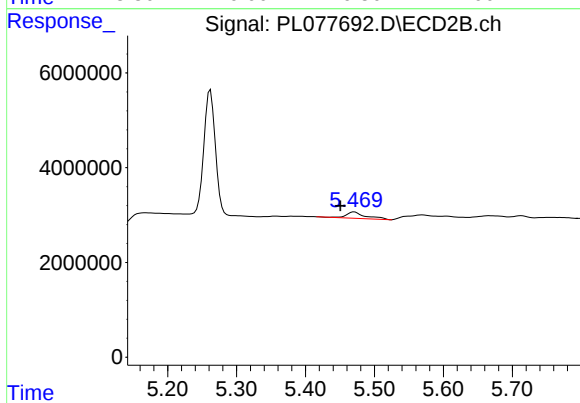

#14 Endrin


R.T.: 5.471 min
Delta R.T.: 0.020 min
Response: 2656257
Conc: 0.93 ng/ml

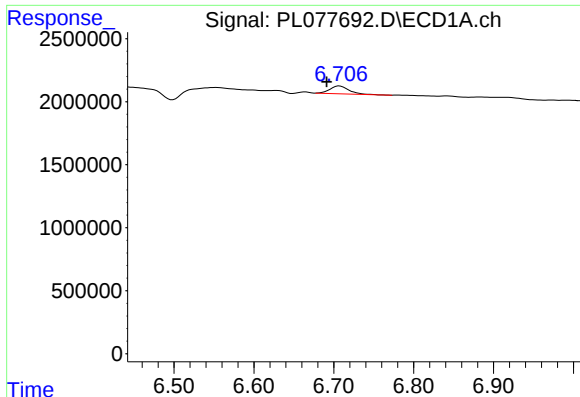

#15 Endosulfan II


R.T.: 6.707 min
Delta R.T.: 0.016 min
Response: 1024447
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

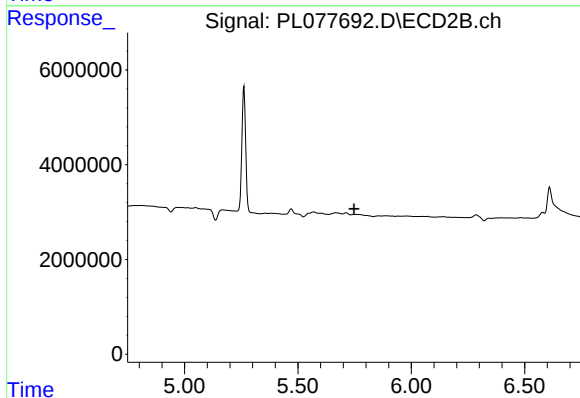


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.747 min
Response: 0
Conc: N.D.

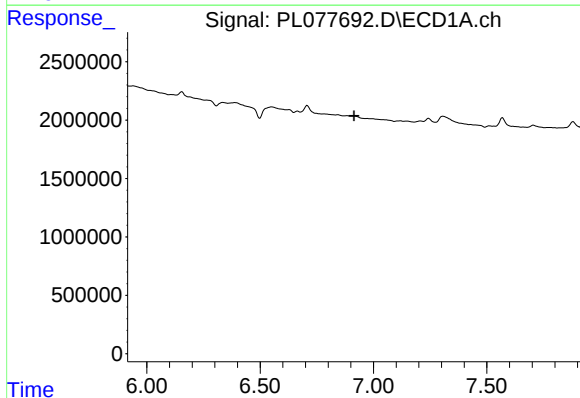


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.915 min
Response: 0
Conc: N.D.

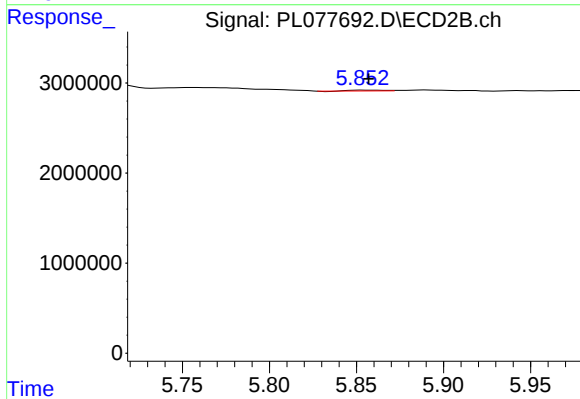

#17 4,4'-DDT


R.T.: 5.853 min
Delta R.T.: -0.004 min
Response: 98383
Conc: 0.04 ng/ml

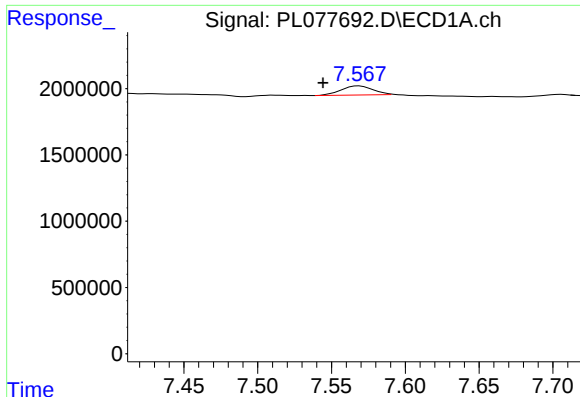

#21 Endrin ketone


R.T.: 7.569 min
Delta R.T.: 0.024 min
Response: 1026914
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

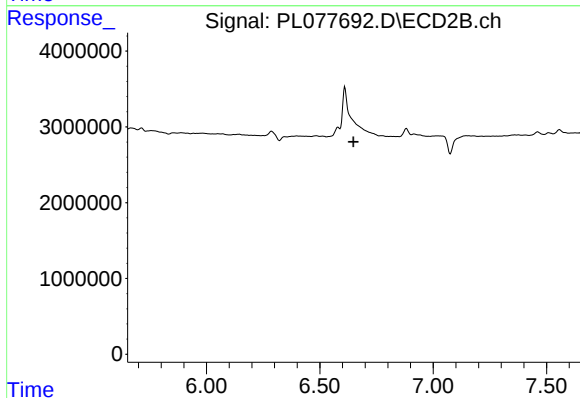


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

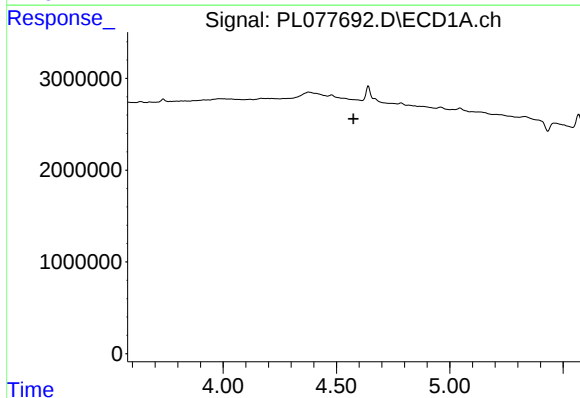


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.575 min
Response: 0
Conc: N.D.

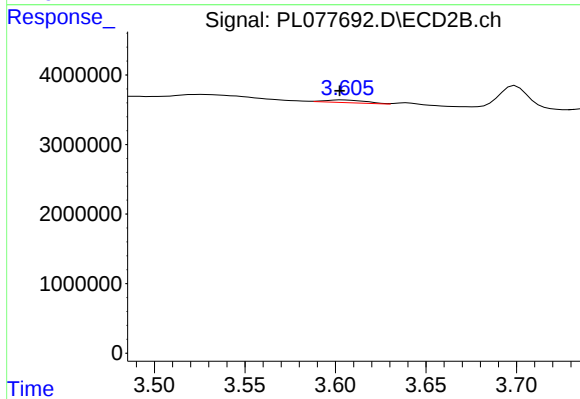

#23 Chlordane-1


R.T.: 3.604 min
Delta R.T.: 0.002 min
Response: 604963
Conc: 5.57 ng/ml

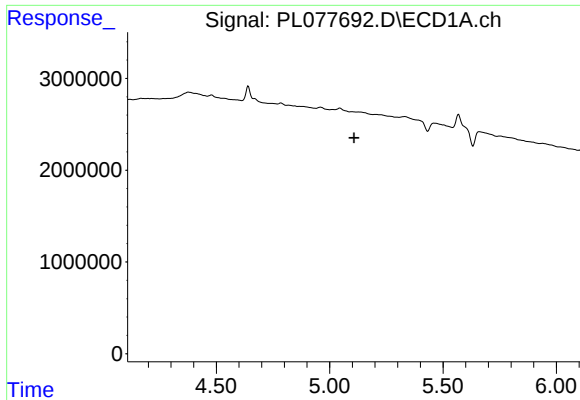

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

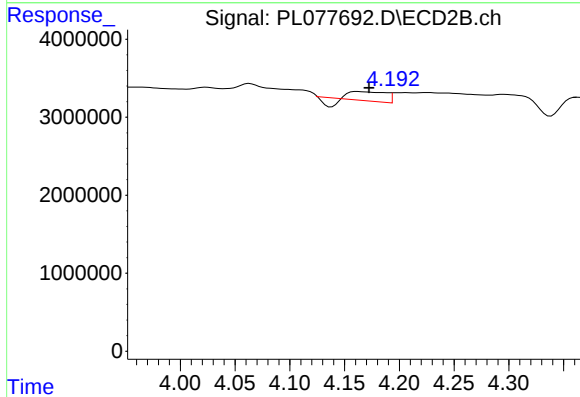


#24 Chlordane-2

R.T.: 4.161 min
Delta R.T.: -0.011 min
Response: 2193661
Conc: 18.31 ng/ml

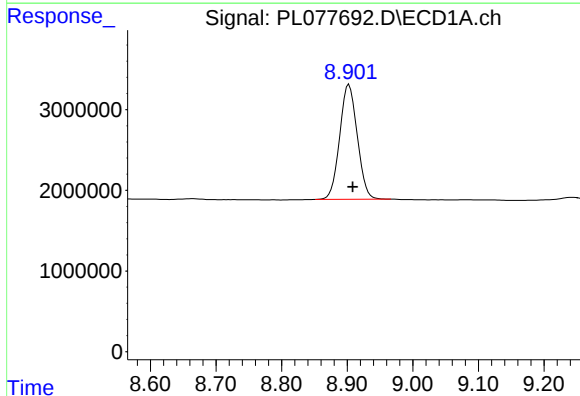

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: -0.006 min
Response: 26573796
Conc: 20.56 ng/ml

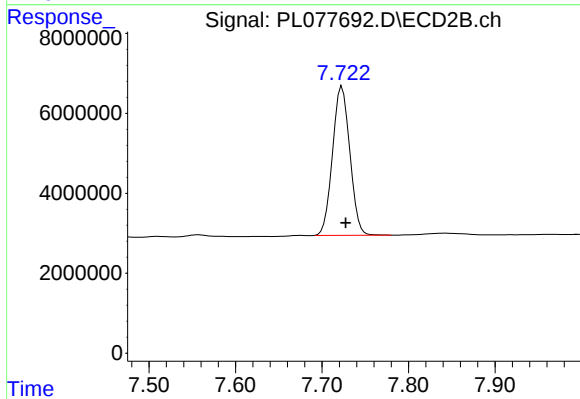

#28 Decachlorobiphenyl

R.T.: 7.723 min
Delta R.T.: -0.004 min
Response: 51697578
Conc: 20.59 ng/ml