

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091223\
 Data File : PL085251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2023 18:02
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:35:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091223CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 12 02:29:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.683	27810998	12845242	10.053	9.957
27)	SA Decachlor...	9.026	7.863	37858678	31229557	21.793	20.648
Target Compounds							
22)	Toxaphene-1	6.190	5.251	17690139	6753101	1039.801	1021.068
23)	Toxaphene-2	7.015	5.612	58345836	8673425	980.300	964.853
24)	Toxaphene-3	7.104	6.657	41271342	40334714	972.960	935.860
25)	Toxaphene-4	7.202	6.973	23678825	26375846	977.231	949.080
26)	Toxaphene-5	7.891	7.107	30165897	15725583	1002.668	922.979

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091223\
Data File : PL085251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2023 18:02
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:35:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091223CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 12 02:29:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

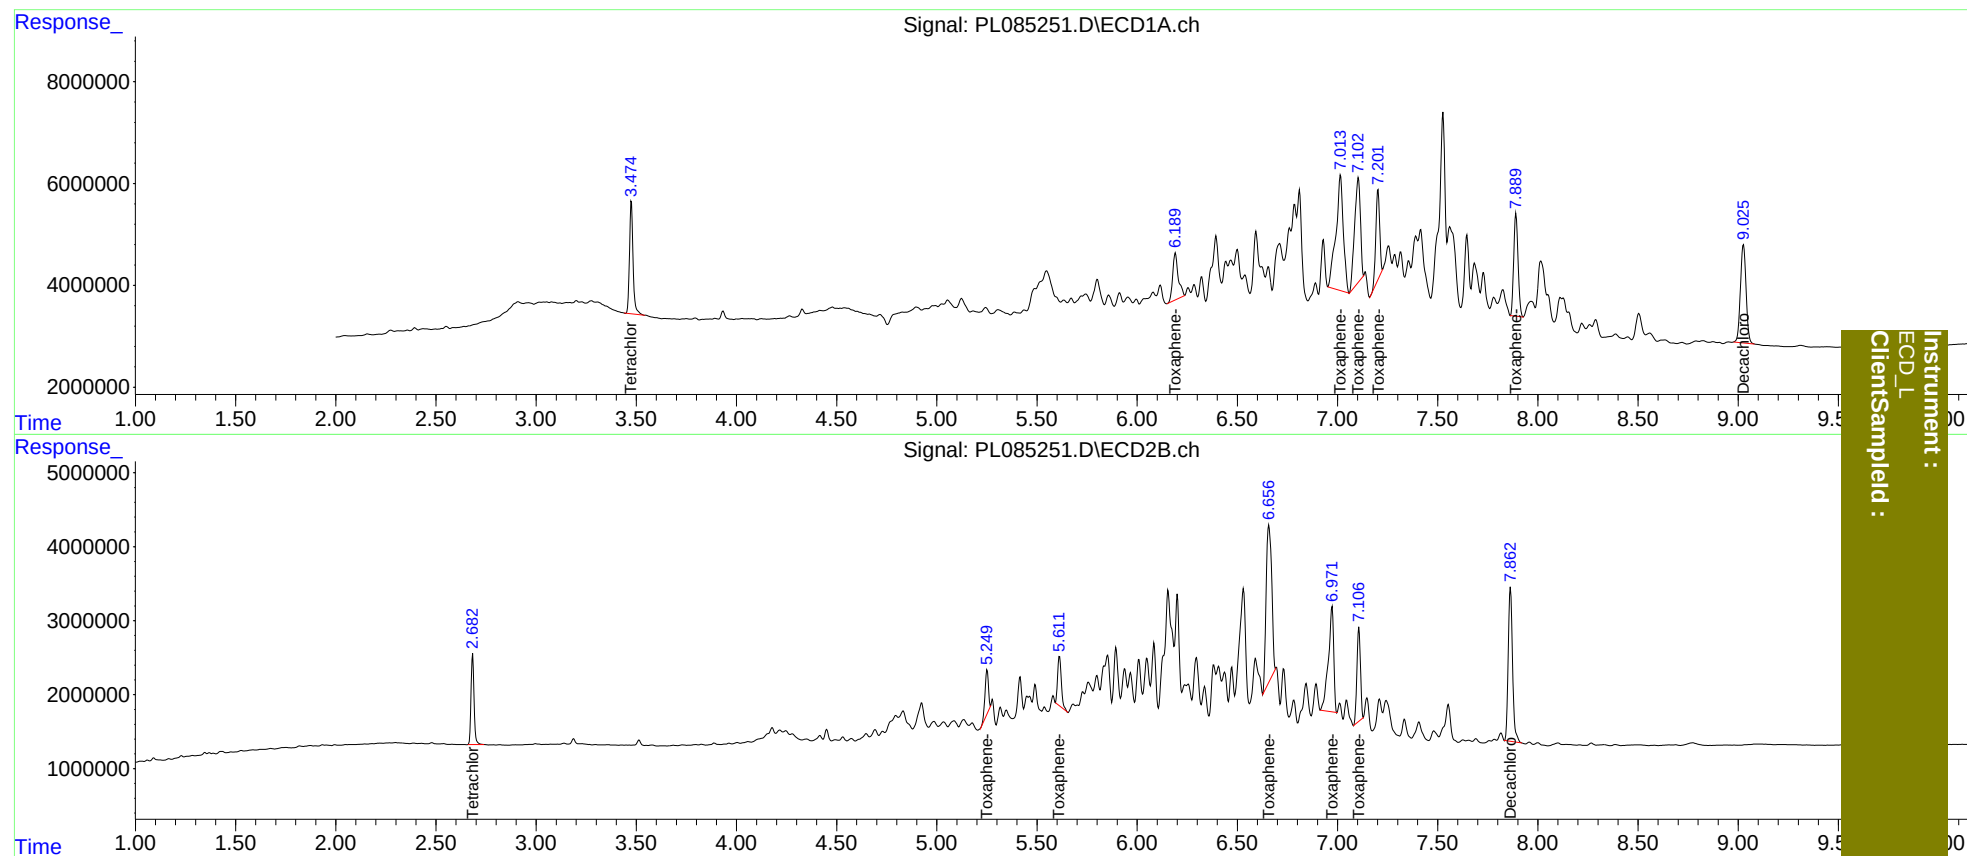

Instrument :
ECD_L
ClientSampled :
PL091223CLP.M Tue Sep 12 02:36:01 2023