

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091223\
 Data File : PL085253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2023 18:30
 Operator : AR\AJ
 Sample : TOXAPH401
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:33:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091223CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 12 02:29:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.683	109.4E6	51264354	39.617	39.678
27)	SA Decachlor...	9.026	7.863	132.1E6	118.3E6	78.405	79.044
Target Compounds							
22)	Toxaphene-1	6.190	5.251	66589523	26188373	3966.660	3987.683
23)	Toxaphene-2	7.014	5.612	234.5E6	36642715	3914.524	4029.024
24)	Toxaphene-3	7.104	6.657	166.1E6	180.5E6	3880.591	4099.646
25)	Toxaphene-4	7.202	6.972	97864076	113.1E6	4008.450	4003.461
26)	Toxaphene-5	7.890	7.107	118.2E6	69896999	3932.476	3999.763

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091223\
Data File : PL085253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2023 18:30
Operator : AR\AJ
Sample : TOXAPH401
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:33:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091223CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 12 02:29:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

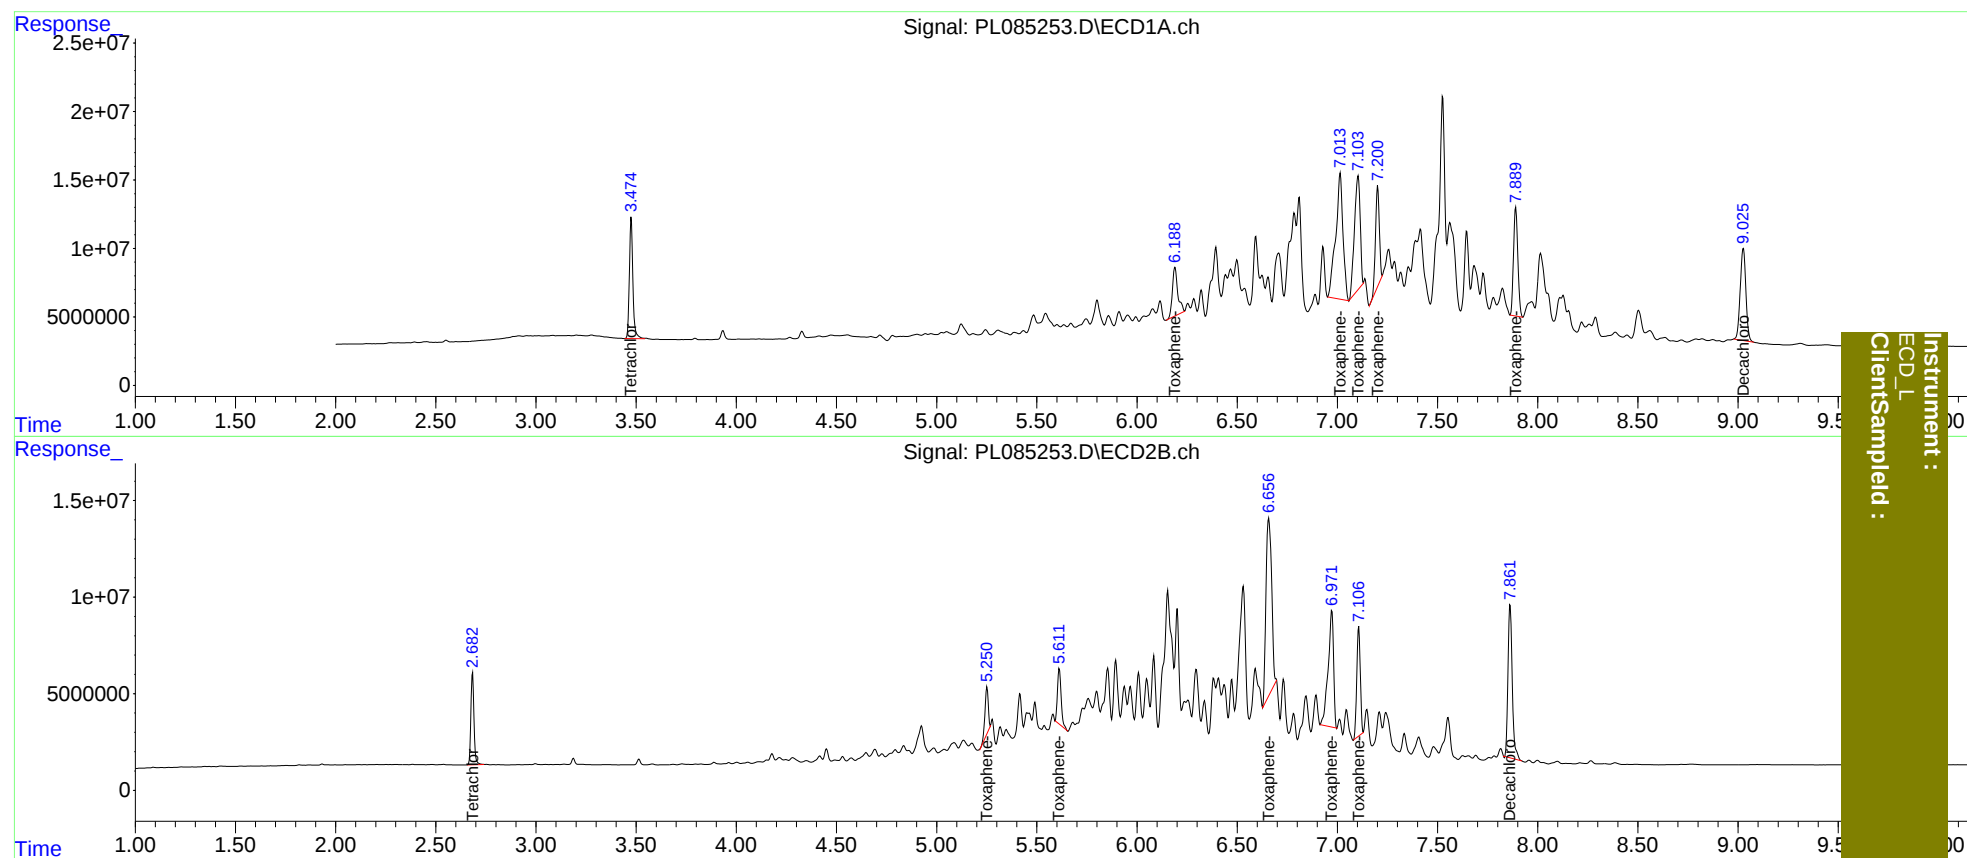

Instrument :
ECD_L
ClientSampled :
PL091223CLP.M Tue Sep 12 02:34:01 2023