

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091319\
 Data File : PL052439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2019 10:58
 Operator : SG\AJ
 Sample : K4850-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AOC-7-(8)

Manual Integrations
 APPROVED

Ankita

9/16/2019 5:55:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 23:18:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 12 03:37:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.311	3.923	138.0E6	42792747	15.322m	19.650 #
28)	SA Decachlor...	7.967	8.944	73241551	17488679	5.220m	5.894

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091319\
Data File : PL052439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2019 10:58
Operator : SG\AJ
Sample : K4850-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AOC-7-(8)



Manual Integrations
APPROVED


Ankita

9/16/2019 5:55:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 23:18:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
Quant Title : GC Extractables
QLast Update : Thu Sep 12 03:37:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

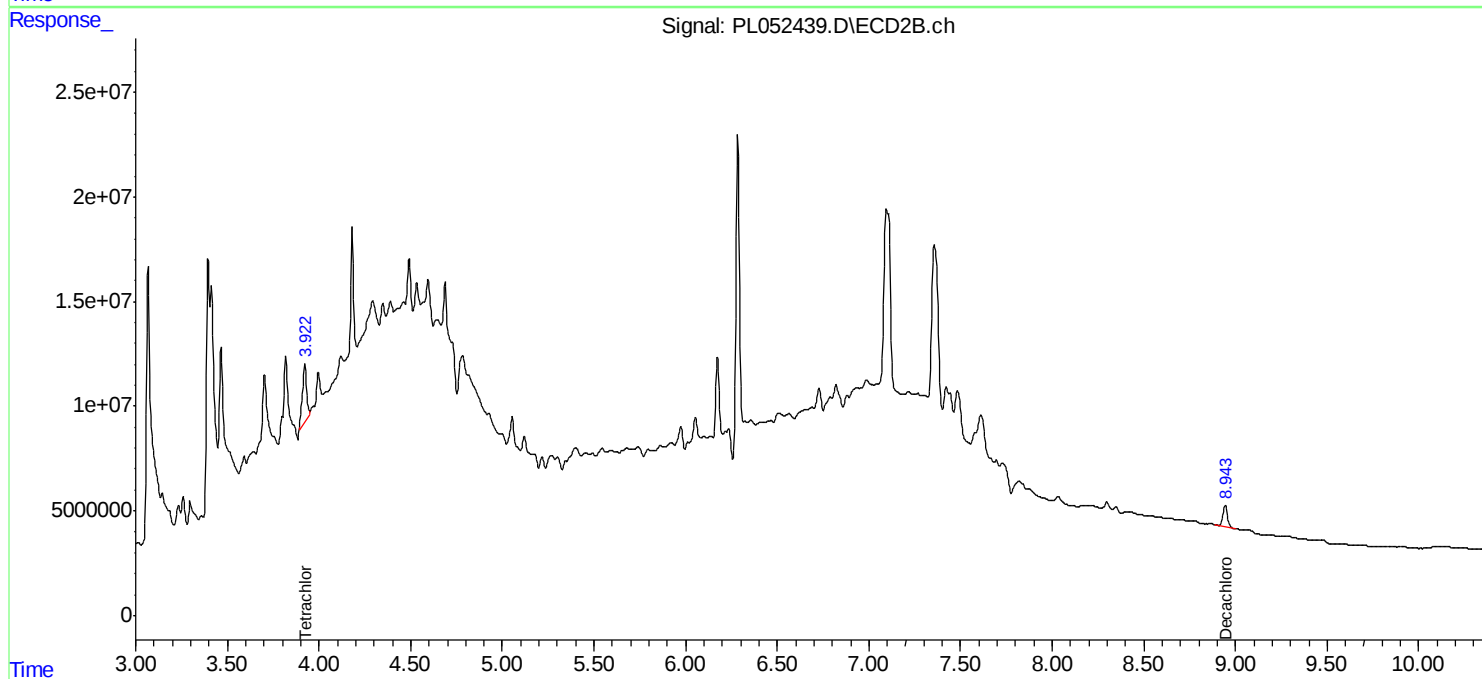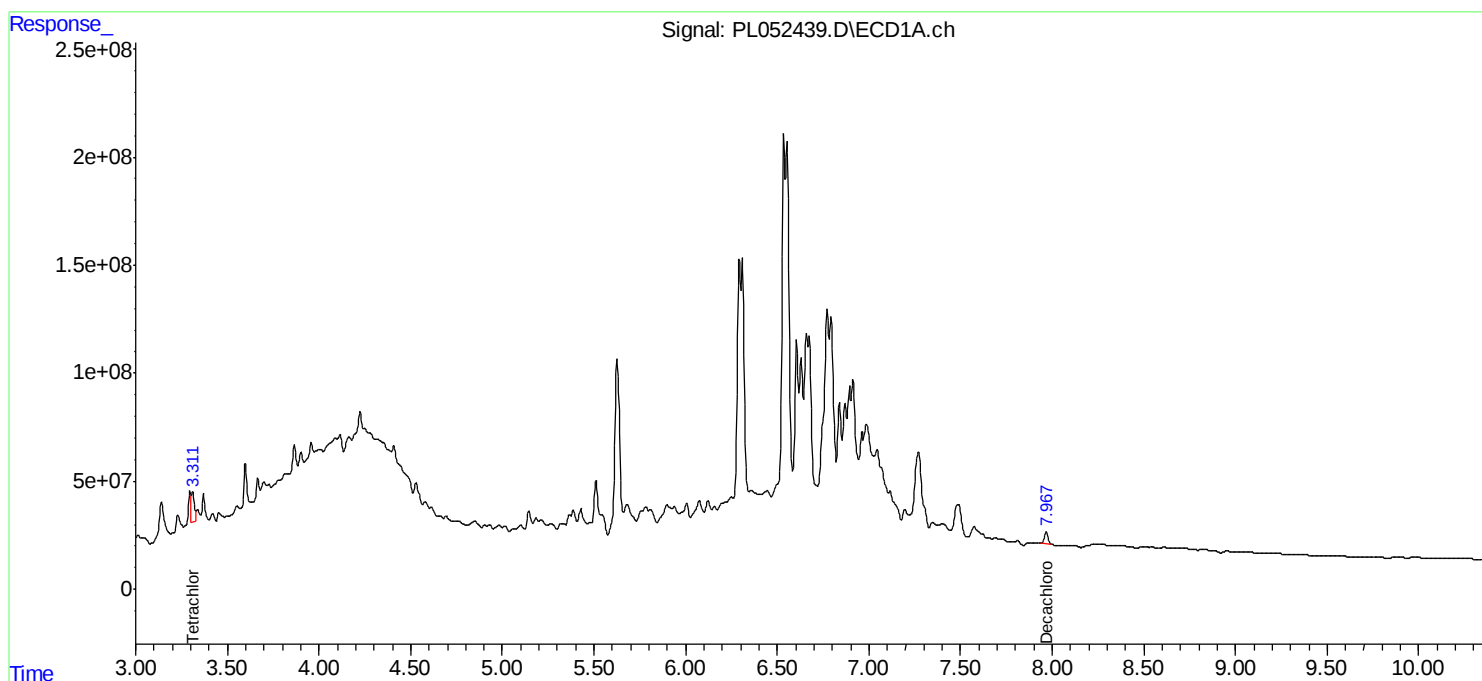

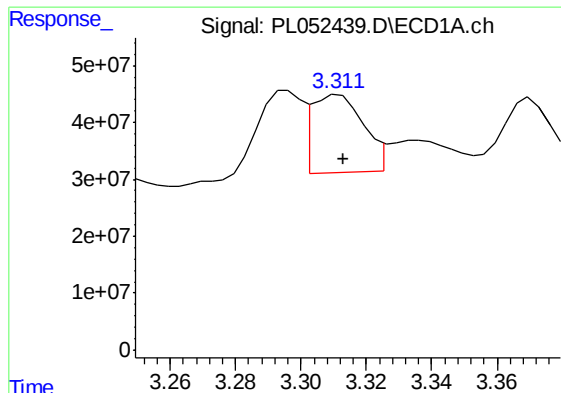

#1 Tetrachloro-m-xylene


R.T.: 3.311 min
Delta R.T.: -0.002 min
Response: 138045484
Conc: 15.32 ng/ml m

Instrument :
ECD_L
ClientSampleId :
AOC-7-(8)

Manual Integrations
APPROVED


Ankita

9/16/2019 5:55:09 PM

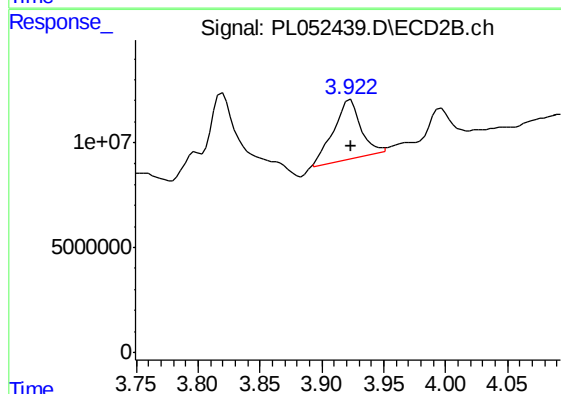


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.001 min
Response: 42792747
Conc: 19.65 ng/ml

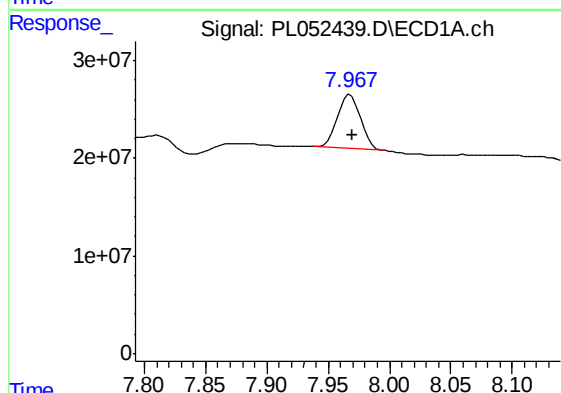

#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.003 min
Response: 73241551
Conc: 5.22 ng/ml m

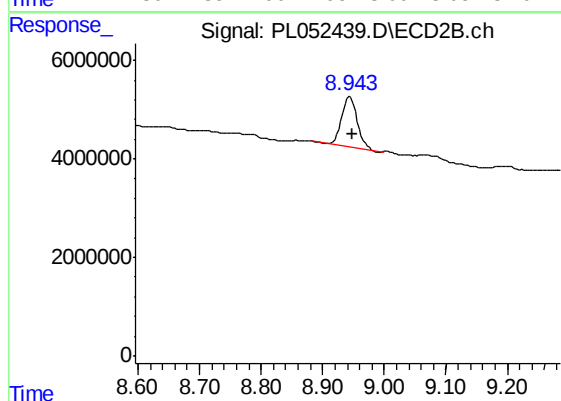

#28 Decachlorobiphenyl

R.T.: 8.944 min
Delta R.T.: -0.004 min
Response: 17488679
Conc: 5.89 ng/ml