

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091319\
 Data File : PL052445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2019 14:11
 Operator : SG\AJ
 Sample : K4666-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-03-091219-A

Manual Integrations
 APPROVED

Ankita
 9/16/2019 5:55:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 09:00:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 12 03:37:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.923	137.3E6	29586950	15.244	13.586
28)	SA Decachlor...	7.969	8.945	123.9E6	31628736	8.833	10.660
Target Compounds							
10)	B gamma-Chl...	5.191	6.014	17571971	4119376	1.073m	1.085m
11)	B alpha-Chl...	5.248	6.085	17577089	8778230	1.106m	2.404m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091319\
Data File : PL052445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2019 14:11
Operator : SG\AJ
Sample : K4666-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PL-03-091219-A


Manual Integrations
APPROVED

Ankita
9/16/2019 5:55:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 09:00:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
Quant Title : GC Extractables
QLast Update : Thu Sep 12 03:37:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

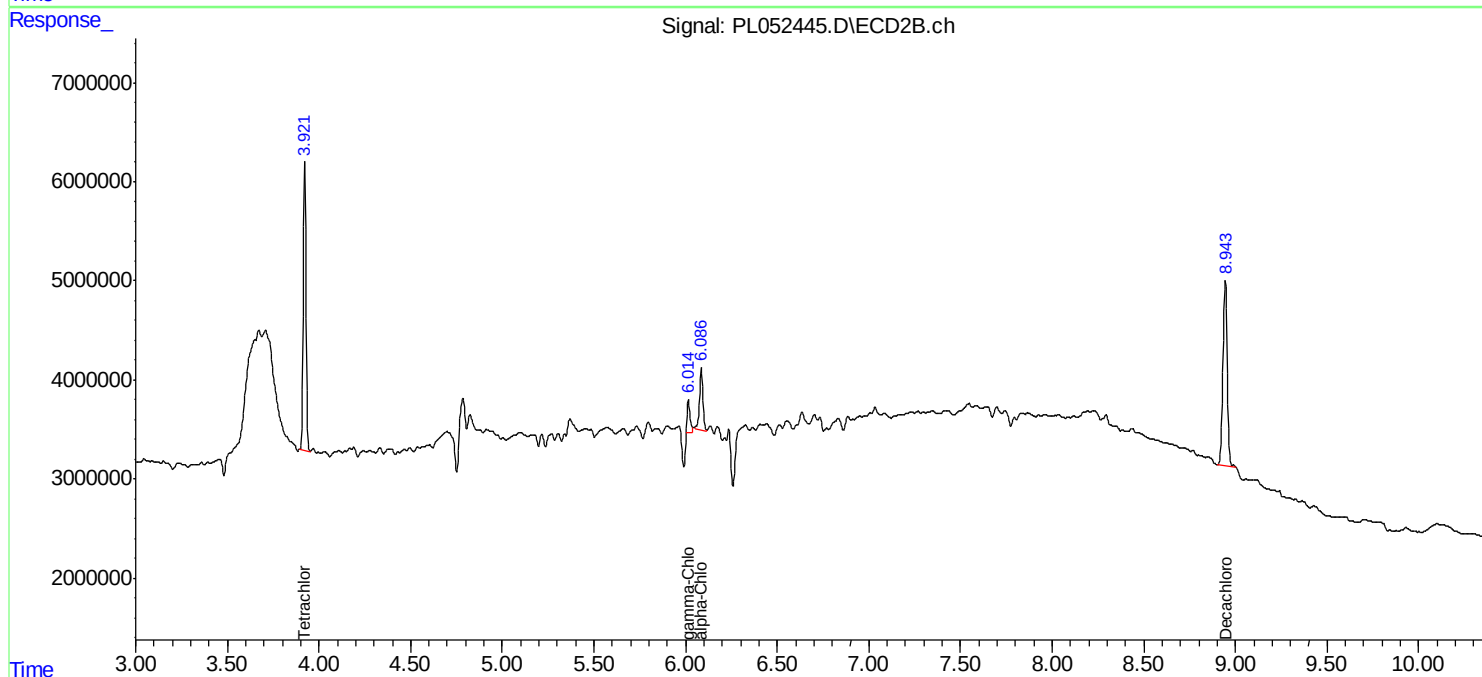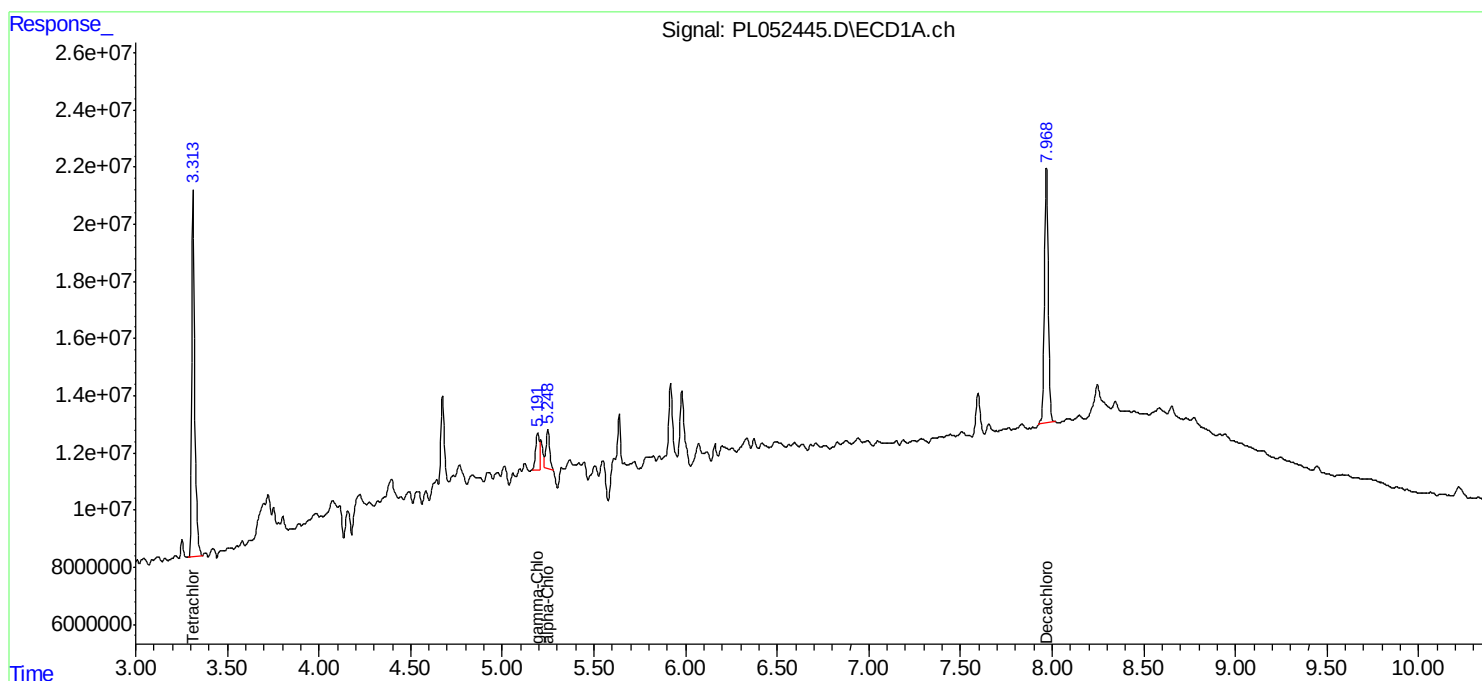

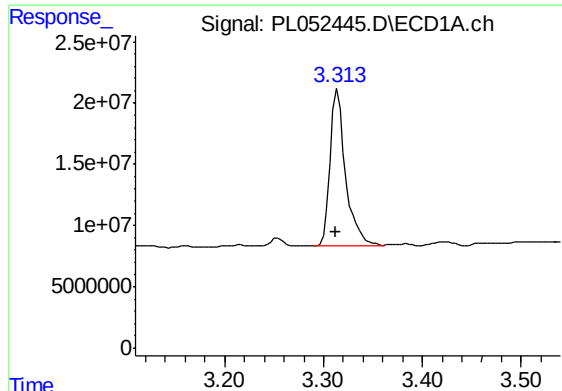


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: 0.001 min
Response: 137348326
Conc: 15.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-03-091219-A


Manual Integrations
APPROVED

Ankita
9/16/2019 5:55:13 PM

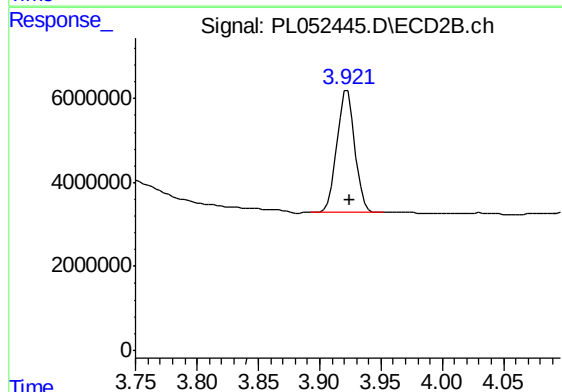


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.001 min
Response: 29586950
Conc: 13.59 ng/ml

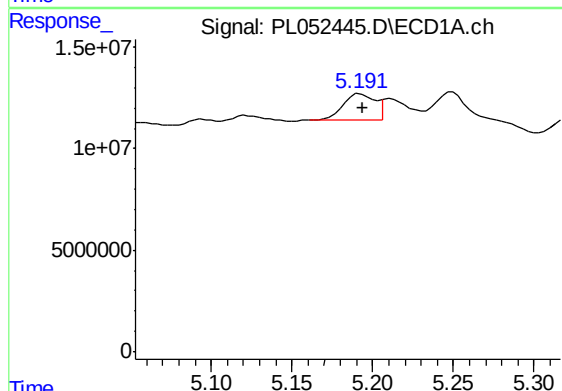


#10 gamma-Chlordane

R.T.: 5.191 min
Delta R.T.: -0.003 min
Response: 17571971
Conc: 1.07 ng/ml m

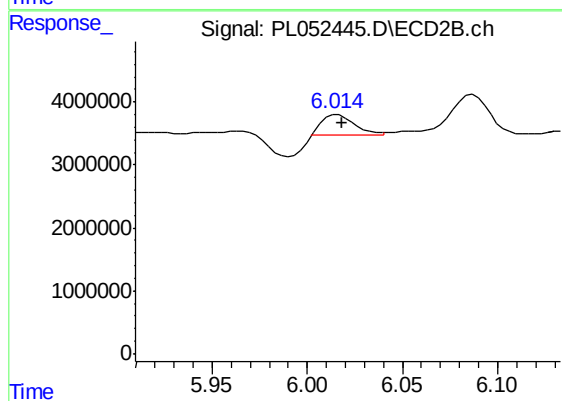

#10 gamma-Chlordane

R.T.: 6.014 min
Delta R.T.: -0.004 min
Response: 4119376
Conc: 1.09 ng/ml m

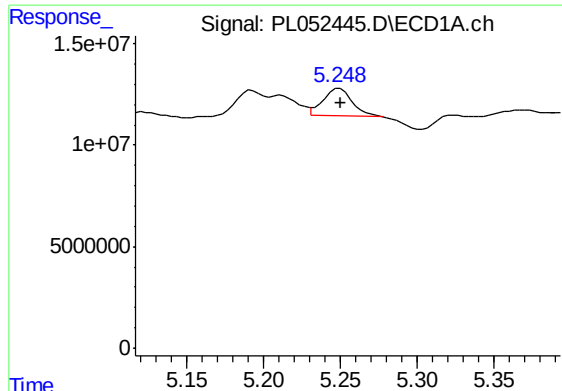


#11 alpha-Chlordane

R.T.: 5.248 min
Delta R.T.: -0.002 min
Response: 17577089
Conc: 1.11 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PL-03-091219-A


Manual Integrations
APPROVED

Ankita
9/16/2019 5:55:13 PM

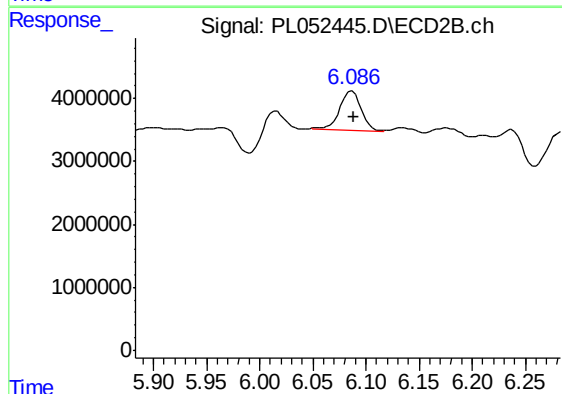


#11 alpha-Chlordane

R.T.: 6.085 min
Delta R.T.: -0.003 min
Response: 8778230
Conc: 2.40 ng/ml m

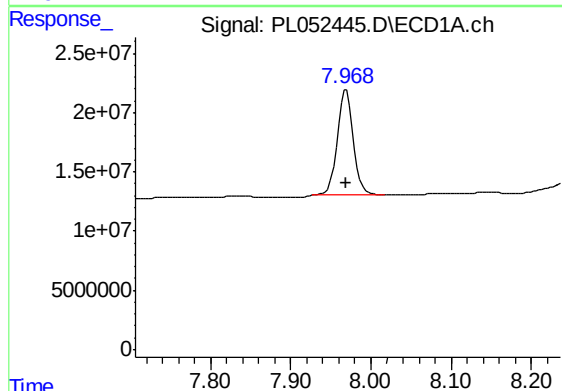

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 123936296
Conc: 8.83 ng/ml

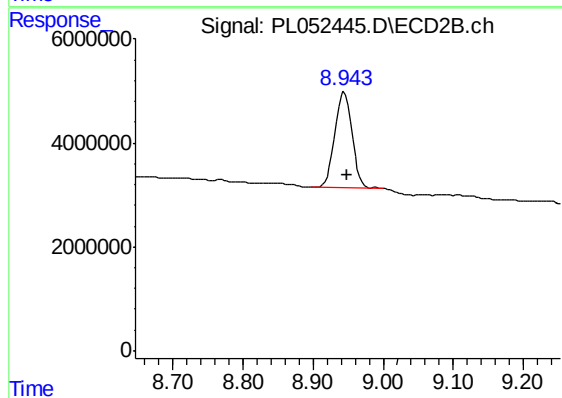

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.004 min
Response: 31628736
Conc: 10.66 ng/ml