

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091319\
 Data File : PL052455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2019 17:09
 Operator : SG\AJ
 Sample : K4861-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-11-D(4-6.5)

Manual Integrations
 APPROVED

Ankita
 9/16/2019 5:55:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 09:03:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 12 03:37:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.313	3.923	197.9E6	46555660	21.964	21.378
28) SA Decachlor...	7.967	8.944	152.8E6	37338220	10.894	12.584
Target Compounds						
17) MA 4,4'-DDT	6.154	7.031	16298246	1679767	1.158m	0.529m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091319\
Data File : PL052455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2019 17:09
Operator : SG\AJ
Sample : K4861-07
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-11-D(4-6.5)


Manual Integrations
APPROVED

Ankita
9/16/2019 5:55:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 09:03:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091119.M
Quant Title : GC Extractables
QLast Update : Thu Sep 12 03:37:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

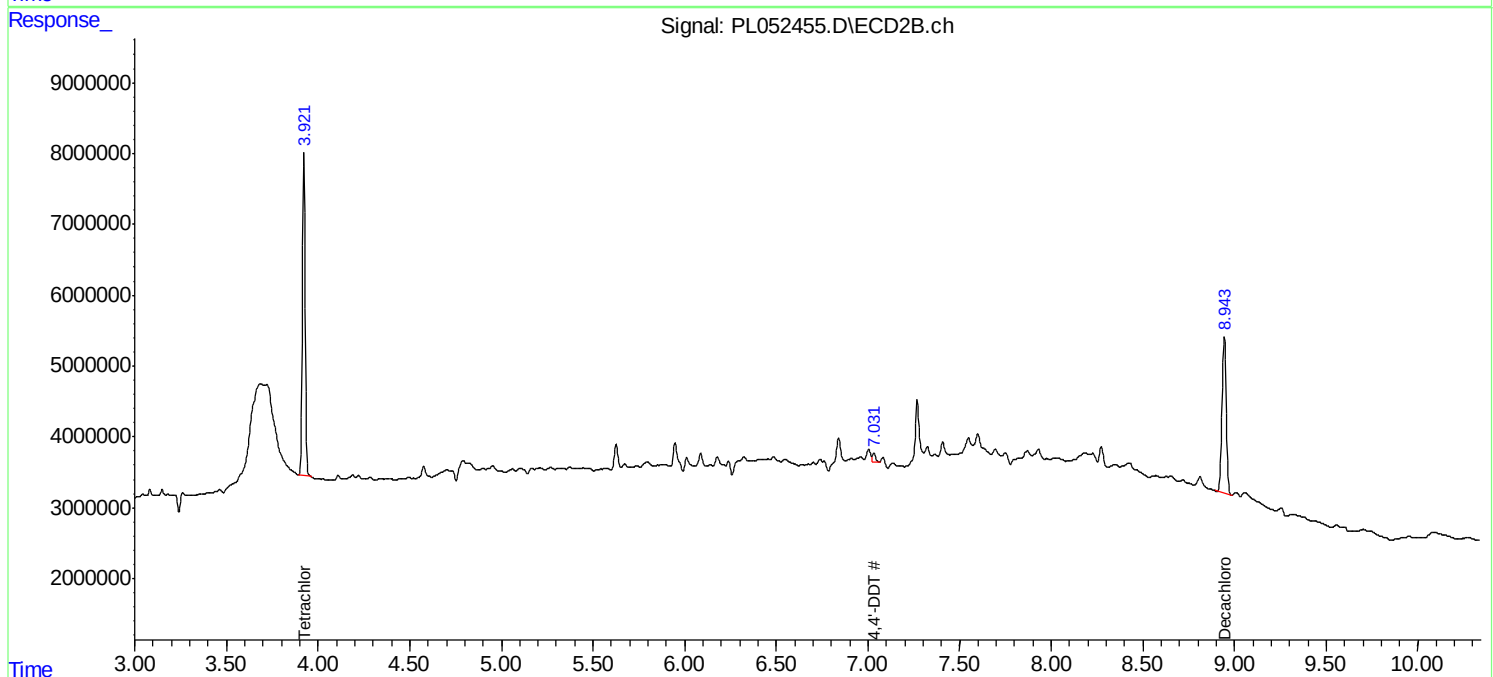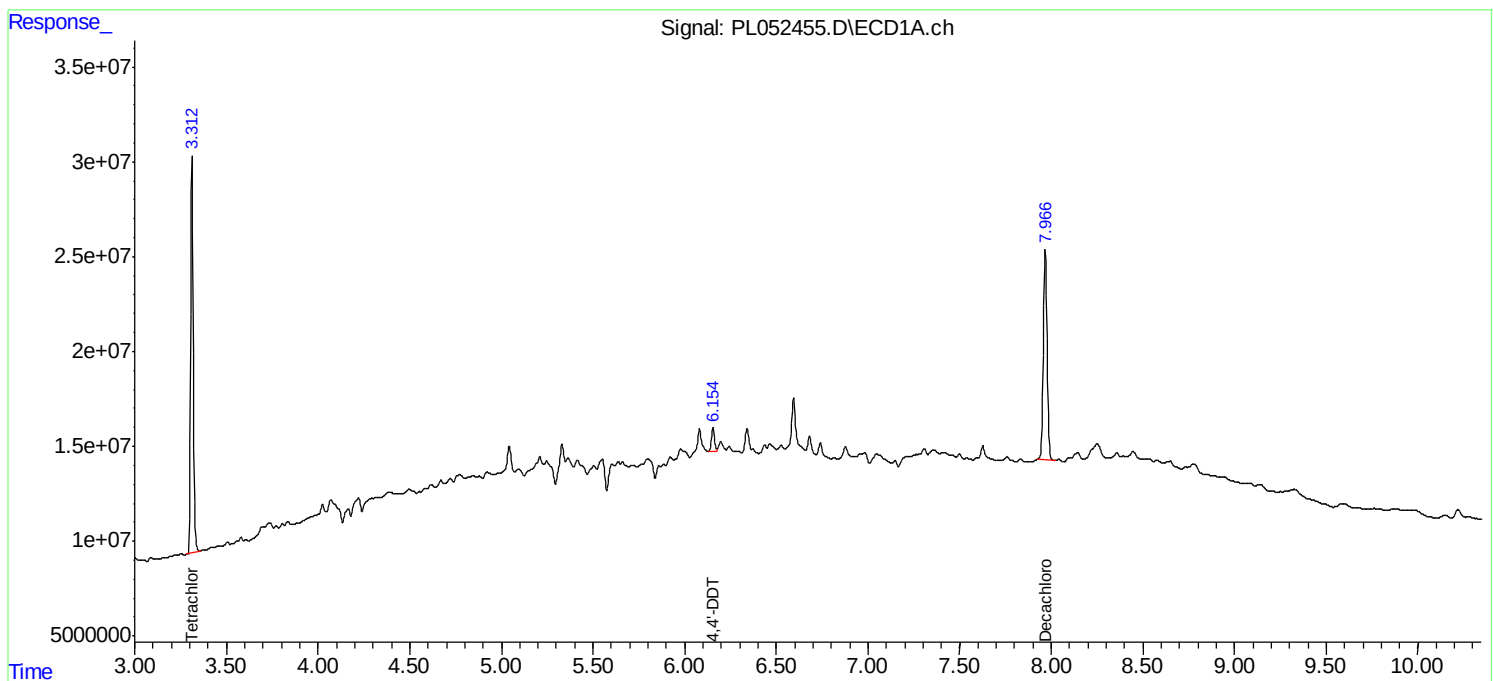

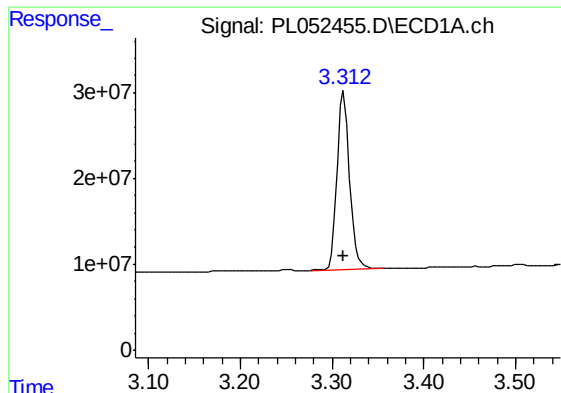


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 197891187
Conc: 21.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11-D(4-6.5)


Manual Integrations
APPROVED

Ankita
9/16/2019 5:55:32 PM

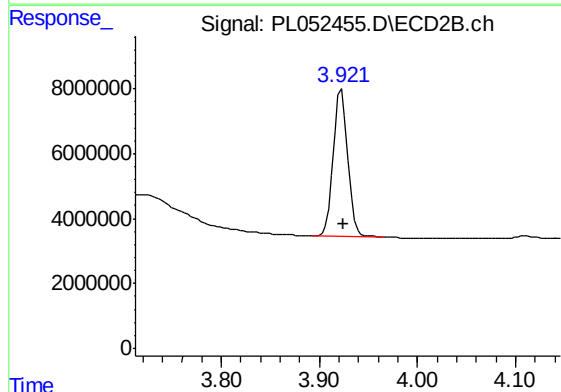


#1 Tetrachloro-m-xylene

R.T.: 3.923 min
Delta R.T.: -0.001 min
Response: 46555660
Conc: 21.38 ng/ml

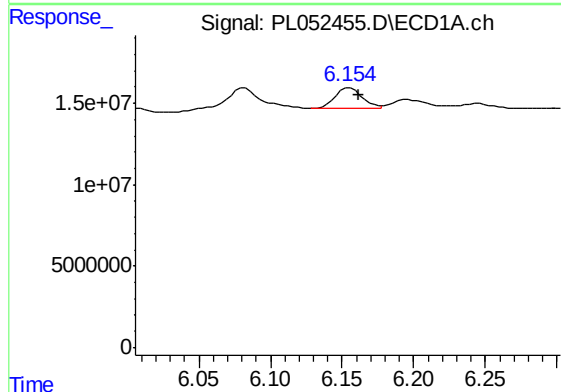


#17 4,4'-DDT

R.T.: 6.154 min
Delta R.T.: -0.008 min
Response: 16298246
Conc: 1.16 ng/ml m

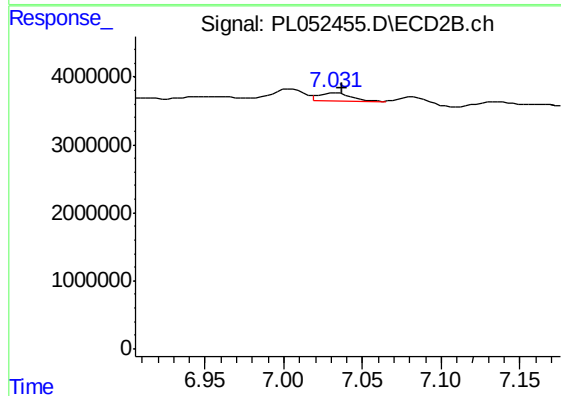

#17 4,4'-DDT

R.T.: 7.031 min
Delta R.T.: -0.005 min
Response: 1679767
Conc: 0.53 ng/ml m

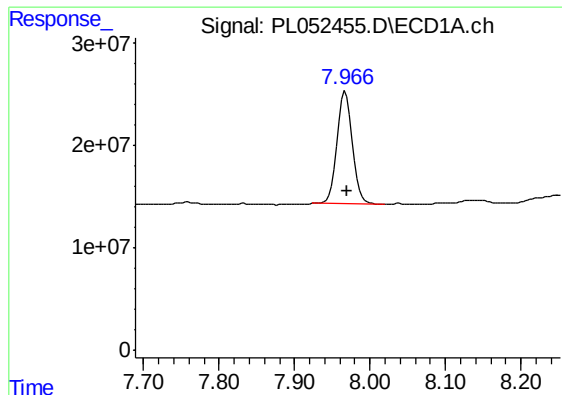


#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.002 min
Response: 152845537
Conc: 10.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11-D(4-6.5)

Manual Integrations
APPROVED

Ankita
9/16/2019 5:55:32 PM

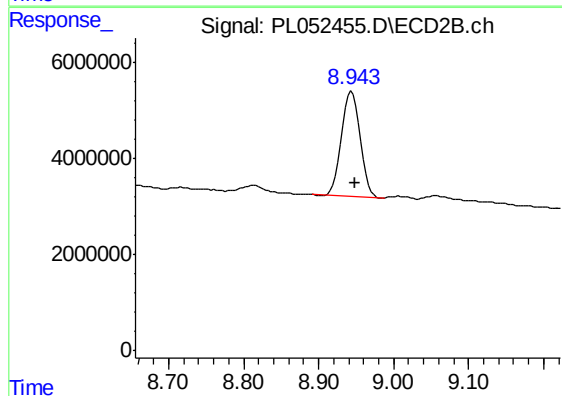

#28 Decachlorobiphenyl

R.T.: 8.944 min
Delta R.T.: -0.004 min
Response: 37338220
Conc: 12.58 ng/ml