

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091321\
 Data File : PL069808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2021 09:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 03:46:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.630	5.565	9230856	26160227	22.657	21.492
28)	SA Decachlor...	10.396	11.485	15672197	24043030	21.281	21.042
Target Compounds							
7)	B delta-BHC	0.000	7.081f	0	702404	N.D.	0.422 #
9)	A Endosulfan I	0.000	8.449	0	272046	N.D.	0.210 #
11)	B alpha-Chl...	0.000	8.366	0	1264923	N.D.	0.929 #
12)	B 4,4'-DDE	0.000	8.592f	0	1235917	N.D.	0.935 #
16)	A 4,4'-DDD	0.000	9.099	0	1209148	N.D.	1.136 #
17)	MA 4,4'-DDT	0.000	9.446f	0	926445	N.D.	0.828 #
19)	B Endosulfa...	0.000	9.587f	0	405792	N.D.	0.360 #
26)	Chlordane-4	0.000	8.366f	0	1264923	N.D.	5.432 #
27)	Chlordane-5	0.000	9.274	0	449300	N.D.	10.684 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091321\
Data File : PL069808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2021 09:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 03:46:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

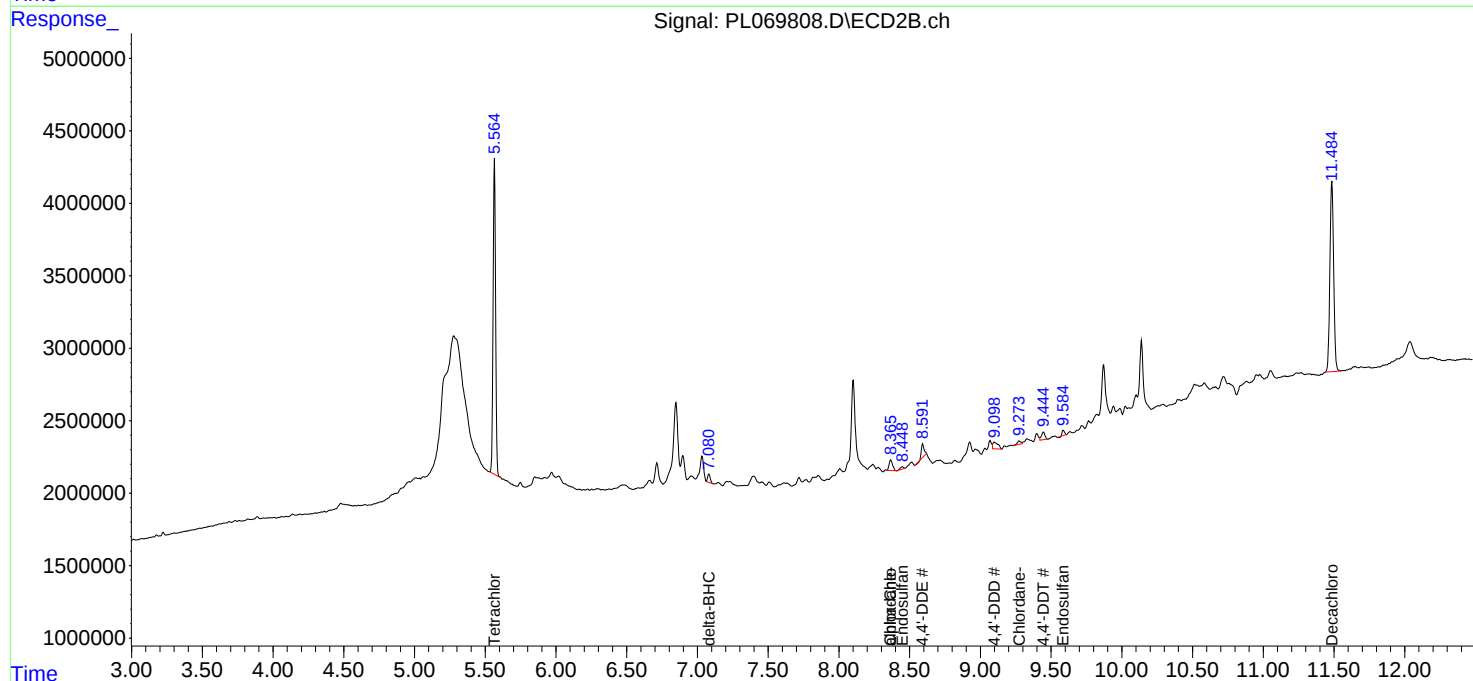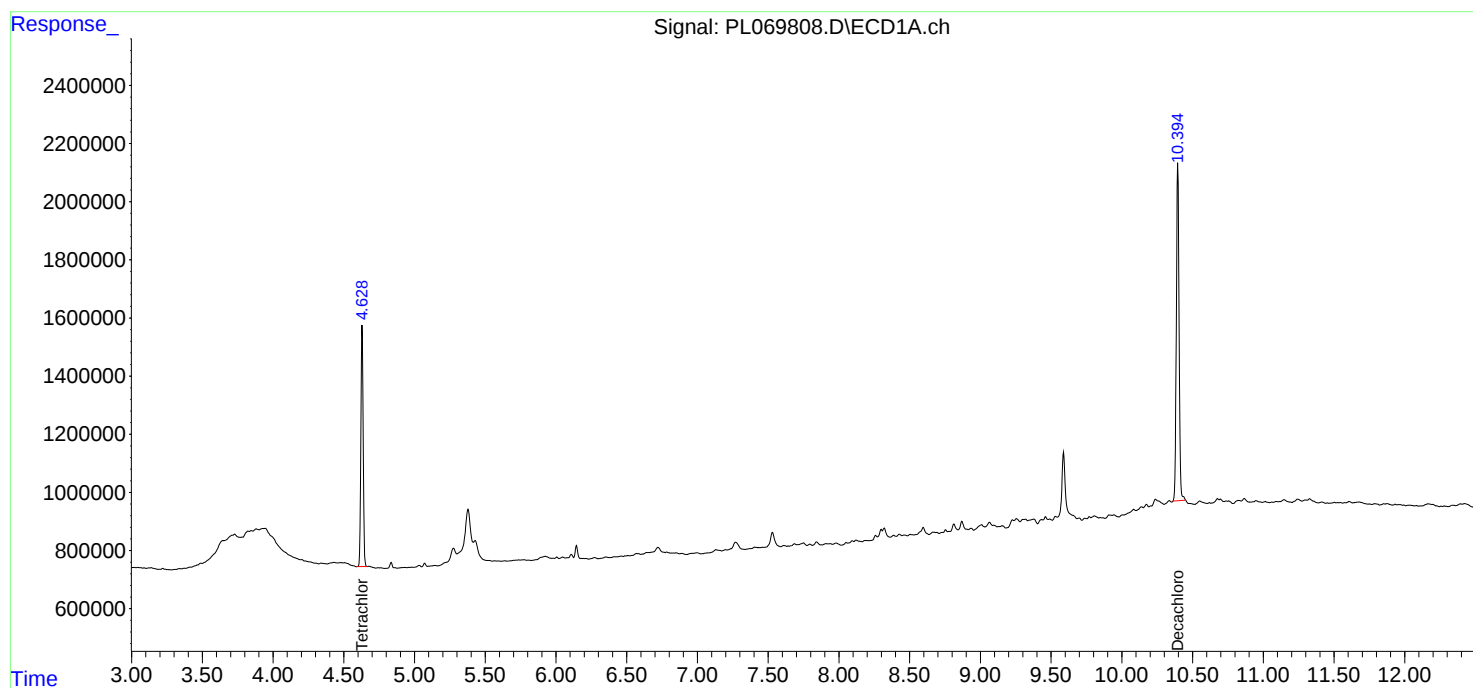


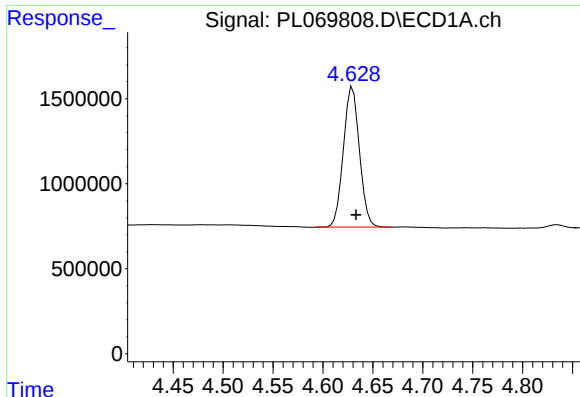

#1 Tetrachloro-m-xylene


R.T.: 4.630 min
Delta R.T.: -0.003 min
Response: 9230856
Conc: 22.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

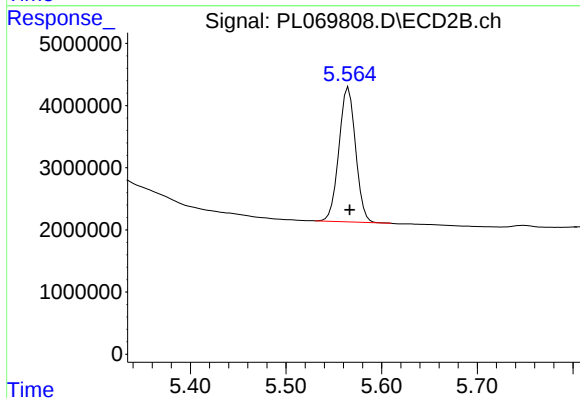


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: -0.001 min
Response: 26160227
Conc: 21.49 ng/ml

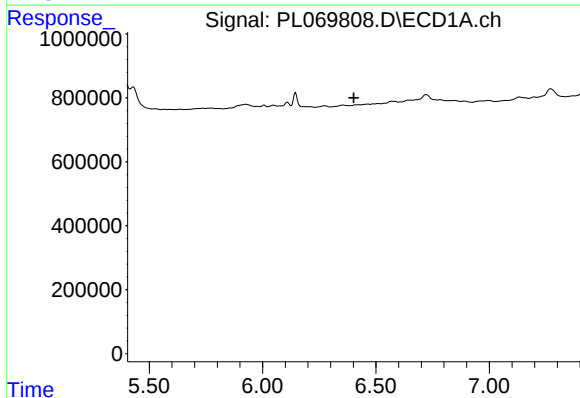


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

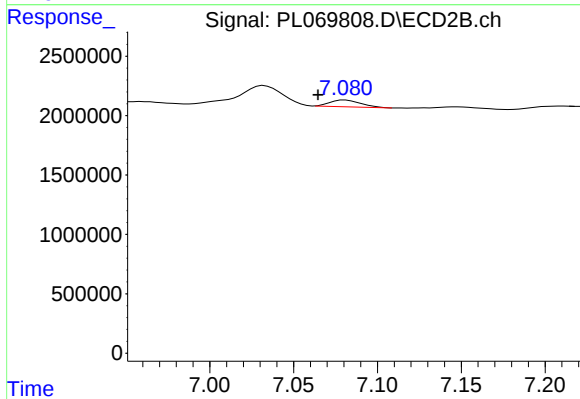

#7 delta-BHC


R.T.: 7.081 min
Delta R.T.: 0.016 min
Response: 702404
Conc: 0.42 ng/ml

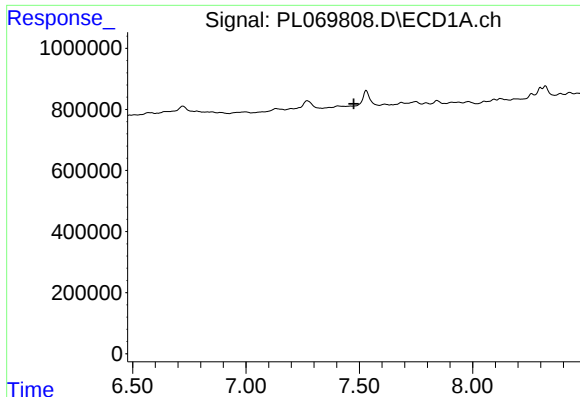

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

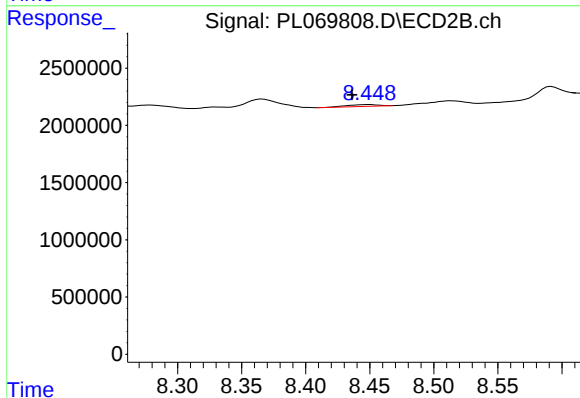


#9 Endosulfan I

R.T.: 8.449 min
Delta R.T.: 0.013 min
Response: 272046
Conc: 0.21 ng/ml

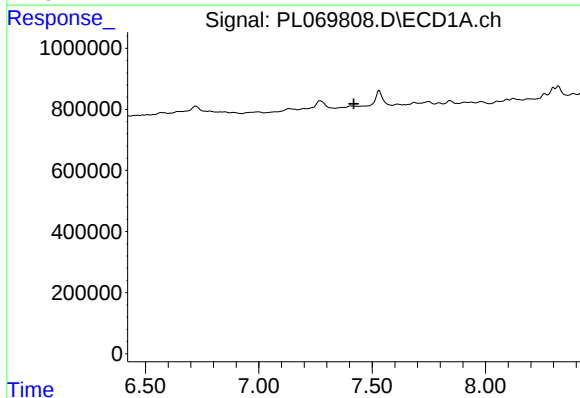


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

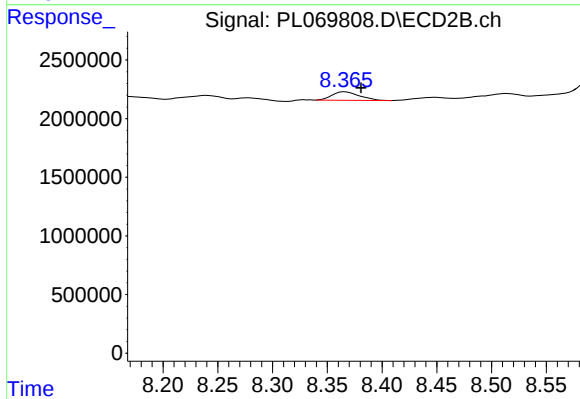

#11 alpha-Chlordane


R.T.: 8.366 min
Delta R.T.: -0.015 min
Response: 1264923
Conc: 0.93 ng/ml

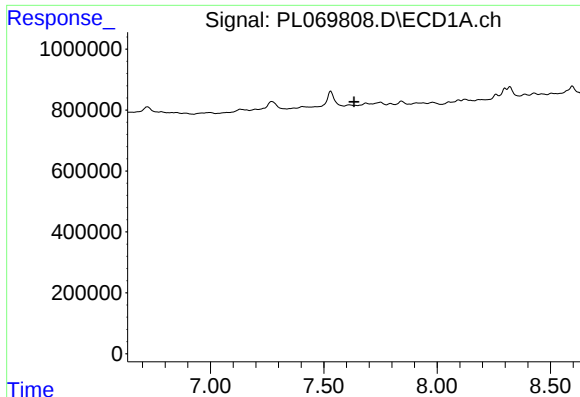

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.633 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

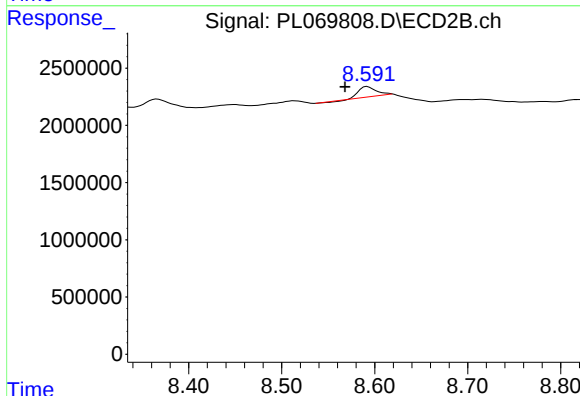


#12 4,4'-DDE

R.T.: 8.592 min
Delta R.T.: 0.024 min
Response: 1235917
Conc: 0.94 ng/ml

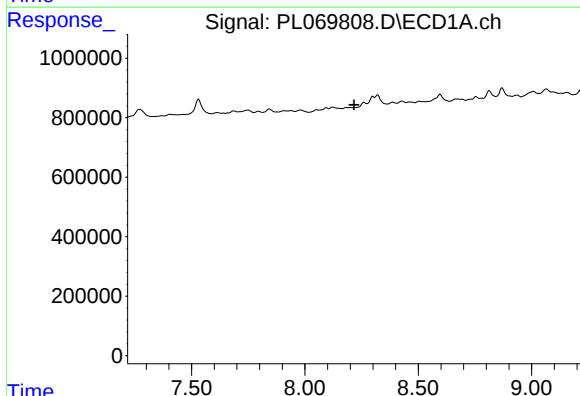


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.218 min
Response: 0
Conc: N.D.

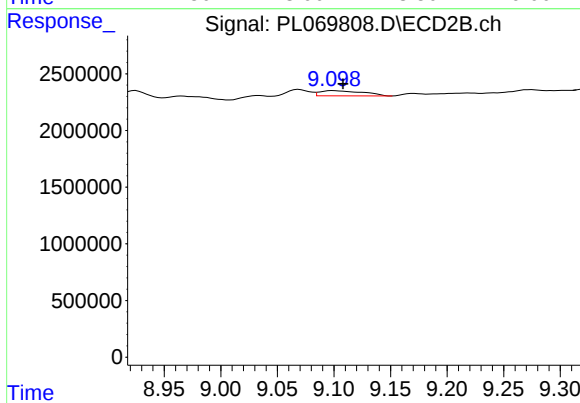

#16 4,4'-DDD


R.T.: 9.099 min
Delta R.T.: -0.009 min
Response: 1209148
Conc: 1.14 ng/ml

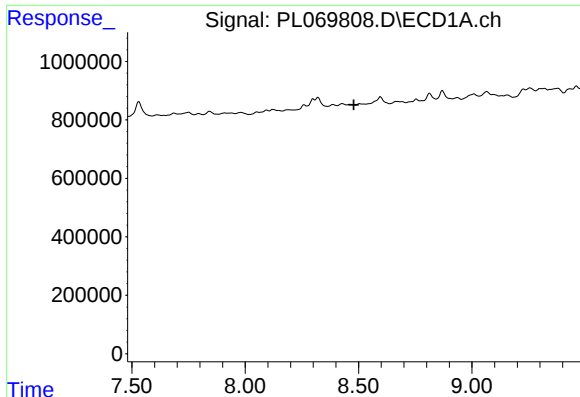

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

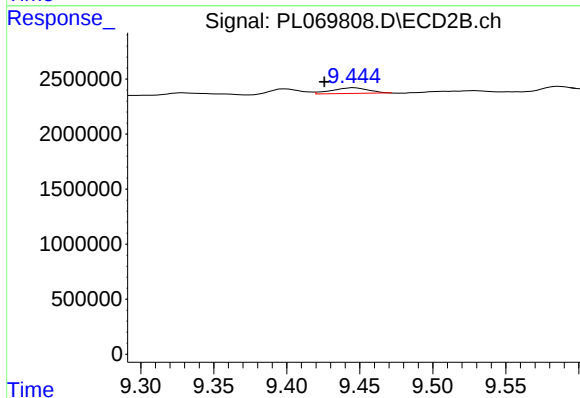


#17 4,4'-DDT

R.T.: 9.446 min
Delta R.T.: 0.021 min
Response: 926445
Conc: 0.83 ng/ml

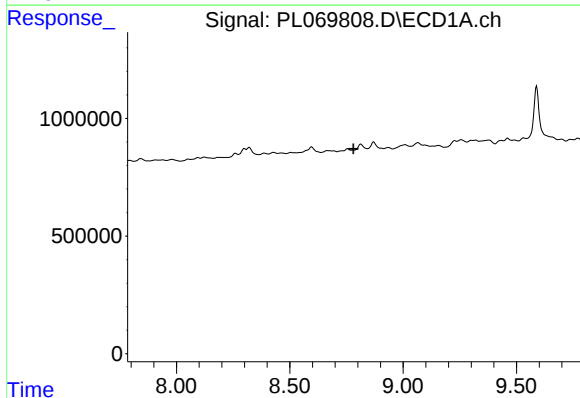


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.781 min
Response: 0
Conc: N.D.

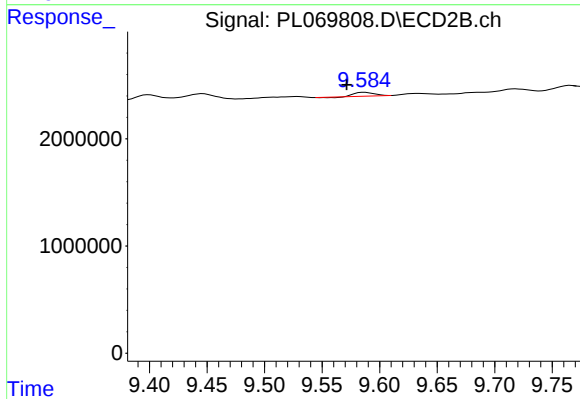

#19 Endosulfan Sulfate


R.T.: 9.587 min
Delta R.T.: 0.015 min
Response: 405792
Conc: 0.36 ng/ml

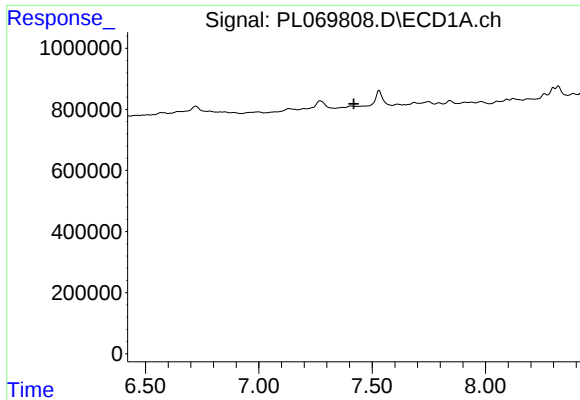

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

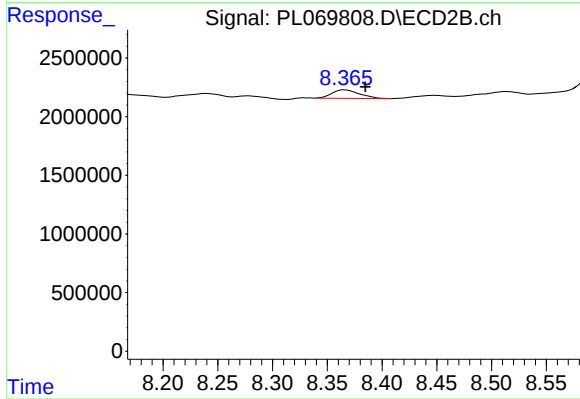


#26 Chlordane-4

R.T.: 8.366 min
Delta R.T.: -0.019 min
Response: 1264923
Conc: 5.43 ng/ml

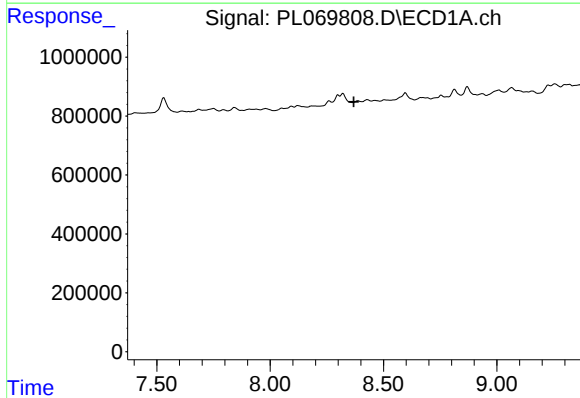


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.369 min
Response: 0
Conc: N.D.

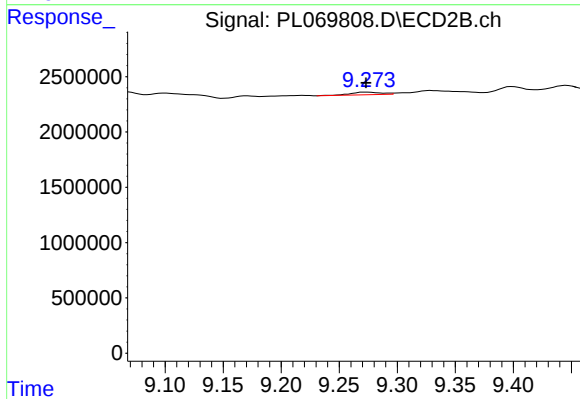

#27 Chlordane-5


R.T.: 9.274 min
Delta R.T.: 0.000 min
Response: 449300
Conc: 10.68 ng/ml

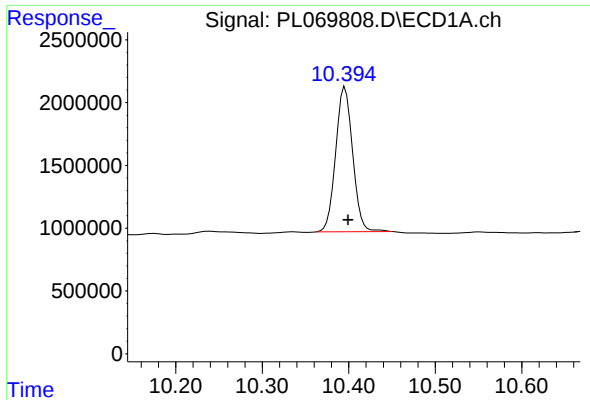

#28 Decachlorobiphenyl

R.T.: 10.396 min
Delta R.T.: -0.003 min
Response: 15672197
Conc: 21.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

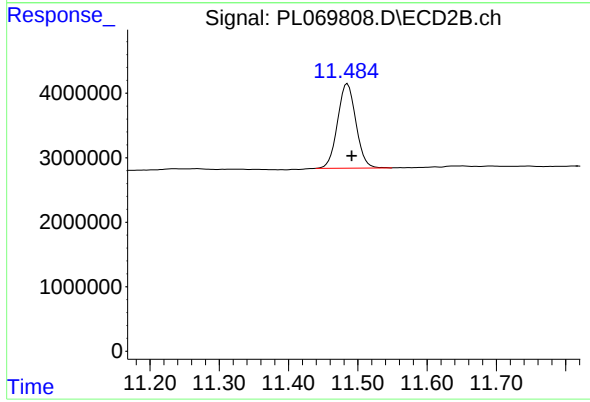

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.006 min
Response: 24043030
Conc: 21.04 ng/ml