

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091321\
 Data File : PL069819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2021 18:24
 Operator : AR\AJ
 Sample : PB139067TB
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 03:50:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.629	5.563	7756187	24616654	19.038	20.223
28)	SA Decachlor...	10.394	11.484	13533541	22836440	18.377	19.986
Target Compounds							
7)	B delta-BHC	0.000	7.080	0	551246	N.D.	0.331 #
22)	Mirex	0.000	10.561f	0	53130	N.D.	0.057 #
23)	Chlordane-1	0.000	6.969f	0	939835	N.D.	22.897 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091321\
Data File : PL069819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2021 18:24
Operator : AR\AJ
Sample : PB139067TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 03:50:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

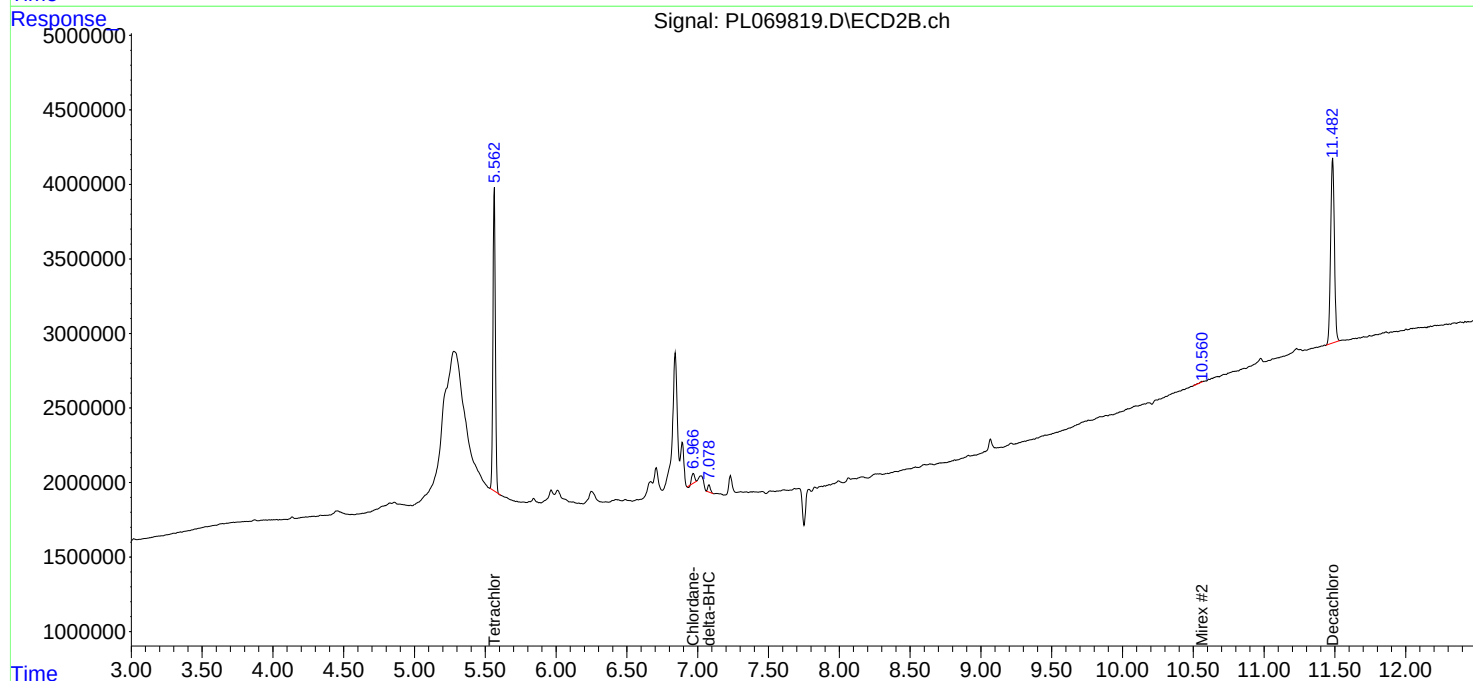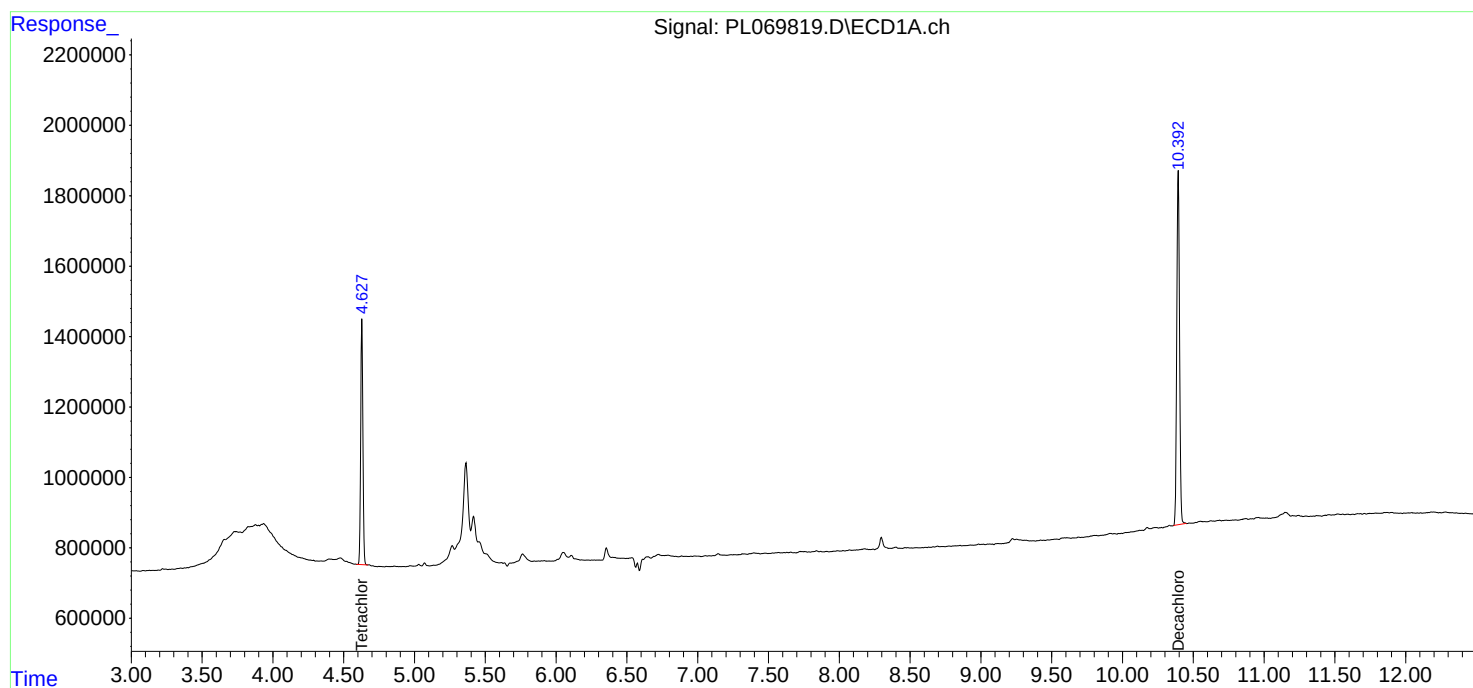


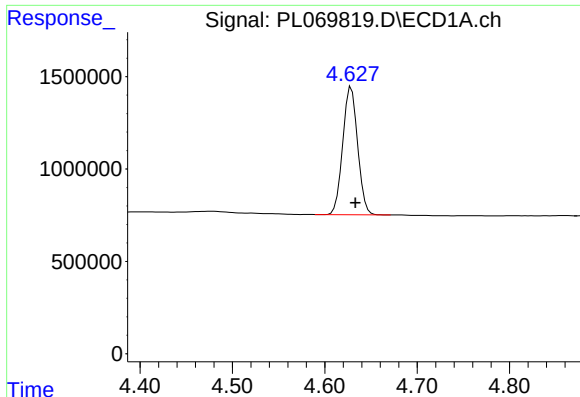

#1 Tetrachloro-m-xylene


R.T.: 4.629 min
Delta R.T.: -0.004 min
Response: 7756187
Conc: 19.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

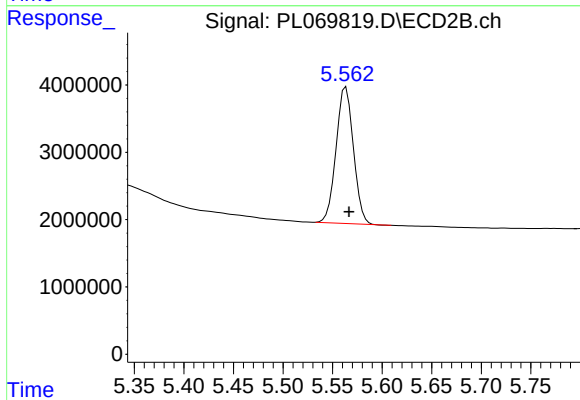


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.003 min
Response: 24616654
Conc: 20.22 ng/ml

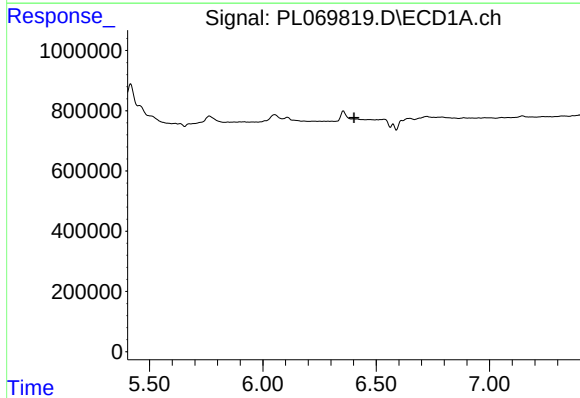


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

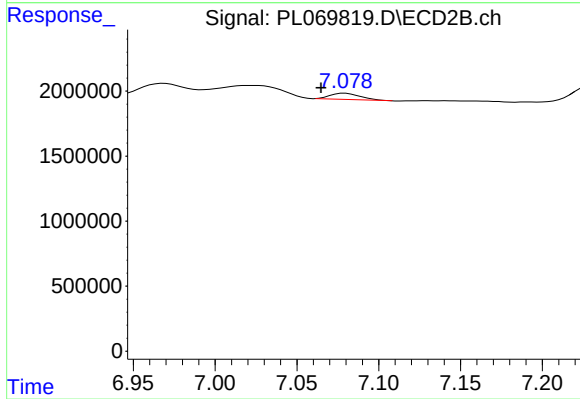

#7 delta-BHC


R.T.: 7.080 min
Delta R.T.: 0.015 min
Response: 551246
Conc: 0.33 ng/ml

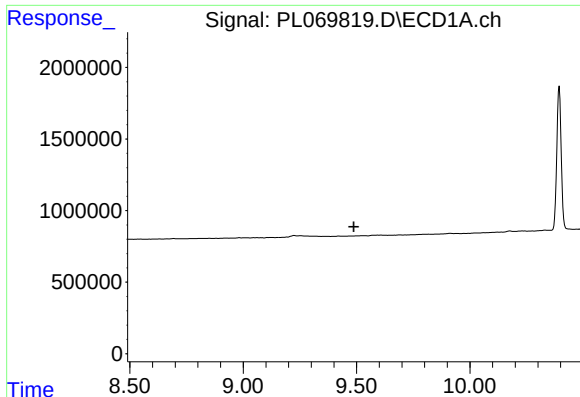

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

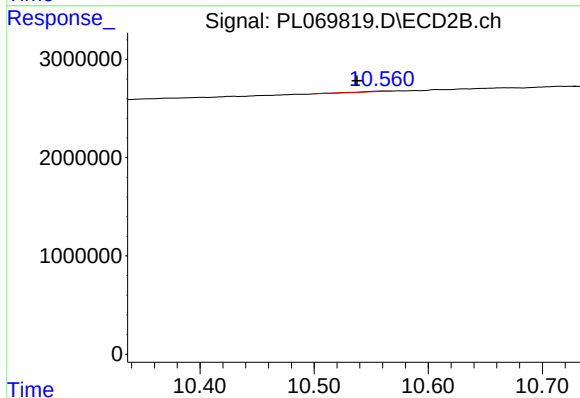


#22 Mirex

R.T.: 10.561 min
Delta R.T.: 0.024 min
Response: 53130
Conc: 0.06 ng/ml

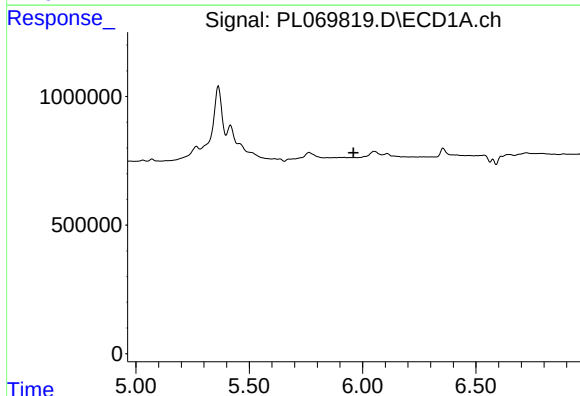


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

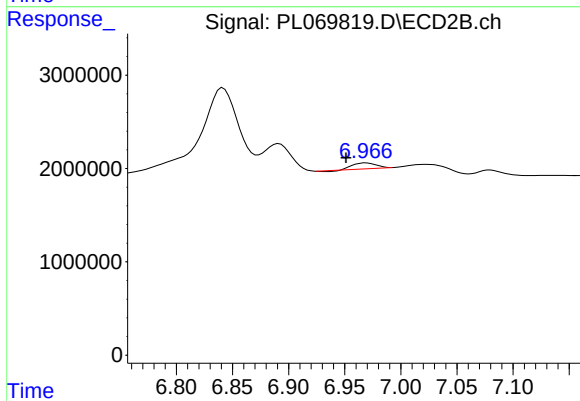

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.018 min
Response: 939835
Conc: 22.90 ng/ml

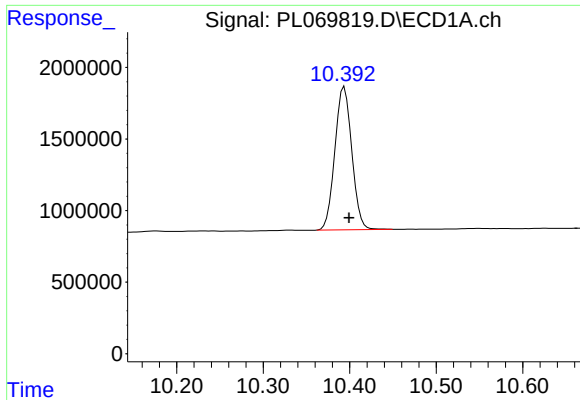

#28 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: -0.005 min
Response: 13533541
Conc: 18.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

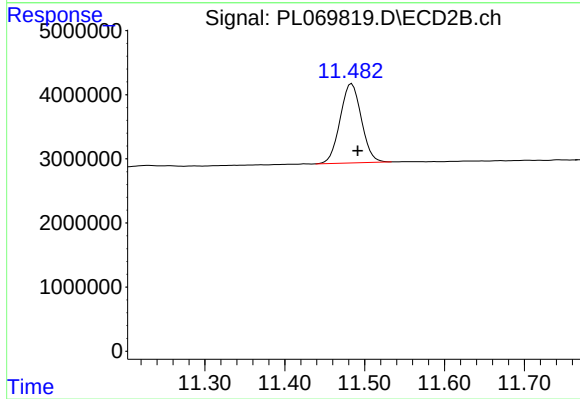

#28 Decachlorobiphenyl

R.T.: 11.484 min
Delta R.T.: -0.008 min
Response: 22836440
Conc: 19.99 ng/ml