

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091322\
 Data File : PL077708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2022 14:18
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 01:39:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.624	77139615	176.6E6	48.122	59.491
28)	SA Decachlor...	8.915	7.729	61605332	113.7E6	47.666	45.280
Target Compounds							
23)	Chlordane-1	4.583	3.602	31652183	53723240	509.137	494.400
24)	Chlordane-2	5.117	4.173	31844548	56426062	477.613	471.043
25)	Chlordane-3	5.829	4.798	122.0E6	166.2E6	495.377	483.079
26)	Chlordane-4	5.907	4.859	145.5E6	176.2E6	488.918	485.557
27)	Chlordane-5	6.766	5.524	23880326	45944826	480.845	488.295



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091322\
Data File : PL077708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2022 14:18
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 01:39:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

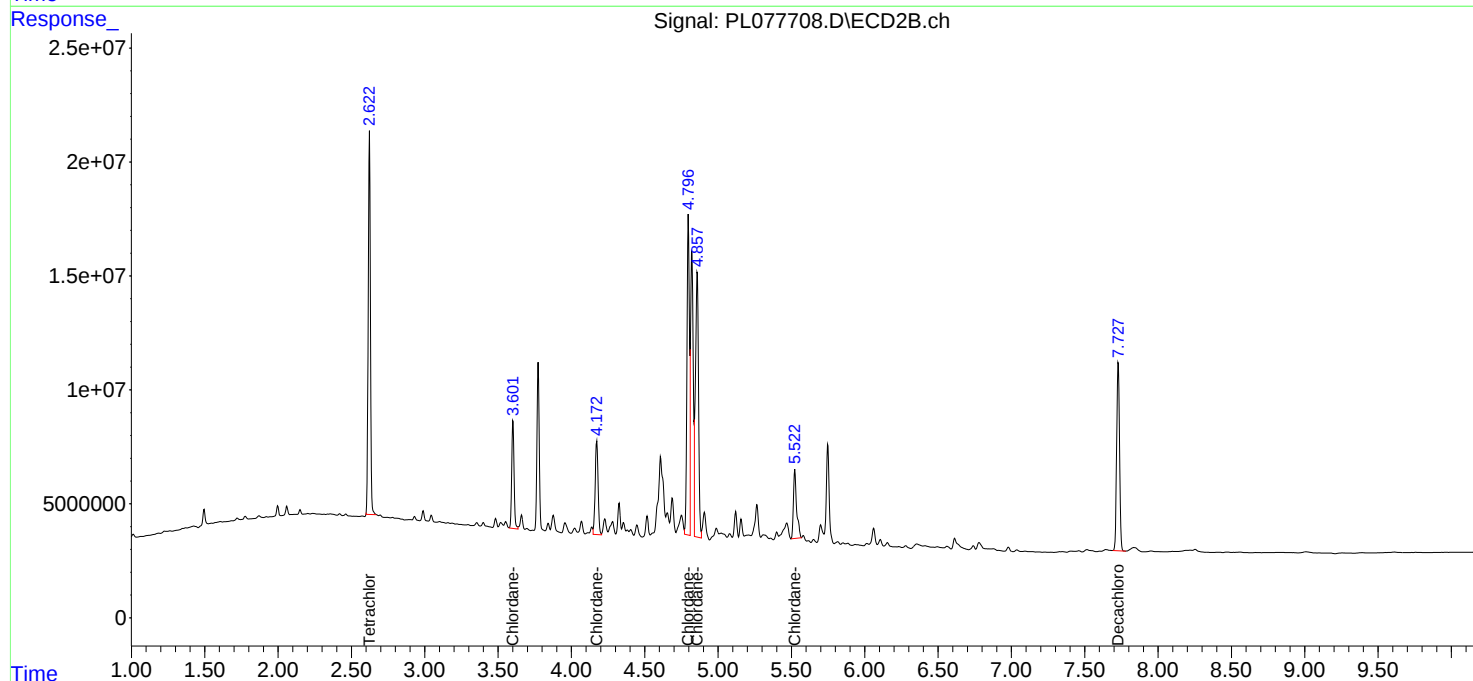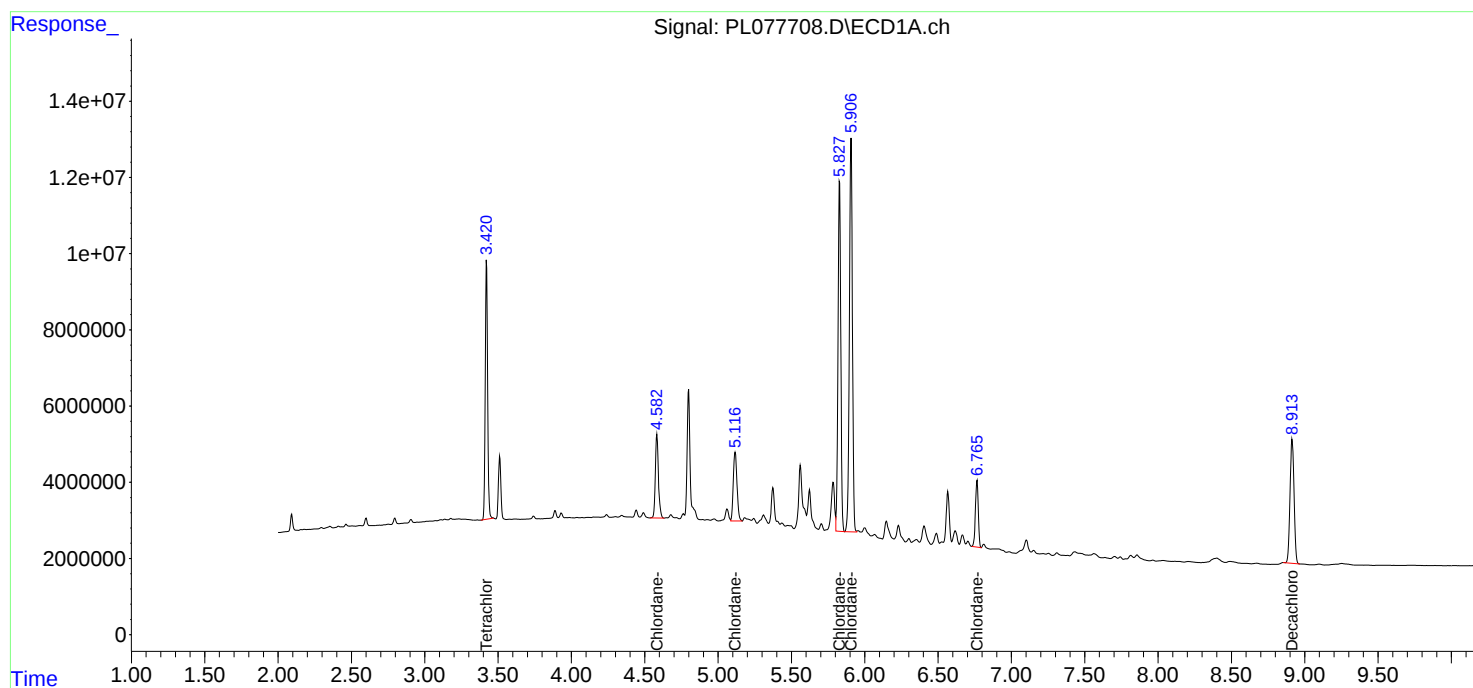


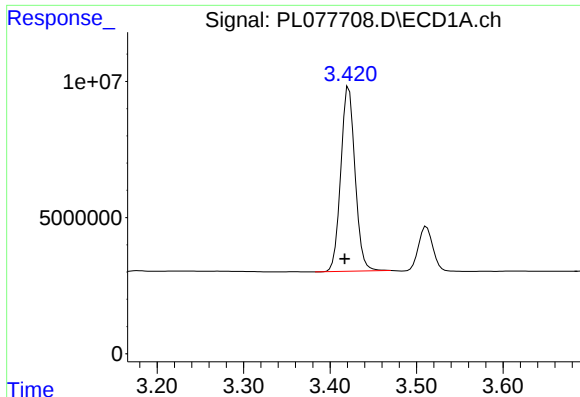

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.005 min
Response: 77139615
Conc: 48.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

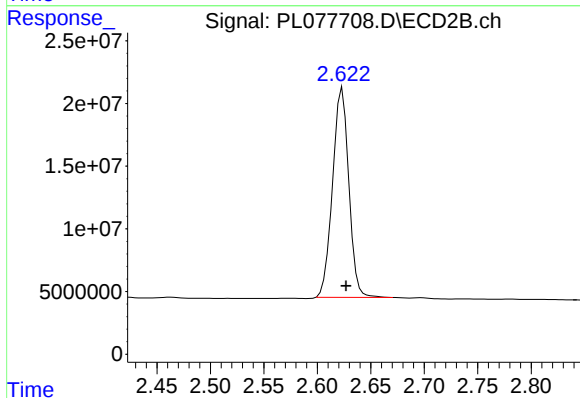


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 176613150
Conc: 59.49 ng/ml

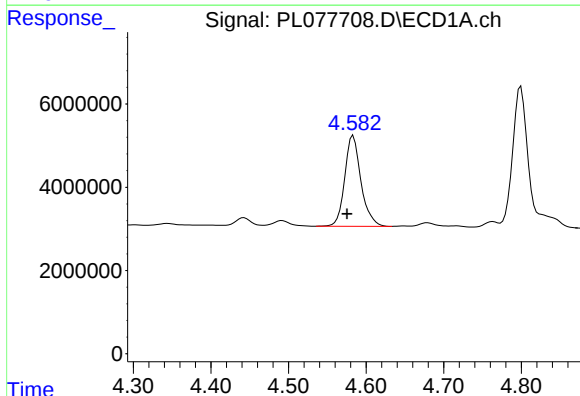


#23 Chlordane-1

R.T.: 4.583 min
Delta R.T.: 0.008 min
Response: 31652183
Conc: 509.14 ng/ml

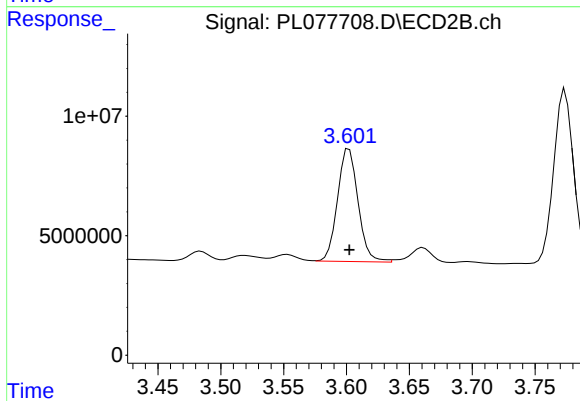

#23 Chlordane-1


R.T.: 3.602 min
Delta R.T.: 0.000 min
Response: 53723240
Conc: 494.40 ng/ml

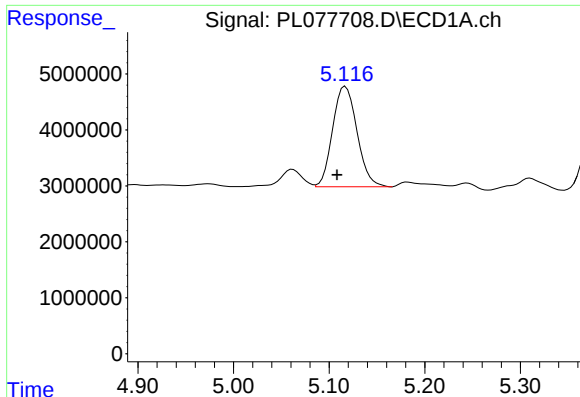

#24 Chlordane-2


R.T.: 5.117 min
Delta R.T.: 0.009 min
Response: 31844548
Conc: 477.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

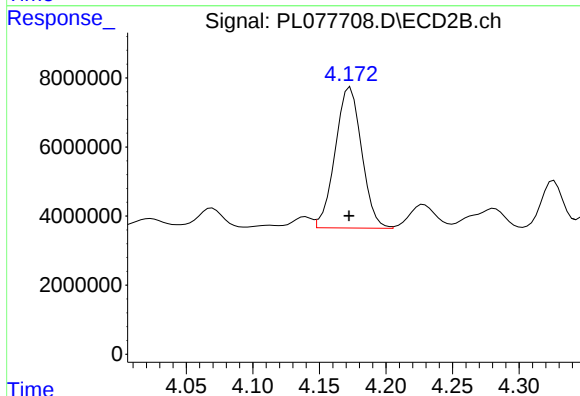


#24 Chlordane-2

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 56426062
Conc: 471.04 ng/ml

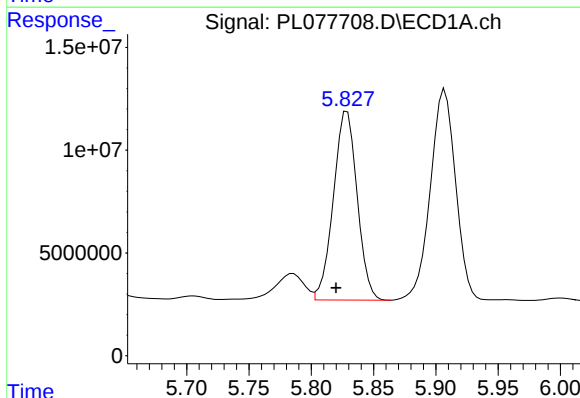


#25 Chlordane-3

R.T.: 5.829 min
Delta R.T.: 0.009 min
Response: 121992610
Conc: 495.38 ng/ml

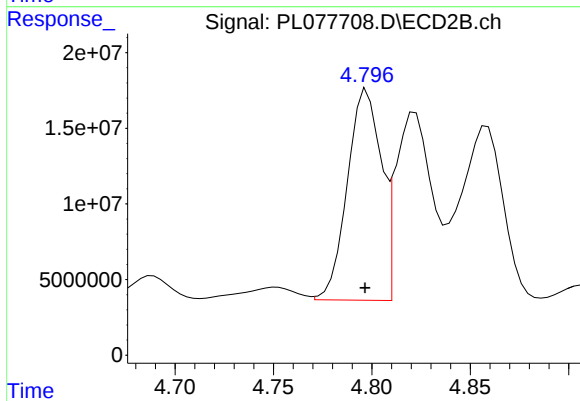

#25 Chlordane-3


R.T.: 4.798 min
Delta R.T.: 0.001 min
Response: 166173236
Conc: 483.08 ng/ml

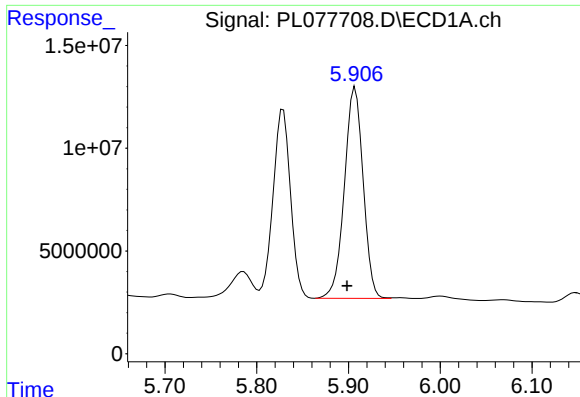

#26 Chlordane-4


R.T.: 5.907 min
Delta R.T.: 0.009 min
Response: 145487550
Conc: 488.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

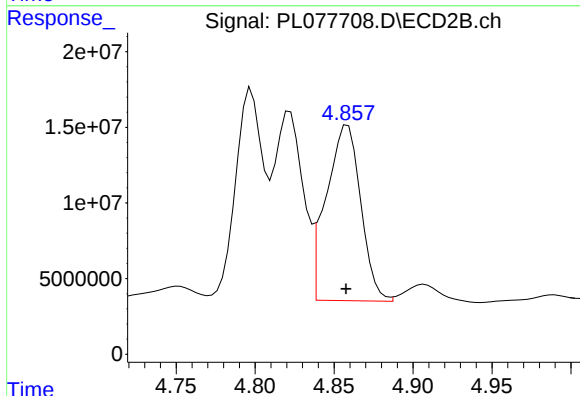


#26 Chlordane-4

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 176168849
Conc: 485.56 ng/ml

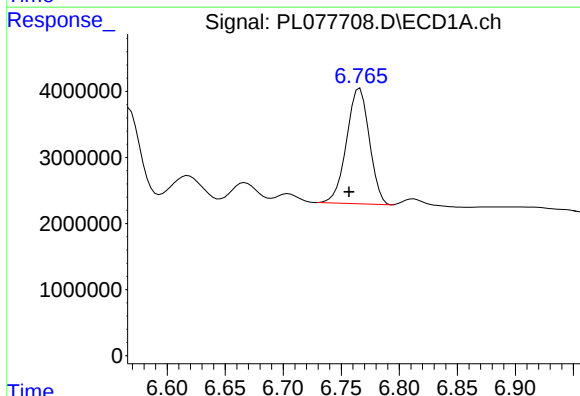


#27 Chlordane-5

R.T.: 6.766 min
Delta R.T.: 0.009 min
Response: 23880326
Conc: 480.84 ng/ml

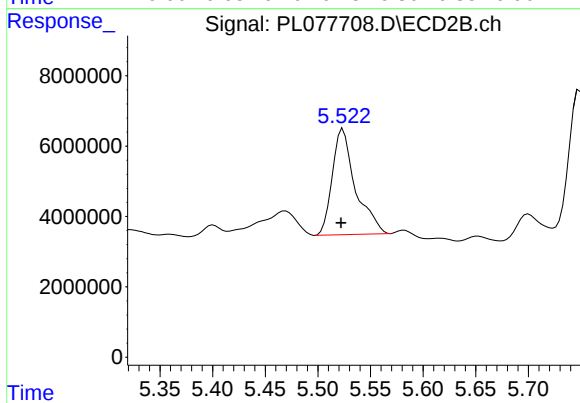

#27 Chlordane-5


R.T.: 5.524 min
Delta R.T.: 0.002 min
Response: 45944826
Conc: 488.29 ng/ml

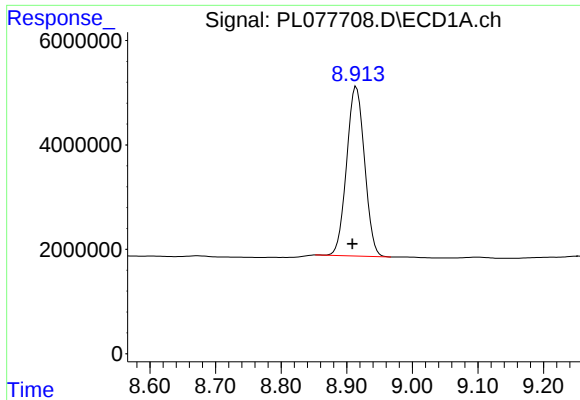

#28 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.006 min
Response: 61605332
Conc: 47.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

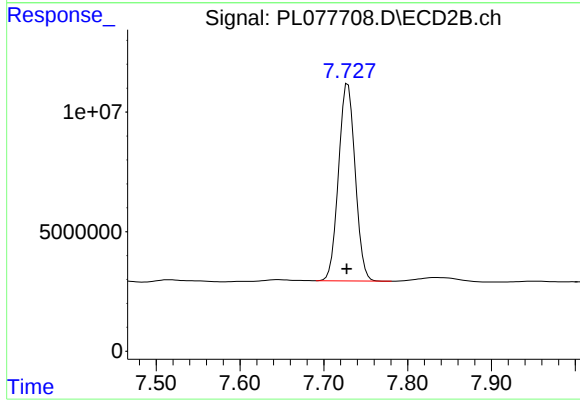

#28 Decachlorobiphenyl

R.T.: 7.729 min
Delta R.T.: 0.001 min
Response: 113662212
Conc: 45.28 ng/ml