

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091323\
 Data File : PL085289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 16:31
 Operator : AR\AJ
 Sample : 04394-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B103-08

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/13/2023
 Supervised By :Ankita Jodhani 09/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 17:44:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.474	2.682	21914025	10073858	8.959	8.866
2) SA Decachlor...	9.021	7.859	13188819	10495234	8.201m	7.885

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091323\
Data File : PL085289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 16:31
Operator : AR\AJ
Sample : 04394-10
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B103-08


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/13/2023
Supervised By : Ankita Jodhani 09/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 17:44:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

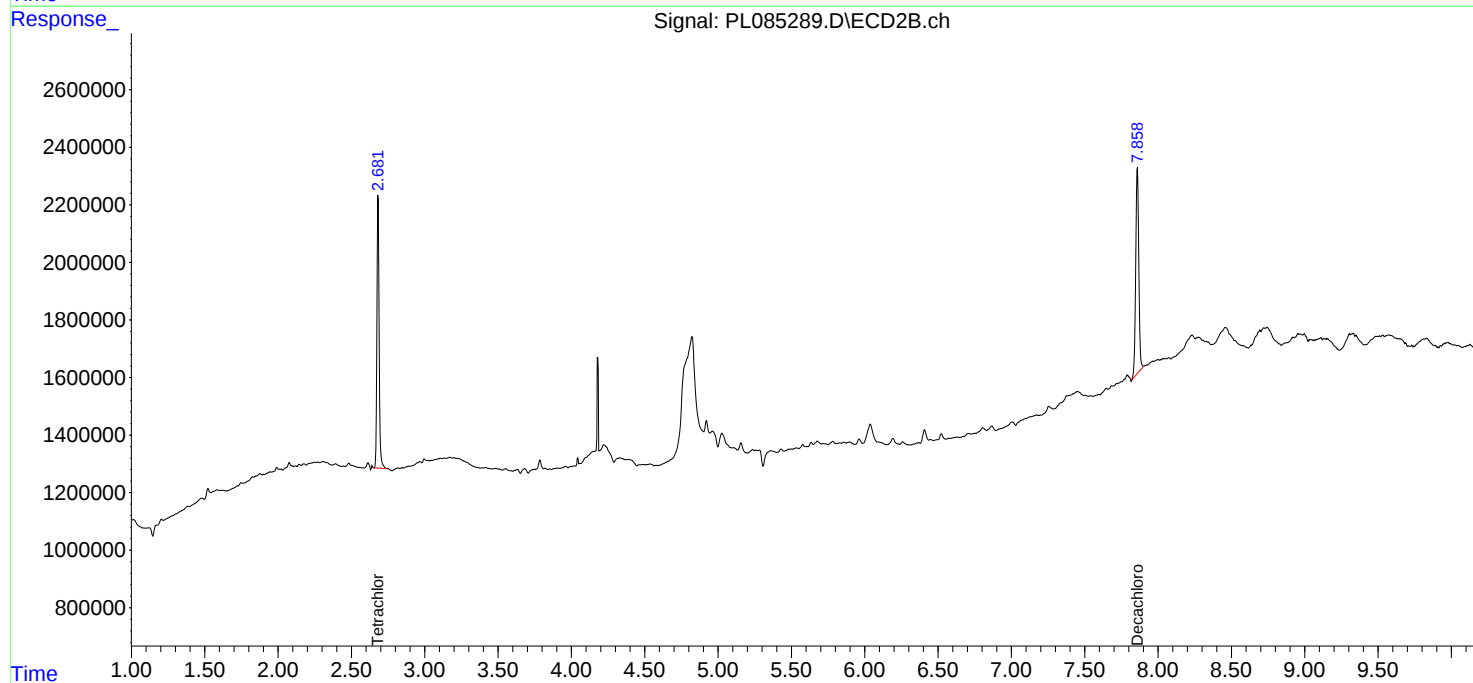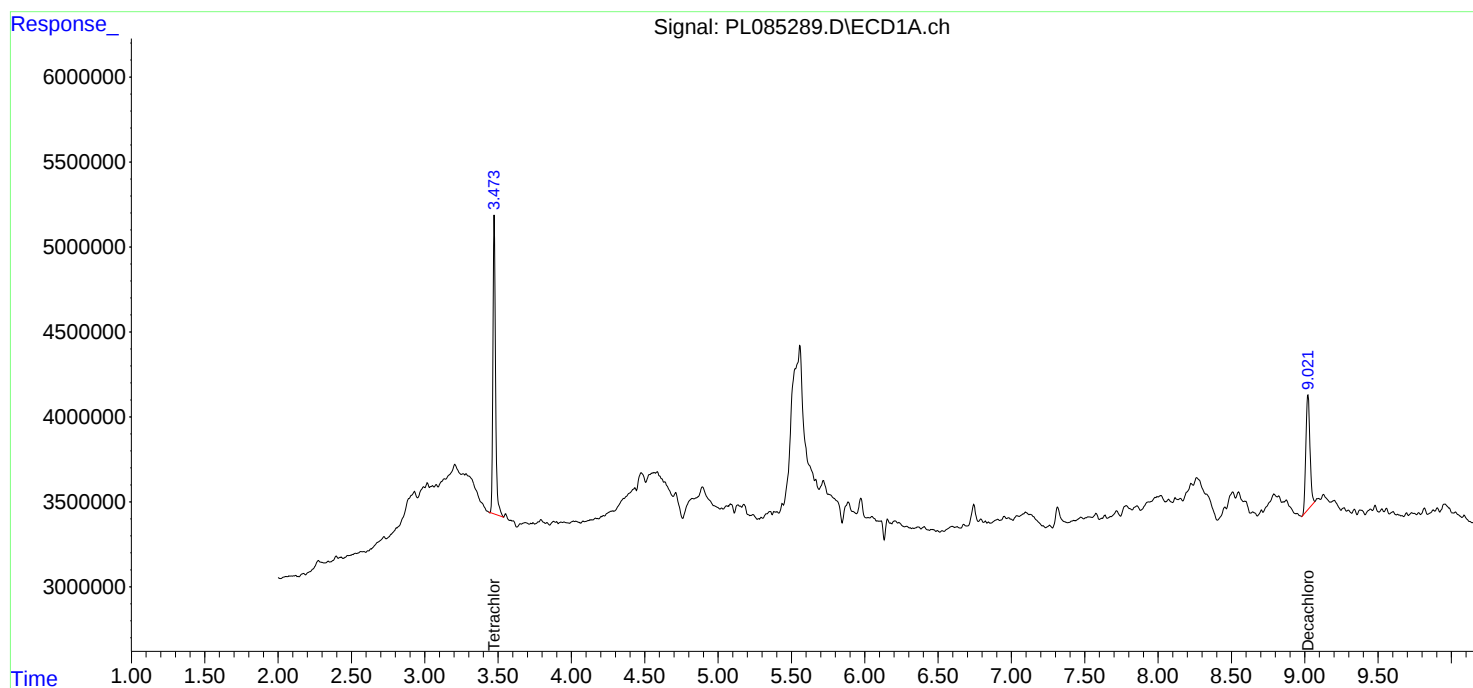

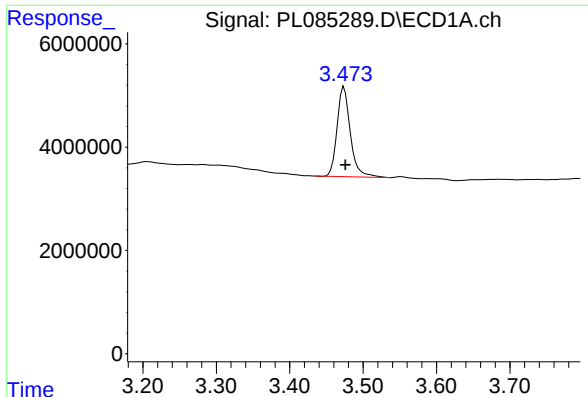


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: -0.002 min
Response: 21914025
Conc: 8.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
B103-08


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/13/2023
Supervised By :Ankita Jodhani 09/13/2023

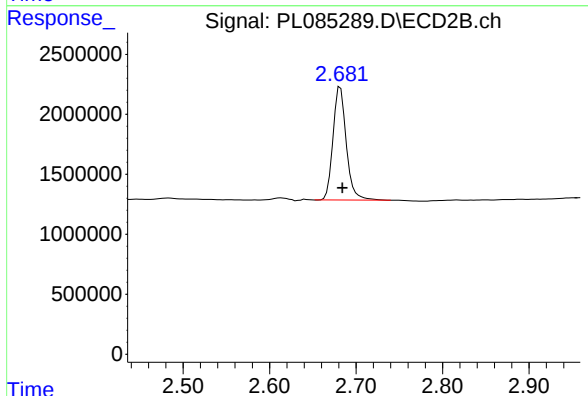


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: -0.002 min
Response: 10073858
Conc: 8.87 ng/ml

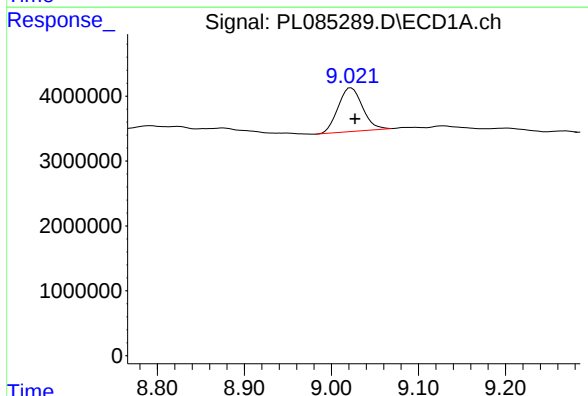

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: -0.006 min
Response: 13188819
Conc: 8.20 ng/ml m

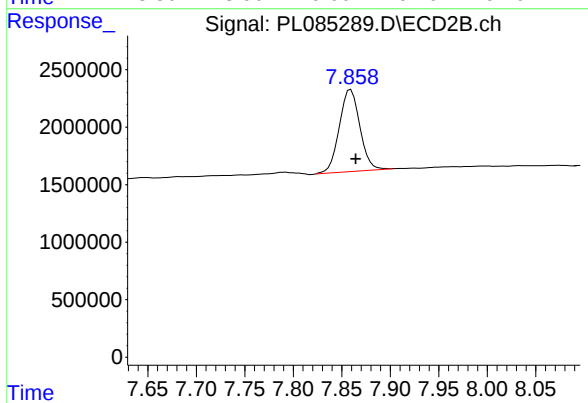

#28 Decachlorobiphenyl

R.T.: 7.859 min
Delta R.T.: -0.005 min
Response: 10495234
Conc: 7.88 ng/ml