

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091323\
 Data File : PL085290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 16:45
 Operator : AR\AJ
 Sample : 04395-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-91123

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 17:45:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.683	25315370	12135207	10.350	10.681
28)	SA Decachlor...	9.022	7.860	14428127	10084797	8.972	7.576
Target Compounds							
12)	B 4,4'-DDE	6.147	5.159	802237	507719	0.386	0.408



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091323\
Data File : PL085290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 16:45
Operator : AR\AJ
Sample : 04395-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-01-91123

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 17:45:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

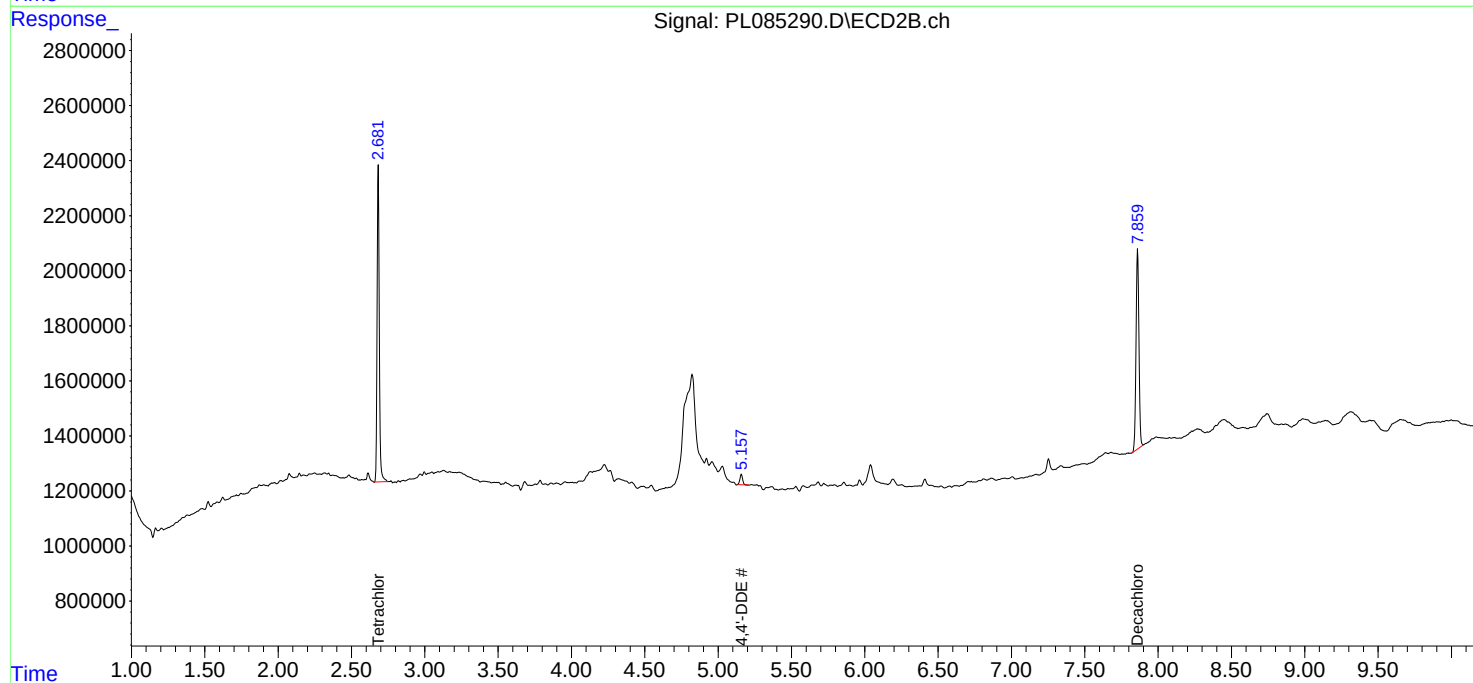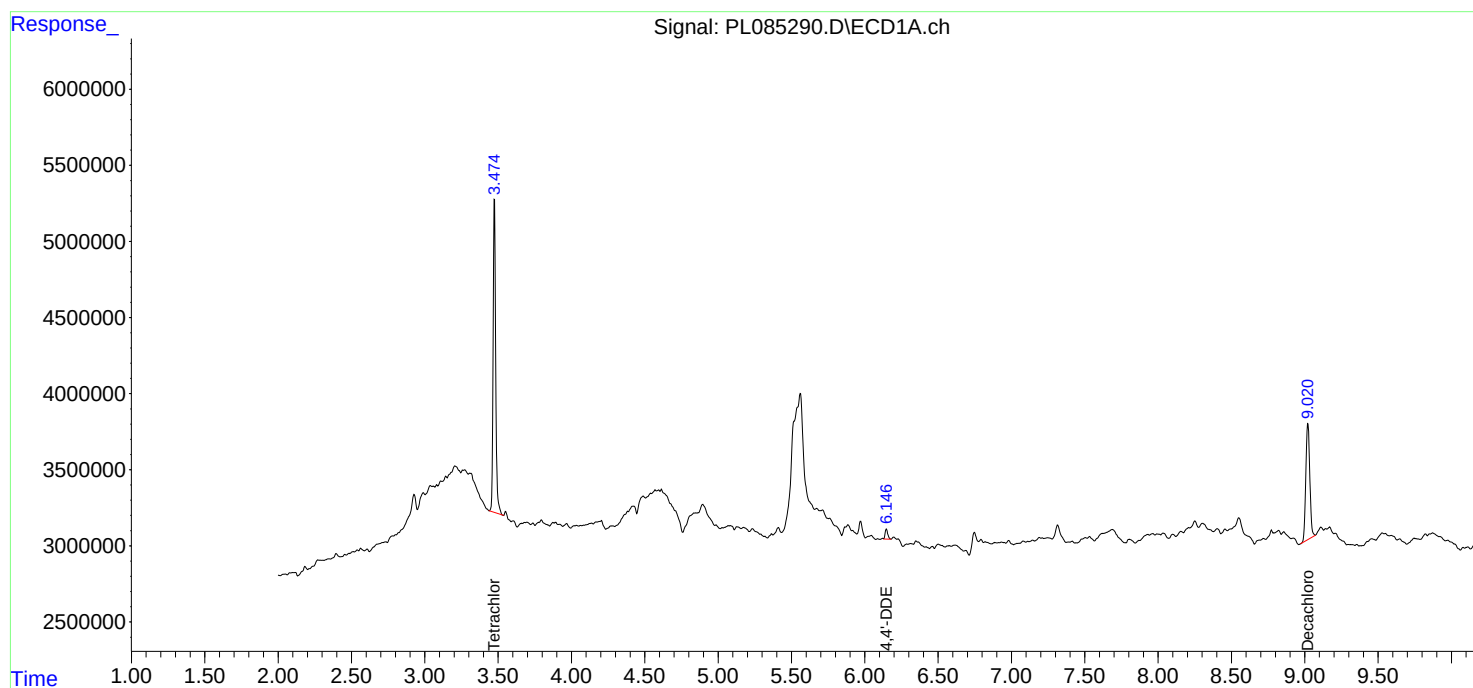


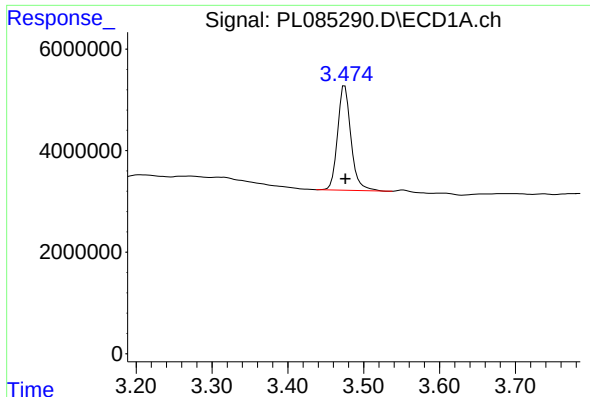

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 25315370
Conc: 10.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-91123

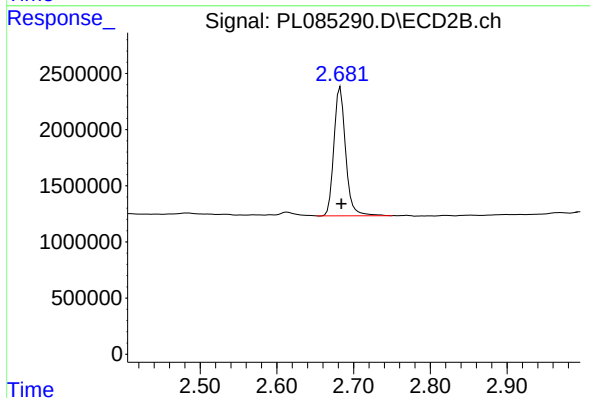


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: -0.001 min
Response: 12135207
Conc: 10.68 ng/ml

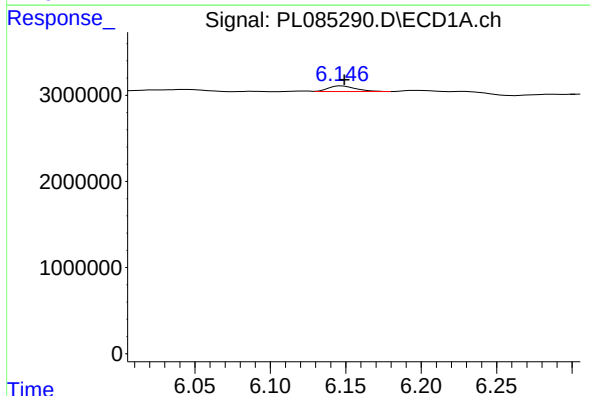


#12 4,4'-DDE

R.T.: 6.147 min
Delta R.T.: -0.002 min
Response: 802237
Conc: 0.39 ng/ml

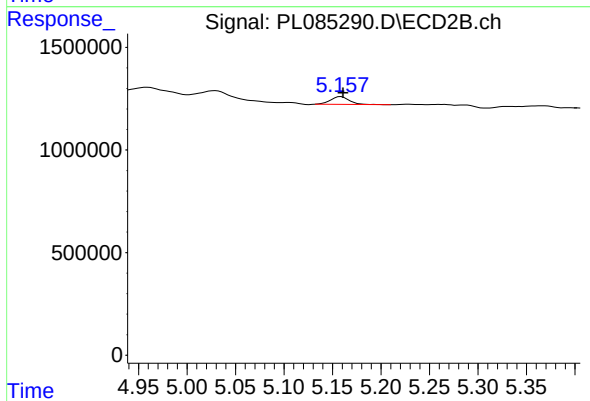

#12 4,4'-DDE


R.T.: 5.159 min
Delta R.T.: -0.002 min
Response: 507719
Conc: 0.41 ng/ml

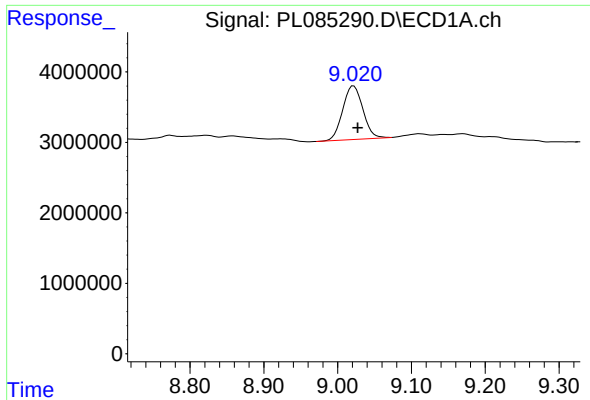

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.005 min
Response: 14428127
Conc: 8.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-91123

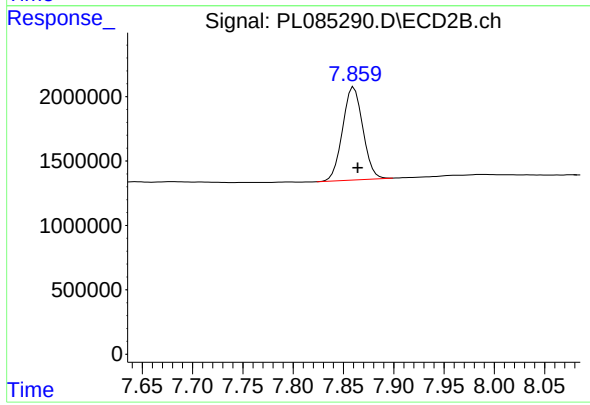

#28 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: -0.004 min
Response: 10084797
Conc: 7.58 ng/ml