

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091324\
 Data File : PL091741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2024 18:26
 Operator : AR\AJ
 Sample : P3980-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-091224

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/15/2024
 Supervised By : Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 03:47:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.784	18966043	26079776	12.169m	13.944
28) SA Decachlor...	9.061	7.925	15164527	22939198	12.478	12.423

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091324\
Data File : PL091741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2024 18:26
Operator : AR\AJ
Sample : P3980-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-02-091224


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/15/2024
Supervised By : Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 03:47:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

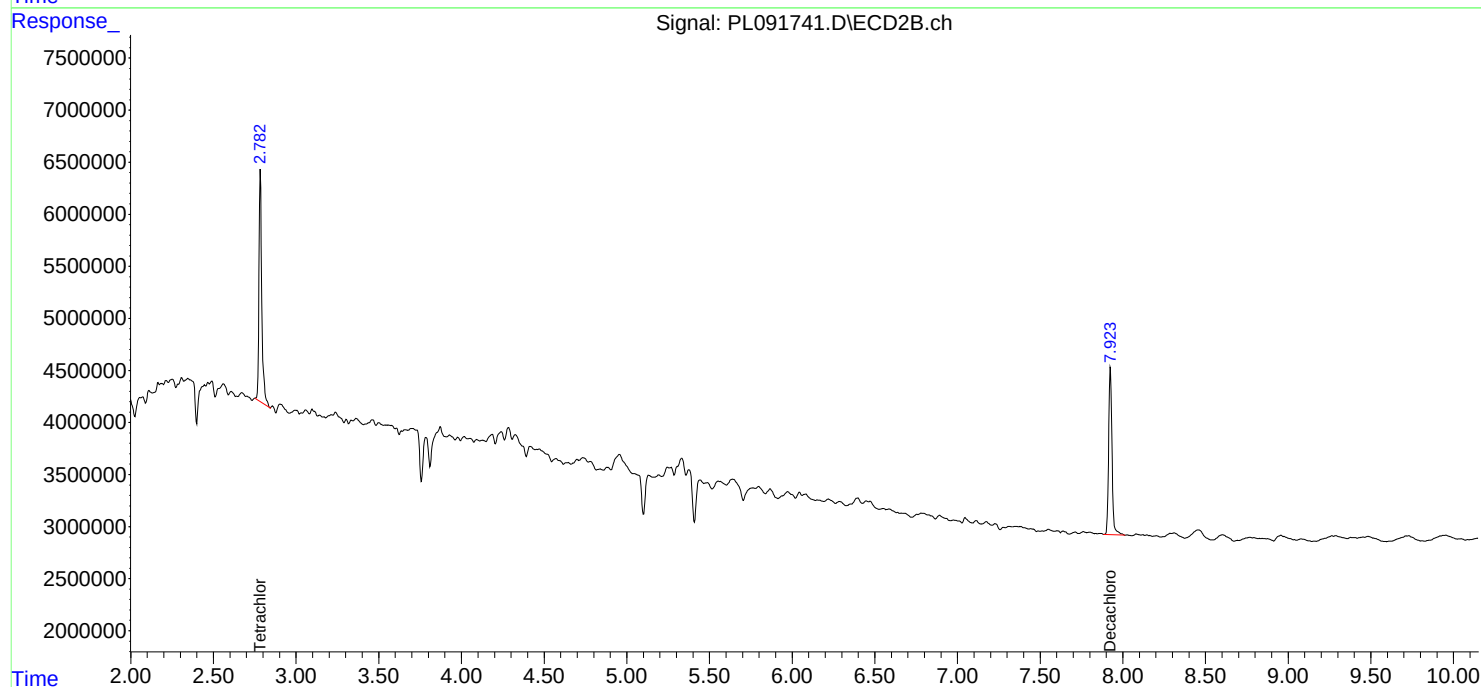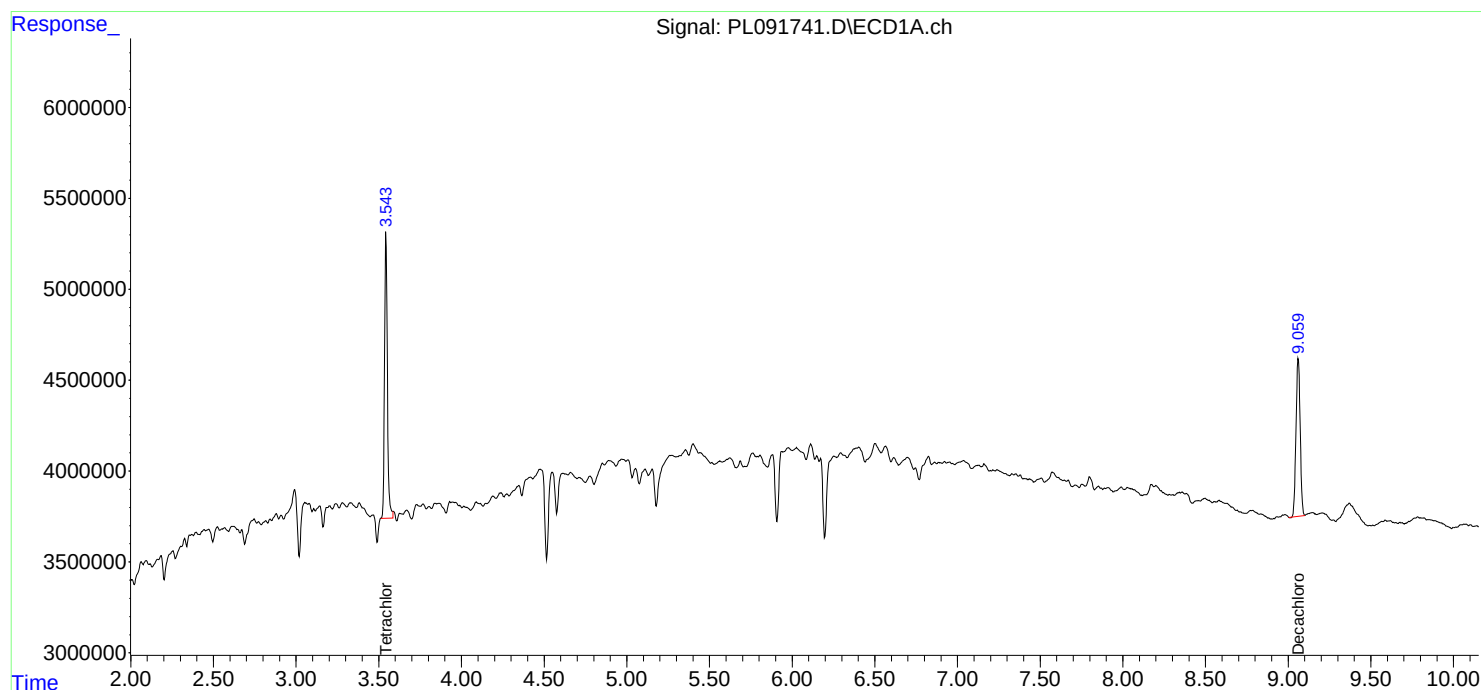

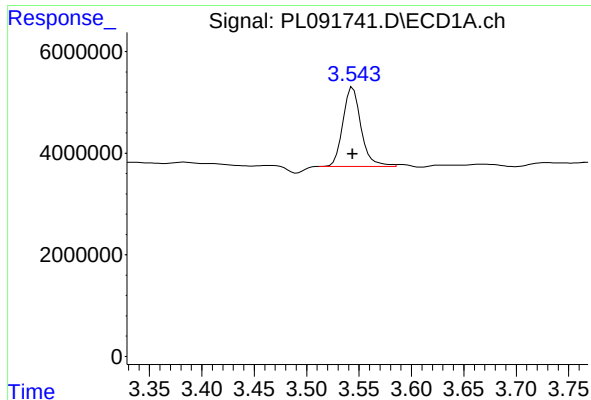


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 18966043
Conc: 12.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-091224


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/15/2024
Supervised By :Ankita Jodhani 09/16/2024

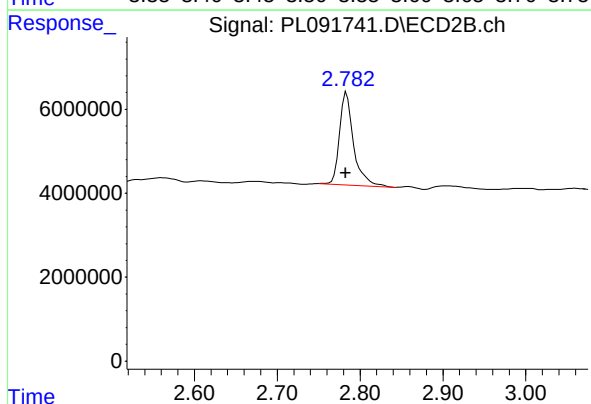


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: 0.001 min
Response: 26079776
Conc: 13.94 ng/ml

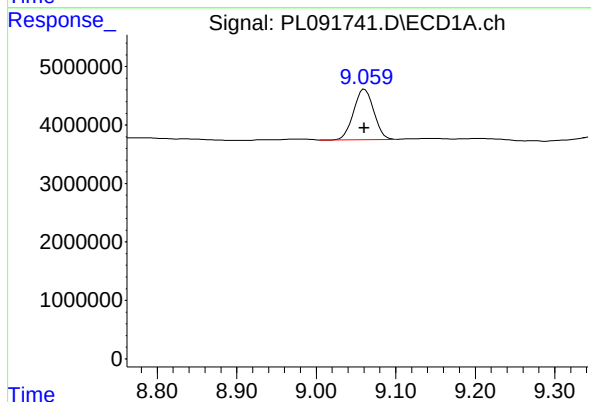

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 15164527
Conc: 12.48 ng/ml

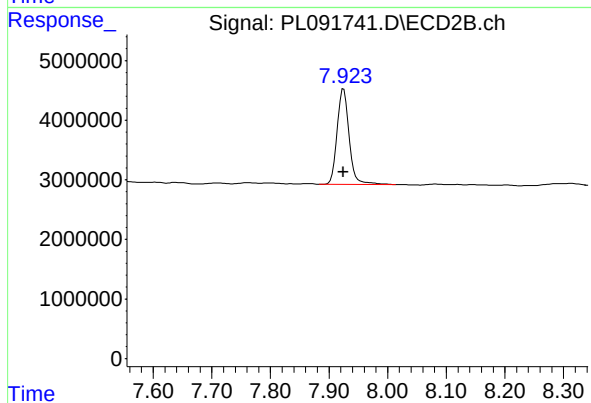

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 22939198
Conc: 12.42 ng/ml