

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091325\
 Data File : PL097158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2025 19:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 01:22:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.526	2.823	79619263	117.4E6	20.188	20.834
28)	SA Decachlor...	9.000	7.982	61435168	110.0E6	20.750	22.938
Target Compounds							
8)	B Heptachlo...	5.643	0.000	35497725	0	6.898	N.D. #
14)	MA Endrin	0.000	5.710	0	36314566	N.D.	6.148 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091325\
Data File : PL097158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2025 19:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 01:22:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

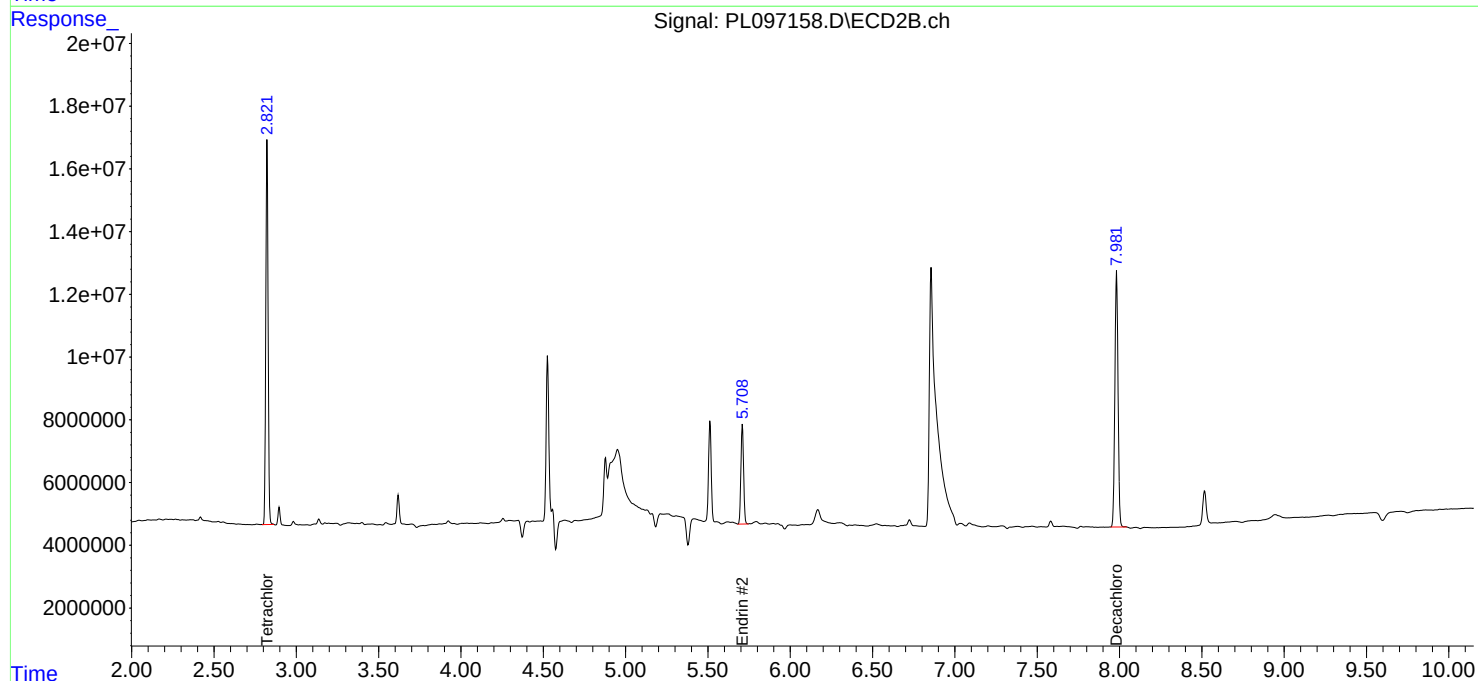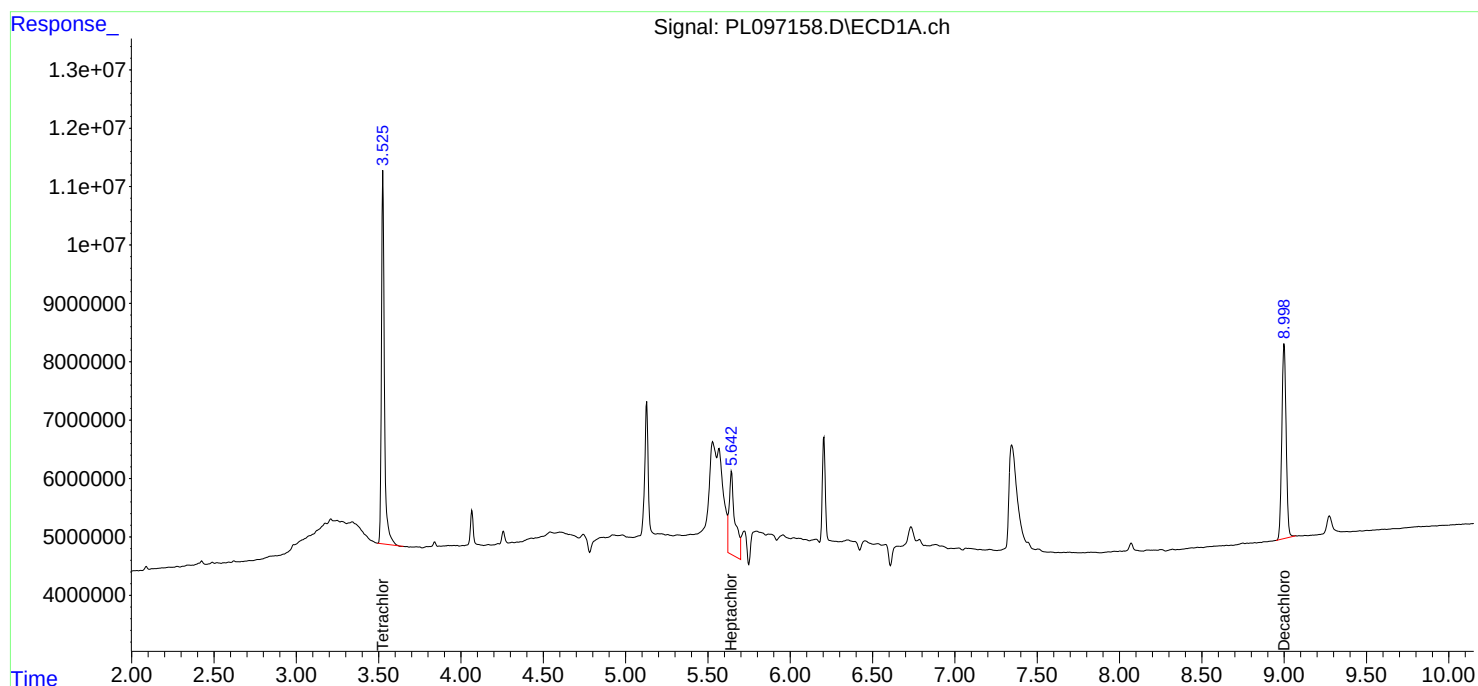


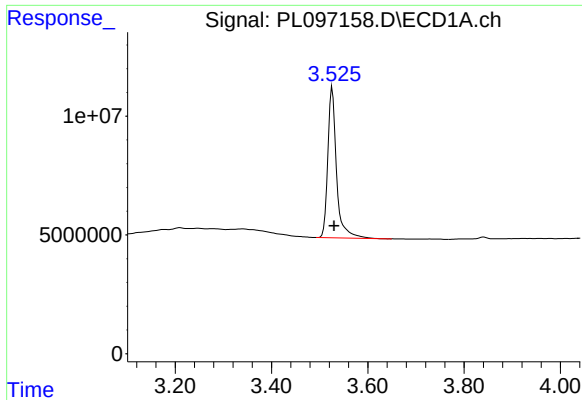

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: -0.004 min
Response: 79619263
Conc: 20.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

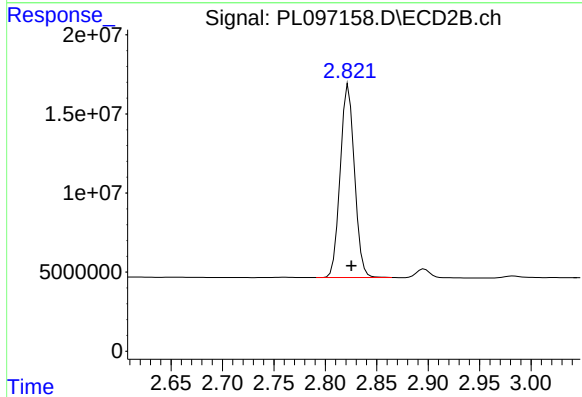


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: -0.003 min
Response: 117434104
Conc: 20.83 ng/ml

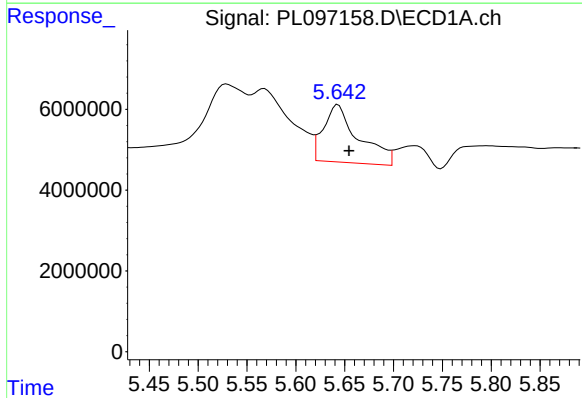


#8 Heptachlor epoxide

R.T.: 5.643 min
Delta R.T.: -0.011 min
Response: 35497725
Conc: 6.90 ng/ml

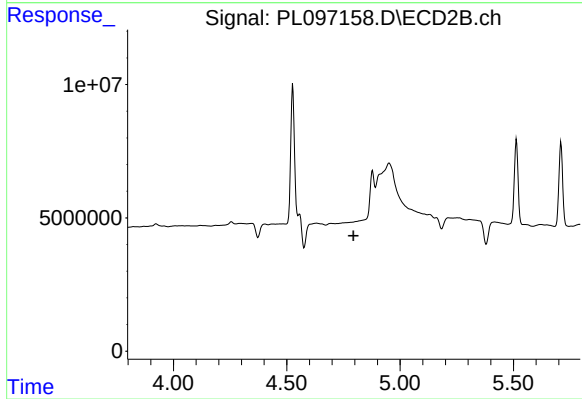

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.795 min
Response: 0
Conc: N.D.

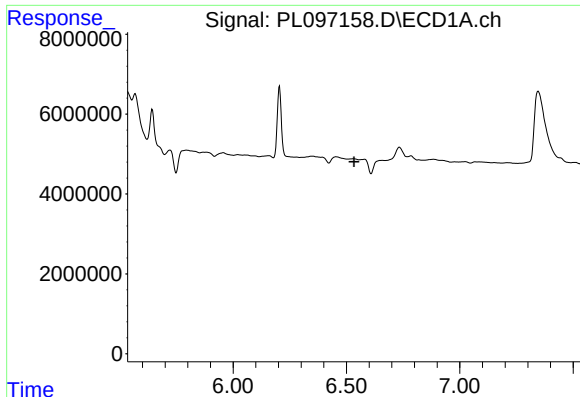

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

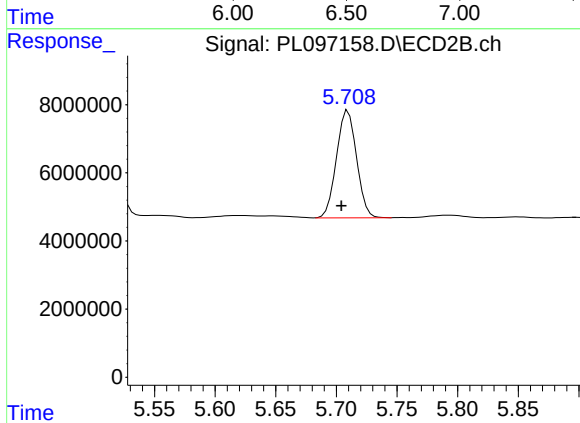


#14 Endrin

R.T.: 5.710 min
Delta R.T.: 0.006 min
Response: 36314566
Conc: 6.15 ng/ml

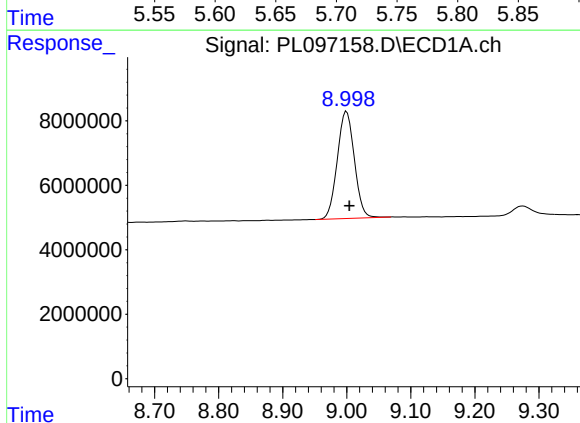

#28 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: -0.004 min
Response: 61435168
Conc: 20.75 ng/ml

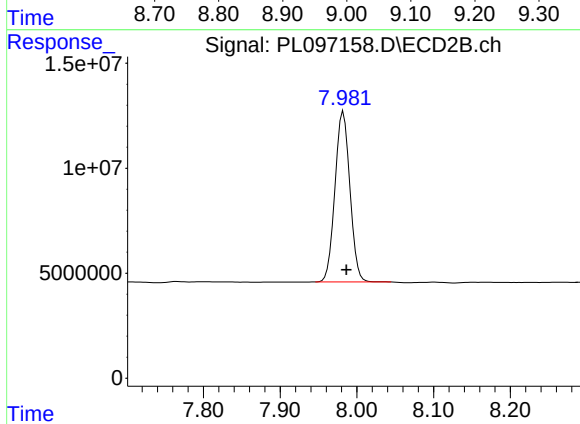

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.004 min
Response: 110005560
Conc: 22.94 ng/ml