

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091325\
 Data File : PL097171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2025 22:37
 Operator : AR\AJ
 Sample : Q3073-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BEL-25-0023

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/12/2025
 Supervised By : mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 01:24:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.526	2.824	37095628	55358794	9.406m	9.821
28) SA Decachlor...	9.005	7.987	35378756	36090888	11.950m	7.526m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091325\
Data File : PL097171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2025 22:37
Operator : AR\AJ
Sample : Q3073-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BEL-25-0023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/12/2025
Supervised By : mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 01:24:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

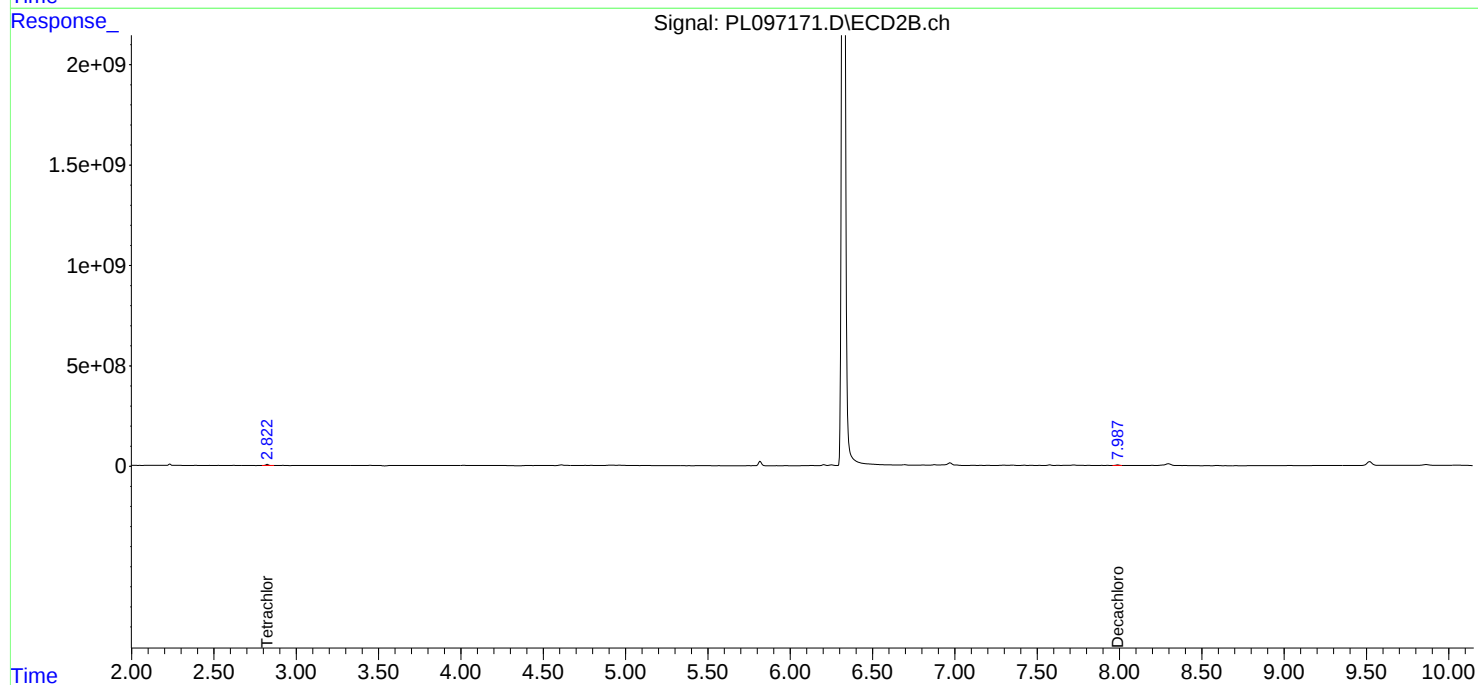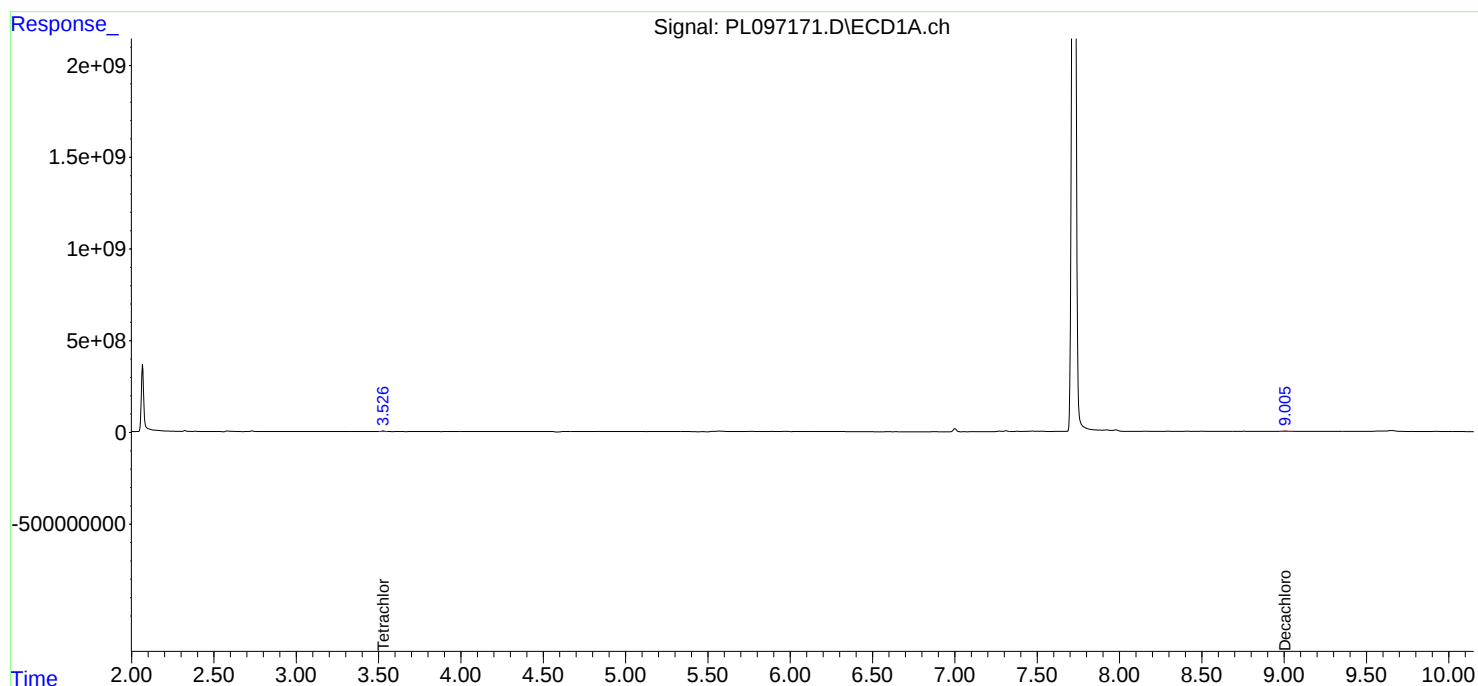

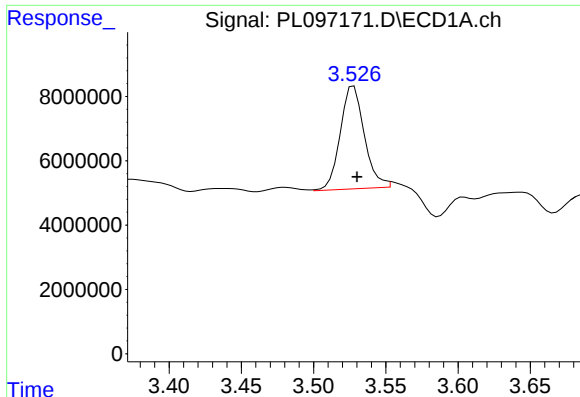


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.004 min
Response: 37095628
Conc: 9.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
BEL-25-0023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/12/2025
Supervised By :mohammad ahmed 09/15/2025

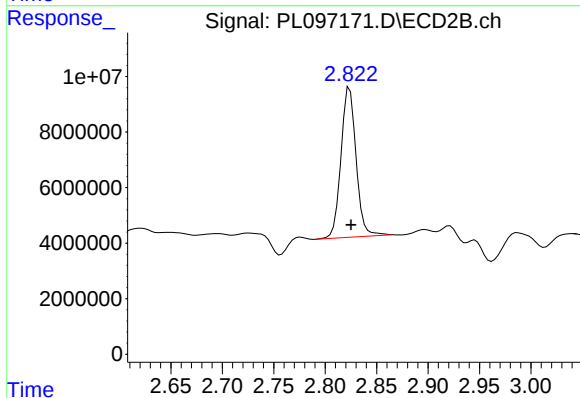


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: -0.001 min
Response: 55358794
Conc: 9.82 ng/ml

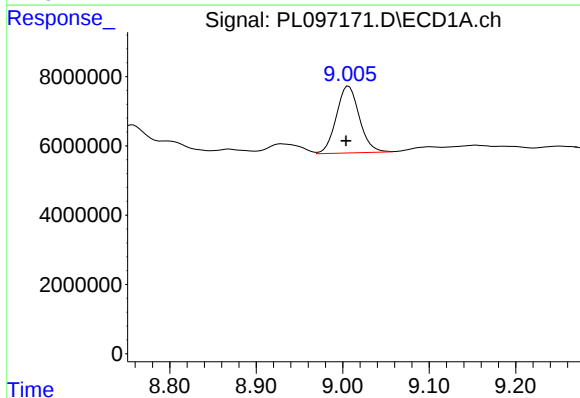

#28 Decachlorobiphenyl

R.T.: 9.005 min
Delta R.T.: 0.002 min
Response: 35378756
Conc: 11.95 ng/ml m

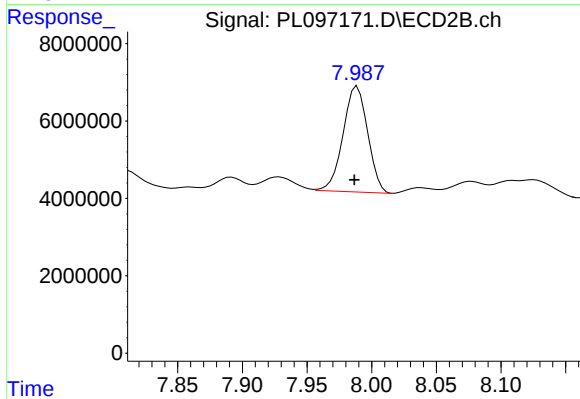

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: 0.000 min
Response: 36090888
Conc: 7.53 ng/ml m