

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 17:46
 Operator : AJ\SJ
 Sample : J4883-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:49:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	136.8E6	53437124	17.646	16.747
28)	SA Decachlor...	7.951	8.888	119.6E6	48213968	14.348	17.751
Target Compounds							
3)	MA gamma-BHC...	4.050f	0.000	91422447	0	7.988	N.D. #
4)	MA Heptachlor	0.000	5.074	0	27350325	N.D.	6.326 #
8)	B Heptachlo...	0.000	5.734	0	13078198	N.D.	3.307 #
10)	B gamma-Chl...	5.215f	0.000	88143425	0	7.968	N.D. #
11)	B alpha-Chl...	5.215	0.000	88143425	0	8.251	N.D. #
15)	B Endosulfa...	0.000	6.789	0	1749015	N.D.	0.530 #
25)	Chlordane-3	5.215	0.000	88143425	0	71.829	N.D. #
26)	Chlordane-4	5.215	0.000	88143425	0	80.405	N.D. #
27)	Chlordane-5	0.000	6.789	0	1749015	N.D.	15.072 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 17:46
Operator : AJ\SJ
Sample : J4883-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:49:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

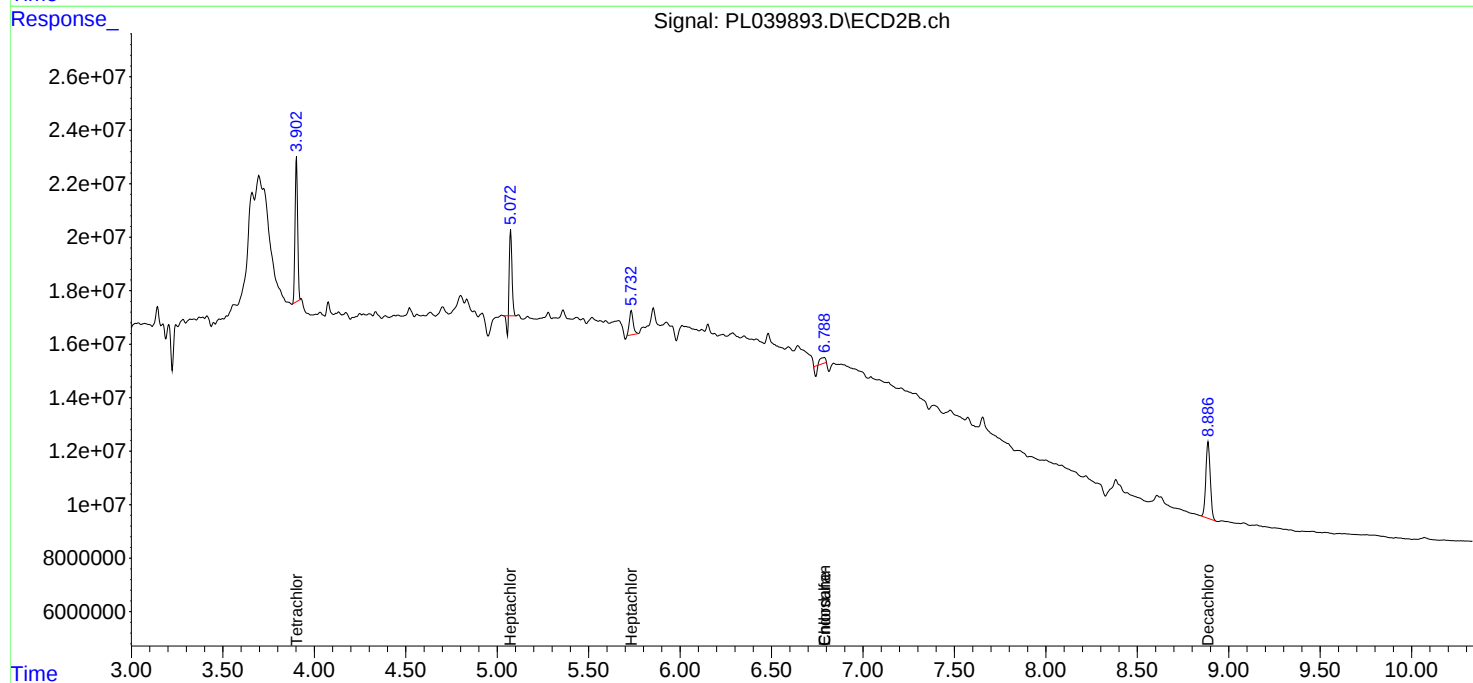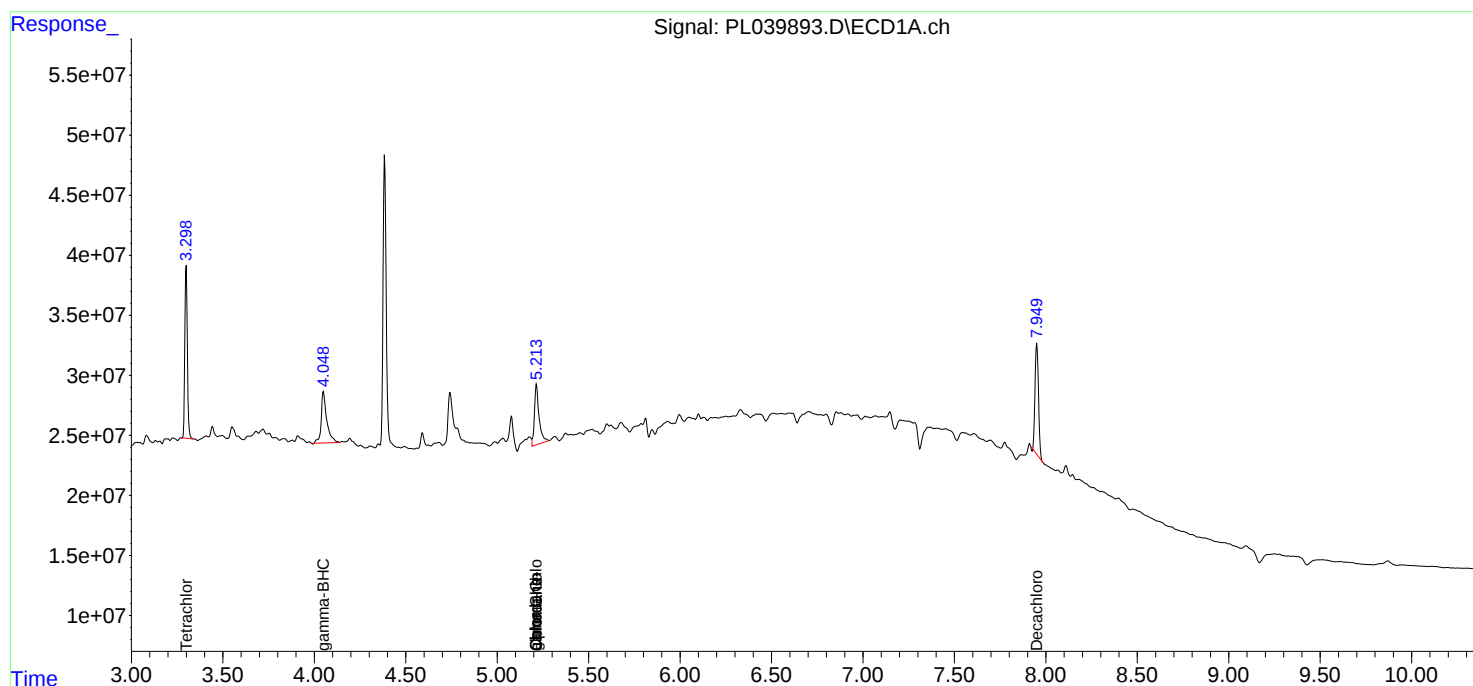


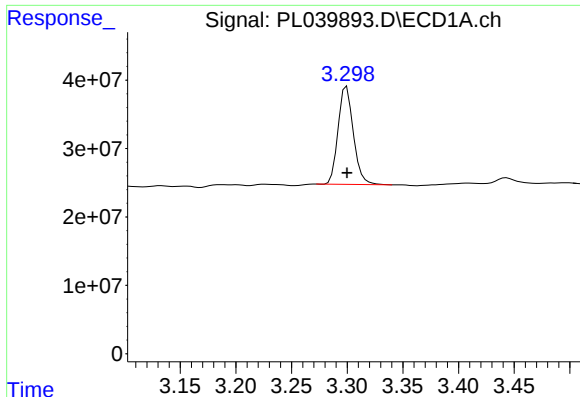

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 136841637
Conc: 17.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

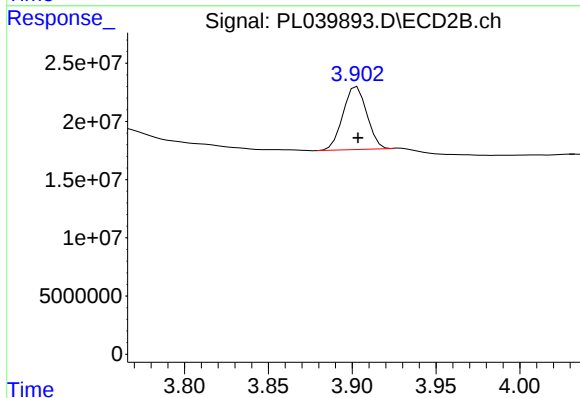


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 53437124
Conc: 16.75 ng/ml

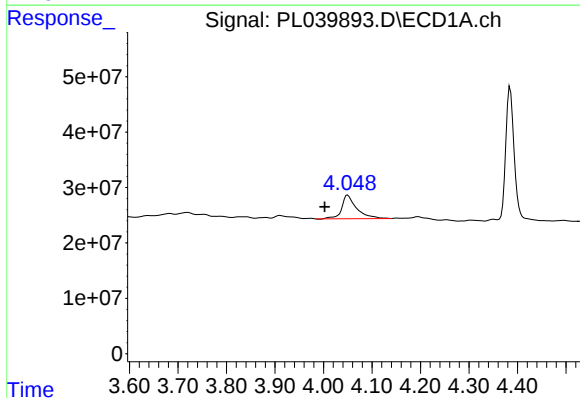


#3 gamma-BHC (Lindane)

R.T.: 4.050 min
Delta R.T.: 0.047 min
Response: 91422447
Conc: 7.99 ng/ml

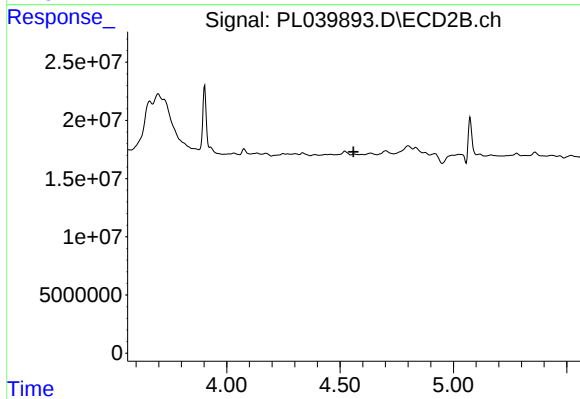

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

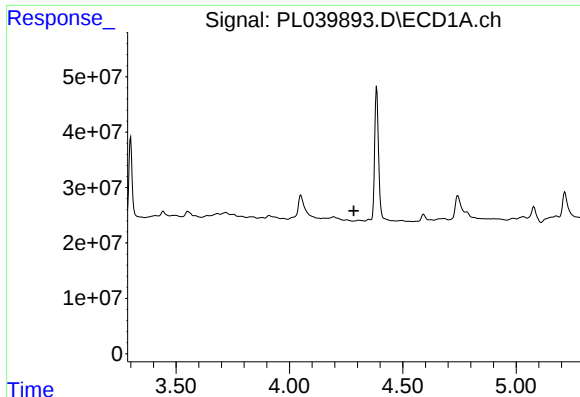

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

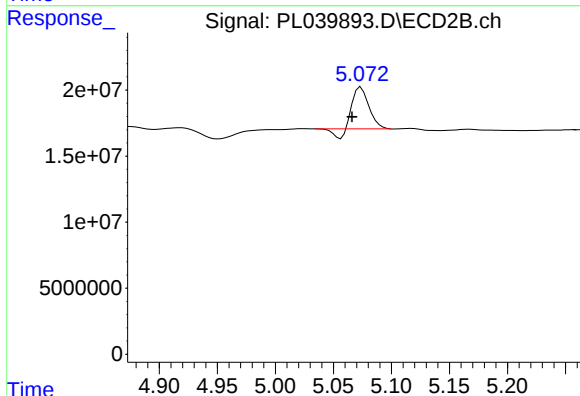


#4 Heptachlor

R.T.: 5.074 min
Delta R.T.: 0.008 min
Response: 27350325
Conc: 6.33 ng/ml

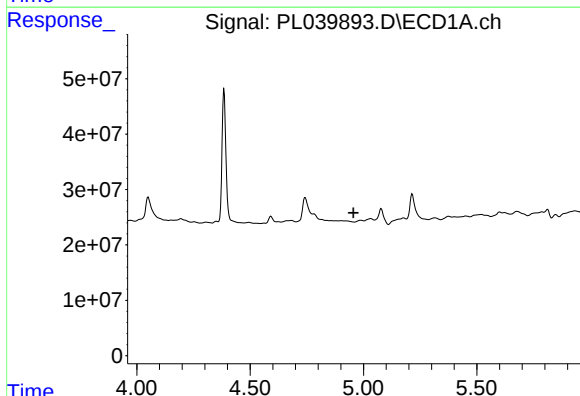


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

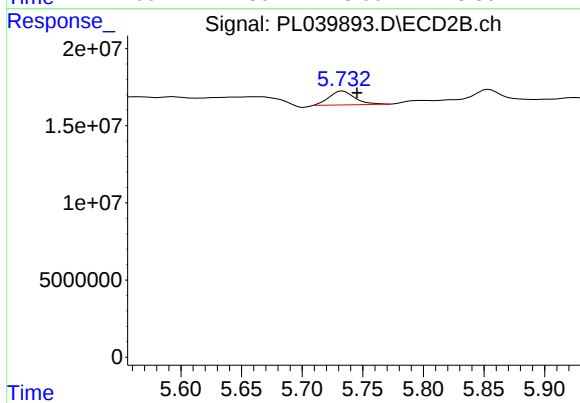

#8 Heptachlor epoxide


R.T.: 5.734 min
Delta R.T.: -0.012 min
Response: 13078198
Conc: 3.31 ng/ml

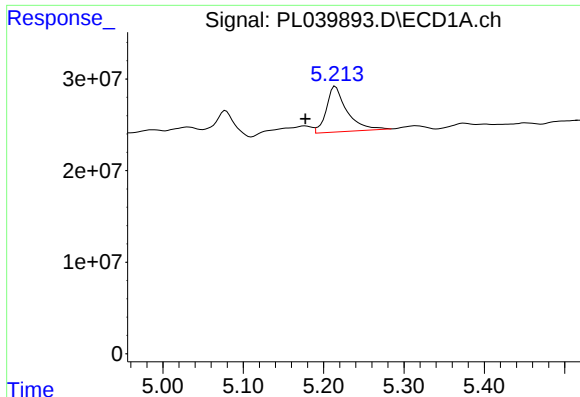

#10 gamma-Chlordane


R.T.: 5.215 min
Delta R.T.: 0.037 min
Response: 88143425
Conc: 7.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

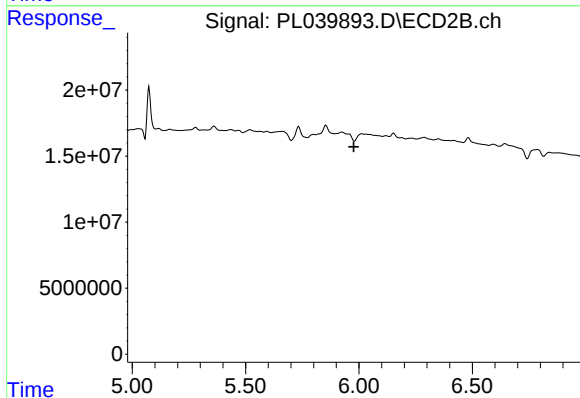


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

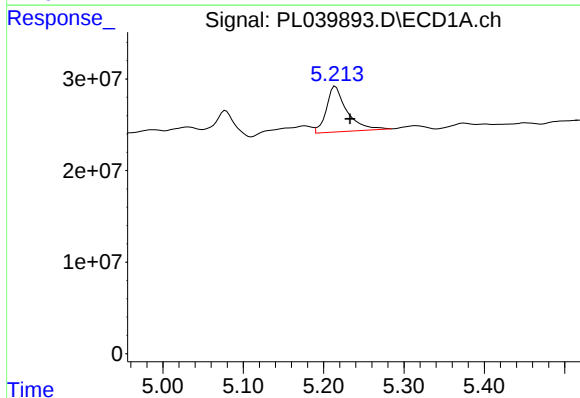


#11 alpha-Chlordane

R.T.: 5.215 min
Delta R.T.: -0.018 min
Response: 88143425
Conc: 8.25 ng/ml

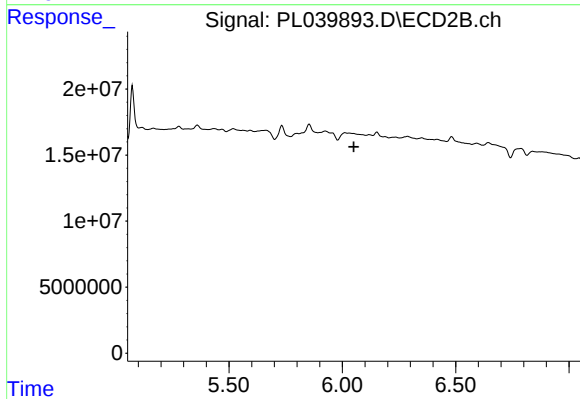

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

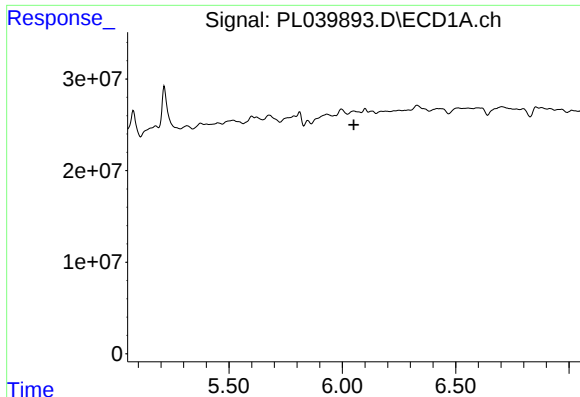

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

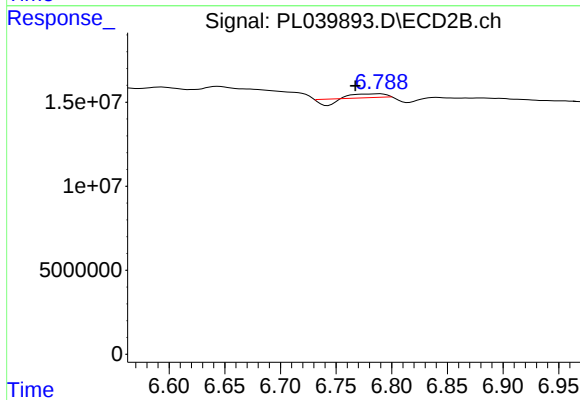


#15 Endosulfan II

R.T.: 6.789 min
Delta R.T.: 0.022 min
Response: 1749015
Conc: 0.53 ng/ml

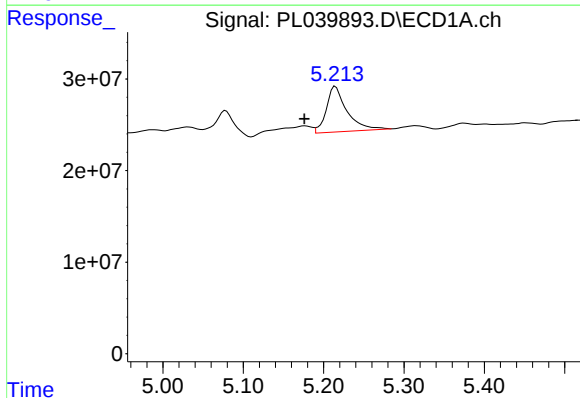


#25 Chlordane-3

R.T.: 5.215 min
Delta R.T.: 0.039 min
Response: 88143425
Conc: 71.83 ng/ml

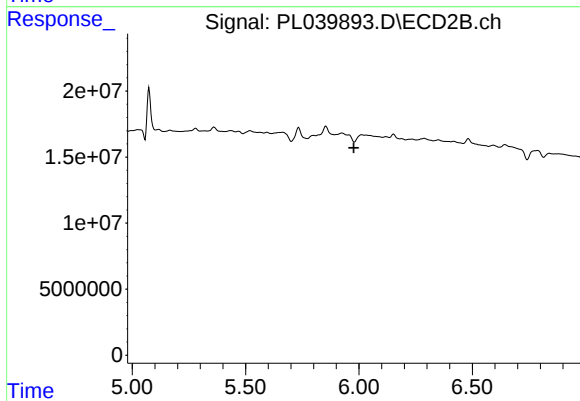

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

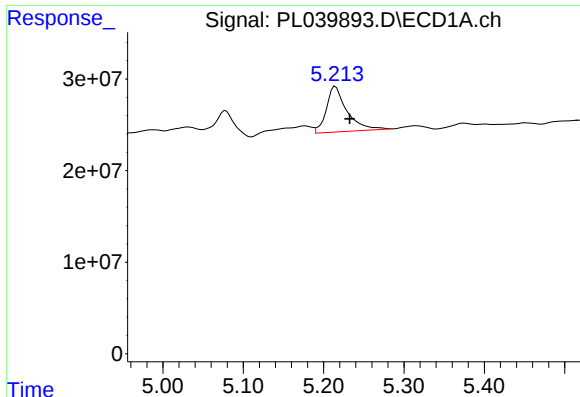

#26 Chlordane-4


R.T.: 5.215 min
Delta R.T.: -0.018 min
Response: 88143425
Conc: 80.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

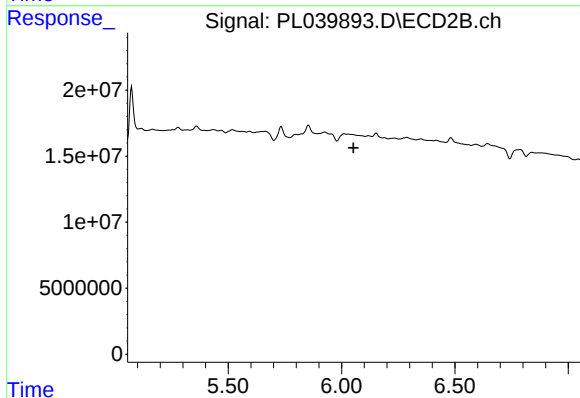


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

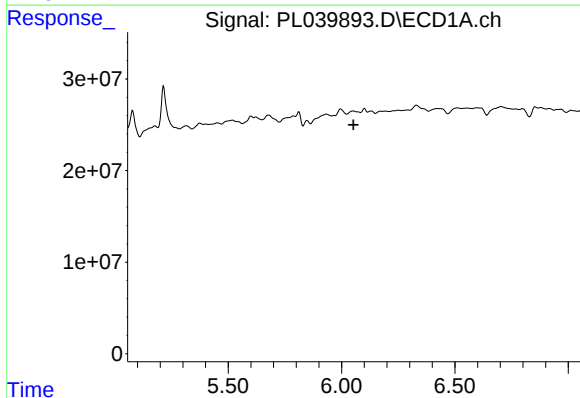


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

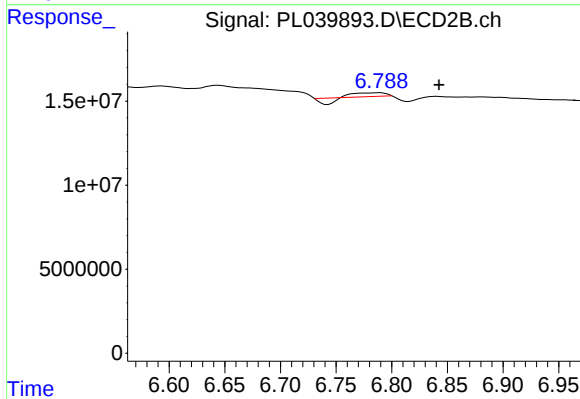

#27 Chlordane-5


R.T.: 6.789 min
Delta R.T.: -0.053 min
Response: 1749015
Conc: 15.07 ng/ml

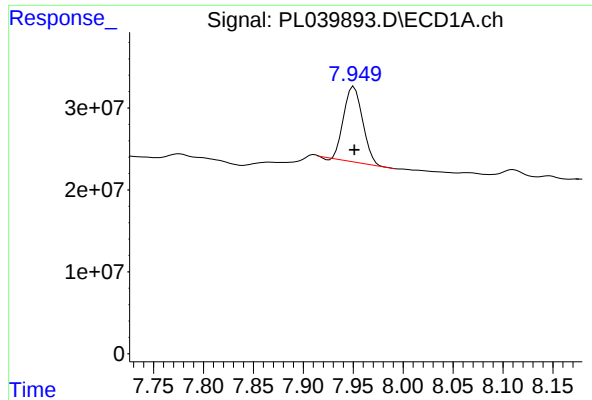

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 119557942
Conc: 14.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

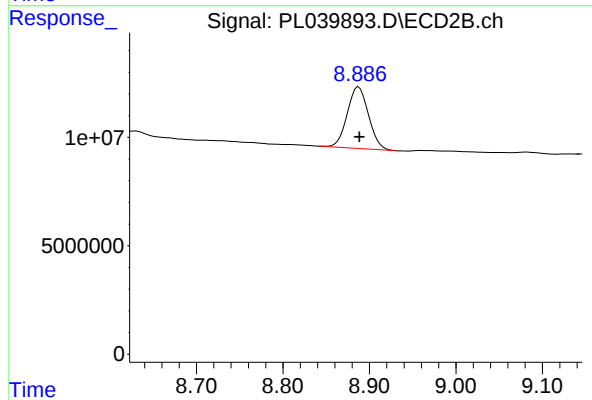

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 48213968
Conc: 17.75 ng/ml