

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 21:04
 Operator : AJ\SJ
 Sample : J4906-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:52:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	125.9E6	62137619	16.231	19.474
28)	SA Decachlor...	7.951	8.889	166.6E6	57116483	19.999	21.029
Target Compounds							
2)	A alpha-BHC	3.742	4.281	96765791	41669938	7.628	8.053
4)	MA Heptachlor	4.316	5.015f	-610432	15185300	N.D.	3.512
5)	MB Aldrin	0.000	5.368	0	23481709	N.D.	5.407 #
20)	A Methoxychlor	6.627f	0.000	31232196	0	6.738	N.D. #
23)	Chlordane-1	4.182	4.878	30610564	15542890	84.456	100.376
24)	Chlordane-2	0.000	5.342	0	34965556	N.D.	229.425 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 21:04
Operator : AJ\SJ
Sample : J4906-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:52:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

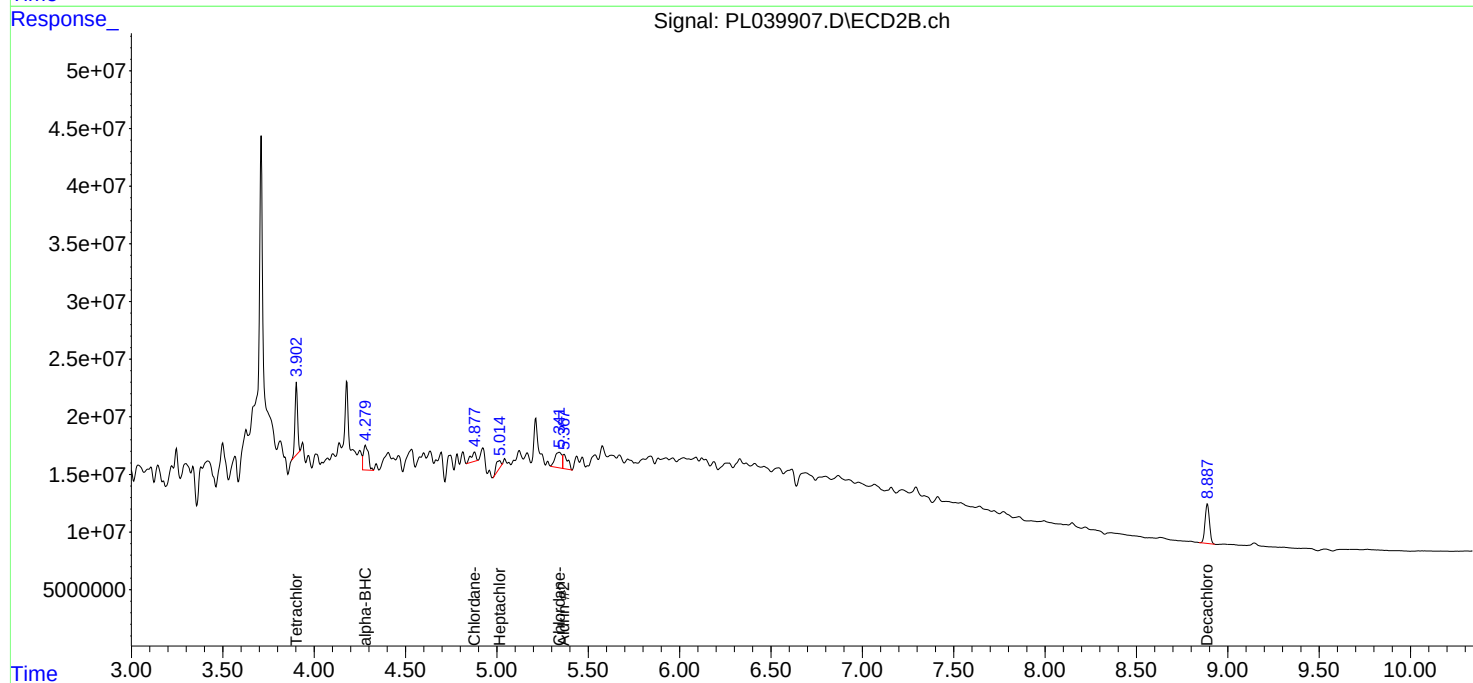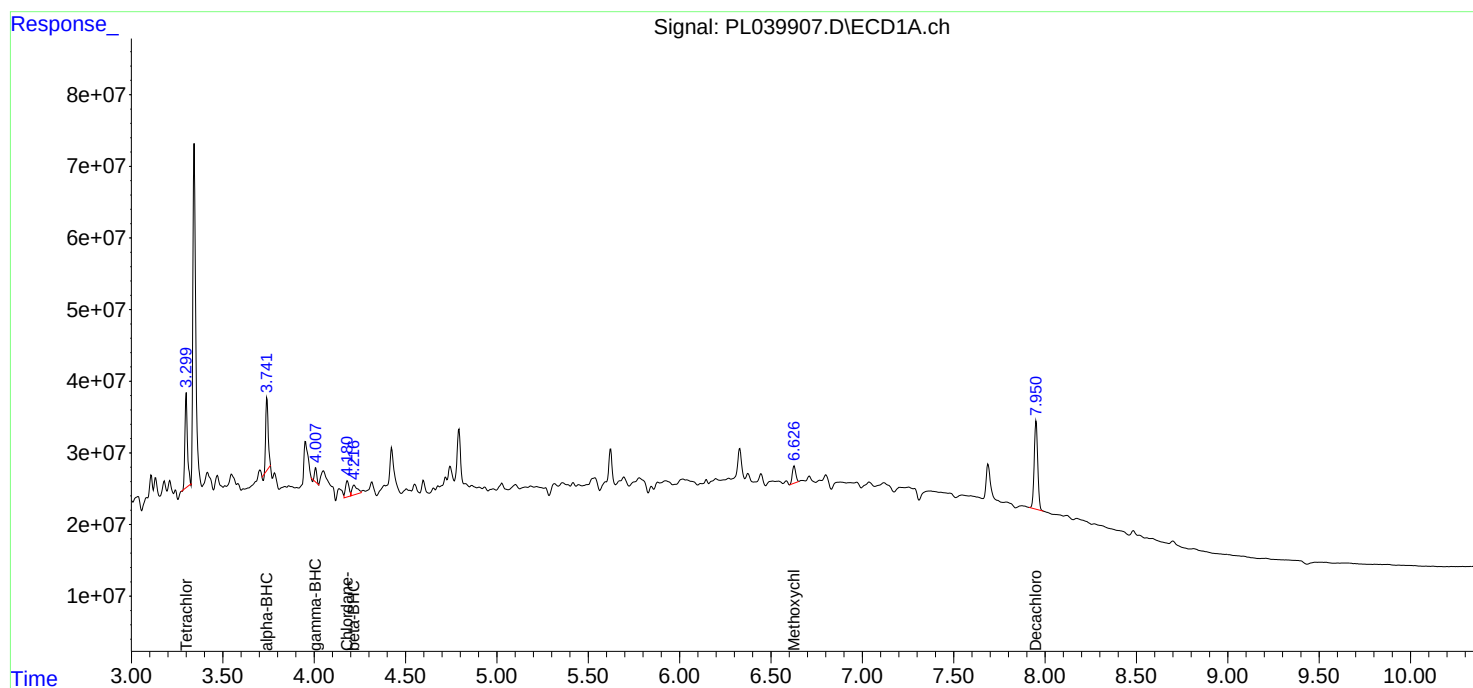


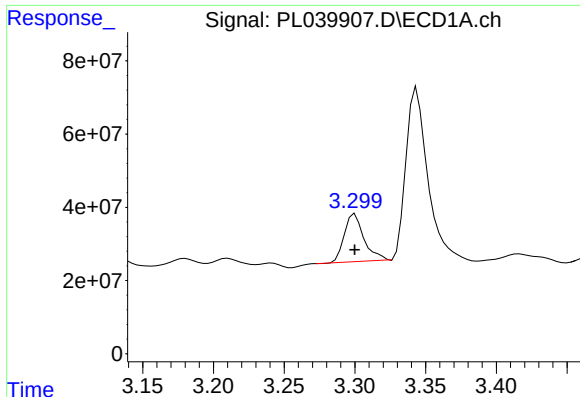

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 125867891
Conc: 16.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

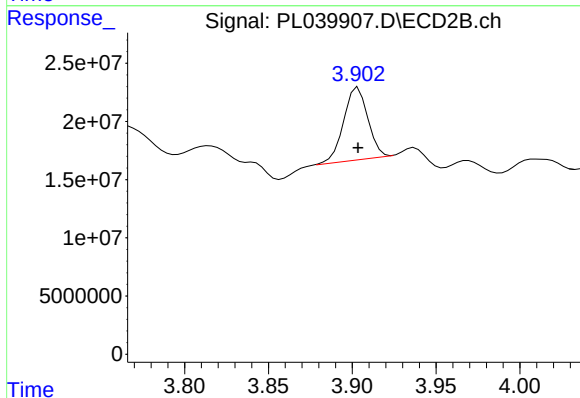


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 62137619
Conc: 19.47 ng/ml

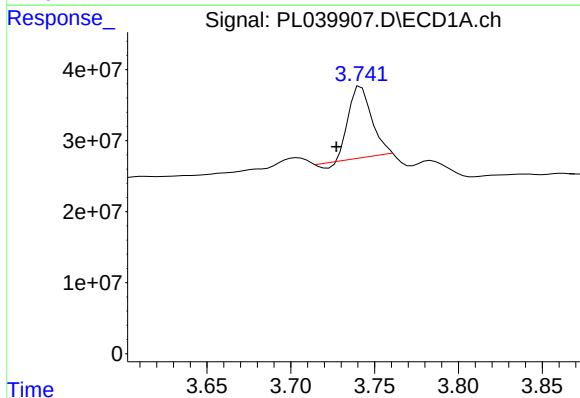


#2 alpha-BHC

R.T.: 3.742 min
Delta R.T.: 0.015 min
Response: 96765791
Conc: 7.63 ng/ml

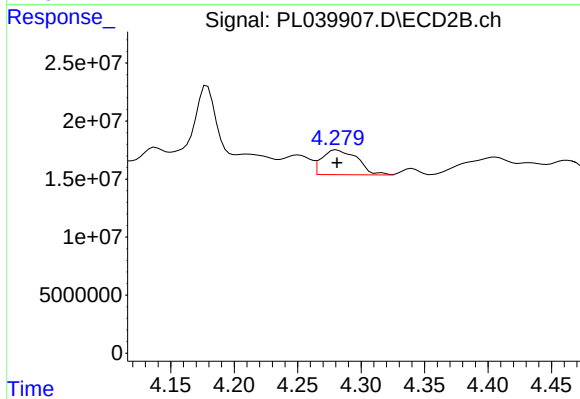

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 41669938
Conc: 8.05 ng/ml

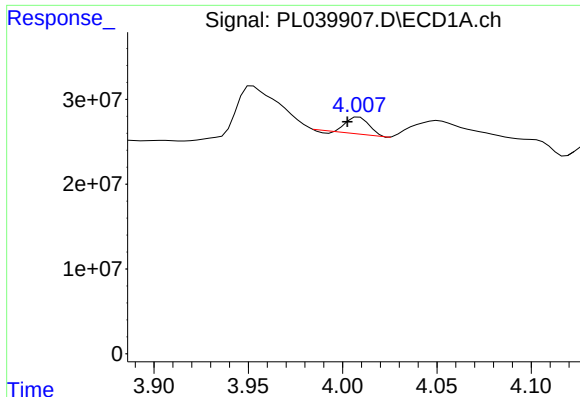

#3 gamma-BHC (Lindane)


R.T.: 4.009 min
Delta R.T.: 0.006 min
Response: 17381907
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

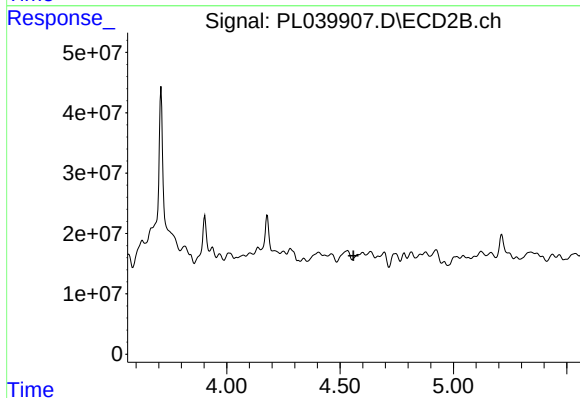


#3 gamma-BHC (Lindane)

R.T.: 4.579 min
Delta R.T.: 0.020 min
Response: -15033900
Conc: N.D.

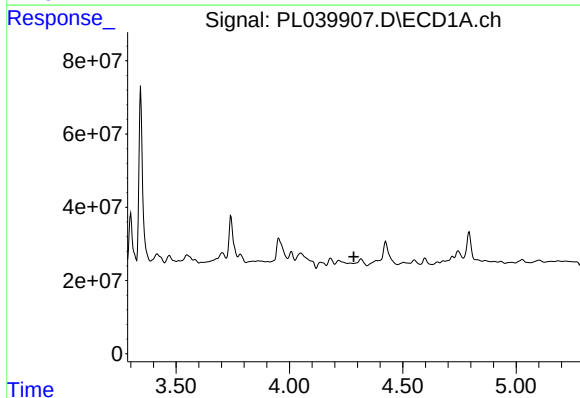


#4 Heptachlor

R.T.: 4.316 min
Delta R.T.: 0.033 min
Response: -610432
Conc: N.D.

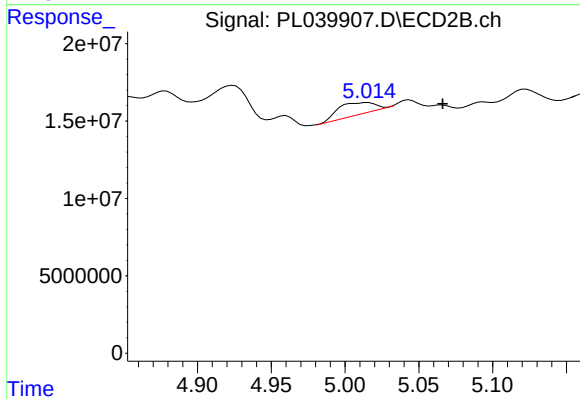

#4 Heptachlor


R.T.: 5.015 min
Delta R.T.: -0.051 min
Response: 15185300
Conc: 3.51 ng/ml

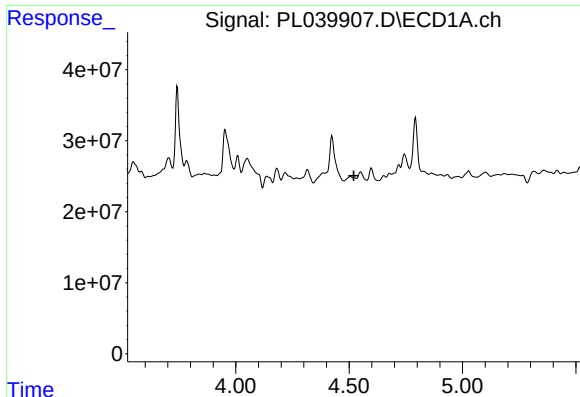

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

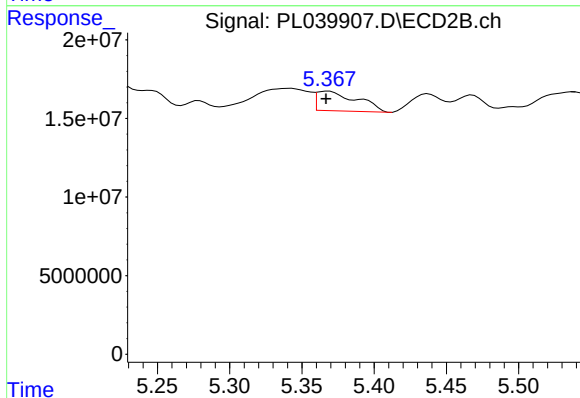


#5 Aldrin

R.T.: 5.368 min
Delta R.T.: 0.001 min
Response: 23481709
Conc: 5.41 ng/ml

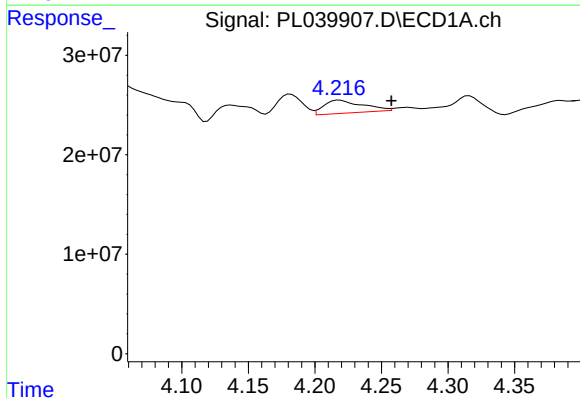


#6 beta-BHC

R.T.: 4.219 min
Delta R.T.: -0.039 min
Response: 26924371
Conc: 5.47 ng/ml

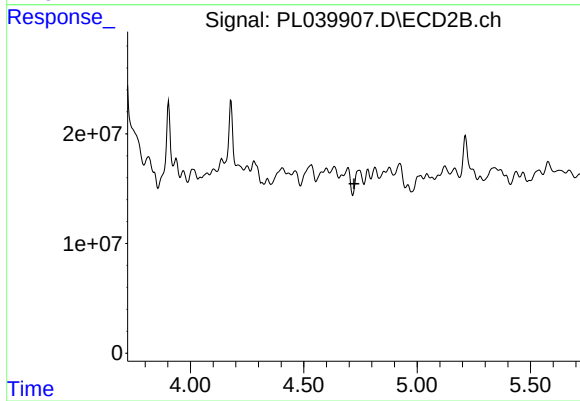

#6 beta-BHC


R.T.: 4.745 min
Delta R.T.: 0.023 min
Response: -24593699
Conc: N.D.

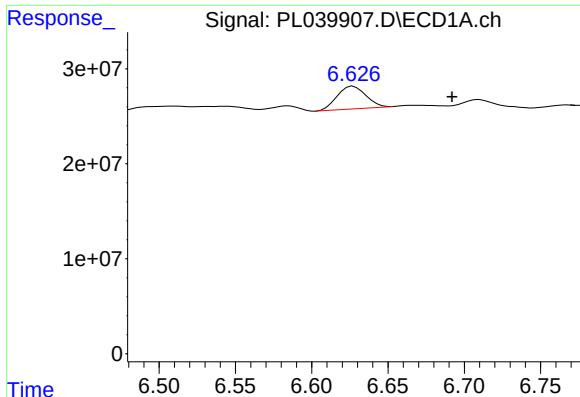

#20 Methoxychlor


R.T.: 6.627 min
Delta R.T.: -0.065 min
Response: 31232196
Conc: 6.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

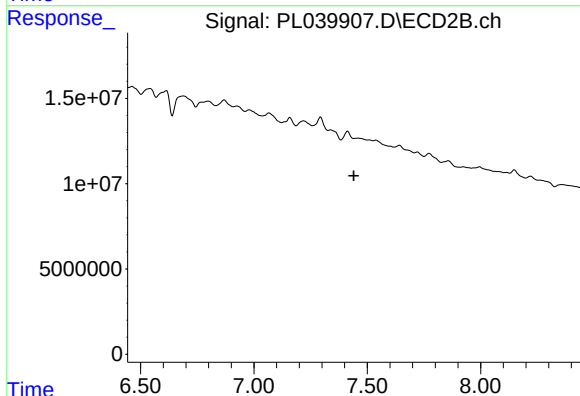


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

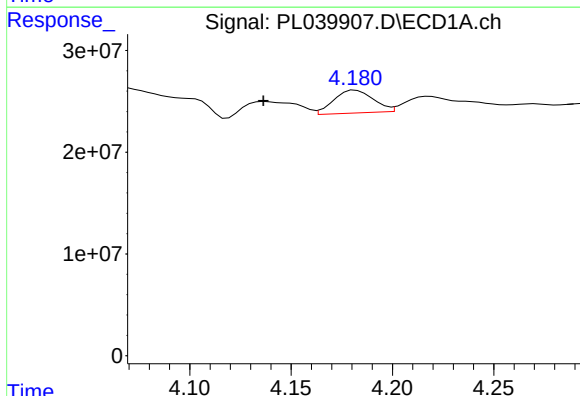


#23 Chlordane-1

R.T.: 4.182 min
Delta R.T.: 0.045 min
Response: 30610564
Conc: 84.46 ng/ml

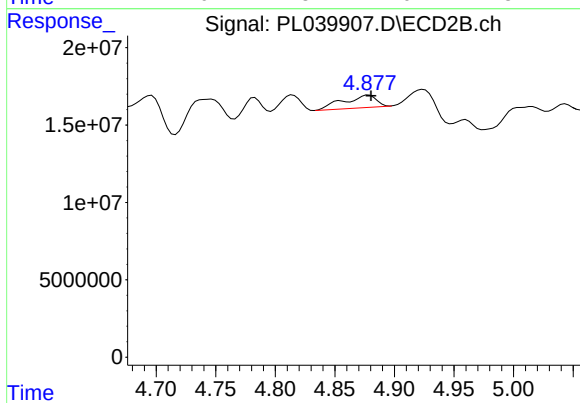

#23 Chlordane-1


R.T.: 4.878 min
Delta R.T.: -0.002 min
Response: 15542890
Conc: 100.38 ng/ml

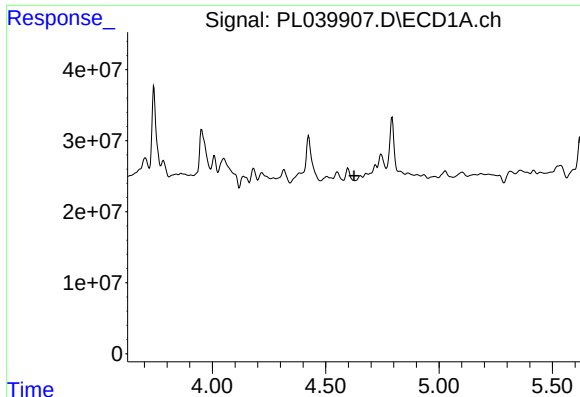

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

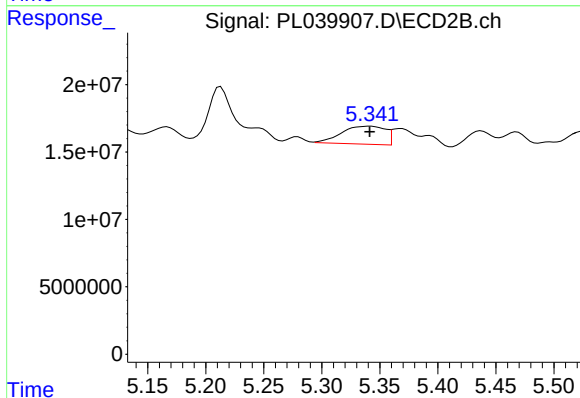


#24 Chlordane-2

R.T.: 5.342 min
Delta R.T.: 0.000 min
Response: 34965556
Conc: 229.43 ng/ml

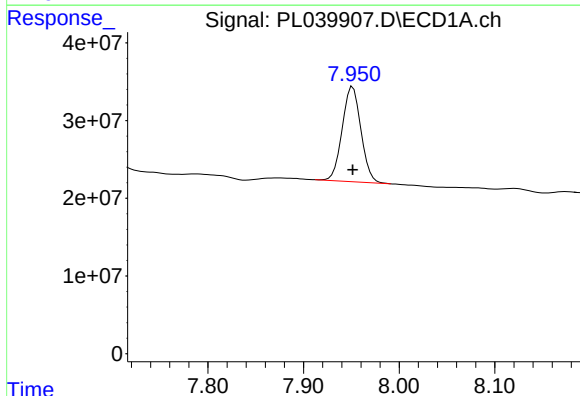

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 166647921
Conc: 20.00 ng/ml

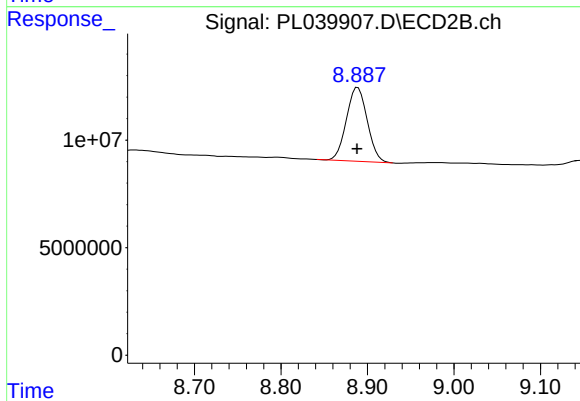

#28 Decachlorobiphenyl

R.T.: 8.889 min
Delta R.T.: 0.000 min
Response: 57116483
Conc: 21.03 ng/ml