

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 21:19
 Operator : AJ\SJ
 Sample : J4898-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:52:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	126.7E6	61910527	16.344	19.403
28)	SA Decachlor...	7.950	8.888	166.8E6	57757682	20.014	21.265
Target Compounds							
2)	A alpha-BHC	3.742	4.281	99134393	39715344	7.814	7.675
4)	MA Heptachlor	4.316	5.015f	468467	13558990	0.041	3.136 #
5)	MB Aldrin	0.000	5.368	0	7058309	N.D.	1.625 #
7)	B delta-BHC	0.000	4.924	0	12886630	N.D.	3.240 #
10)	B gamma-Chl...	0.000	5.926f	0	5008502	N.D.	1.323 #
20)	A Methoxychlor	6.628f	0.000	30875449	0	6.661	N.D. #
23)	Chlordane-1	4.182	4.878	30038929	9800237	82.879	63.290
24)	Chlordane-2	0.000	5.342	0	24945224	N.D.	163.677 #
25)	Chlordane-3	0.000	5.926	0	5008502	N.D.	9.783 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 21:19
Operator : AJ\SJ
Sample : J4898-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:52:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

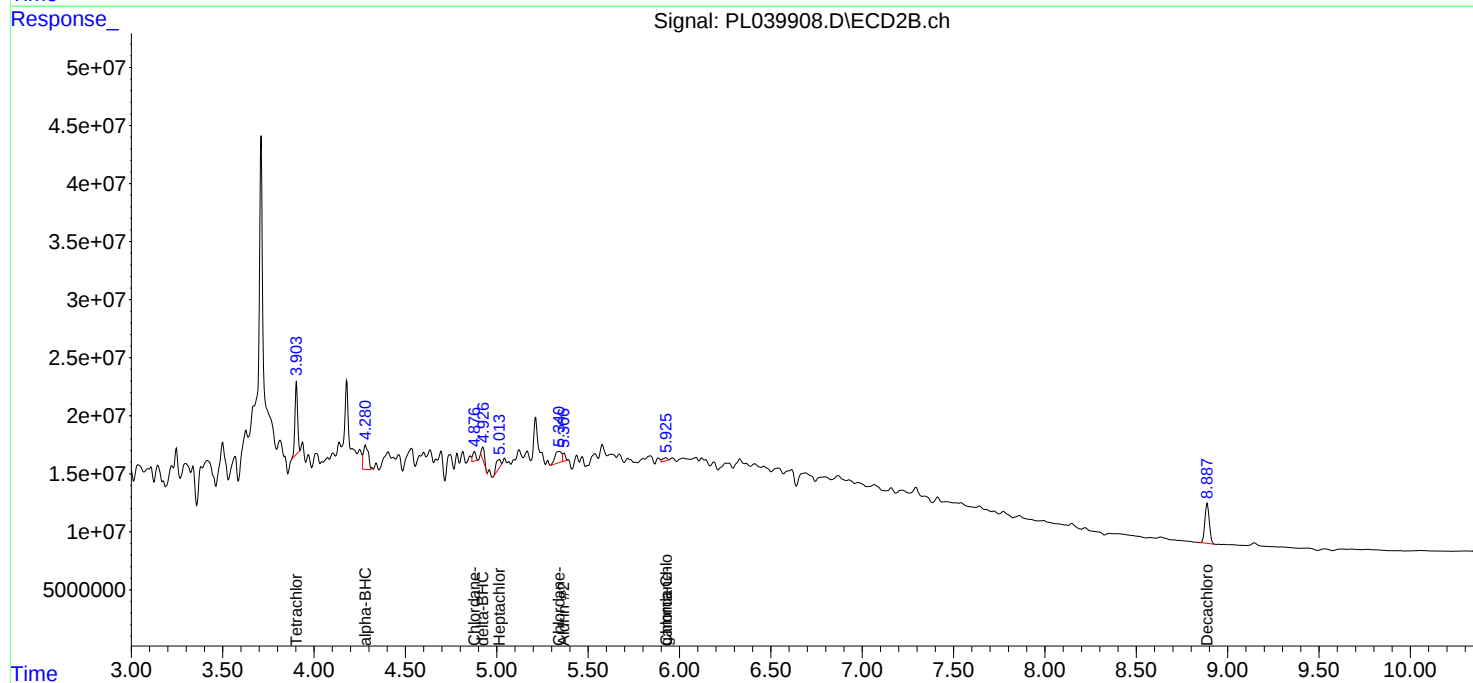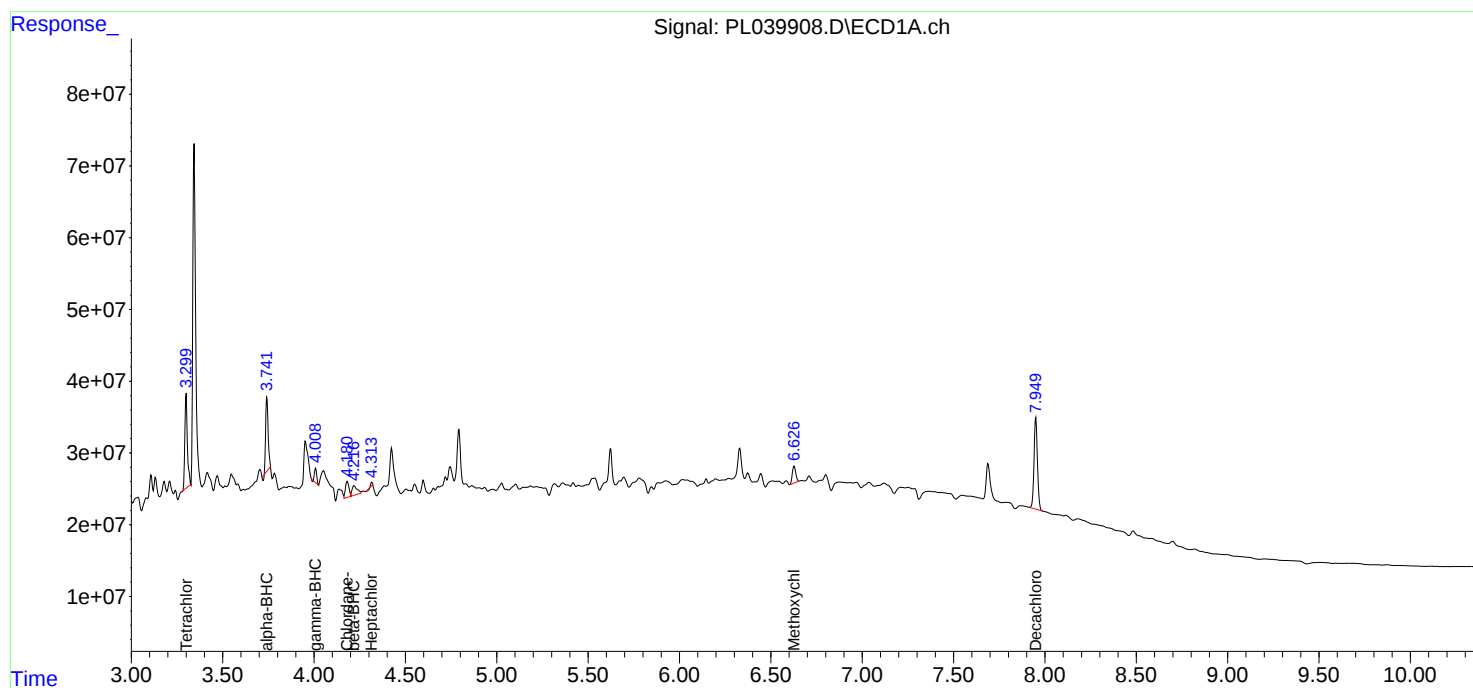


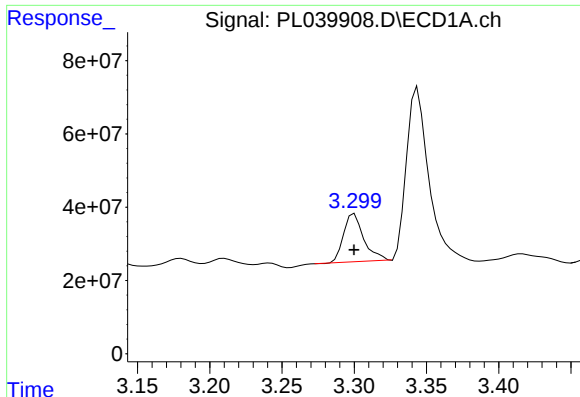

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 126744557
Conc: 16.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

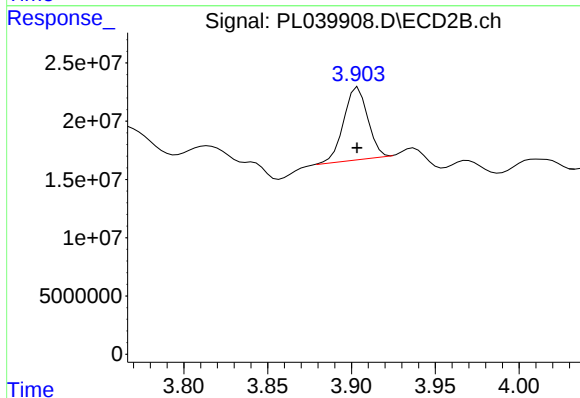


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 61910527
Conc: 19.40 ng/ml

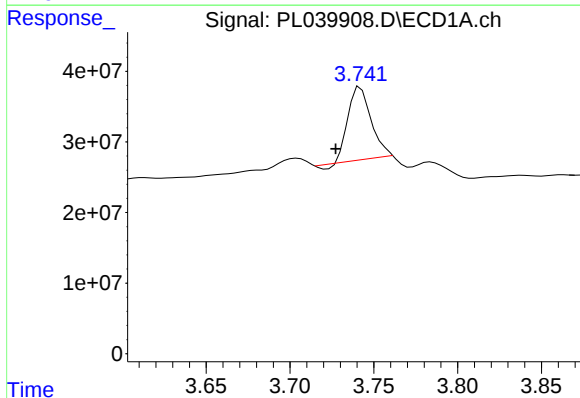


#2 alpha-BHC

R.T.: 3.742 min
Delta R.T.: 0.015 min
Response: 99134393
Conc: 7.81 ng/ml

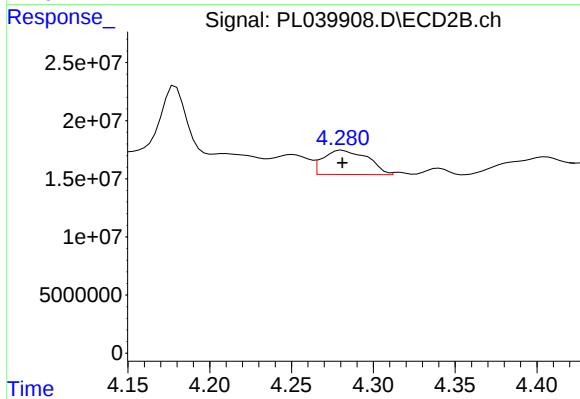

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 39715344
Conc: 7.67 ng/ml

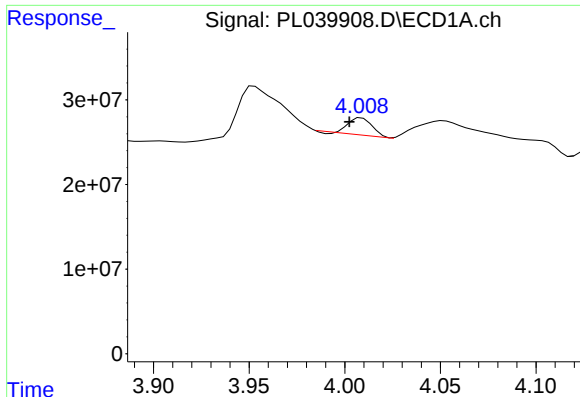

#3 gamma-BHC (Lindane)


R.T.: 4.009 min
Delta R.T.: 0.006 min
Response: 18024245
Conc: 1.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

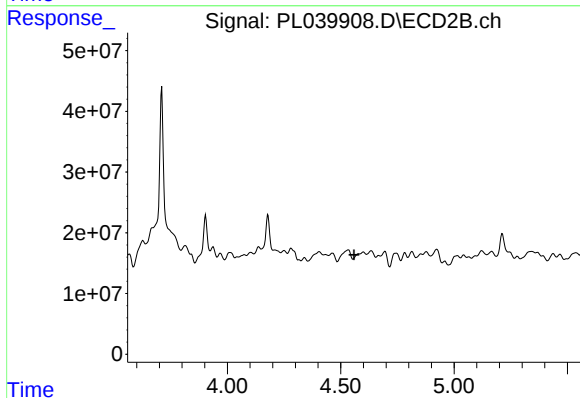


#3 gamma-BHC (Lindane)

R.T.: 4.579 min
Delta R.T.: 0.019 min
Response: -15097339
Conc: N.D.

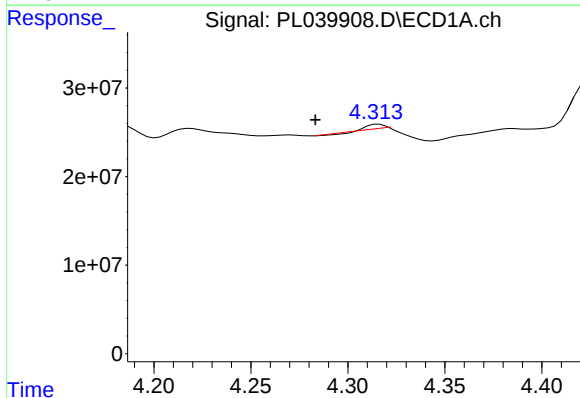


#4 Heptachlor

R.T.: 4.316 min
Delta R.T.: 0.033 min
Response: 468467
Conc: 0.04 ng/ml

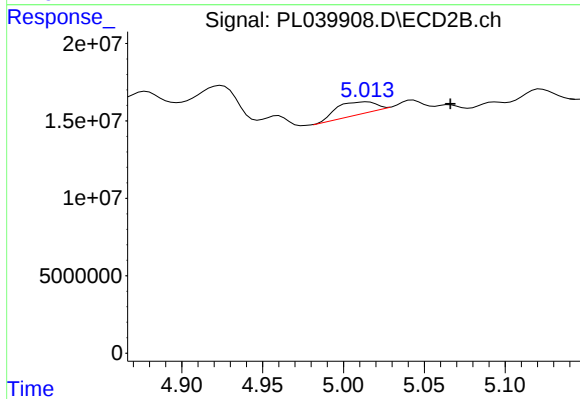

#4 Heptachlor


R.T.: 5.015 min
Delta R.T.: -0.052 min
Response: 13558990
Conc: 3.14 ng/ml

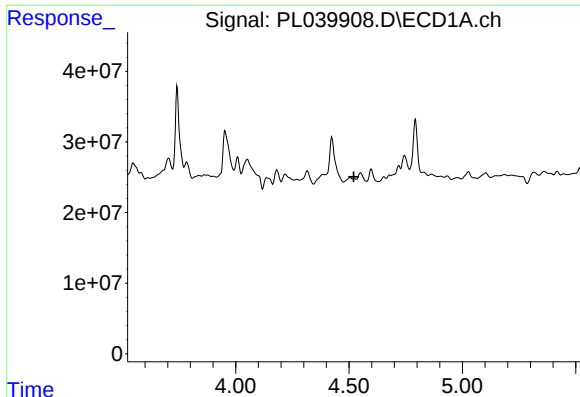

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

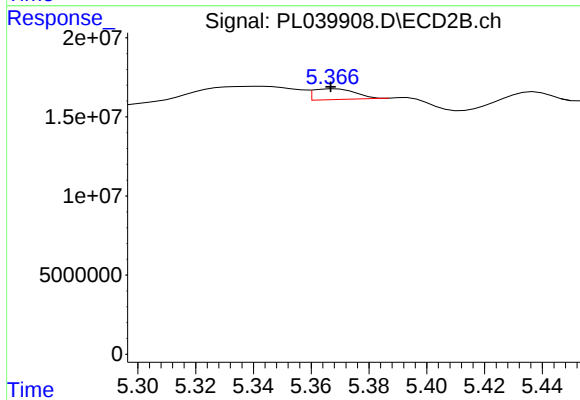


#5 Aldrin

R.T.: 5.368 min
Delta R.T.: 0.002 min
Response: 7058309
Conc: 1.63 ng/ml

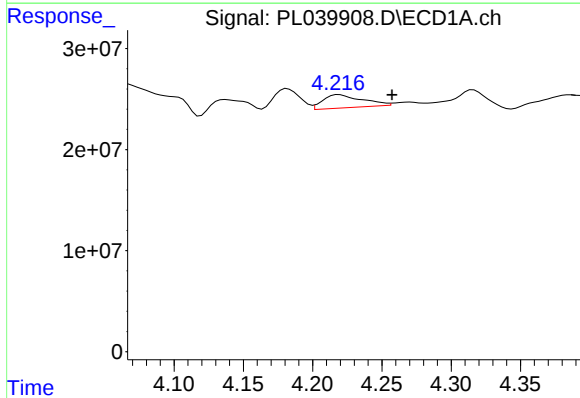


#6 beta-BHC

R.T.: 4.219 min
Delta R.T.: -0.038 min
Response: 25732197
Conc: 5.23 ng/ml

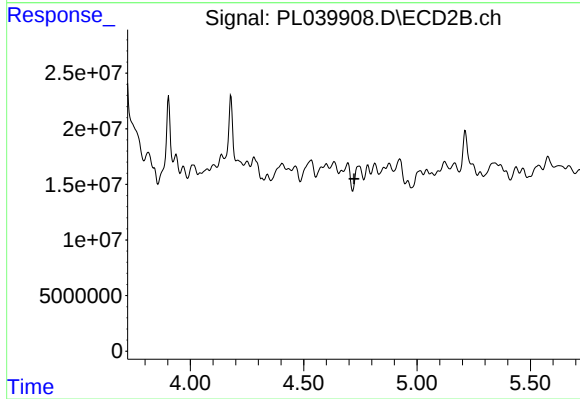

#6 beta-BHC


R.T.: 4.746 min
Delta R.T.: 0.023 min
Response: -17544122
Conc: N.D.

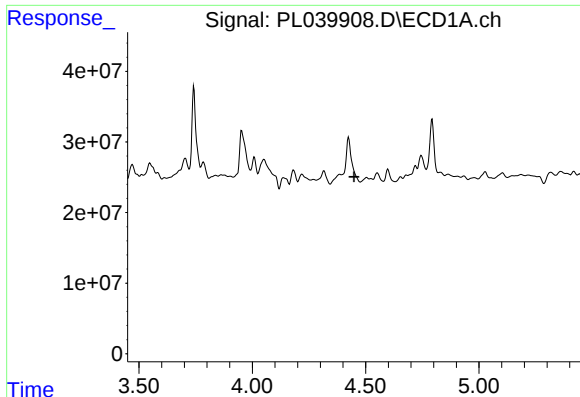

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

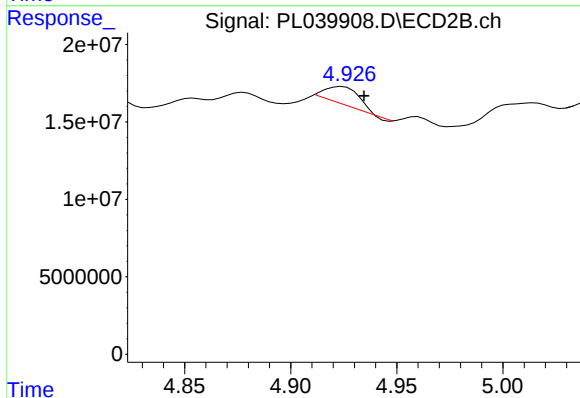


#7 delta-BHC

R.T.: 4.924 min
Delta R.T.: -0.010 min
Response: 12886630
Conc: 3.24 ng/ml

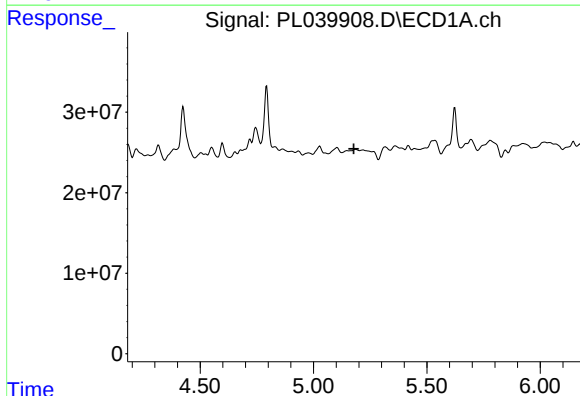


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

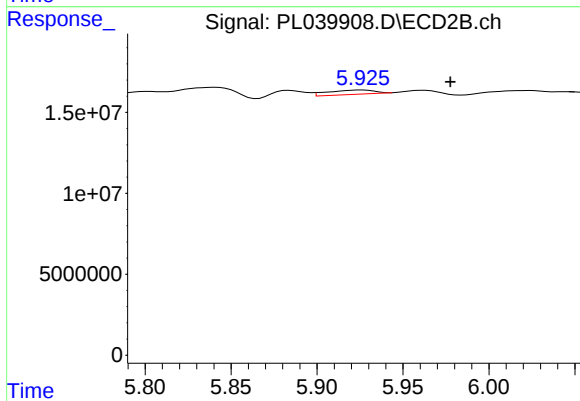

#10 gamma-Chlordane


R.T.: 5.926 min
Delta R.T.: -0.052 min
Response: 5008502
Conc: 1.32 ng/ml

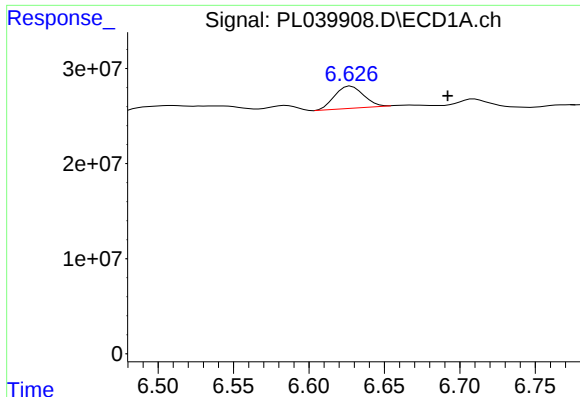

#20 Methoxychlor


R.T.: 6.628 min
Delta R.T.: -0.064 min
Response: 30875449
Conc: 6.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

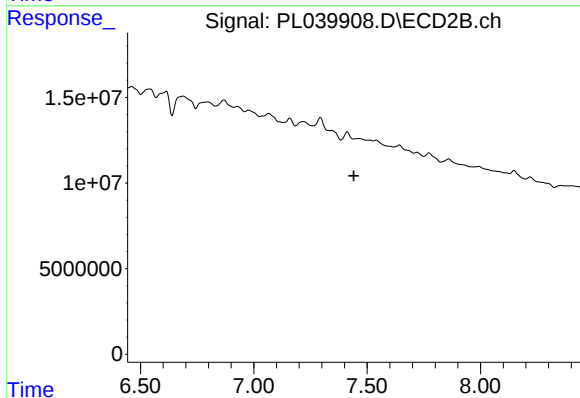


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

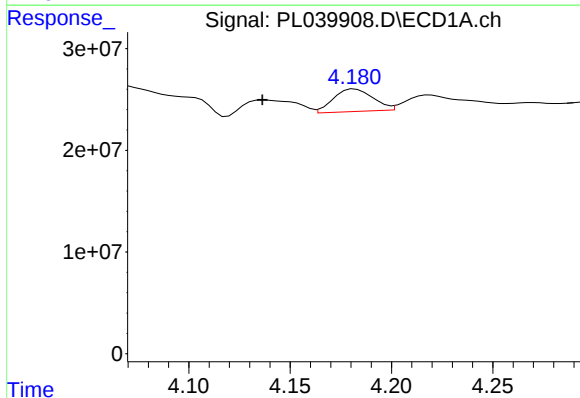


#23 Chlordane-1

R.T.: 4.182 min
Delta R.T.: 0.046 min
Response: 30038929
Conc: 82.88 ng/ml

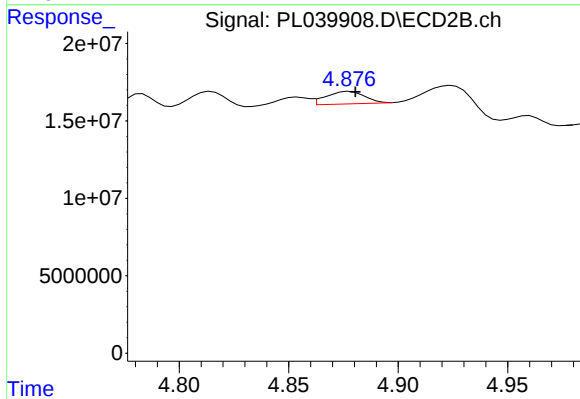

#23 Chlordane-1


R.T.: 4.878 min
Delta R.T.: -0.002 min
Response: 9800237
Conc: 63.29 ng/ml

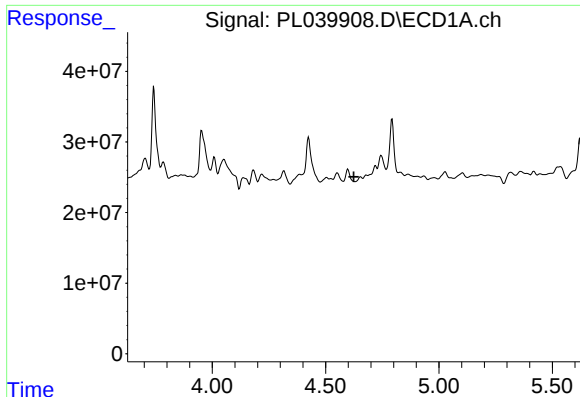

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

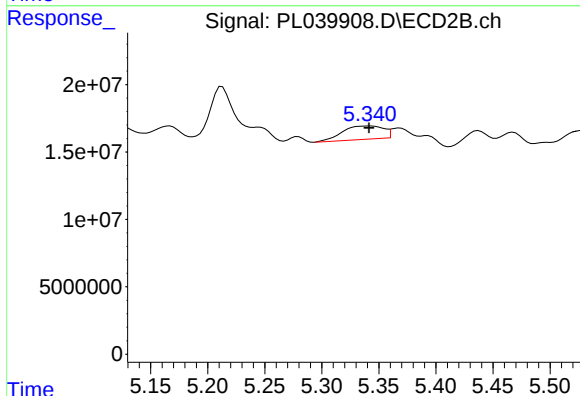


#24 Chlordane-2

R.T.: 5.342 min
Delta R.T.: 0.000 min
Response: 24945224
Conc: 163.68 ng/ml

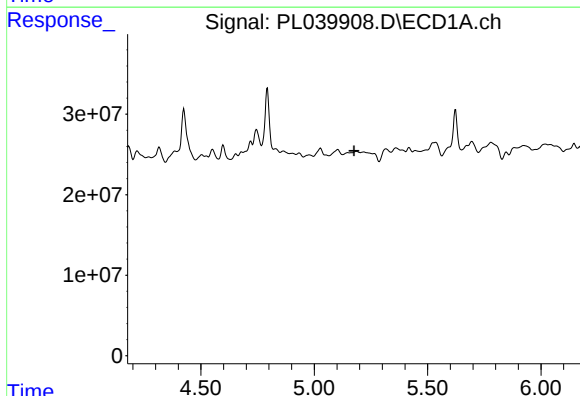


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

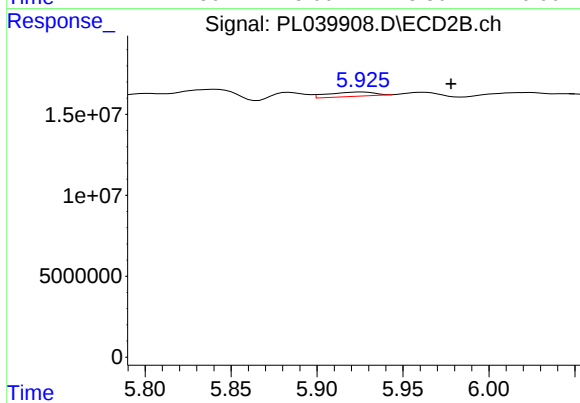

#25 Chlordane-3


R.T.: 5.926 min
Delta R.T.: -0.052 min
Response: 5008502
Conc: 9.78 ng/ml

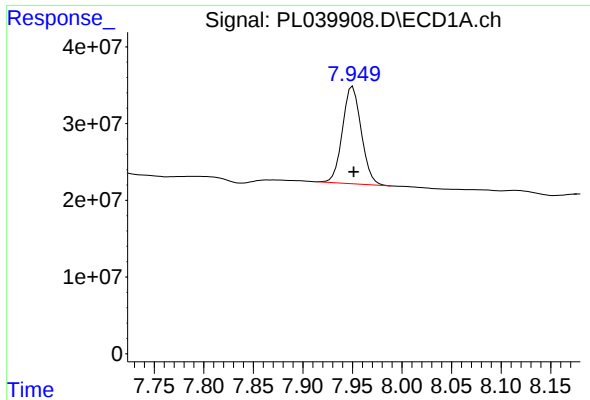

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 166765479
Conc: 20.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

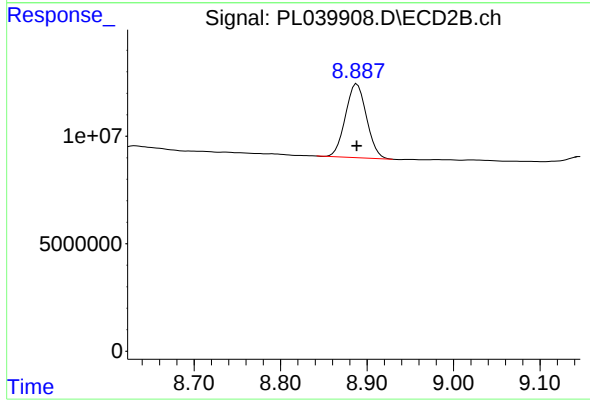

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 57757682
Conc: 21.27 ng/ml