

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 21:33
 Operator : AJ\SJ
 Sample : J4906-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:52:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	125.6E6	59212998	16.192	18.557
28)	SA Decachlor...	7.951	8.888	164.2E6	60222340	19.703	22.173
Target Compounds							
2)	A alpha-BHC	3.742	4.281	79957916	40625245	6.303	7.851
4)	MA Heptachlor	4.316	5.015f	578130	12291402	0.050	2.843 #
5)	MB Aldrin	0.000	5.369	0	6714108	N.D.	1.546 #
7)	B delta-BHC	0.000	4.924	0	11375843	N.D.	2.860 #
19)	B Endosulfa...	0.000	7.068f	0	5622699	N.D.	1.915 #
20)	A Methoxychlor	6.627f	0.000	36668634	0	7.911	N.D. #
23)	Chlordane-1	4.181	4.878	29519926	8547217	81.447	55.198 #
24)	Chlordane-2	4.598	5.341	13037207	22292114	34.617	146.269 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 21:33
Operator : AJ\SJ
Sample : J4906-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:52:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

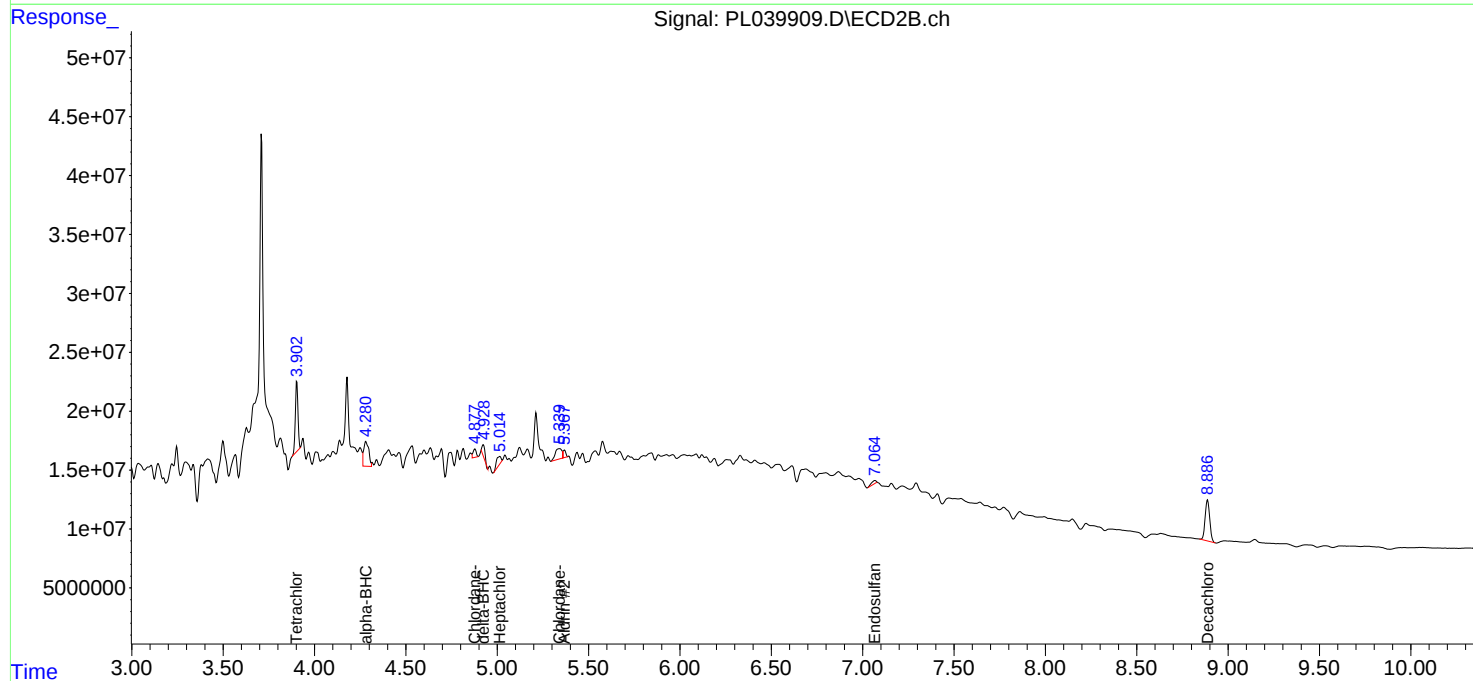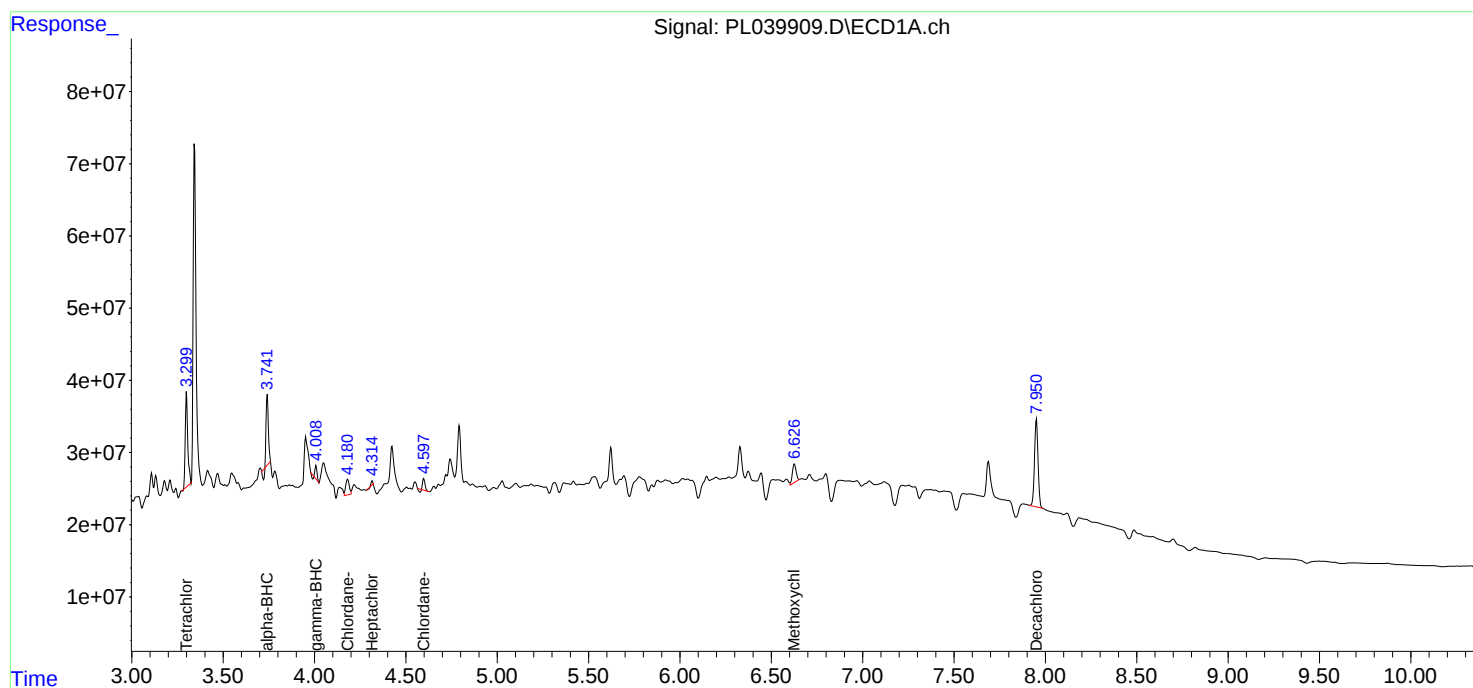


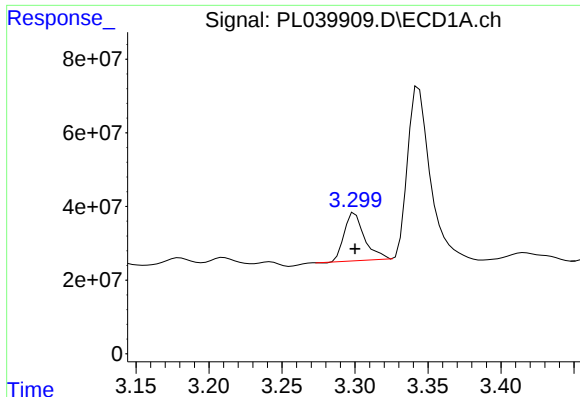

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 125564062
Conc: 16.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

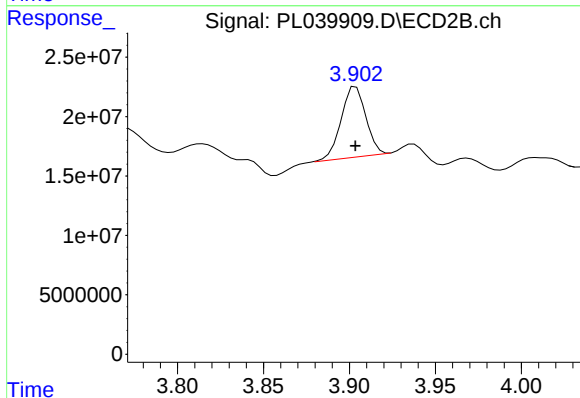


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 59212998
Conc: 18.56 ng/ml

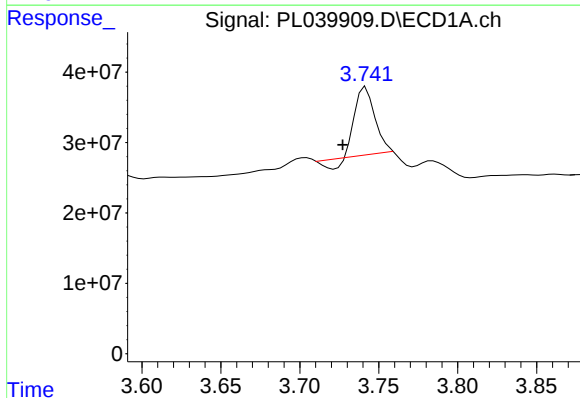


#2 alpha-BHC

R.T.: 3.742 min
Delta R.T.: 0.015 min
Response: 79957916
Conc: 6.30 ng/ml

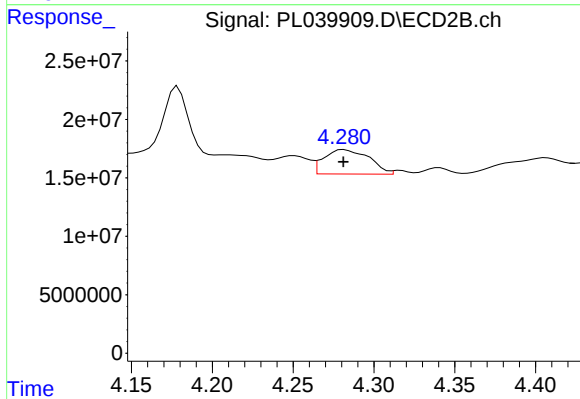

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 40625245
Conc: 7.85 ng/ml

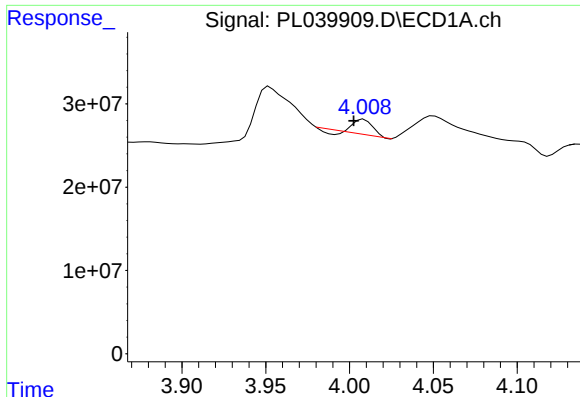

#3 gamma-BHC (Lindane)


R.T.: 4.008 min
Delta R.T.: 0.006 min
Response: 12902661
Conc: 1.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

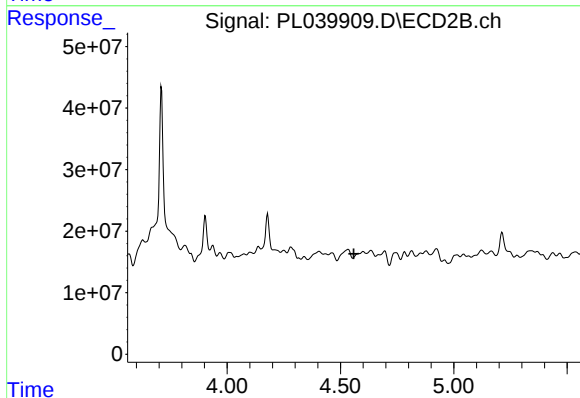


#3 gamma-BHC (Lindane)

R.T.: 4.579 min
Delta R.T.: 0.019 min
Response: -13984895
Conc: N.D.

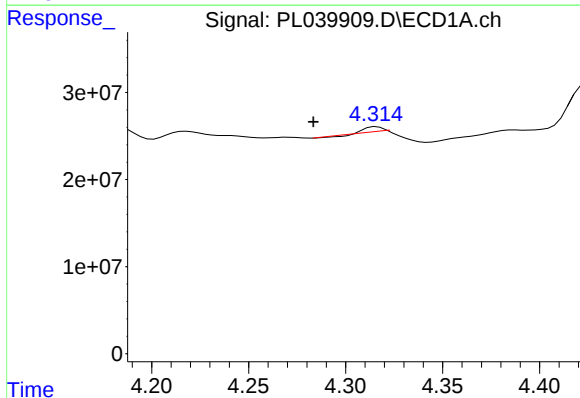


#4 Heptachlor

R.T.: 4.316 min
Delta R.T.: 0.033 min
Response: 578130
Conc: 0.05 ng/ml

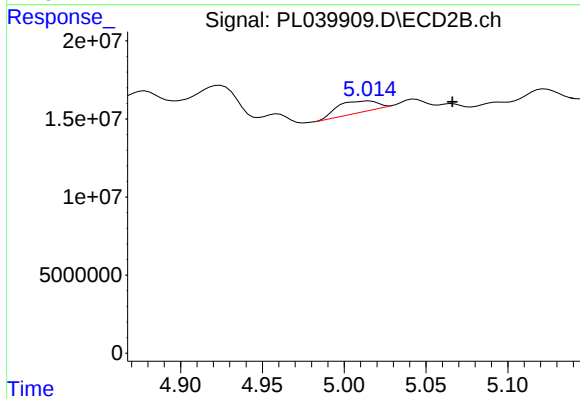

#4 Heptachlor


R.T.: 5.015 min
Delta R.T.: -0.051 min
Response: 12291402
Conc: 2.84 ng/ml

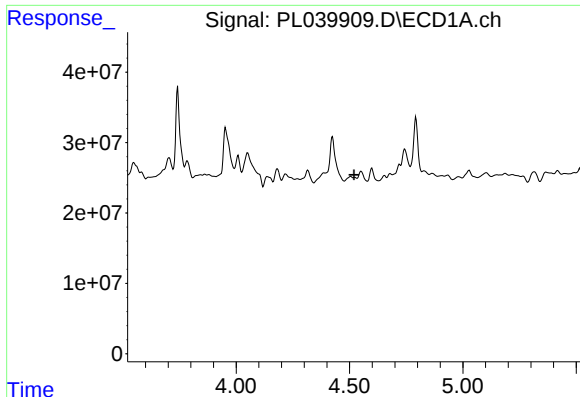

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

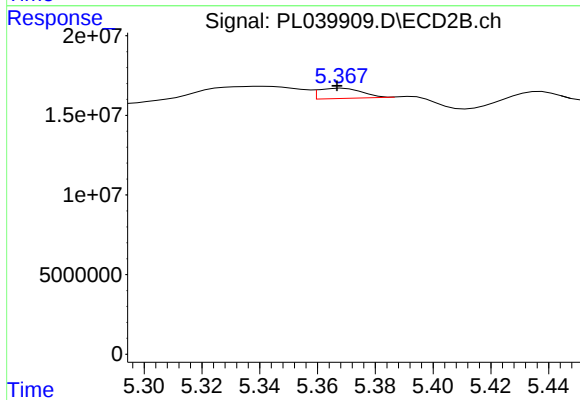


#5 Aldrin

R.T.: 5.369 min
Delta R.T.: 0.002 min
Response: 6714108
Conc: 1.55 ng/ml

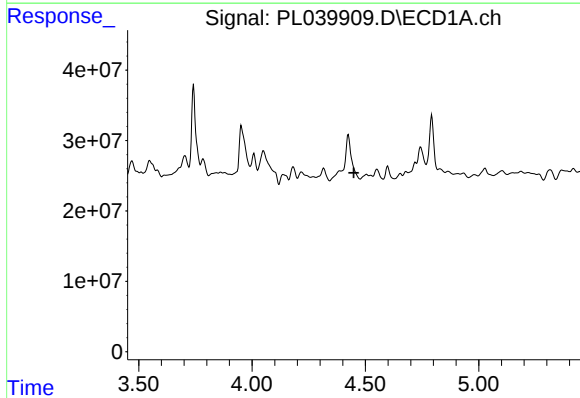


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.449 min
Response: 0
Conc: N.D.

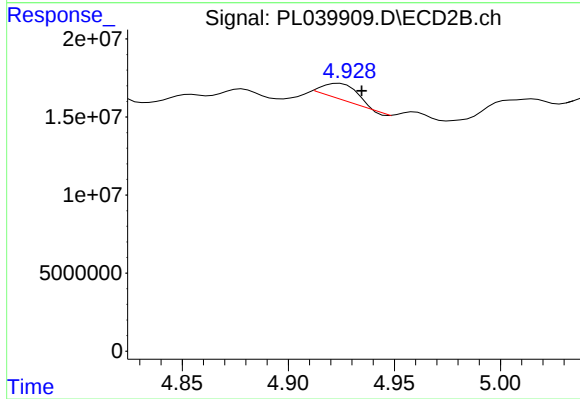

#7 delta-BHC


R.T.: 4.924 min
Delta R.T.: -0.010 min
Response: 11375843
Conc: 2.86 ng/ml

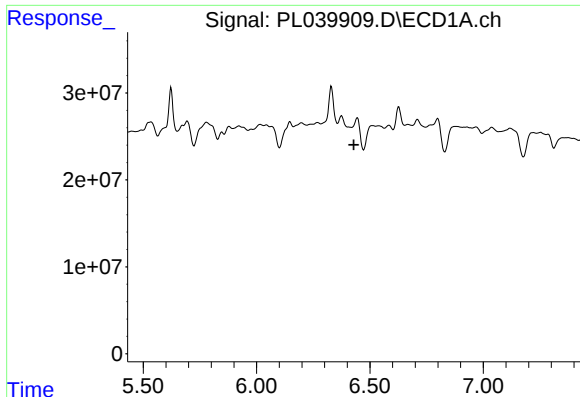

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

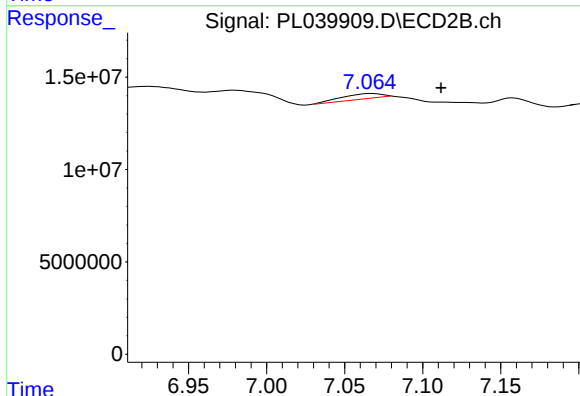


#19 Endosulfan Sulfate

R.T.: 7.068 min
Delta R.T.: -0.044 min
Response: 5622699
Conc: 1.92 ng/ml

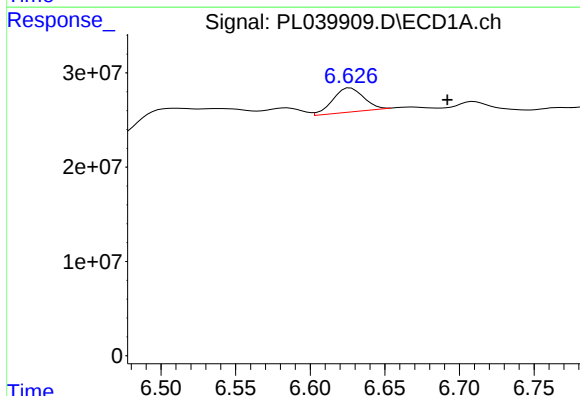


#20 Methoxychlor

R.T.: 6.627 min
Delta R.T.: -0.065 min
Response: 36668634
Conc: 7.91 ng/ml

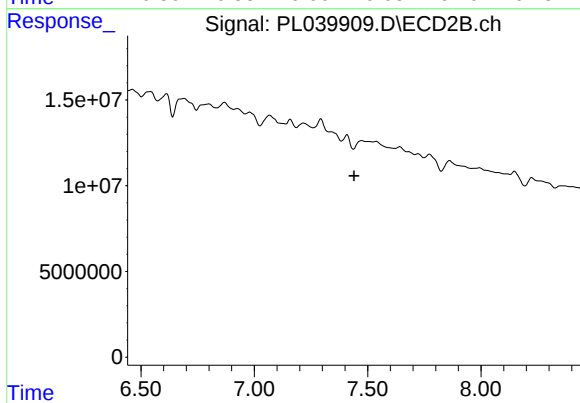

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.441 min
Response: 0
Conc: N.D.

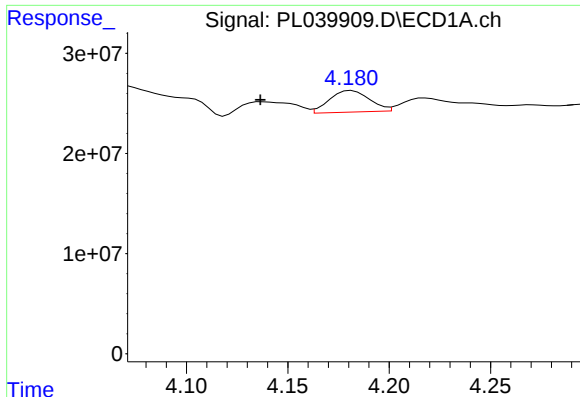

#23 Chlordane-1


R.T.: 4.181 min
Delta R.T.: 0.045 min
Response: 29519926
Conc: 81.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

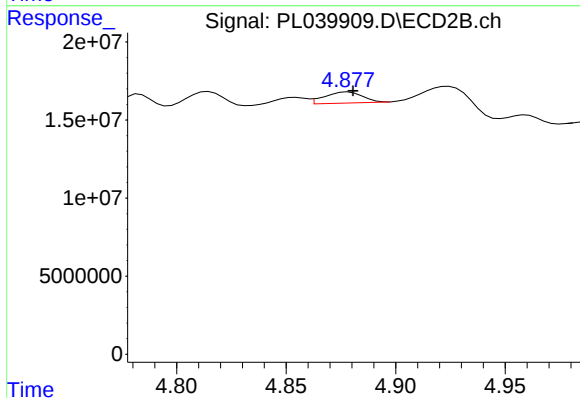


#23 Chlordane-1

R.T.: 4.878 min
Delta R.T.: -0.002 min
Response: 8547217
Conc: 55.20 ng/ml

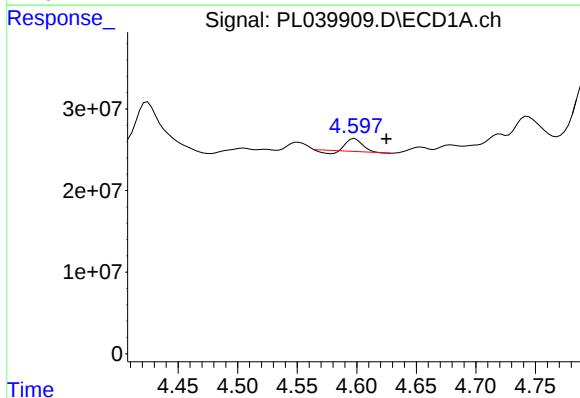


#24 Chlordane-2

R.T.: 4.598 min
Delta R.T.: -0.027 min
Response: 13037207
Conc: 34.62 ng/ml

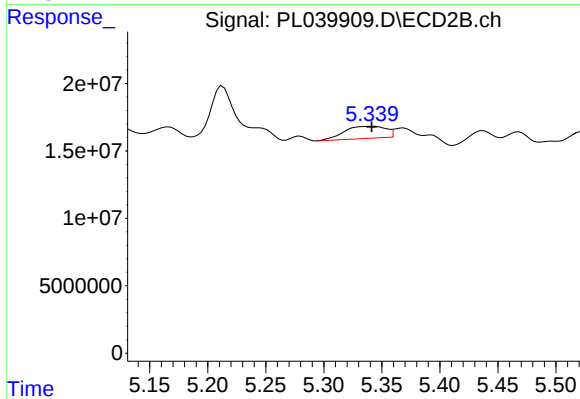

#24 Chlordane-2


R.T.: 5.341 min
Delta R.T.: 0.000 min
Response: 22292114
Conc: 146.27 ng/ml

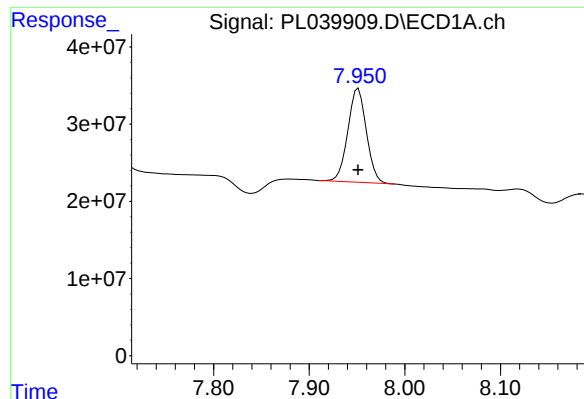

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 164175528
Conc: 19.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

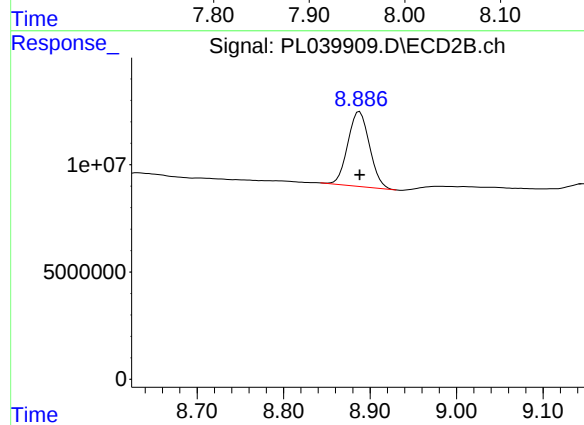

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 60222340
Conc: 22.17 ng/ml