

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 01:20
 Operator : AJ\SJ
 Sample : J4906-09
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:19:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	169.2E6	72280363	21.816	22.653
28)	SA Decachlor...	7.951	8.889	154.3E6	58254824	18.514	21.448
Target Compounds							
10)	B gamma-Chl...	5.180	0.000	13297007	0	1.202	N.D. #
11)	B alpha-Chl...	5.180f	0.000	13297007	0	1.245	N.D. #
15)	B Endosulfa...	0.000	6.791	0	936730	N.D.	0.284 #
25)	Chlordane-3	5.180	0.000	13297007	0	10.836	N.D. #
26)	Chlordane-4	5.180	0.000	13297007	0	12.130	N.D. #
27)	Chlordane-5	0.000	6.791	0	936730	N.D.	8.072 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 01:20
Operator : AJ\SJ
Sample : J4906-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:19:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

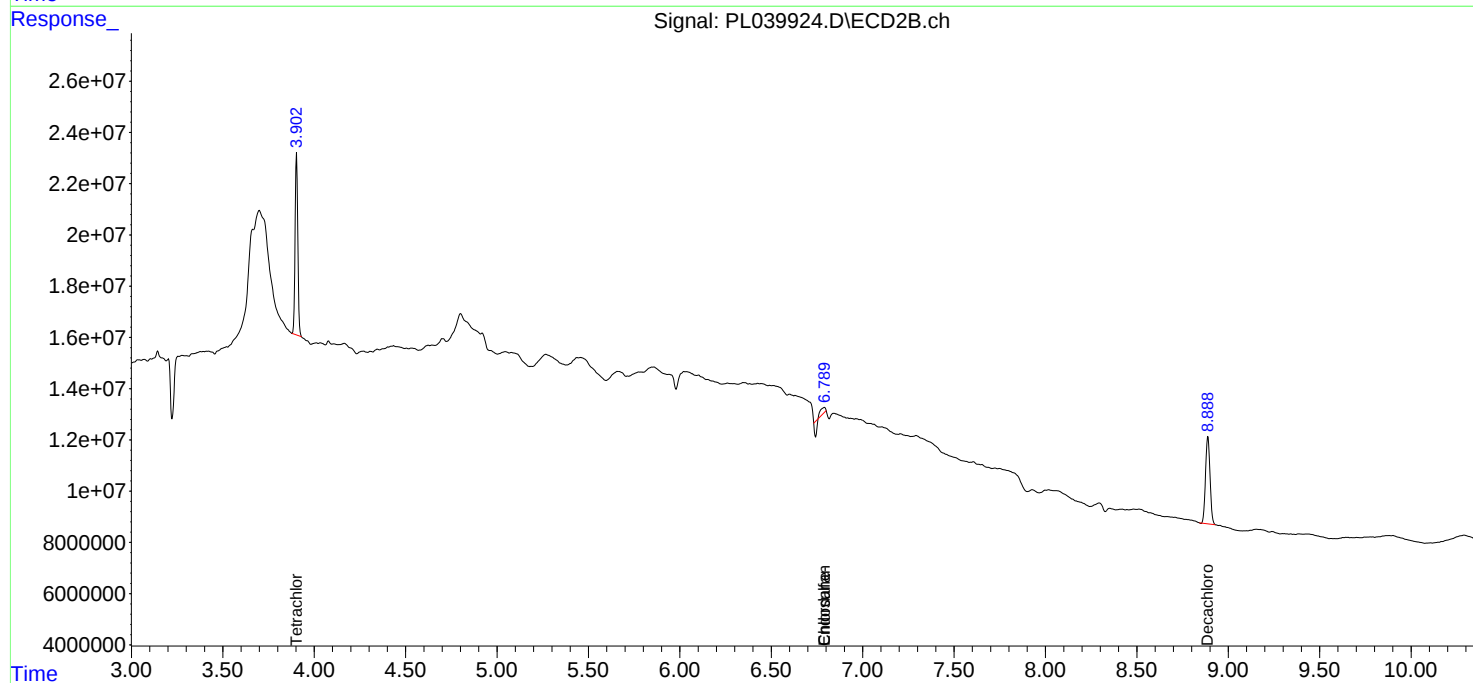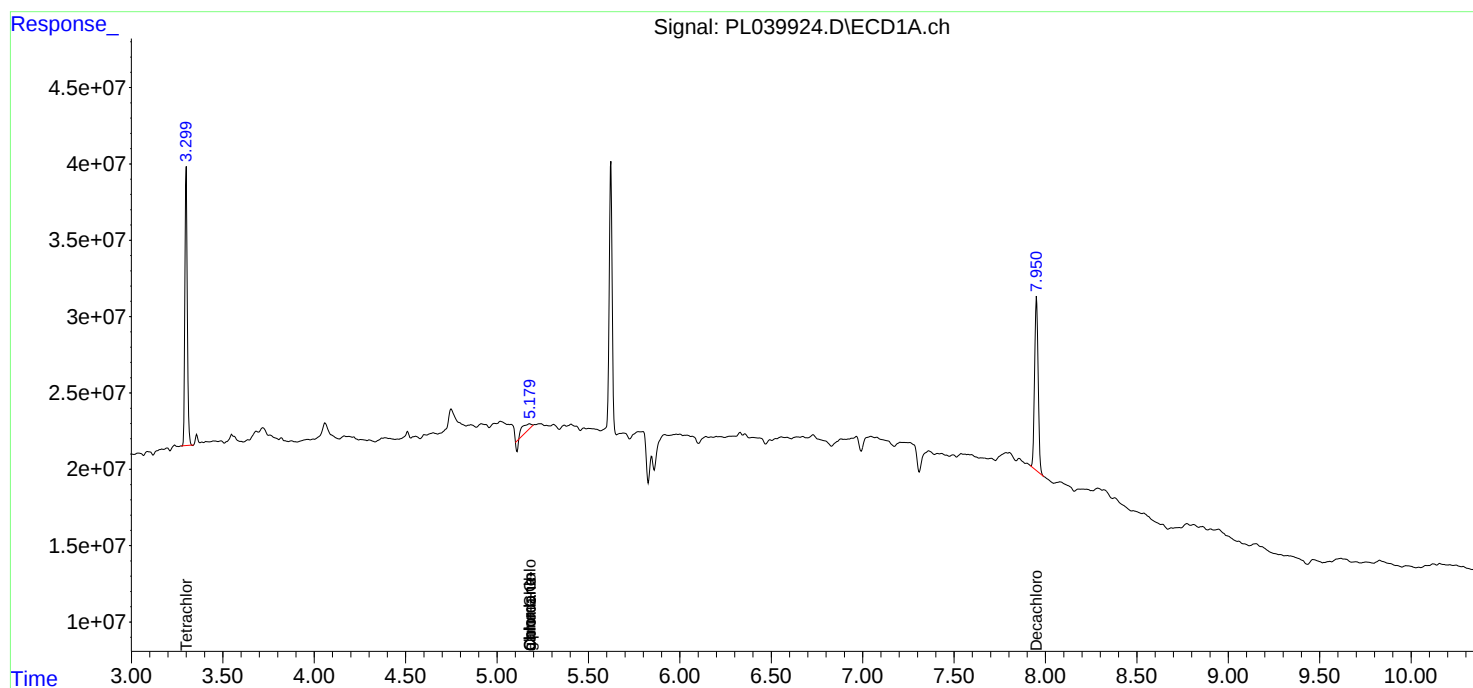


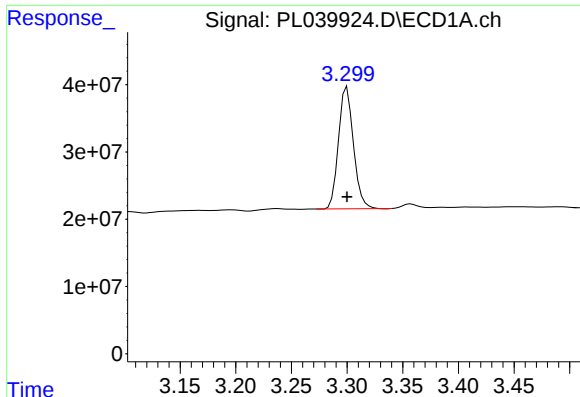

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 169178845
Conc: 21.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

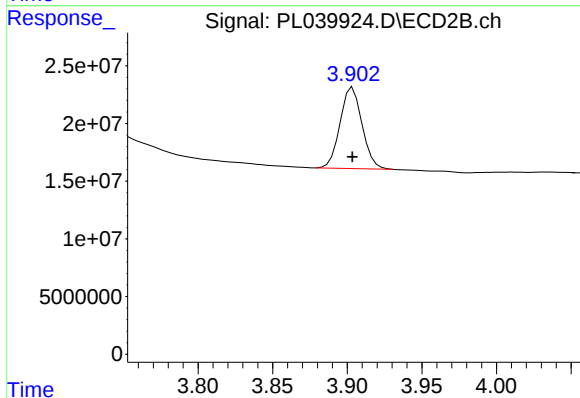


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 72280363
Conc: 22.65 ng/ml

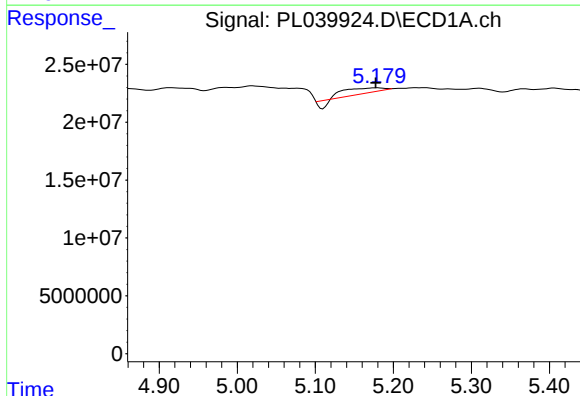


#10 gamma-Chlordane

R.T.: 5.180 min
Delta R.T.: 0.002 min
Response: 13297007
Conc: 1.20 ng/ml

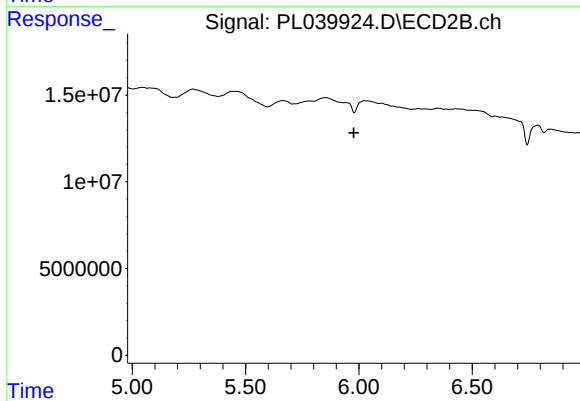

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

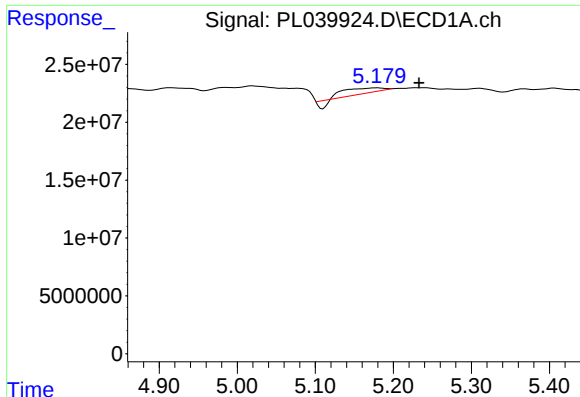

#11 alpha-Chlordane


R.T.: 5.180 min
Delta R.T.: -0.053 min
Response: 13297007
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

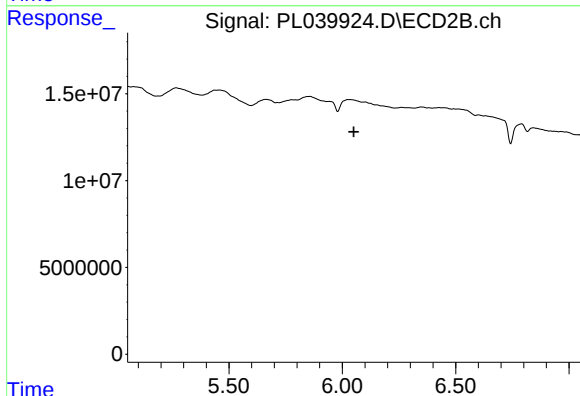


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

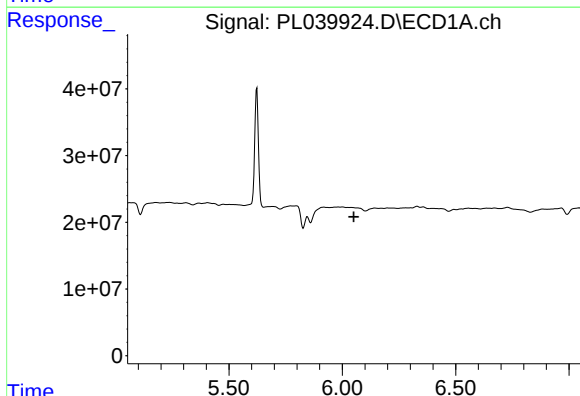


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

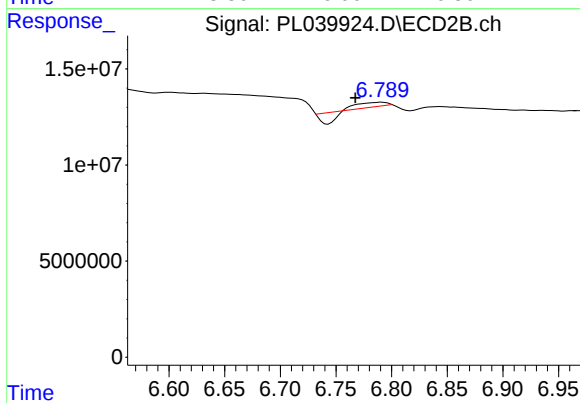

#15 Endosulfan II


R.T.: 6.791 min
Delta R.T.: 0.024 min
Response: 936730
Conc: 0.28 ng/ml

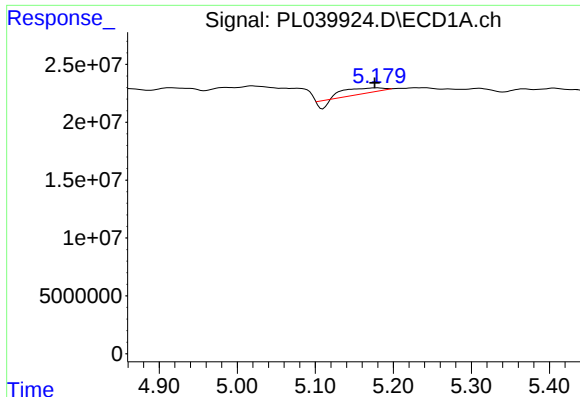

#25 Chlordane-3


R.T.: 5.180 min
Delta R.T.: 0.003 min
Response: 13297007
Conc: 10.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

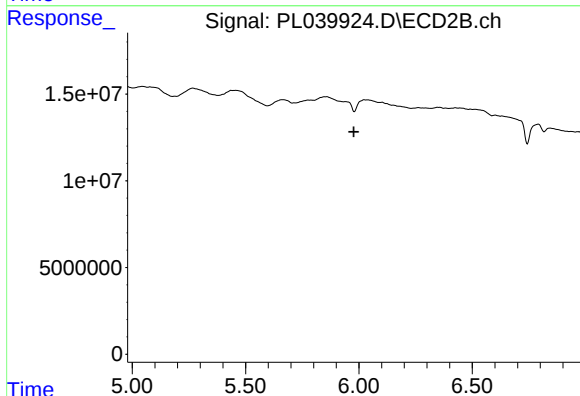


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

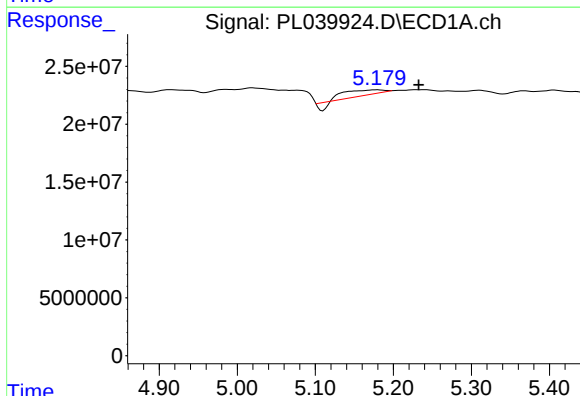


#26 Chlordane-4

R.T.: 5.180 min
Delta R.T.: -0.053 min
Response: 13297007
Conc: 12.13 ng/ml

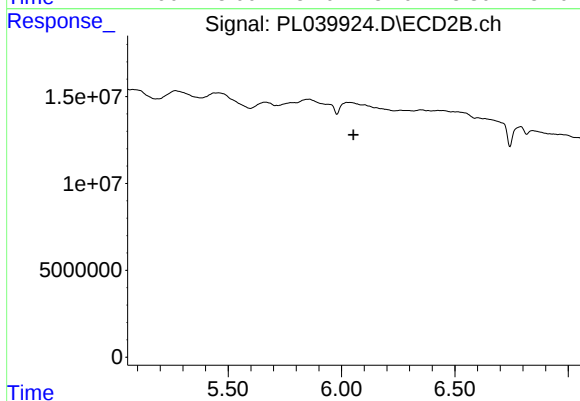

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

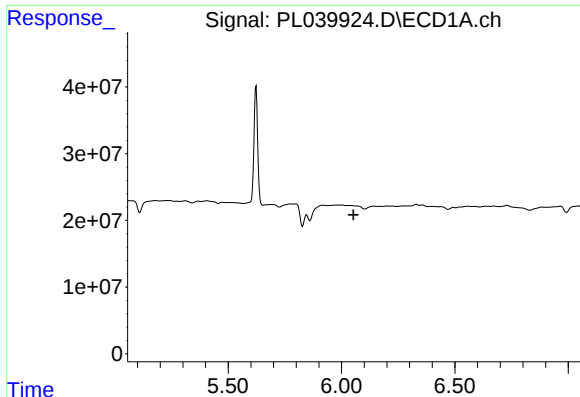

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

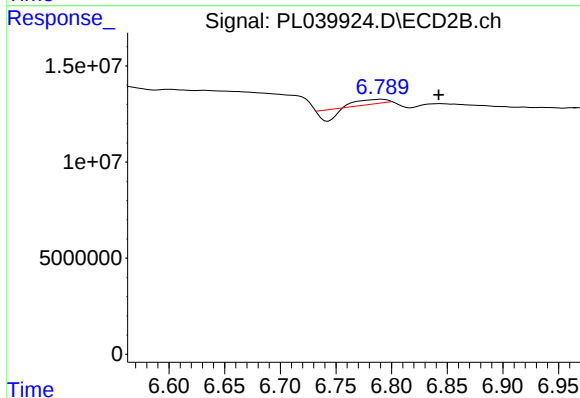


#27 Chlordane-5

R.T.: 6.791 min
Delta R.T.: -0.051 min
Response: 936730
Conc: 8.07 ng/ml

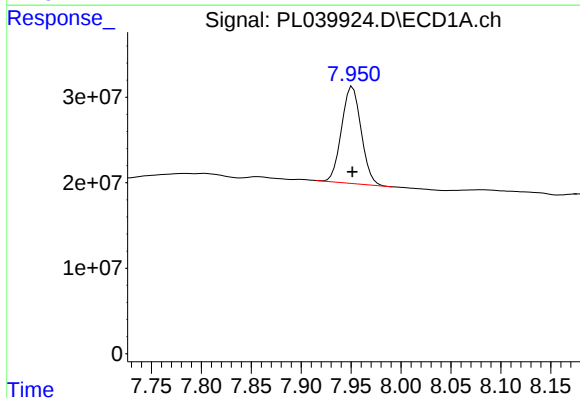

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 154267641
Conc: 18.51 ng/ml

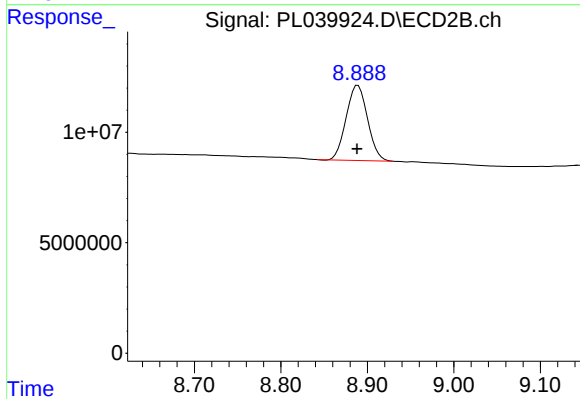

#28 Decachlorobiphenyl

R.T.: 8.889 min
Delta R.T.: 0.000 min
Response: 58254824
Conc: 21.45 ng/ml