

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 01:34
 Operator : AJ\SJ
 Sample : J4906-13
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:20:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	151.0E6	64477241	19.471	20.207
28)	SA Decachlor...	7.951	8.889	129.2E6	47119786	15.511	17.349
Target Compounds							
15)	B Endosulfa...	0.000	6.787	0	2648403	N.D.	0.802 #
27)	Chlordane-5	0.000	6.787	0	2648403	N.D.	22.823 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 01:34
Operator : AJ\SJ
Sample : J4906-13
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:20:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

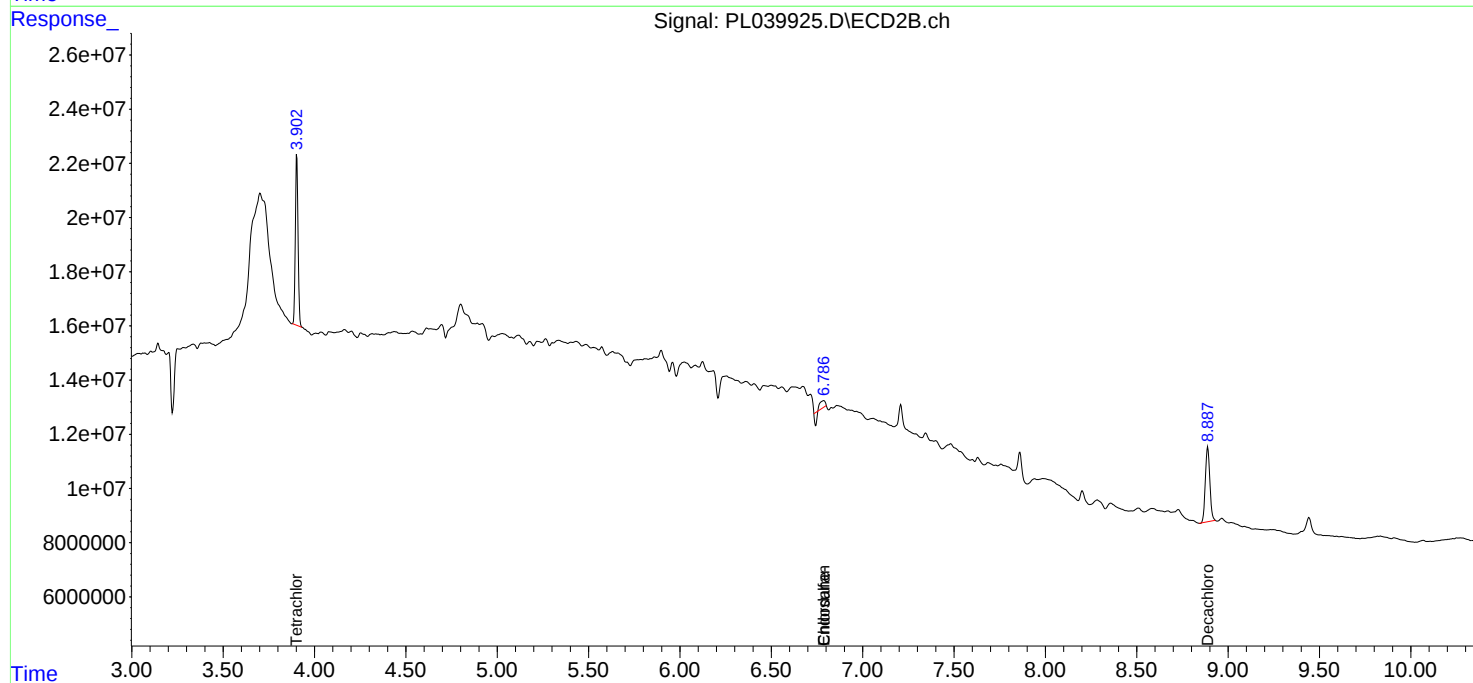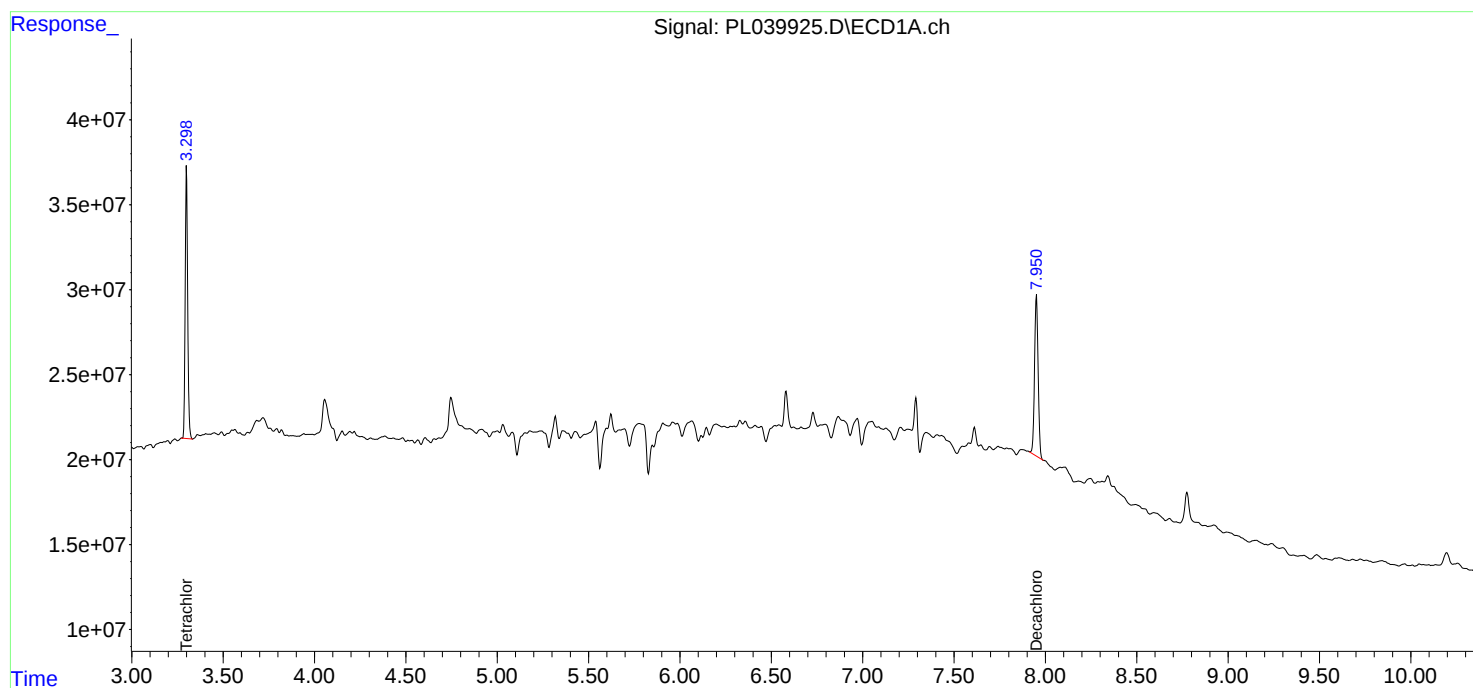


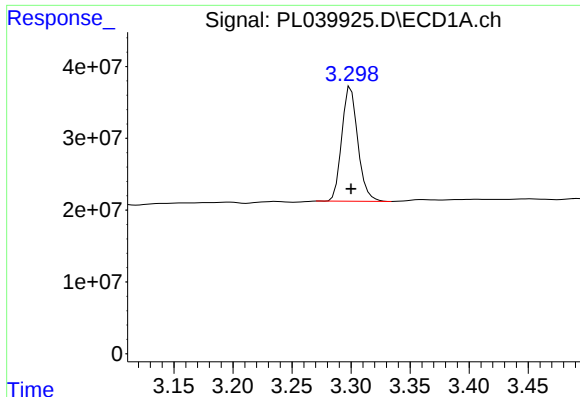

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 150995564
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

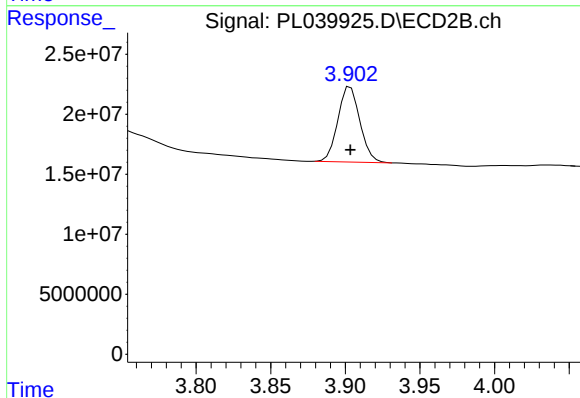


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 64477241
Conc: 20.21 ng/ml

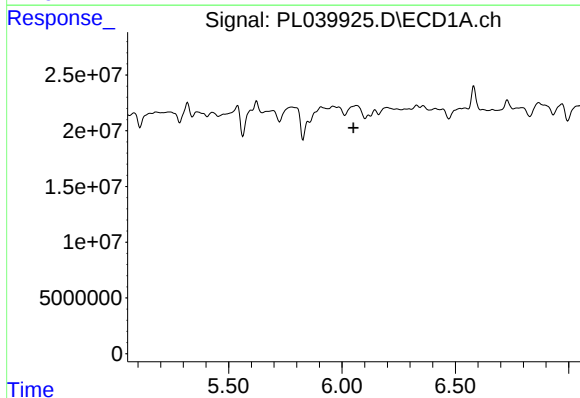


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

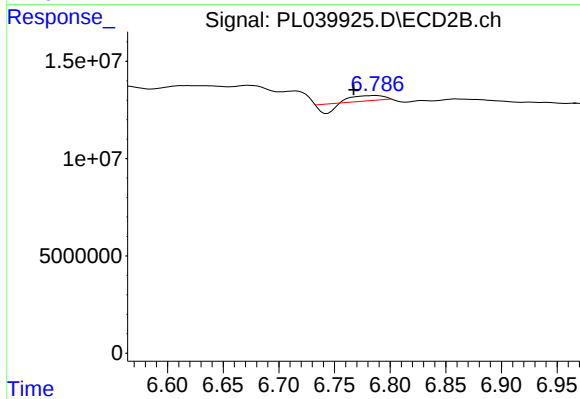

#15 Endosulfan II


R.T.: 6.787 min
Delta R.T.: 0.020 min
Response: 2648403
Conc: 0.80 ng/ml

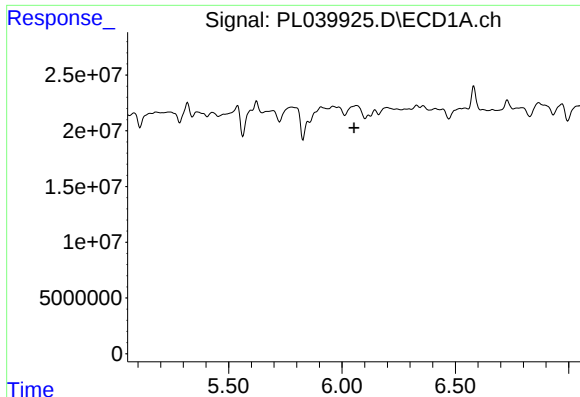

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 6.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

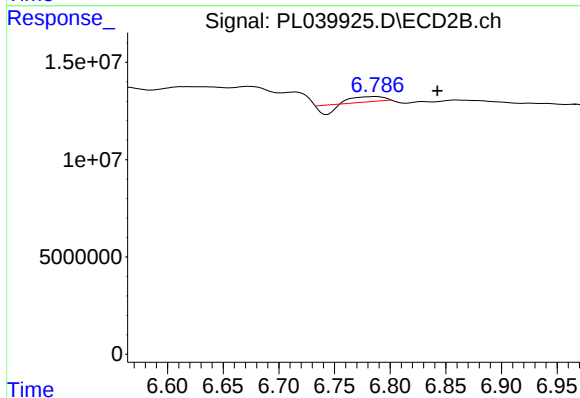


#27 Chlorodane-5

R.T.: 6.787 min
Delta R.T.: -0.055 min
Response: 2648403
Conc: 22.82 ng/ml

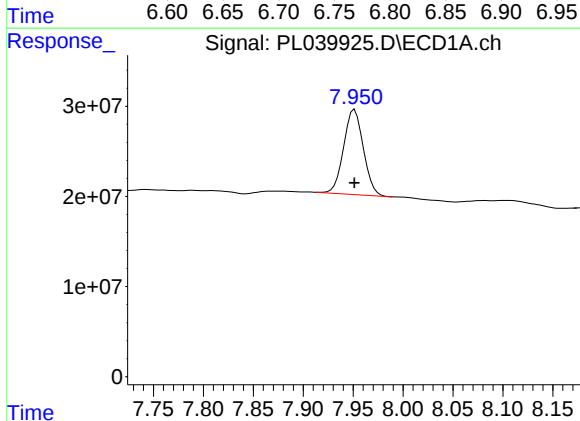

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 129247859
Conc: 15.51 ng/ml

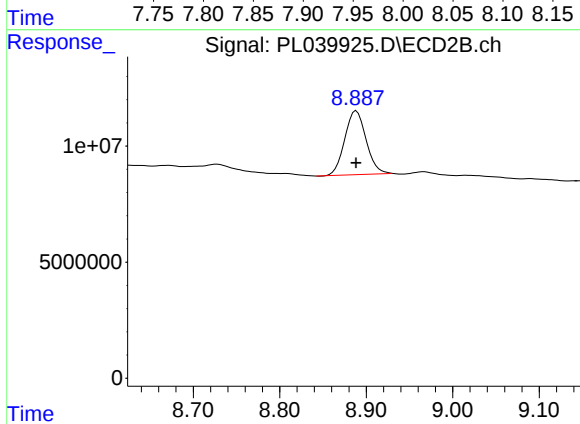

#28 Decachlorobiphenyl

R.T.: 8.889 min
Delta R.T.: 0.000 min
Response: 47119786
Conc: 17.35 ng/ml