

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 11:54
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 12:38:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 12:37:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	771.7E6	306.5E6	95.247	95.713
28)	SA Decachlor...	7.951	8.887	766.9E6	250.6E6	92.731	93.421
Target Compounds							
23)	Chlordane-1	4.137	4.881	355.9E6	151.9E6	1002.842	957.664
24)	Chlordane-2	4.626	5.341	361.9E6	146.0E6	940.377	947.540
25)	Chlordane-3	5.178	5.978	1172.0E6	509.3E6	897.932	962.939
26)	Chlordane-4	5.233	6.053	1075.0E6	595.9E6	948.852	953.422
27)	Chlordane-5	6.052	6.843	367.5E6	114.9E6	956.110	982.619



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 11:54
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 12:38:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 12:37:34 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

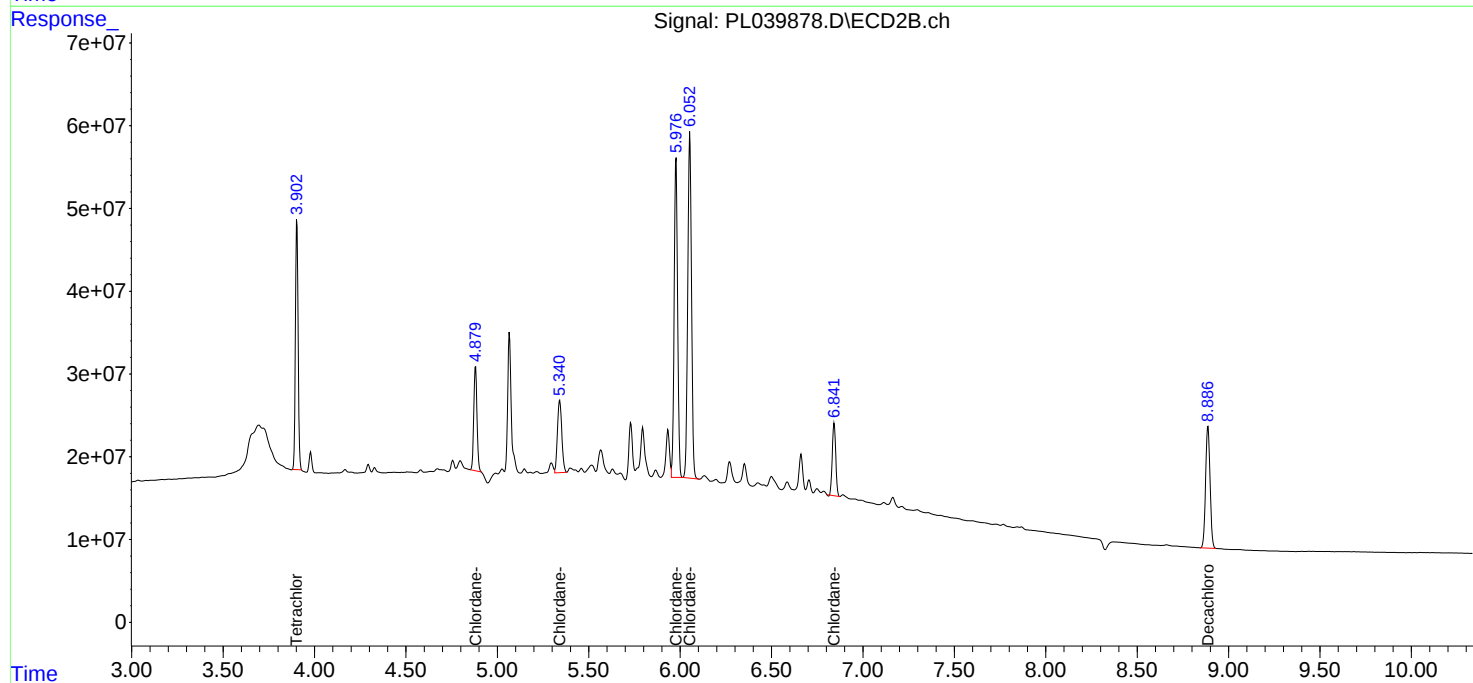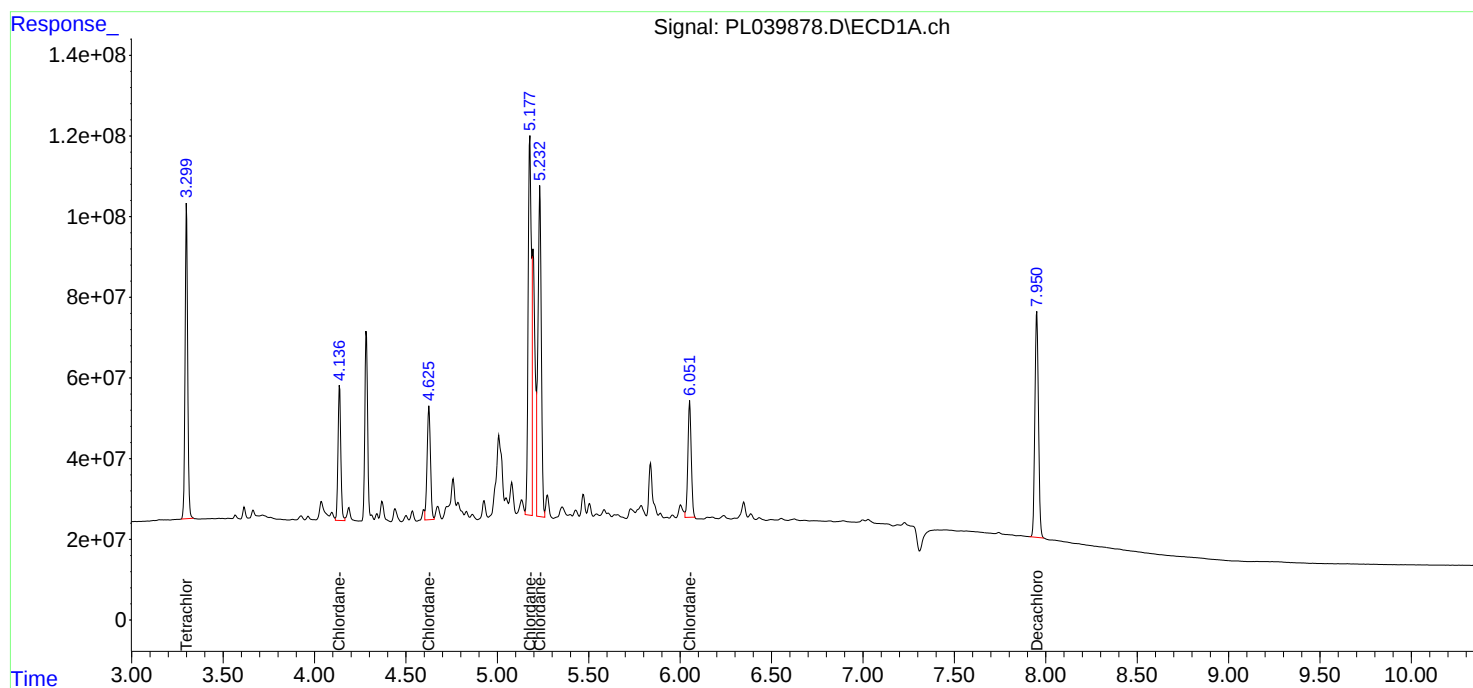


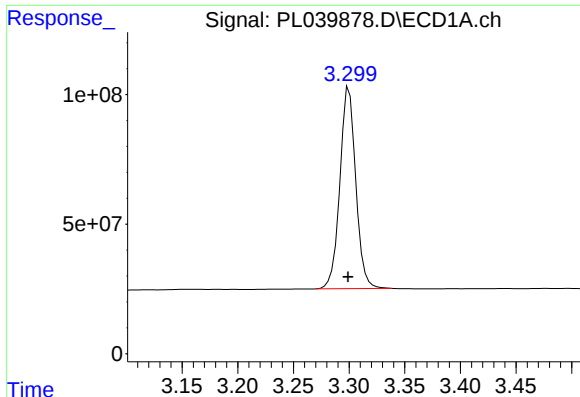

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.001 min
Response: 771675955
Conc: 95.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

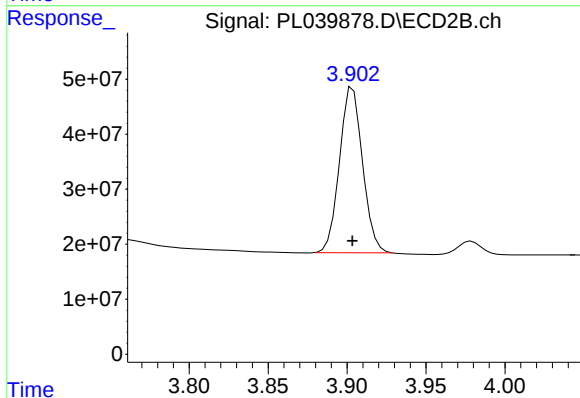


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 306511470
Conc: 95.71 ng/ml

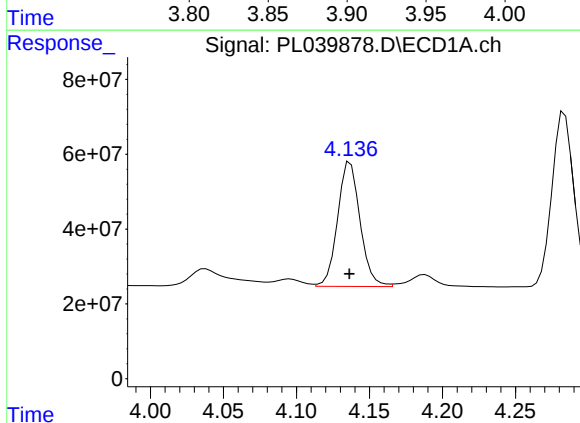


#23 Chlordane-1

R.T.: 4.137 min
Delta R.T.: 0.000 min
Response: 355893431
Conc: 1002.84 ng/ml

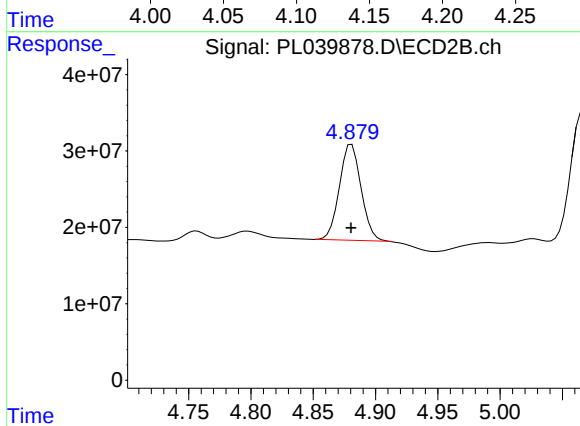

#23 Chlordane-1


R.T.: 4.881 min
Delta R.T.: 0.000 min
Response: 151865592
Conc: 957.66 ng/ml

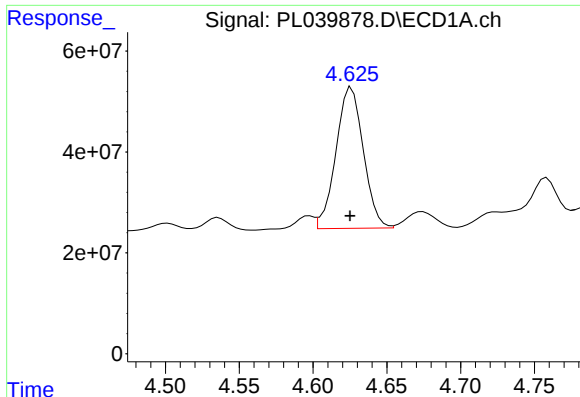

#24 Chlordane-2


R.T.: 4.626 min
Delta R.T.: 0.001 min
Response: 361930453
Conc: 940.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

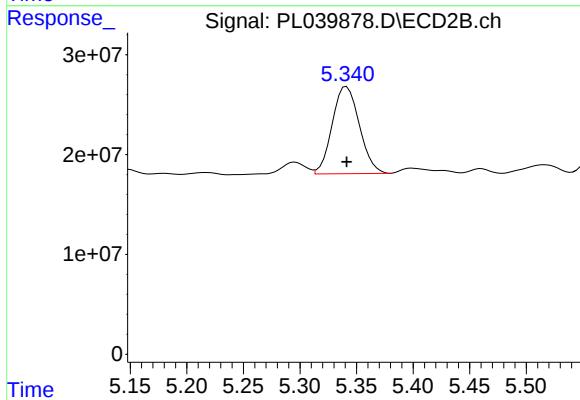


#24 Chlordane-2

R.T.: 5.341 min
Delta R.T.: 0.000 min
Response: 145980895
Conc: 947.54 ng/ml

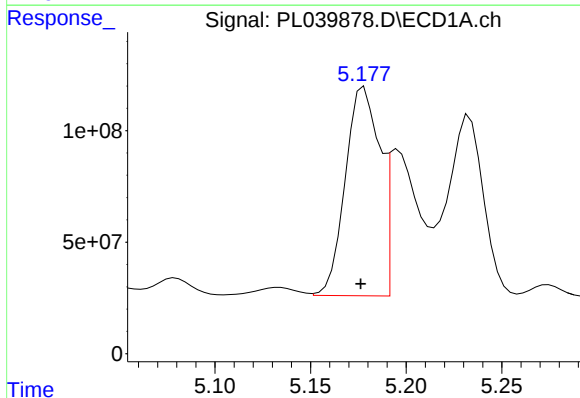


#25 Chlordane-3

R.T.: 5.178 min
Delta R.T.: 0.002 min
Response: 1171959261
Conc: 897.93 ng/ml

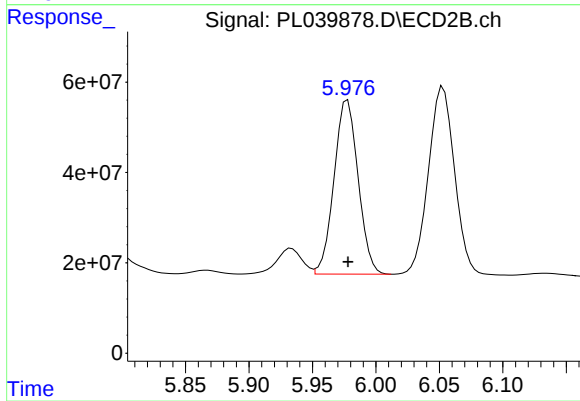

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 509267161
Conc: 962.94 ng/ml

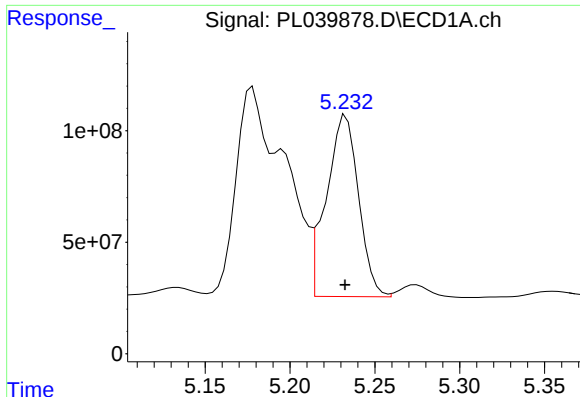

#26 Chlordane-4


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 1075009257
Conc: 948.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

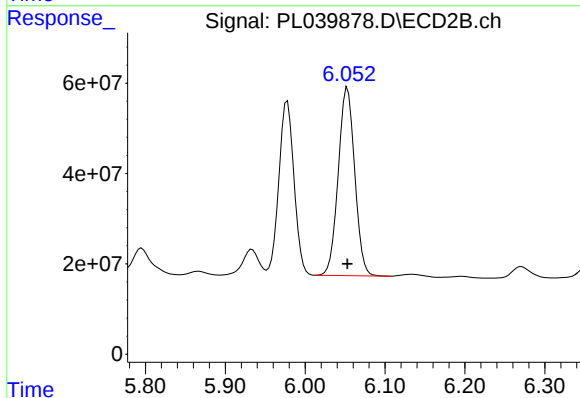


#26 Chlordane-4

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 595912262
Conc: 953.42 ng/ml

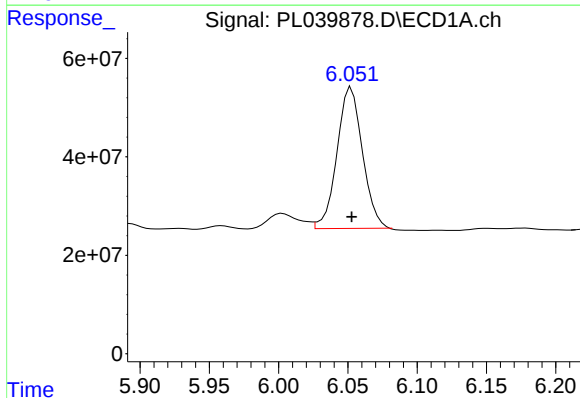


#27 Chlordane-5

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 367472666
Conc: 956.11 ng/ml

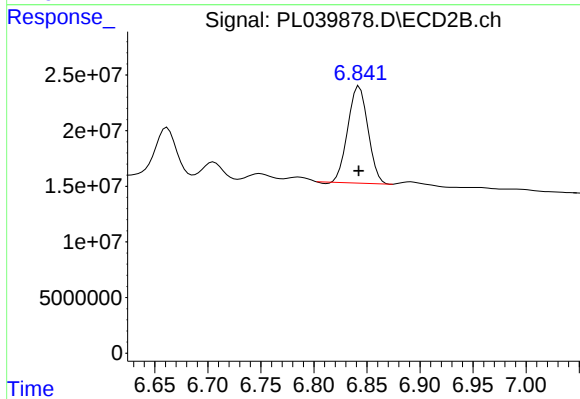

#27 Chlordane-5


R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 114945324
Conc: 982.62 ng/ml

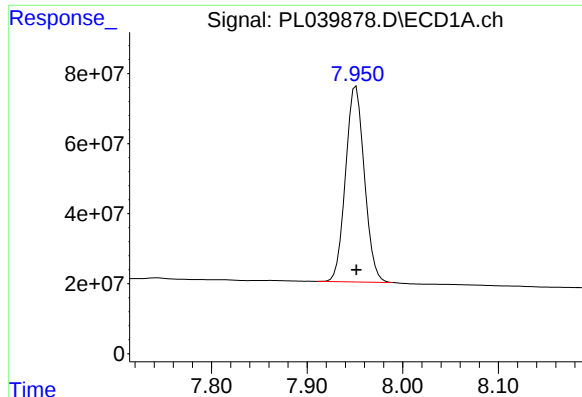

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 766885073
Conc: 92.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

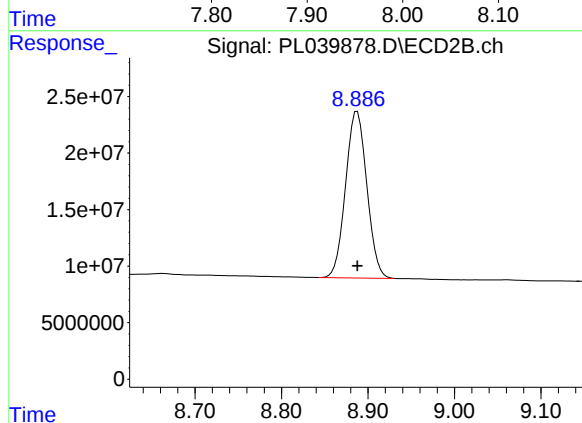

#28 Decachlorobiphenyl

R.T.: 8.887 min
Delta R.T.: 0.000 min
Response: 250594628
Conc: 93.42 ng/ml