

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 12:08
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 12:38:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 12:37:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	592.5E6	236.2E6	73.128	73.751
28)	SA Decachlor...	7.952	8.889	595.0E6	194.1E6	71.949	72.368
Target Compounds							
23)	Chlordane-1	4.136	4.881	274.1E6	116.9E6	772.359	737.166
24)	Chlordane-2	4.625	5.341	280.3E6	112.4E6	728.280	729.853
25)	Chlordane-3	5.178	5.978	923.3E6	390.1E6	707.444	737.702
26)	Chlordane-4	5.232	6.054	825.7E6	458.6E6	728.785	733.676
27)	Chlordane-5	6.053	6.843	281.0E6	87366659	730.998	746.861



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 12:08
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 12:38:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 12:37:34 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

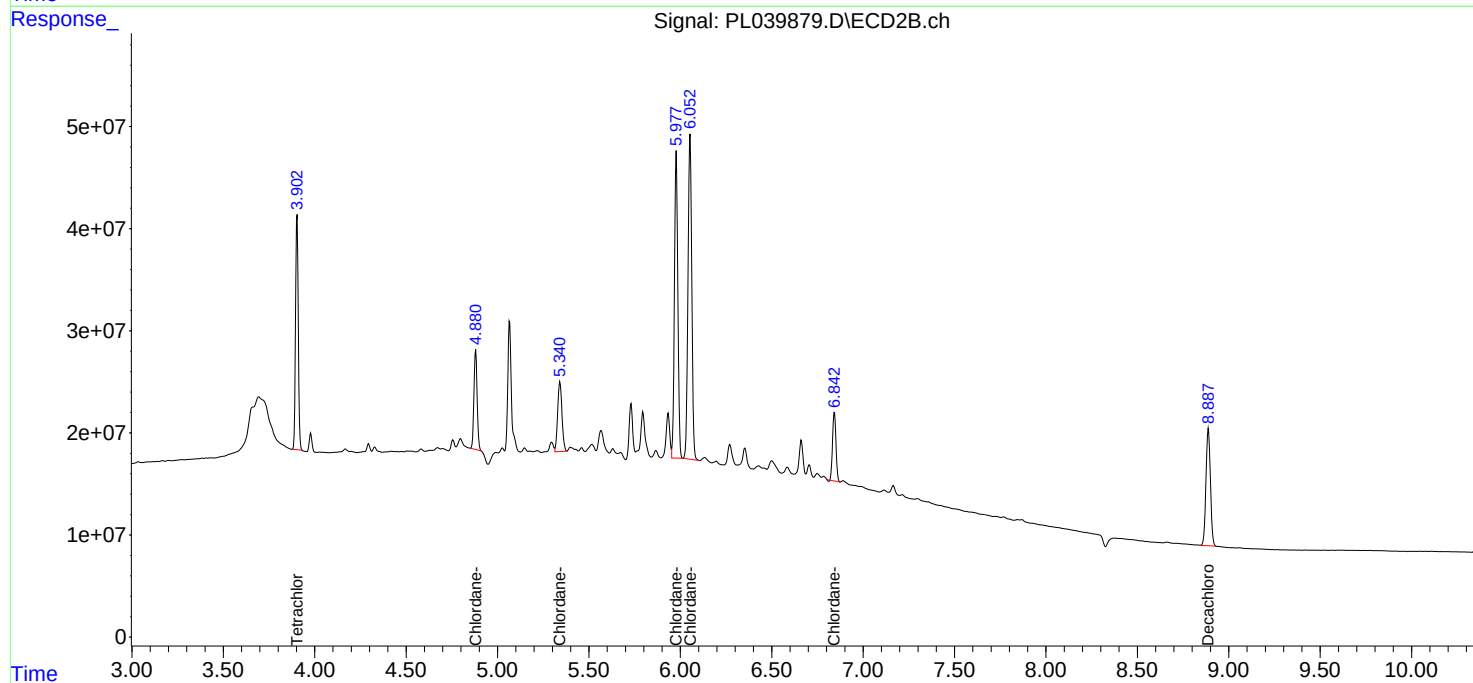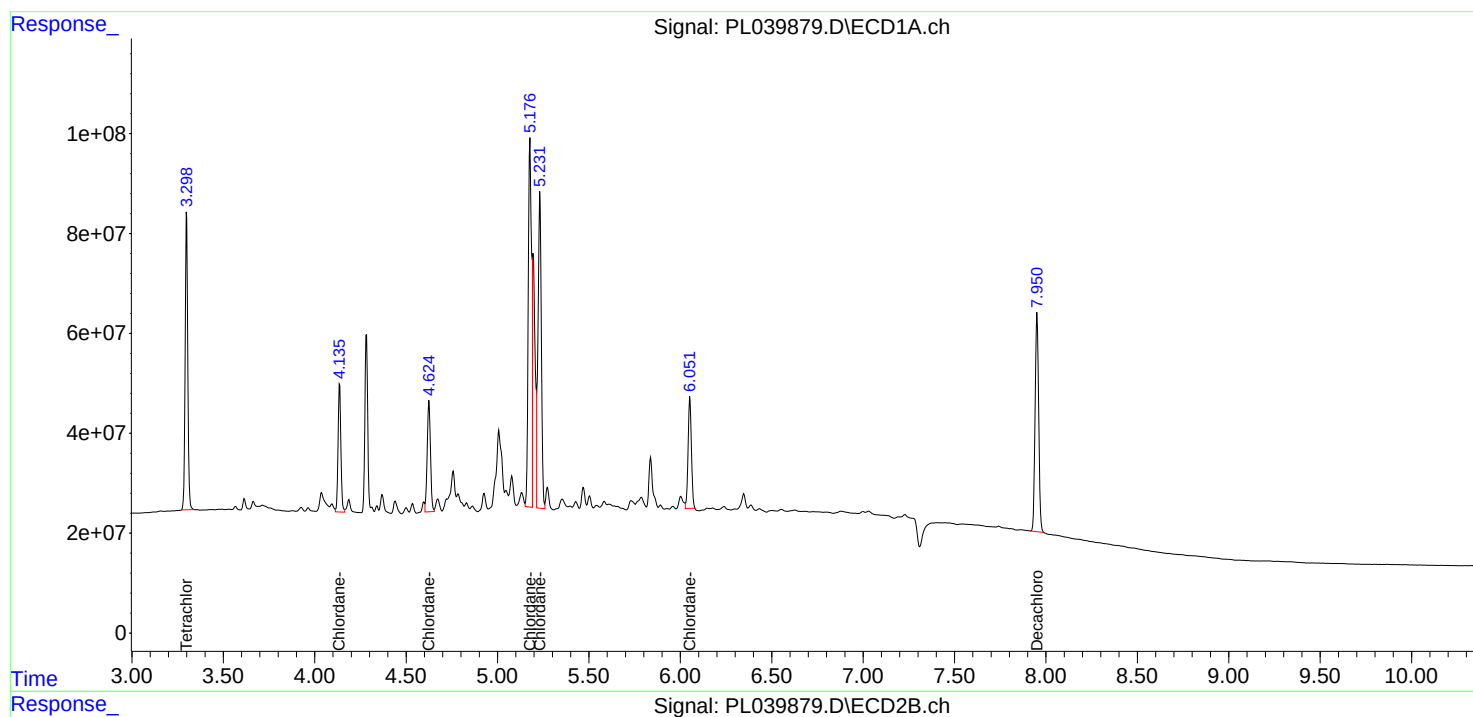


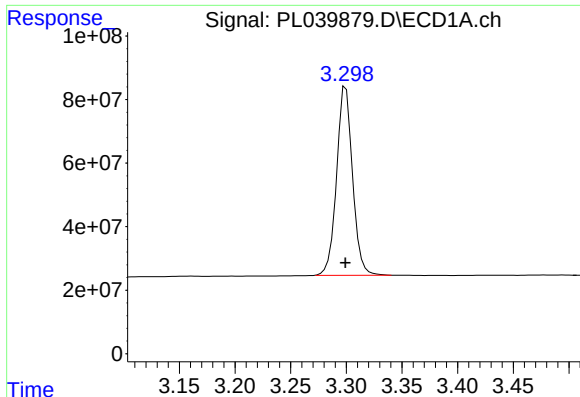

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 592473775
Conc: 73.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

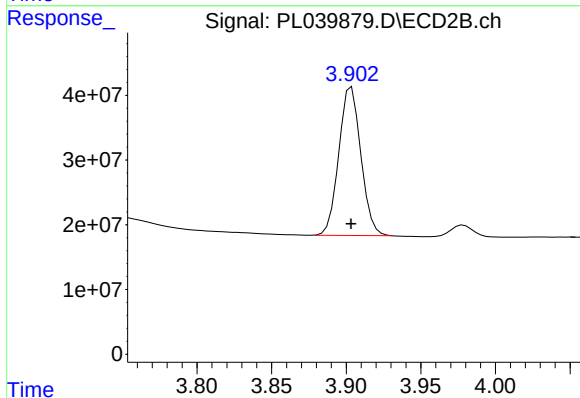


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 236179957
Conc: 73.75 ng/ml

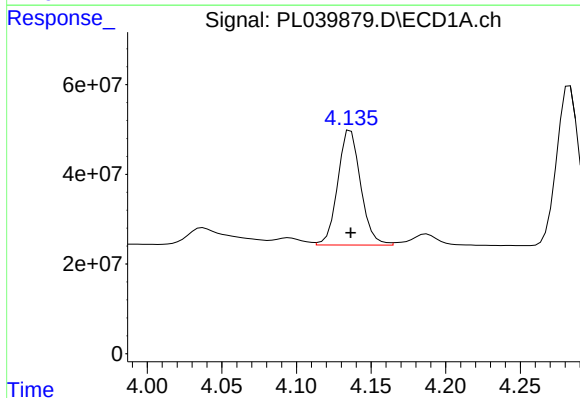


#23 Chlordane-1

R.T.: 4.136 min
Delta R.T.: 0.000 min
Response: 274098649
Conc: 772.36 ng/ml

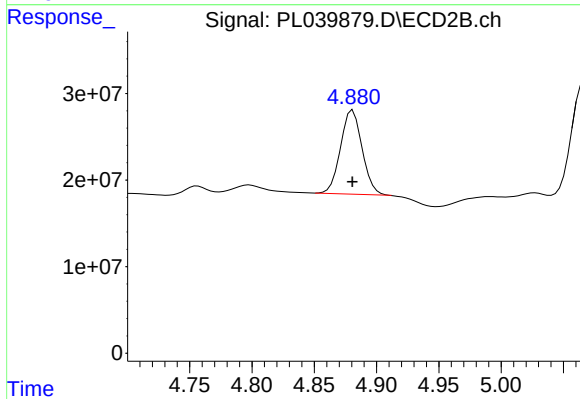

#23 Chlordane-1


R.T.: 4.881 min
Delta R.T.: 0.000 min
Response: 116899103
Conc: 737.17 ng/ml

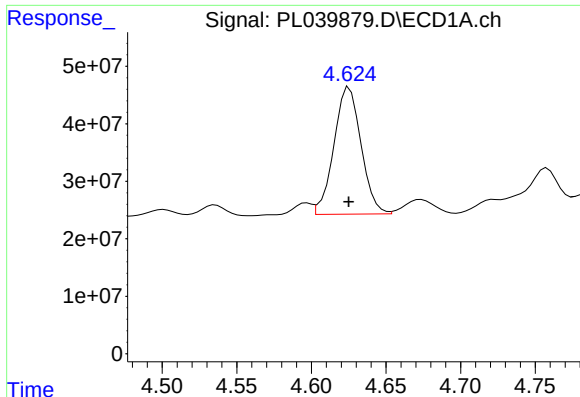

#24 Chlordane-2


R.T.: 4.625 min
Delta R.T.: 0.000 min
Response: 280299055
Conc: 728.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

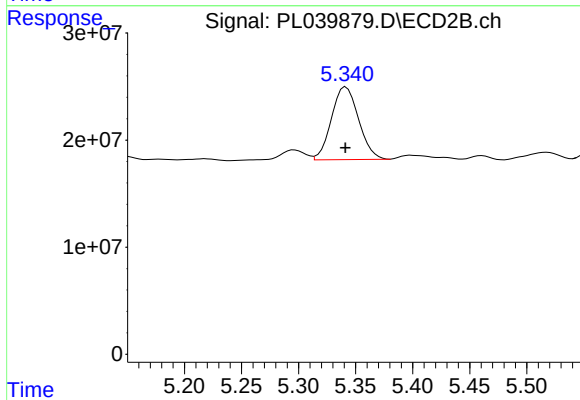


#24 Chlordane-2

R.T.: 5.341 min
Delta R.T.: 0.000 min
Response: 112443373
Conc: 729.85 ng/ml

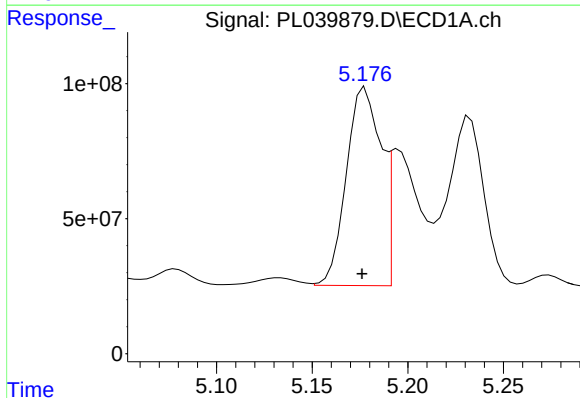


#25 Chlordane-3

R.T.: 5.178 min
Delta R.T.: 0.002 min
Response: 923339641
Conc: 707.44 ng/ml

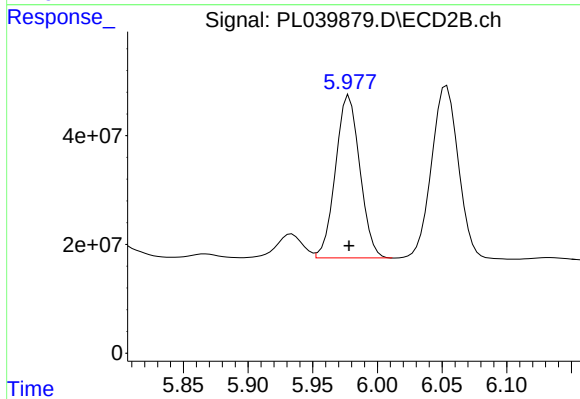

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 390146869
Conc: 737.70 ng/ml

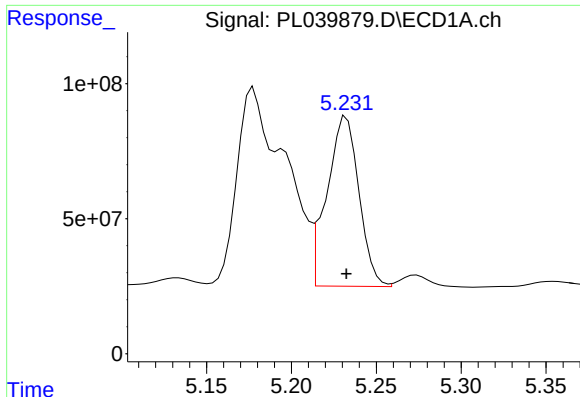

#26 Chlordane-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 825682776
Conc: 728.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

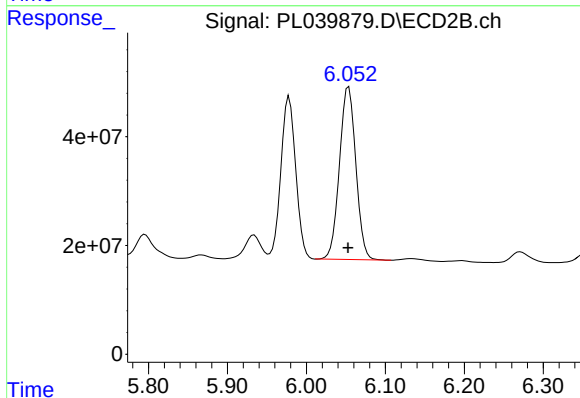


#26 Chlordane-4

R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 458565198
Conc: 733.68 ng/ml

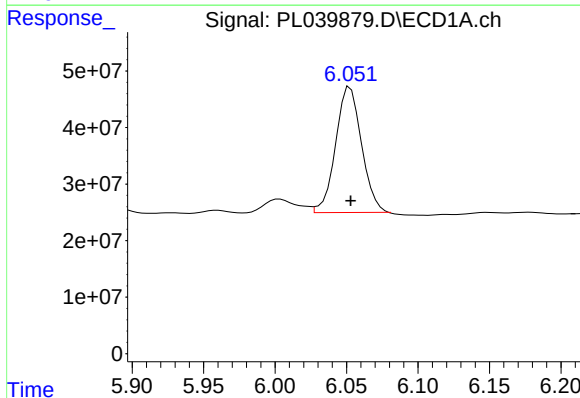


#27 Chlordane-5

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 280952627
Conc: 731.00 ng/ml

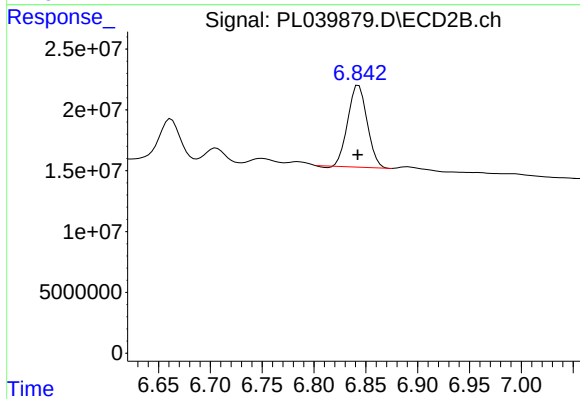

#27 Chlordane-5

R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 87366659
Conc: 746.86 ng/ml

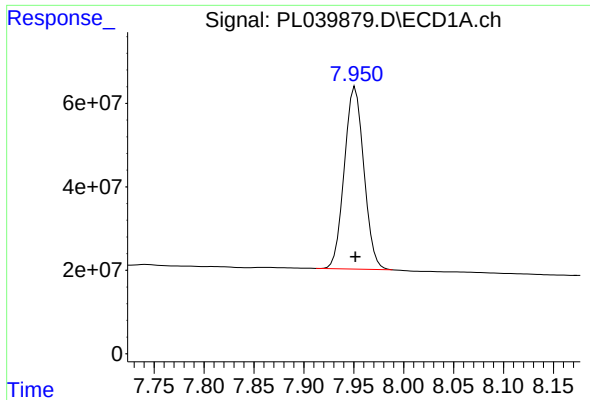

#28 Decachlorobiphenyl


R.T.: 7.952 min

Delta R.T.: 0.000 min

Response: 595017647

Conc: 71.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

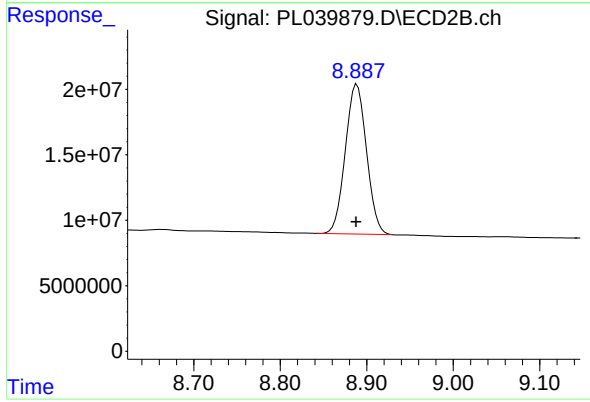

#28 Decachlorobiphenyl

R.T.: 8.889 min

Delta R.T.: 0.000 min

Response: 194121891

Conc: 72.37 ng/ml