

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 12:22
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 12:37:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 12:37:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.299	3.903	405.1E6	160.1E6	50.000	50.000
28)	SA Decachlor...	7.952	8.888	413.5E6	134.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.136	4.880	177.4E6	79289560	500.000	500.000
24)	Chlordane-2	4.625	5.341	192.4E6	77031505	500.000	500.000
25)	Chlordane-3	5.178	5.978	615.6E6	264.4E6	471.670	500.000
26)	Chlordane-4	5.232	6.053	566.5E6	312.5E6	500.000	500.000
27)	Chlordane-5	6.053	6.842	192.2E6	58489239	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 12:22
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 12:37:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 12:37:34 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

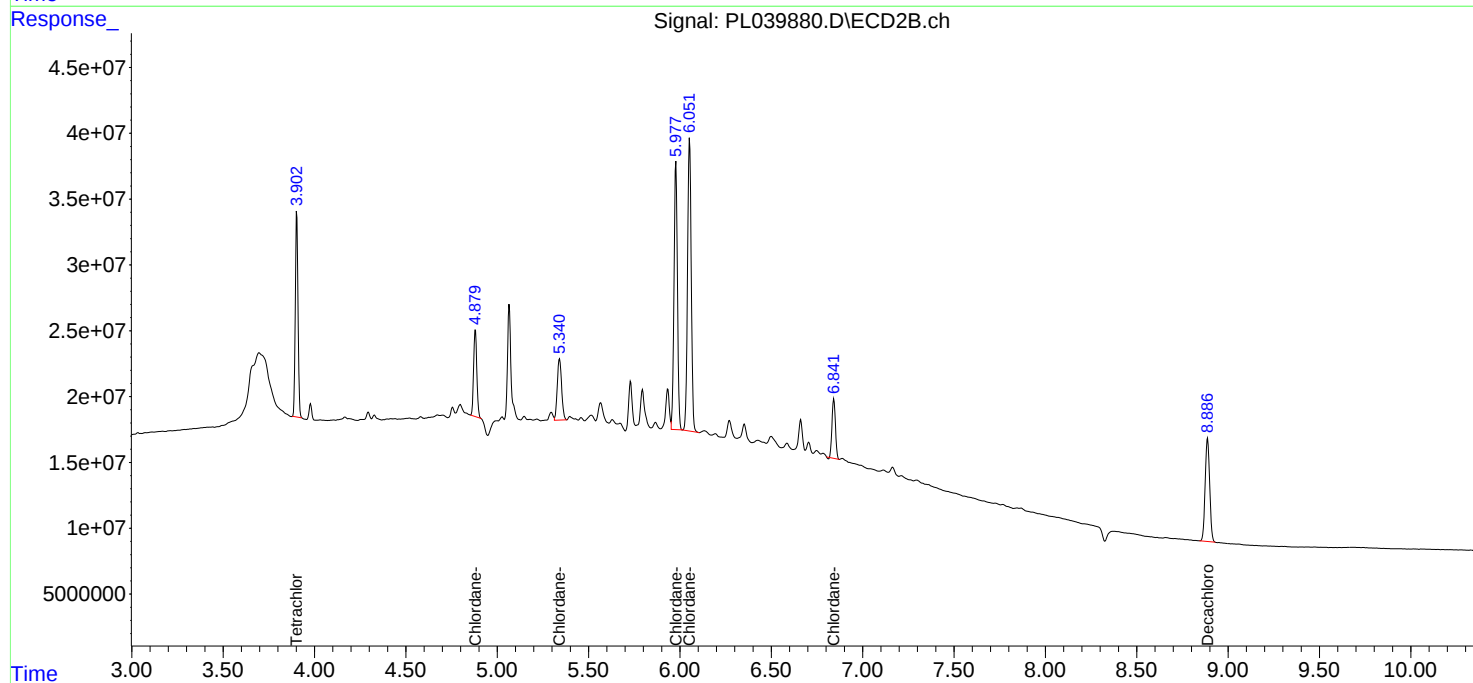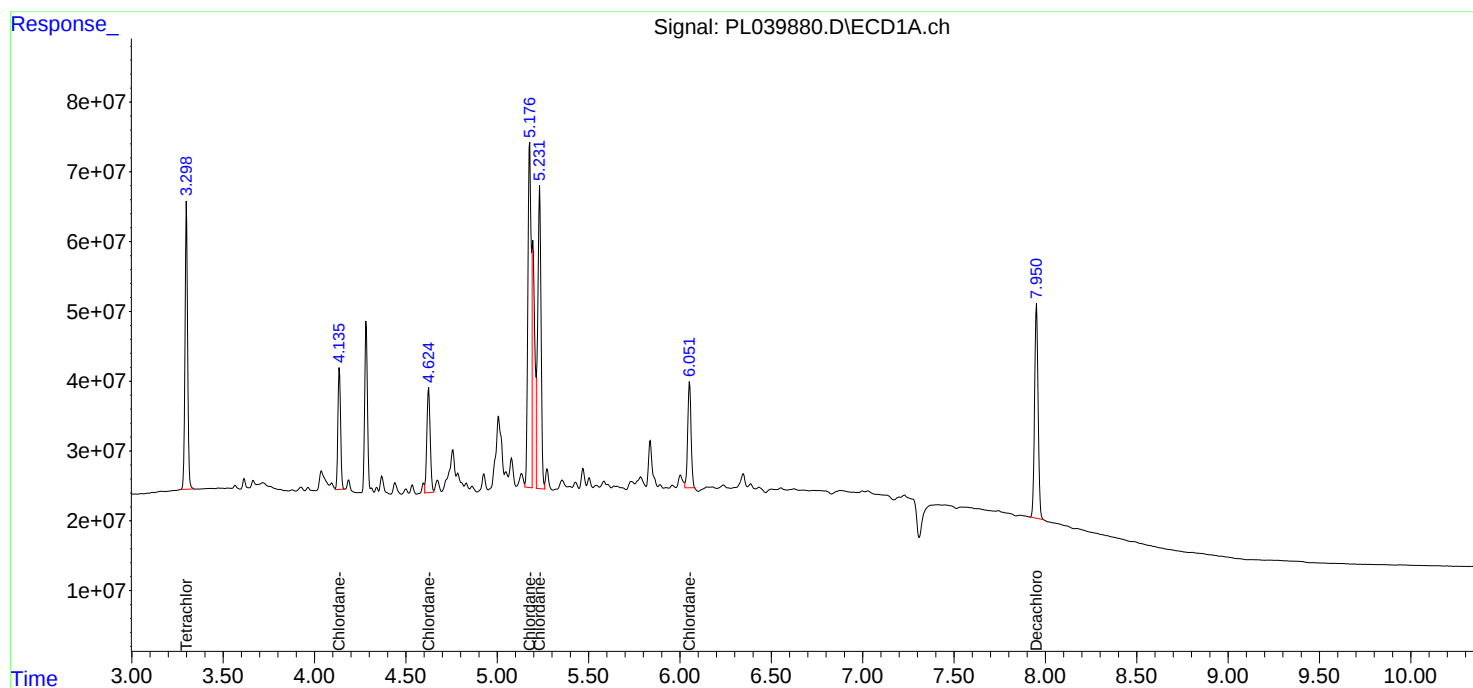


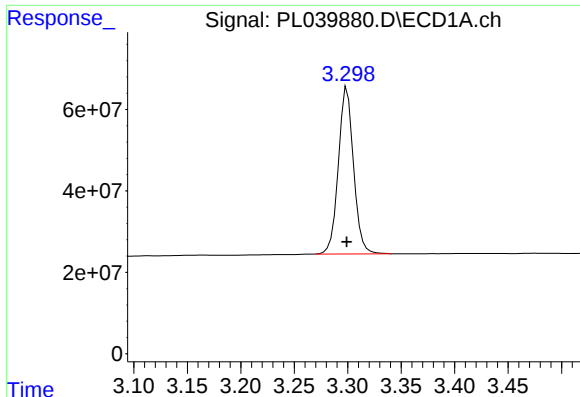

#1 Tetrachloro-m-xylene


R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 405091813
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

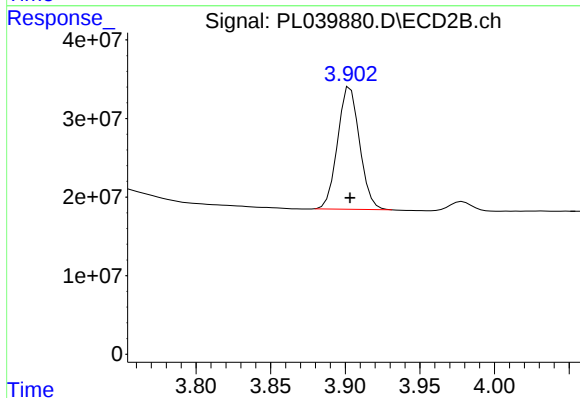


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 160119527
Conc: 50.00 ng/ml

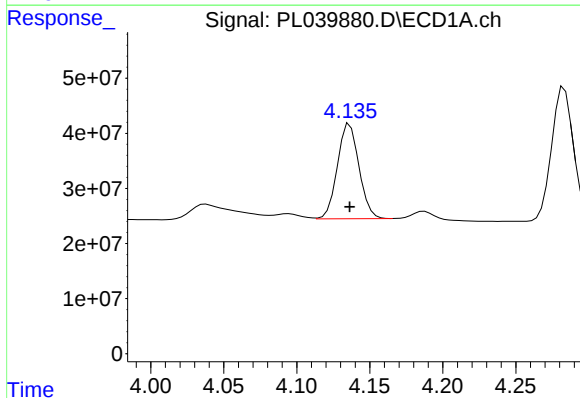


#23 Chlordane-1

R.T.: 4.136 min
Delta R.T.: 0.000 min
Response: 177442427
Conc: 500.00 ng/ml

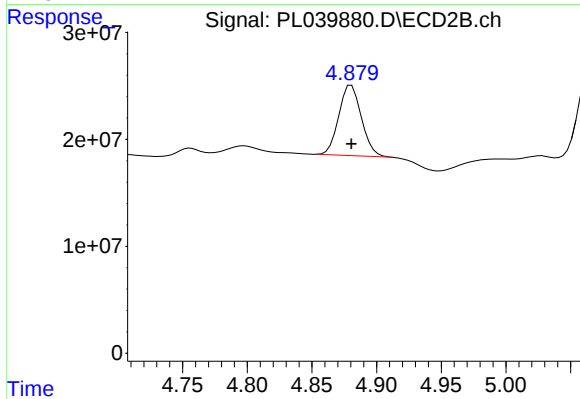

#23 Chlordane-1


R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 79289560
Conc: 500.00 ng/ml

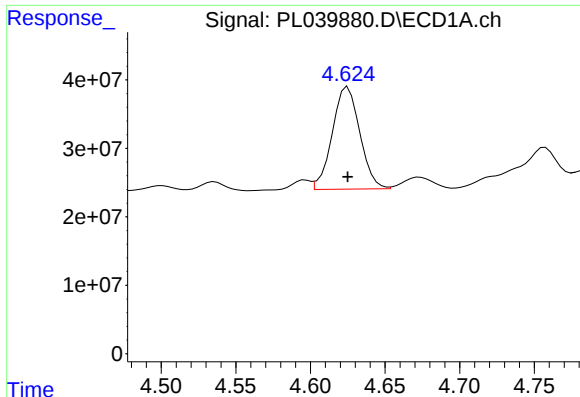

#24 Chlordane-2


R.T.: 4.625 min
Delta R.T.: 0.000 min
Response: 192439057
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

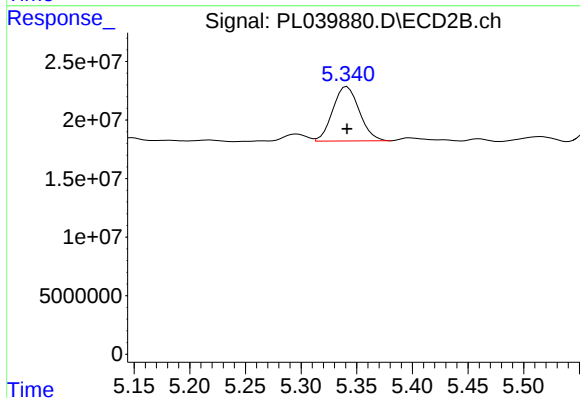


#24 Chlordane-2

R.T.: 5.341 min
Delta R.T.: 0.000 min
Response: 77031505
Conc: 500.00 ng/ml

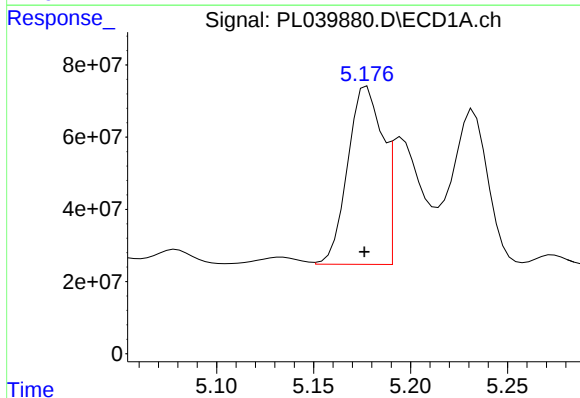


#25 Chlordane-3

R.T.: 5.178 min
Delta R.T.: 0.002 min
Response: 615612874
Conc: 471.67 ng/ml

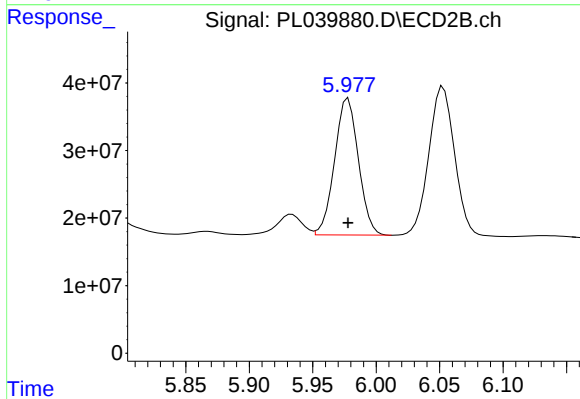

#25 Chlordane-3


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 264433810
Conc: 500.00 ng/ml

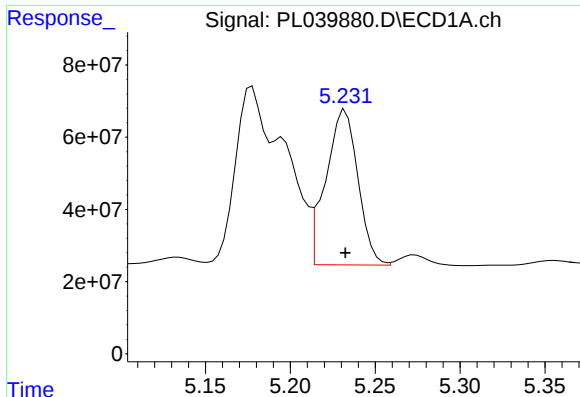

#26 Chlordane-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 566478649
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

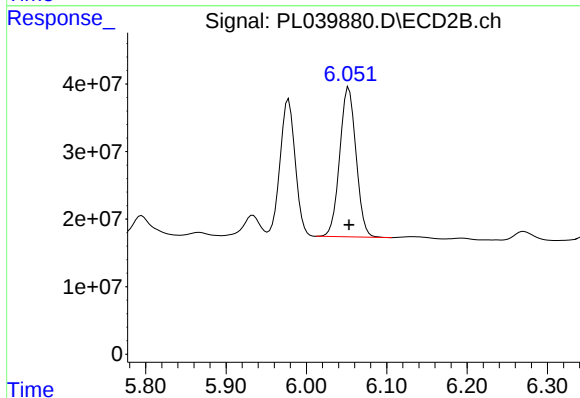


#26 Chlordane-4

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 312512189
Conc: 500.00 ng/ml

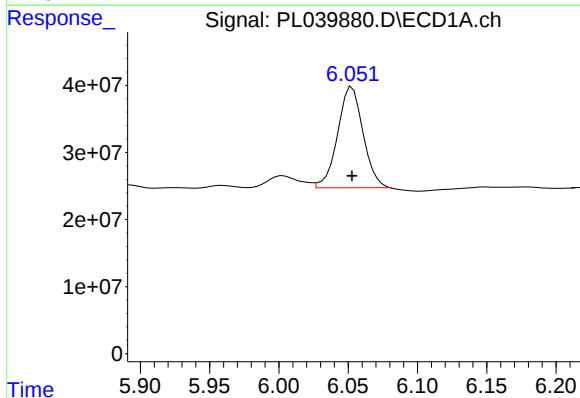


#27 Chlordane-5

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 192170683
Conc: 500.00 ng/ml

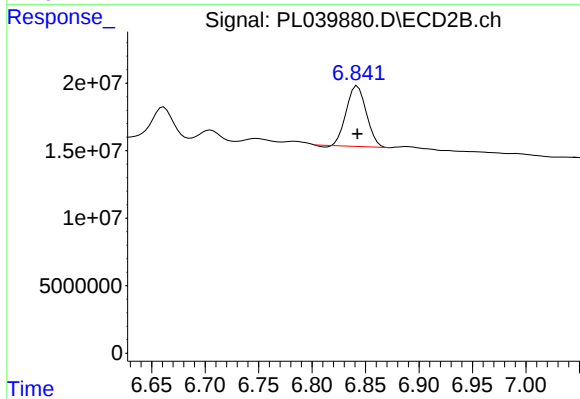

#27 Chlordane-5


R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 58489239
Conc: 500.00 ng/ml

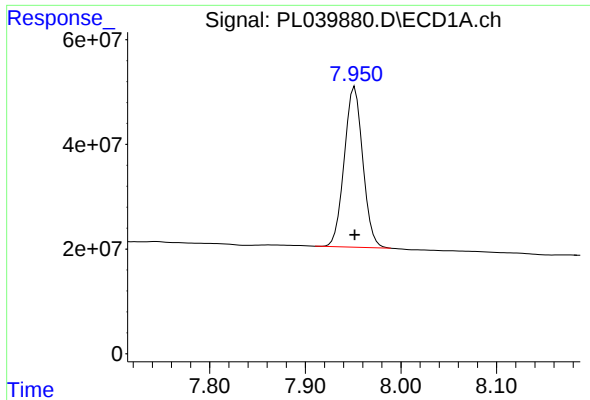

#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 413500859
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

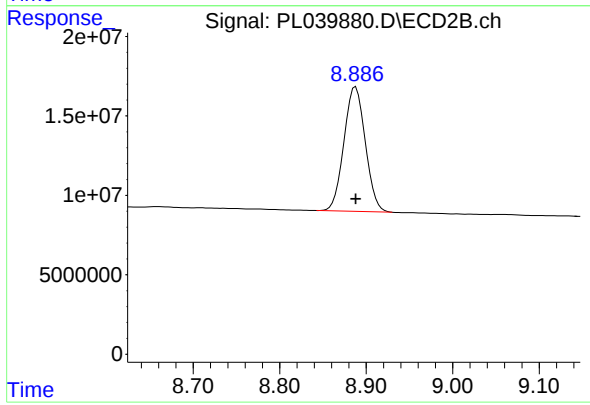

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 134120629
Conc: 50.00 ng/ml