

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 12:37
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Manual Integrations
 APPROVED

Sohil
 9/17/2018 11:10:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 13:30:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 12:40:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.299	3.903	196.9E6	77567265	24.903	24.712
28)	SA Decachlor...	7.951	8.888	206.2E6	68686652	25.913	26.497
Target Compounds							
23)	Chlordane-1	4.135	4.881	86639993	39213945	241.507m	252.282
24)	Chlordane-2	4.626	5.341	98563878	37709780	263.883	251.416
25)	Chlordane-3	5.176	5.978	303.5E6	127.7E6	245.547m	245.749
26)	Chlordane-4	5.232	6.053	266.9E6	154.0E6	241.962	252.185
27)	Chlordane-5	6.052	6.843	100.8E6	28408387	268.428	244.610

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 12:37
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PCHLORICC250


Manual Integrations
APPROVED

Sohil
9/17/2018 11:10:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 13:30:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 12:40:47 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

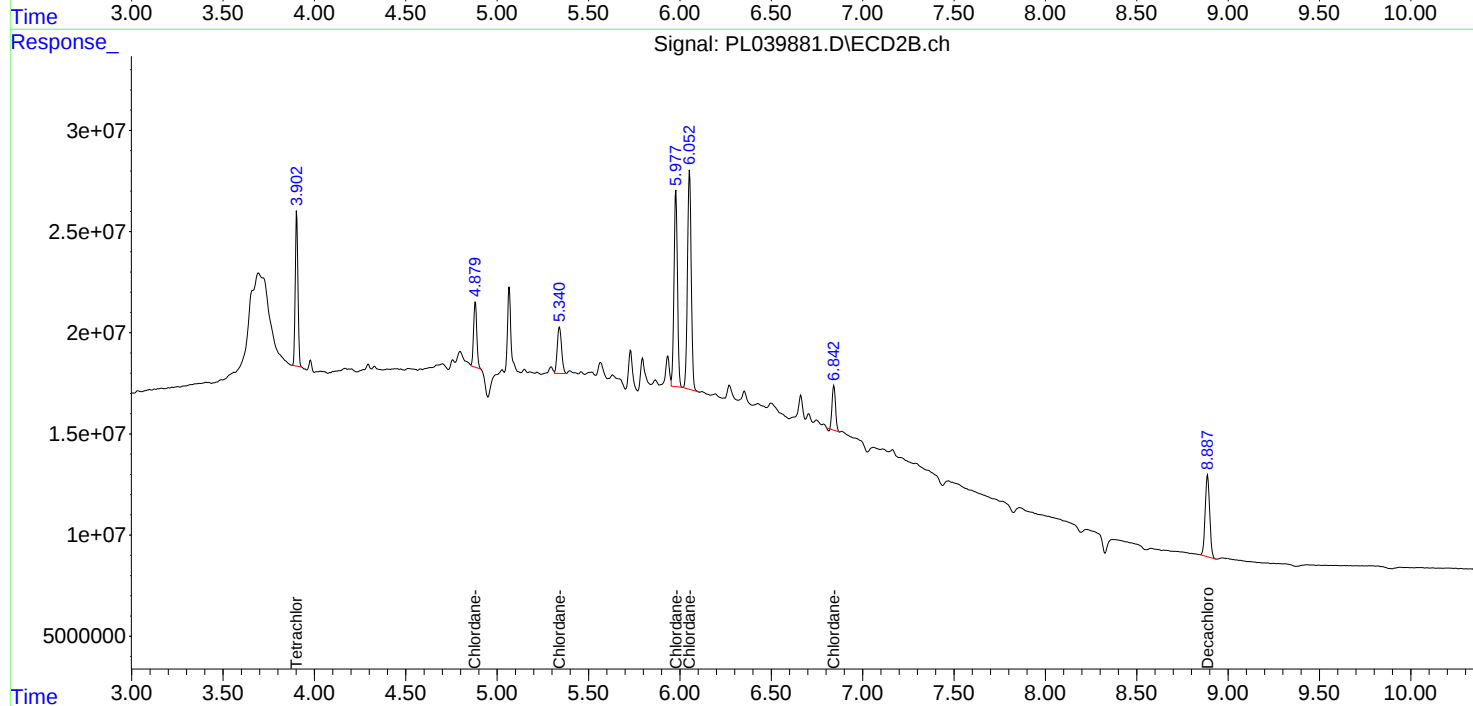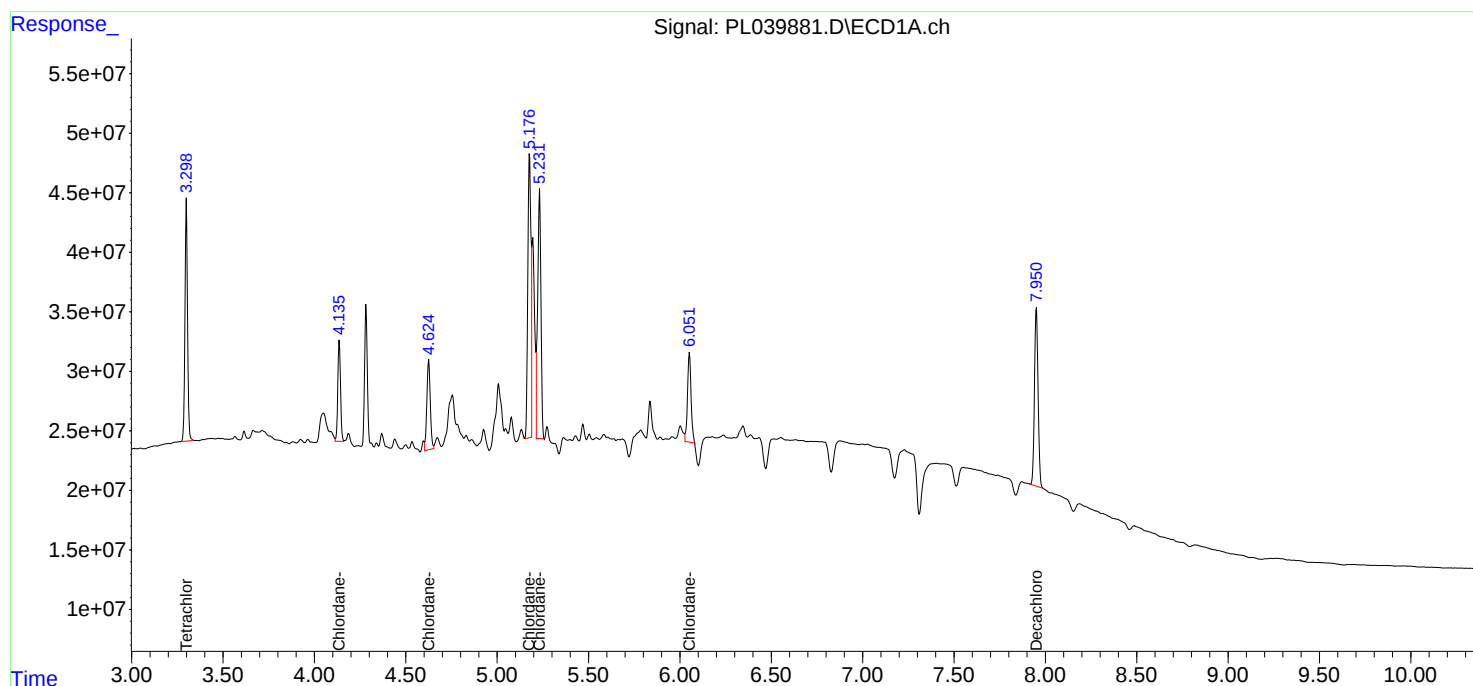

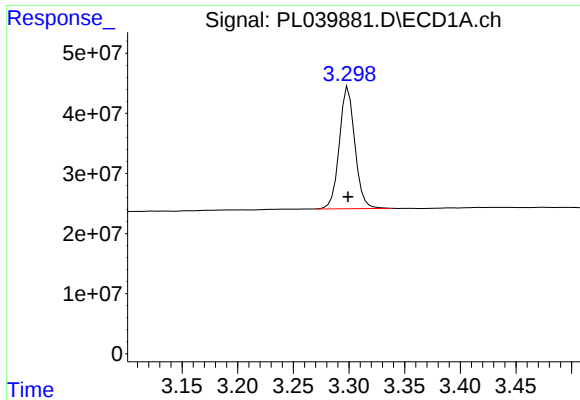


#1 Tetrachloro-m-xylene

R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 196882425
Conc: 24.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250


Manual Integrations
APPROVED

Sohil
9/17/2018 11:10:58 AM

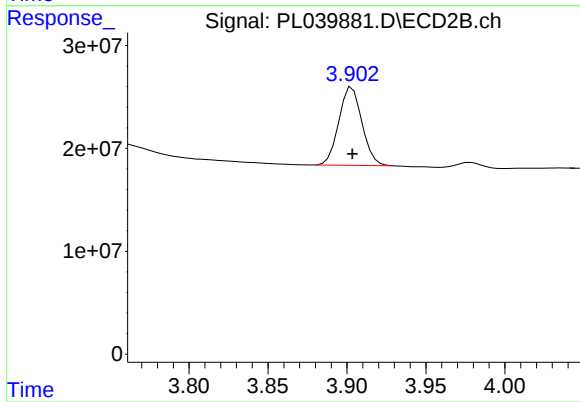


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 77567265
Conc: 24.71 ng/ml

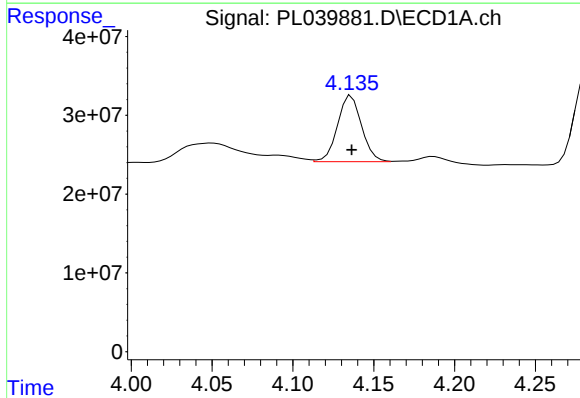


#23 Chlordane-1

R.T.: 4.135 min
Delta R.T.: -0.002 min
Response: 86639993
Conc: 241.51 ng/ml m

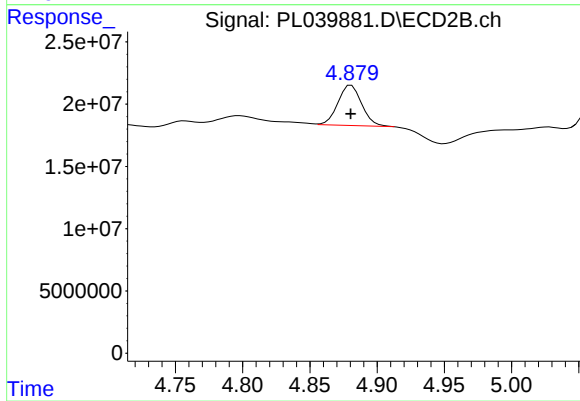

#23 Chlordane-1

R.T.: 4.881 min
Delta R.T.: 0.000 min
Response: 39213945
Conc: 252.28 ng/ml

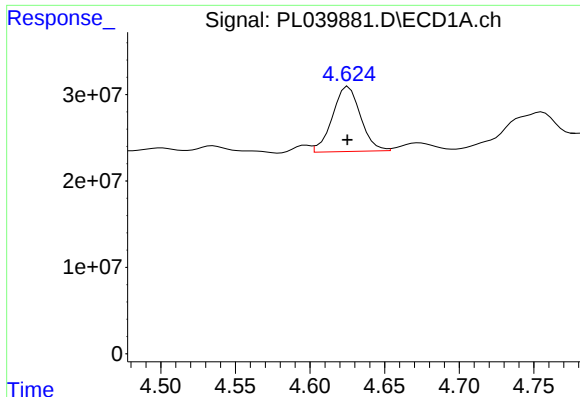


#24 Chlordane-2

R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 98563878
Conc: 263.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250


Manual Integrations
APPROVED

Sohil
9/17/2018 11:10:58 AM

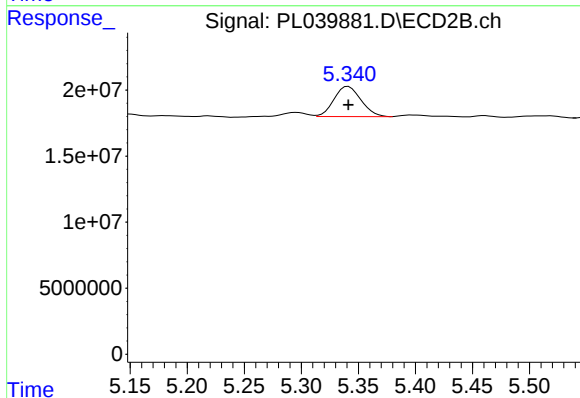


#24 Chlordane-2

R.T.: 5.341 min
Delta R.T.: 0.000 min
Response: 37709780
Conc: 251.42 ng/ml

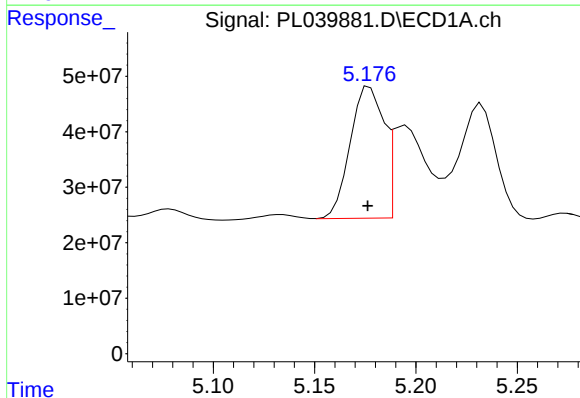


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 303517441
Conc: 245.55 ng/ml m

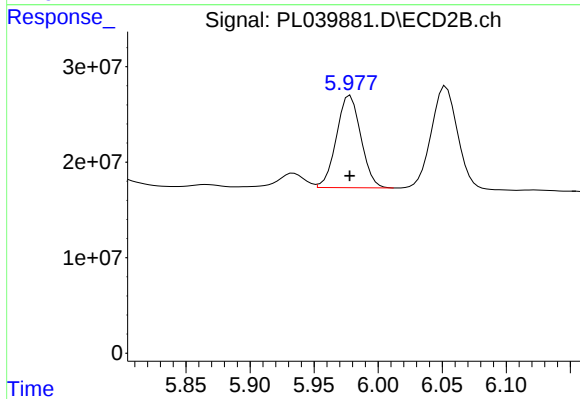

#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 127652629
Conc: 245.75 ng/ml

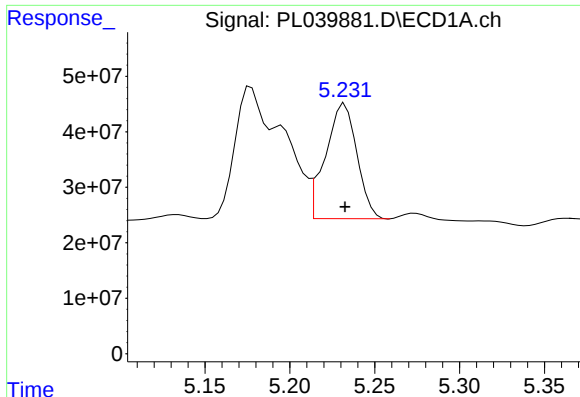


#26 Chlordane-4

R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 266874151
Conc: 241.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250


Manual Integrations
APPROVED

Sohil
9/17/2018 11:10:58 AM

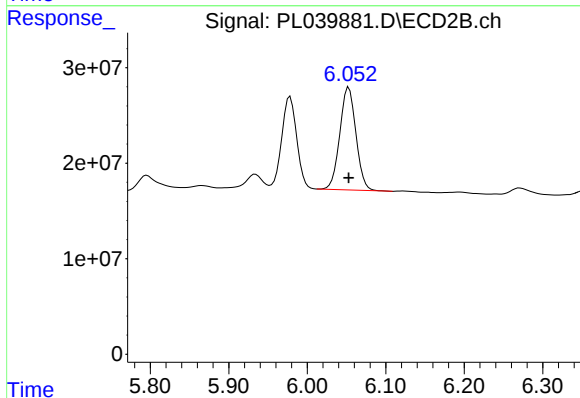


#26 Chlordane-4

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 154030750
Conc: 252.18 ng/ml

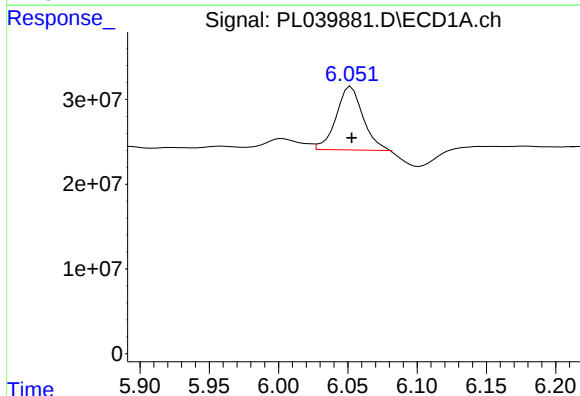


#27 Chlordane-5

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 100787503
Conc: 268.43 ng/ml

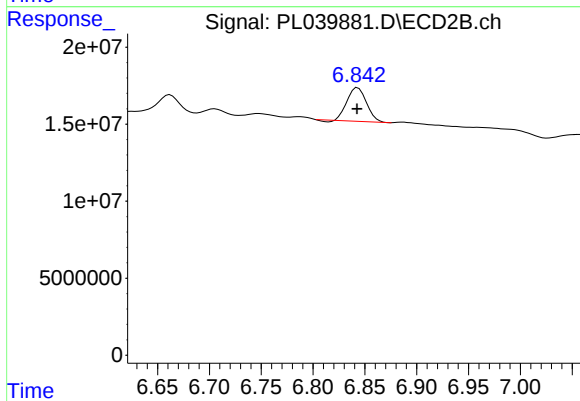

#27 Chlordane-5

R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 28408387
Conc: 244.61 ng/ml

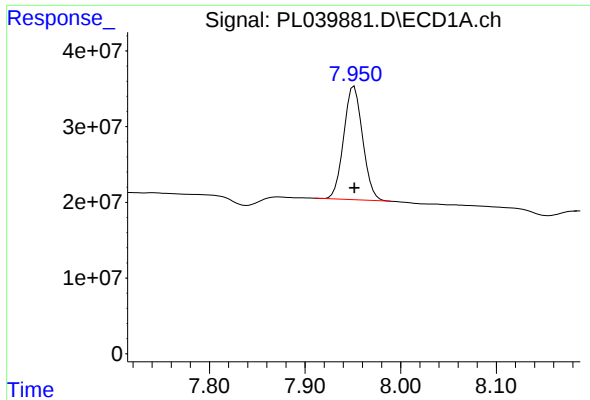


#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 206200498
Conc: 25.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Manual Integrations
APPROVED

Sohil
9/17/2018 11:10:58 AM

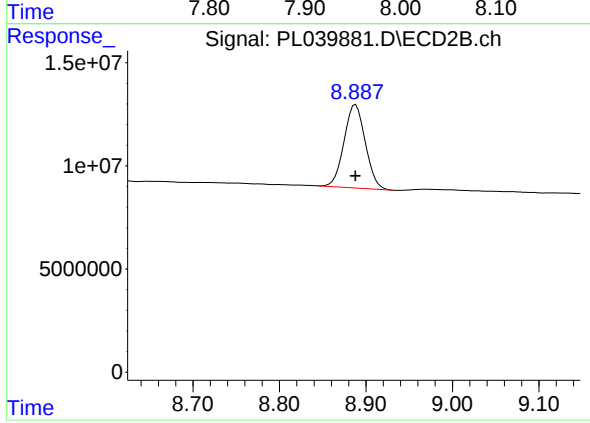

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 68686652
Conc: 26.50 ng/ml