

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
 Data File : PL039885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 14:51
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL091418CHLOR

Manual Integrations
 APPROVED

Sohil
 9/17/2018 11:11:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 15:03:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 13:34:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	397.1E6	159.4E6	51.200	49.945
28)	SA Decachlor...	7.952	8.888	412.6E6	134.0E6	49.512	49.348
Target Compounds							
23)	Chlordane-1	4.136	4.880	174.7E6	78474479	481.915	506.790
24)	Chlordane-2	4.625	5.340	184.6E6	76214812	490.142	500.081
25)	Chlordane-3	5.176	5.977	554.1E6	264.5E6	451.512m	516.570
26)	Chlordane-4	5.232	6.053	561.6E6	312.9E6	512.341	505.464
27)	Chlordane-5	6.053	6.842	192.9E6	59402369	520.304	511.910

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091418\
Data File : PL039885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 14:51
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ICVPL091418CHLOR


Manual Integrations
APPROVED

Sohil
9/17/2018 11:11:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 15:03:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 13:34:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

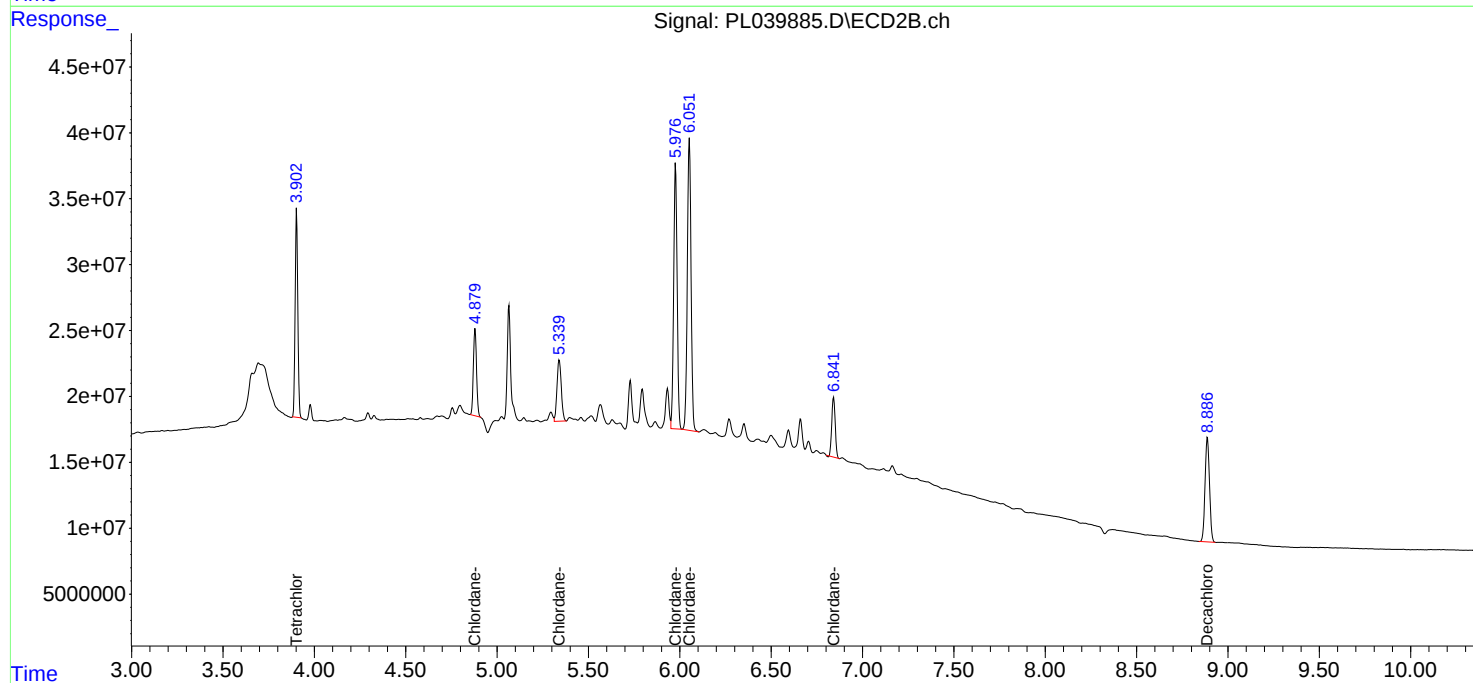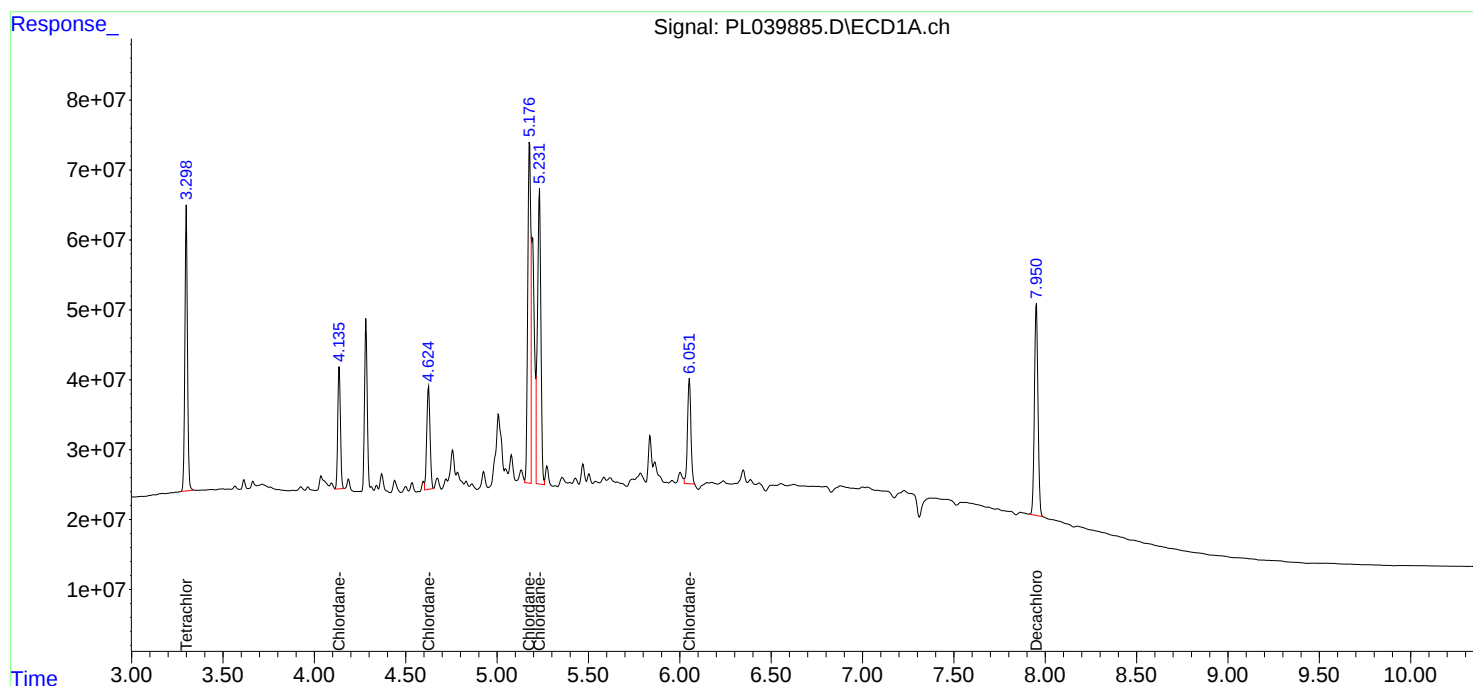

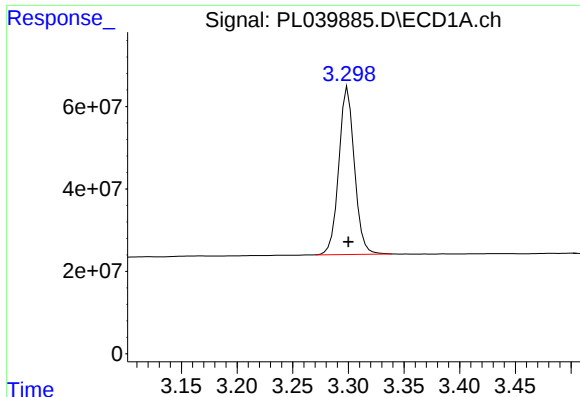


#1 Tetrachloro-m-xylene

R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 397052546
Conc: 51.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091418CHLOR


Manual Integrations
APPROVED

Sohil
9/17/2018 11:11:02 AM

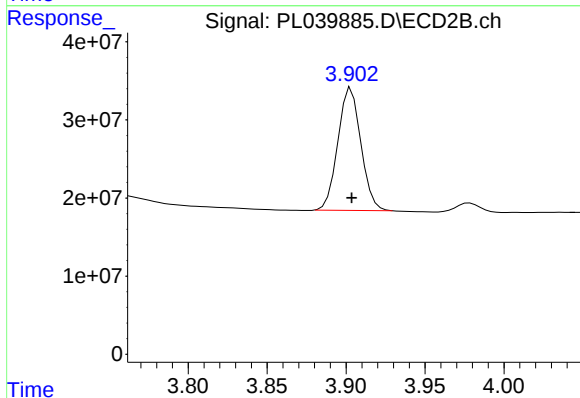


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 159365823
Conc: 49.95 ng/ml

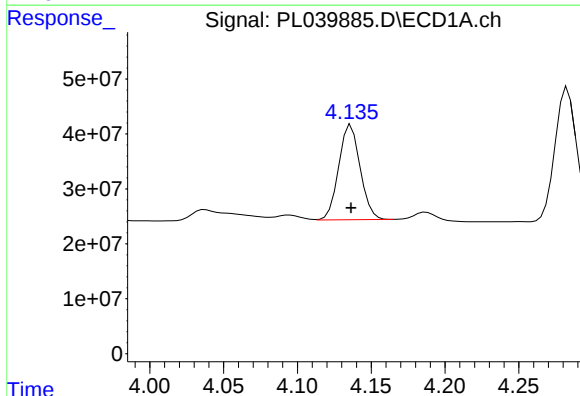


#23 Chlordane-1

R.T.: 4.136 min
Delta R.T.: 0.000 min
Response: 174666478
Conc: 481.91 ng/ml

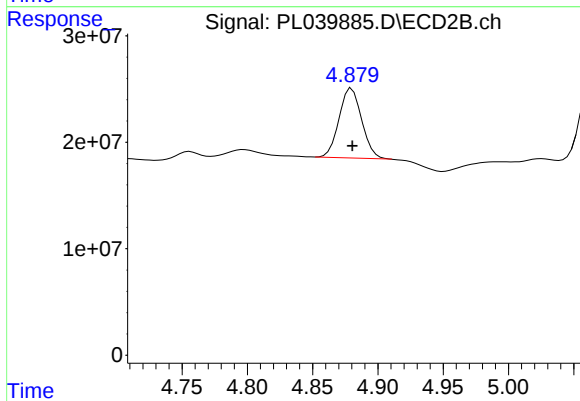

#23 Chlordane-1

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 78474479
Conc: 506.79 ng/ml

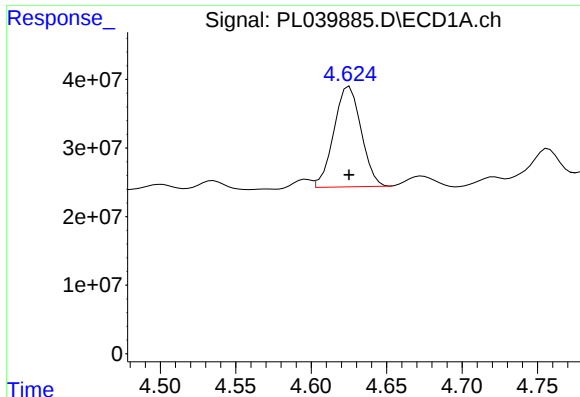


#24 Chlordane-2

R.T.: 4.625 min
Delta R.T.: 0.000 min
Response: 184596026
Conc: 490.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091418CHLOR


Manual Integrations
APPROVED

Sohil
9/17/2018 11:11:02 AM

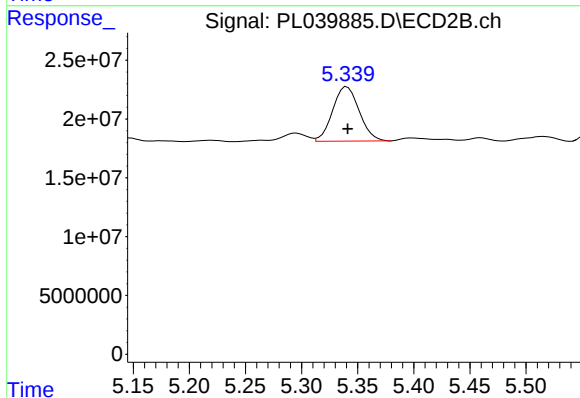


#24 Chlordane-2

R.T.: 5.340 min
Delta R.T.: 0.000 min
Response: 76214812
Conc: 500.08 ng/ml

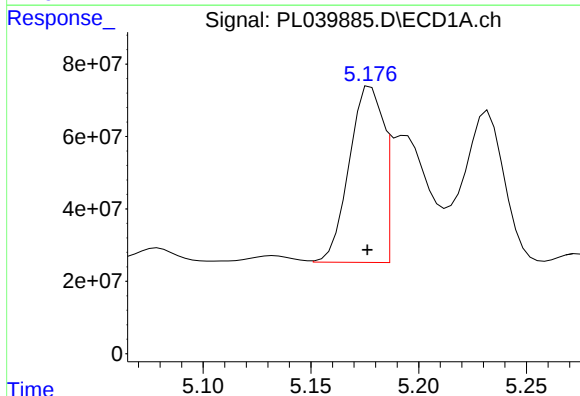


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 554061246
Conc: 451.51 ng/ml m

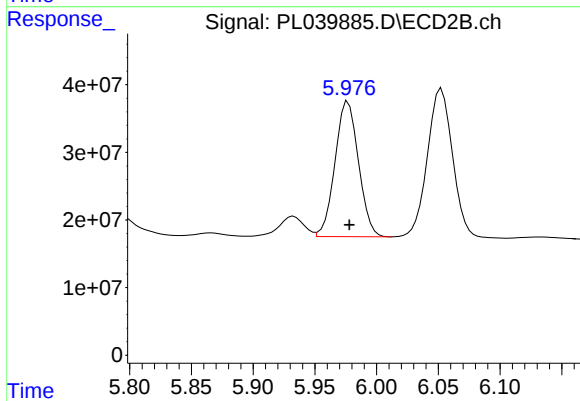

#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: -0.001 min
Response: 264453408
Conc: 516.57 ng/ml

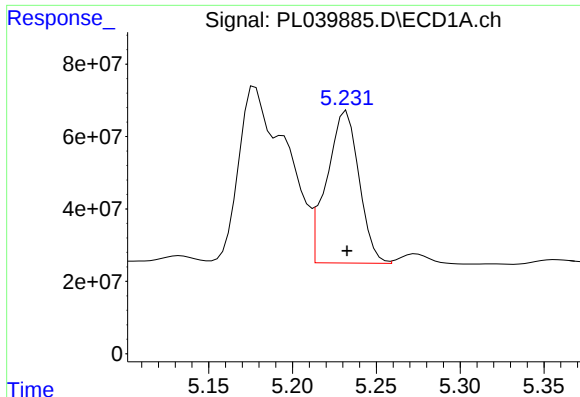


#26 Chlordane-4

R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 561648627
Conc: 512.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091418CHLOR


Manual Integrations
APPROVED

Sohil
9/17/2018 11:11:02 AM

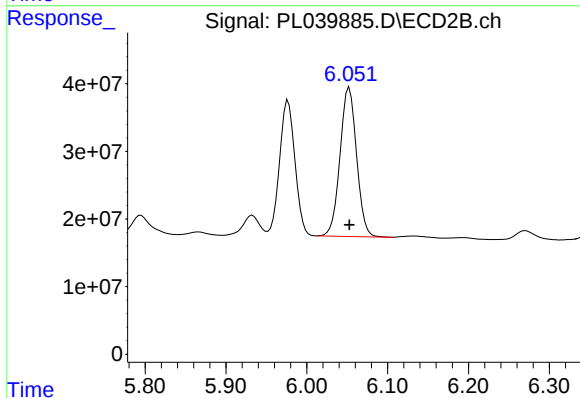


#26 Chlordane-4

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 312861886
Conc: 505.46 ng/ml

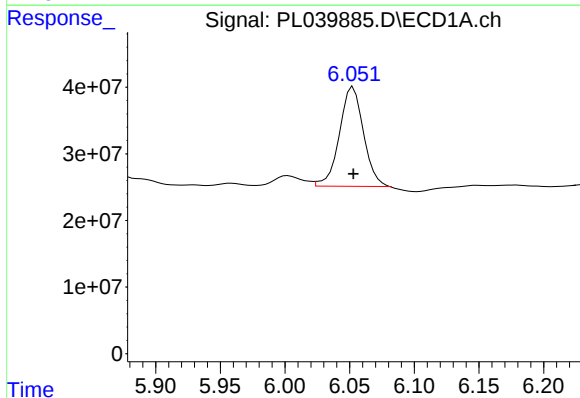


#27 Chlordane-5

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 192903998
Conc: 520.30 ng/ml

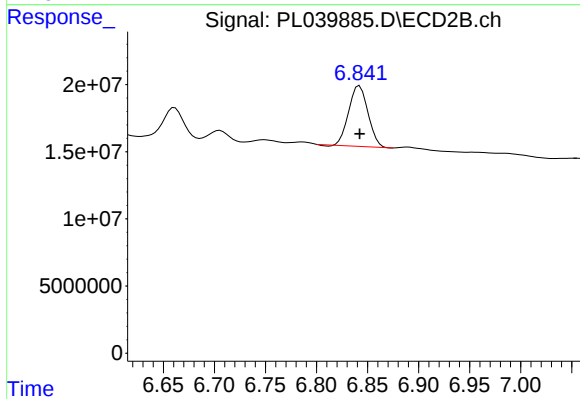

#27 Chlordane-5

R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 59402369
Conc: 511.91 ng/ml

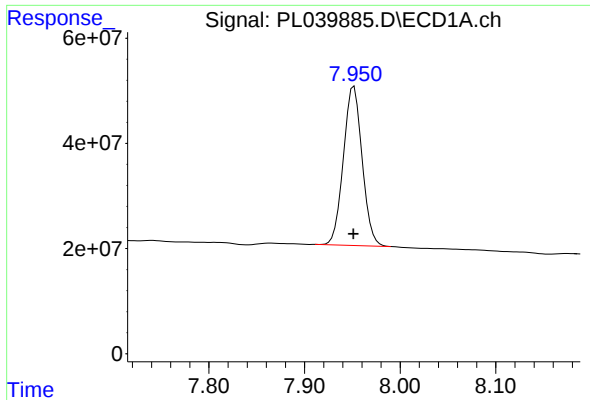


#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 412568009
Conc: 49.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091418CHLOR

Manual Integrations
APPROVED

Sohil
9/17/2018 11:11:02 AM

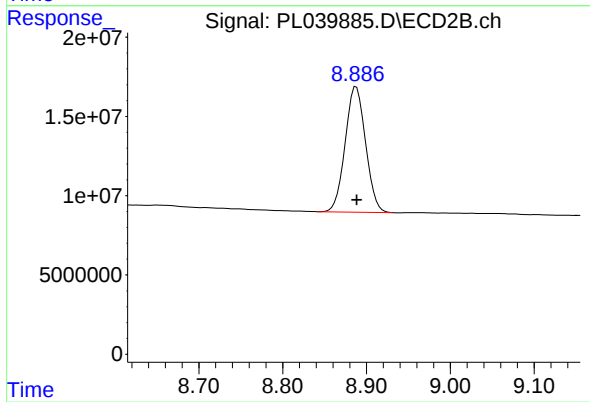

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 134032260
Conc: 49.35 ng/ml