

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
 Data File : PL061410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2020 12:31
 Operator : DD\AJ
 Sample : L3863-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 16:32:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.007	23433850	34646203	13.587	11.264
28)	SA Decachlor...	8.210	9.093	20340083	32449028	12.192	13.723
Target Compounds							
10)	B gamma-Chl...	0.000	6.122	0	3653270	N.D.	1.060 #
11)	B alpha-Chl...	0.000	6.194	0	5718980	N.D.	1.643 #
17)	MA 4,4'-DDT	0.000	7.142	0	3791062	N.D.	1.515 #
23)	Chlordane-1	4.319	0.000	2730311	0	52.048	N.D. #
25)	Chlordane-3	0.000	6.122	0	3653270	N.D.	8.457 #
26)	Chlordane-4	0.000	6.194	0	5718980	N.D.	10.925 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
Data File : PL061410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2020 12:31
Operator : DD\AJ
Sample : L3863-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 16:32:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

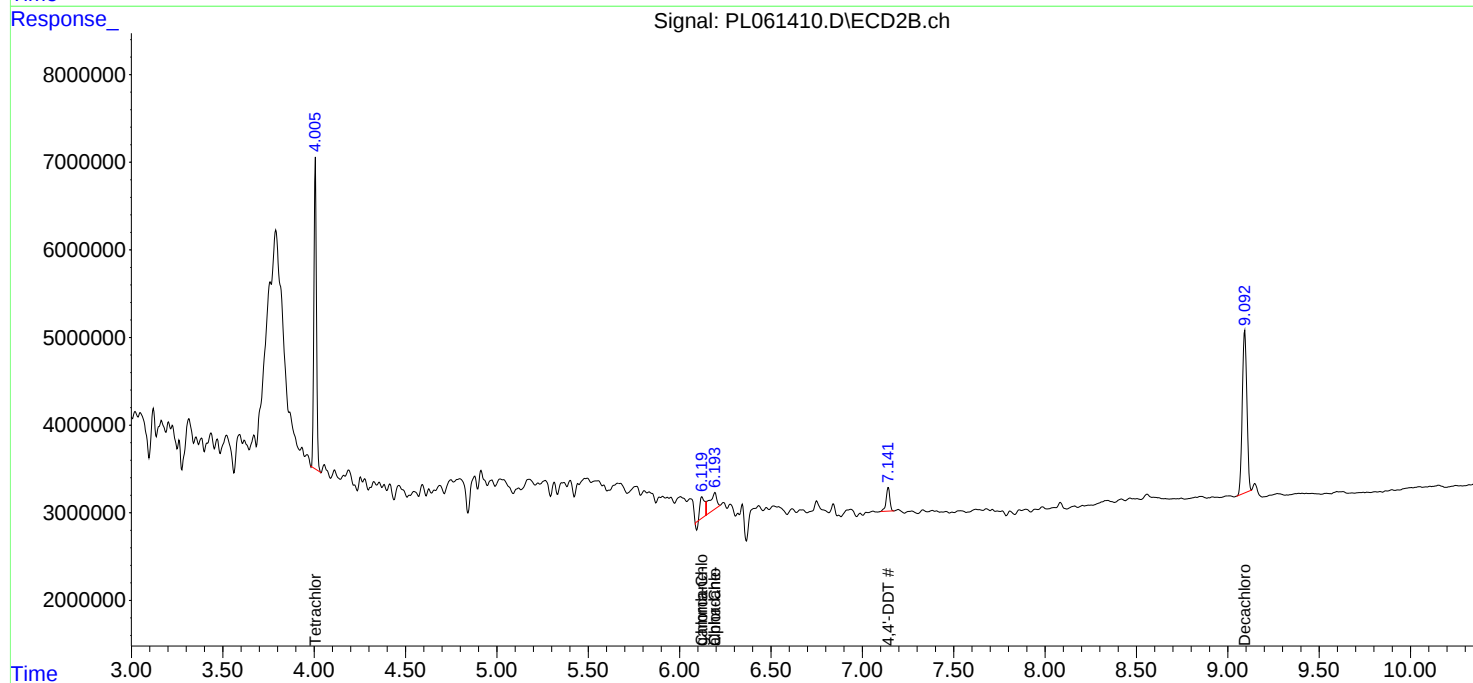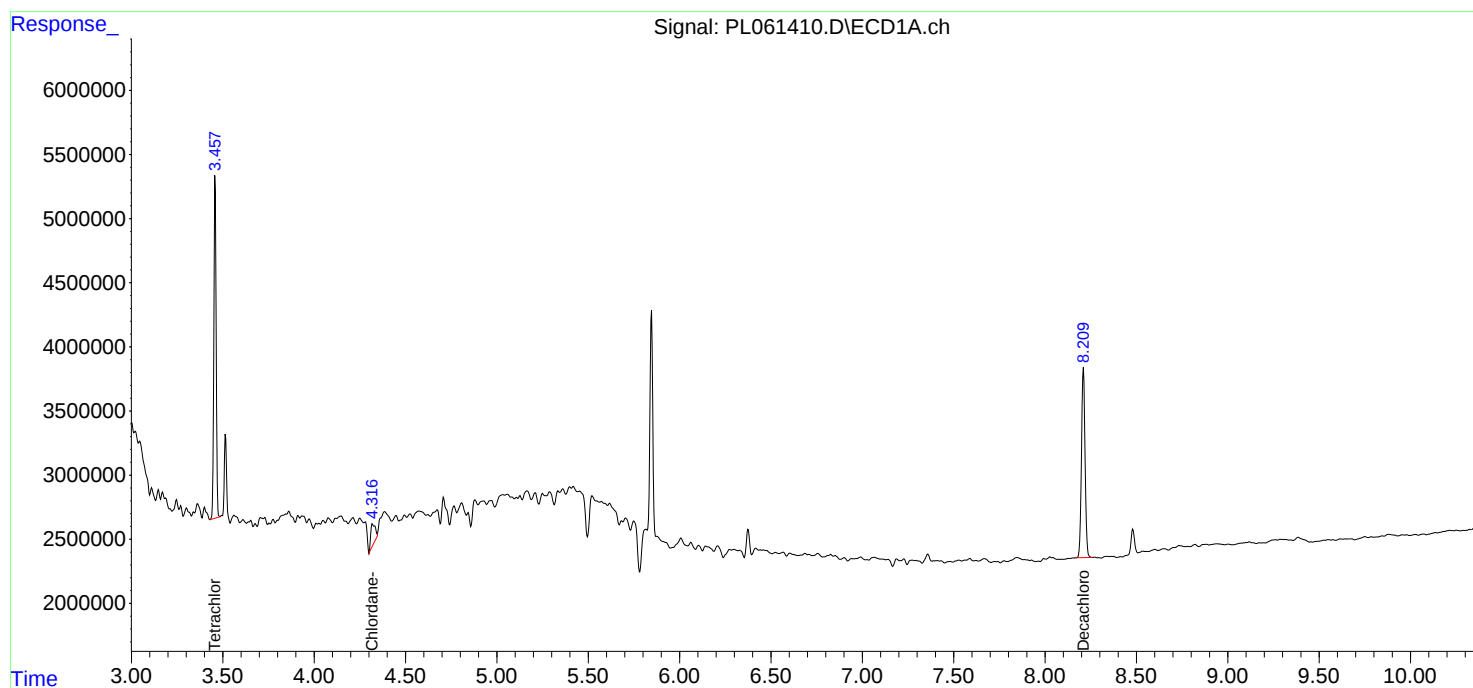


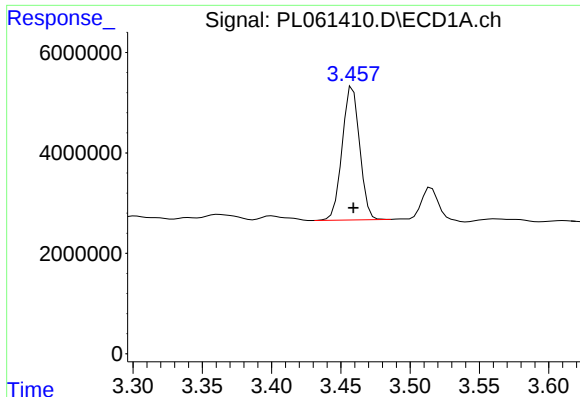

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 23433850
Conc: 13.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

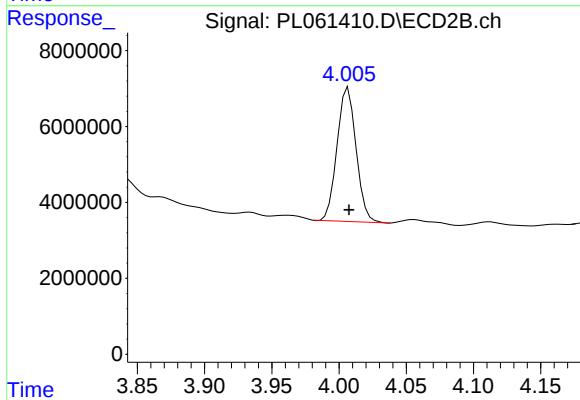


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 34646203
Conc: 11.26 ng/ml

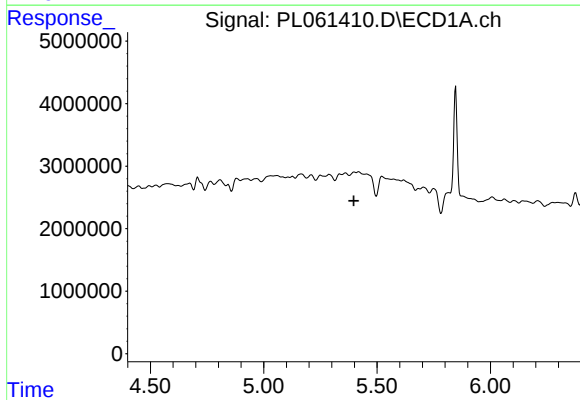


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

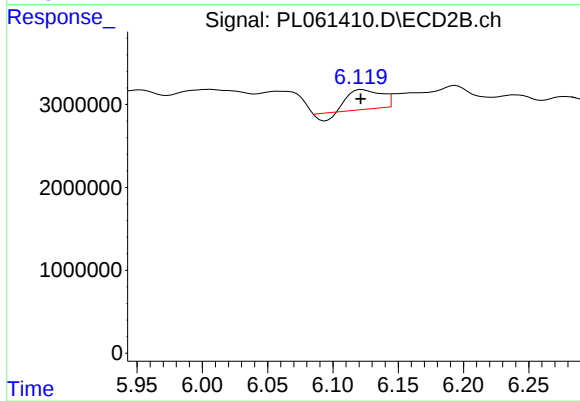

#10 gamma-Chlordane


R.T.: 6.122 min
Delta R.T.: 0.001 min
Response: 3653270
Conc: 1.06 ng/ml

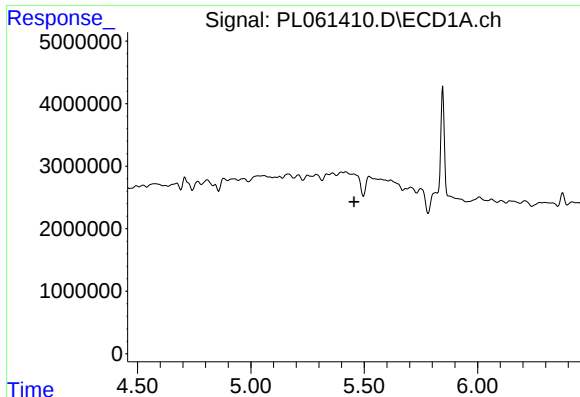

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

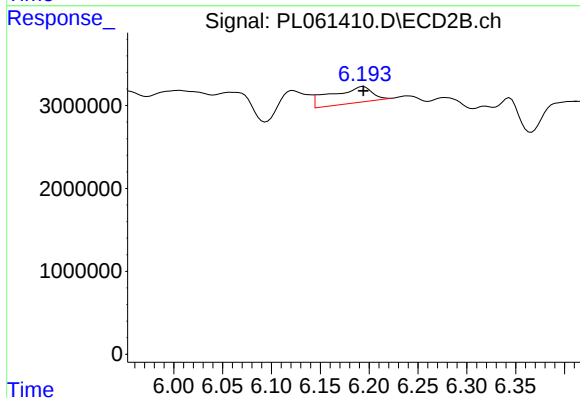


#11 alpha-Chlordane

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 5718980
Conc: 1.64 ng/ml

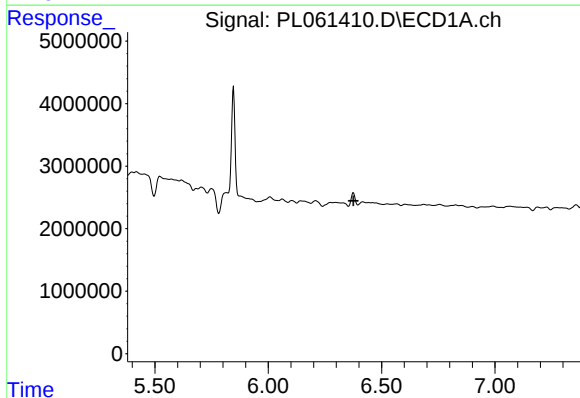


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

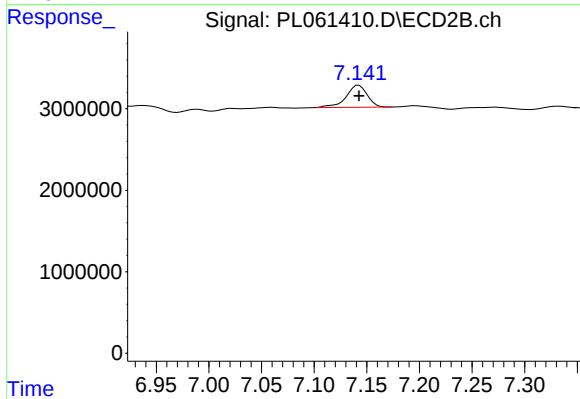

#17 4,4'-DDT


R.T.: 7.142 min
Delta R.T.: 0.000 min
Response: 3791062
Conc: 1.51 ng/ml

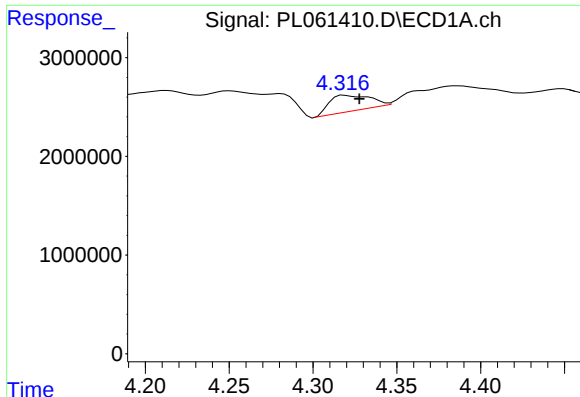

#23 Chlordane-1


R.T.: 4.319 min
Delta R.T.: -0.009 min
Response: 2730311
Conc: 52.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

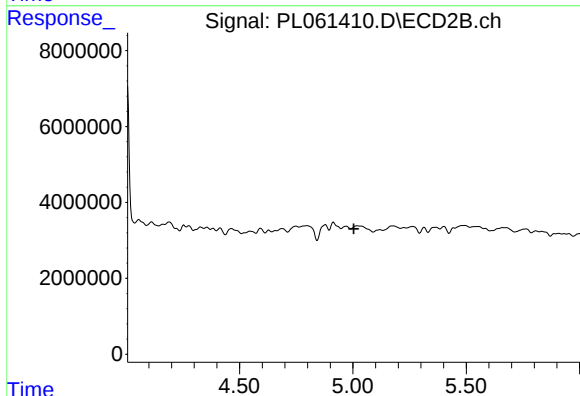


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

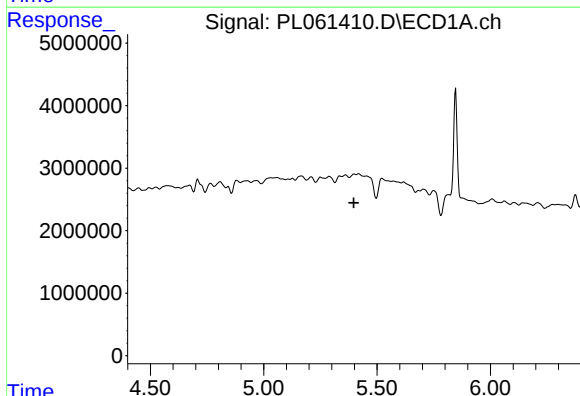


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

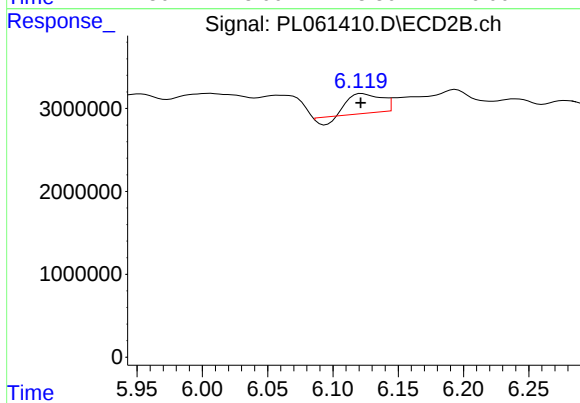

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.001 min
Response: 3653270
Conc: 8.46 ng/ml

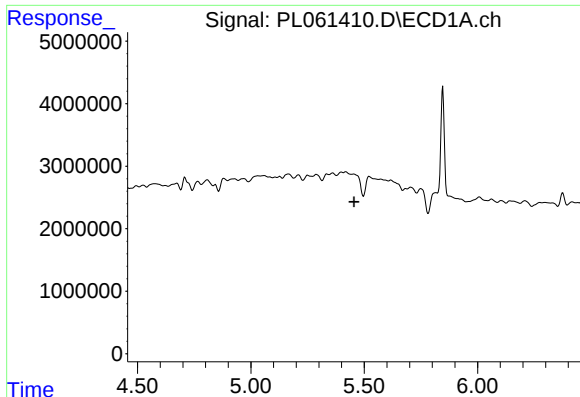

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

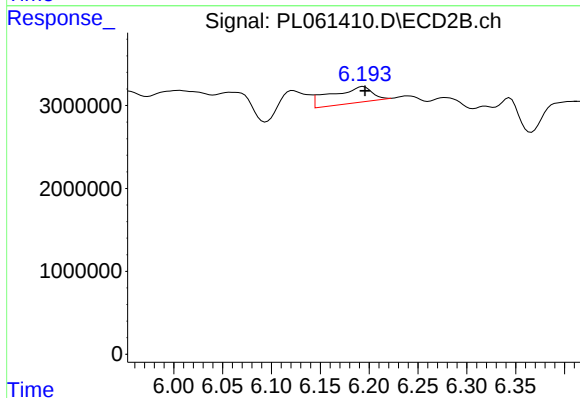


#26 Chlordane-4

R.T.: 6.194 min
Delta R.T.: -0.002 min
Response: 5718980
Conc: 10.93 ng/ml

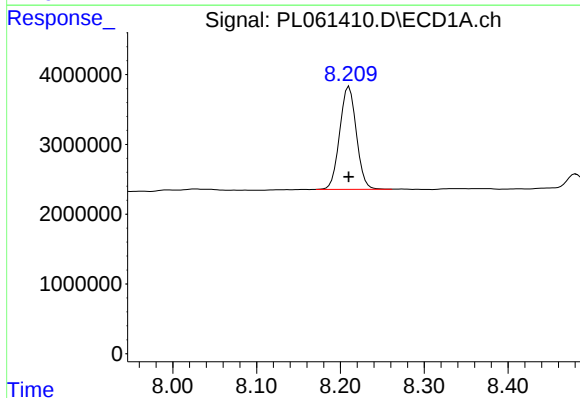

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 20340083
Conc: 12.19 ng/ml

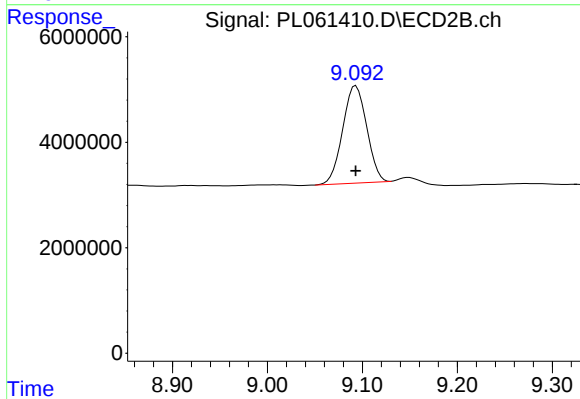

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 32449028
Conc: 13.72 ng/ml