

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
 Data File : PL061425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2020 16:03
 Operator : DD\AJ
 Sample : L3981-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B20-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:31:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	24975905	43497673	14.481	14.141
28)	SA Decachlor...	8.210	9.093	20205964	28910090	12.112	12.226
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	11179419	N.D.	2.421 #
8)	B Heptachlo...	0.000	5.876	0	2614263	N.D.	0.876 #
12)	B 4,4'-DDE	0.000	6.349	0	4570651	N.D.	1.426 #
14)	MA Endrin	0.000	6.713	0	2760710	N.D.	0.987 #
16)	A 4,4'-DDD	0.000	6.849	0	5429558	N.D.	2.114 #
17)	MA 4,4'-DDT	6.373	7.117f	4116391	2133396	2.998	0.852 #
19)	B Endosulfa...	6.683f	0.000	5063675	0	3.077	N.D. #
20)	A Methoxychlor	0.000	7.622f	0	5938385	N.D.	4.128 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
Data File : PL061425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2020 16:03
Operator : DD\AJ
Sample : L3981-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B20-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:31:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

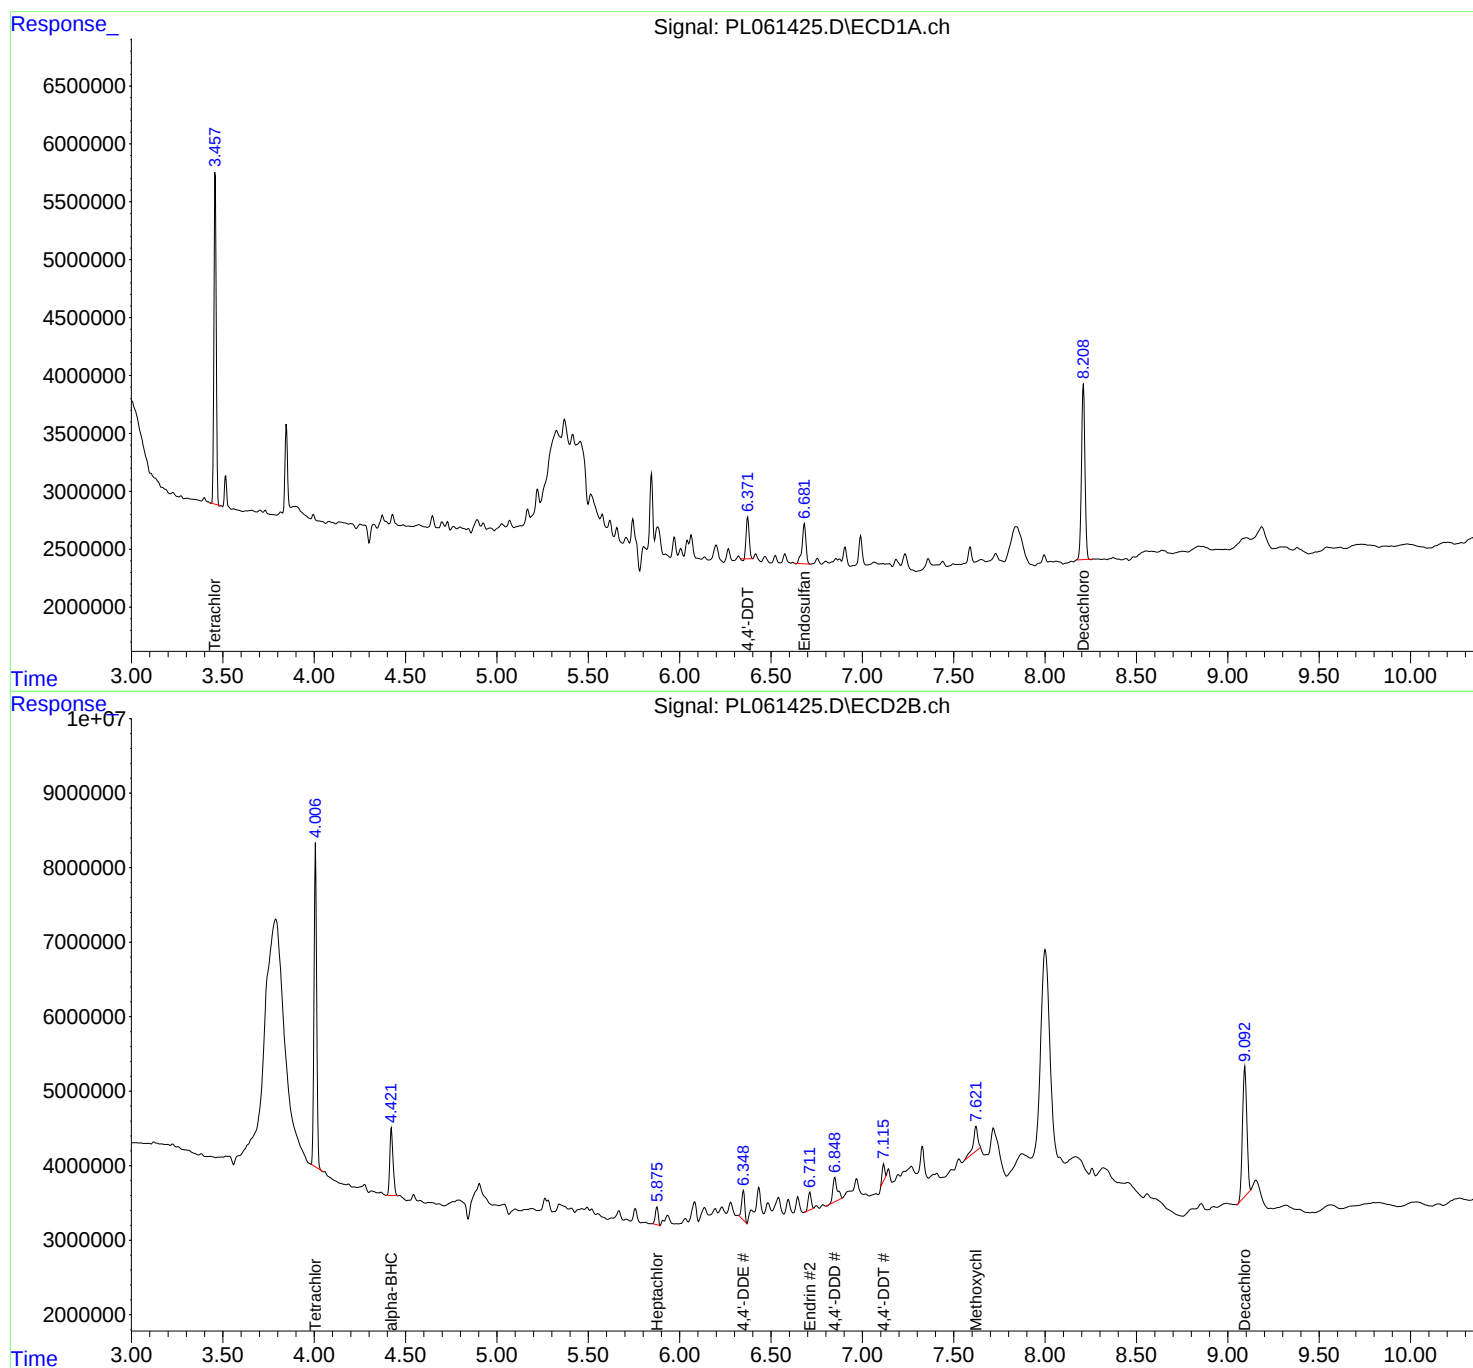


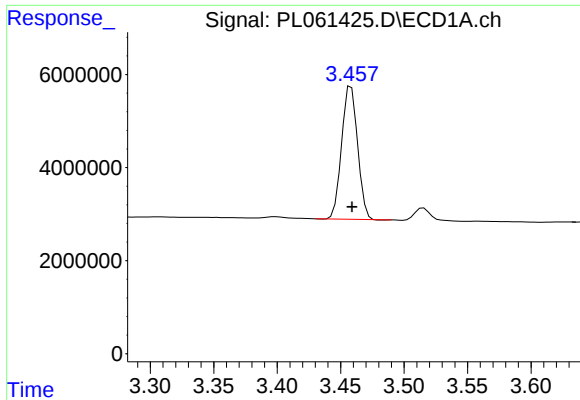

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 24975905
Conc: 14.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
B20-0-2

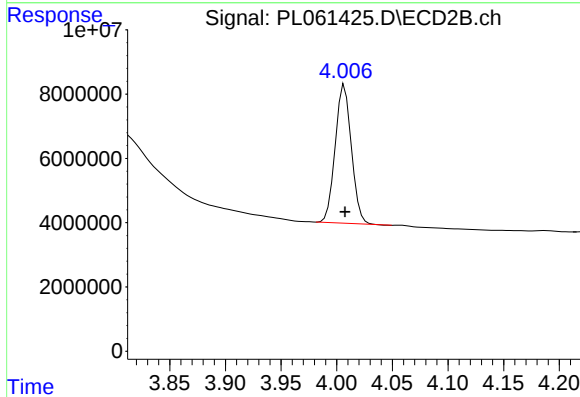


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 43497673
Conc: 14.14 ng/ml

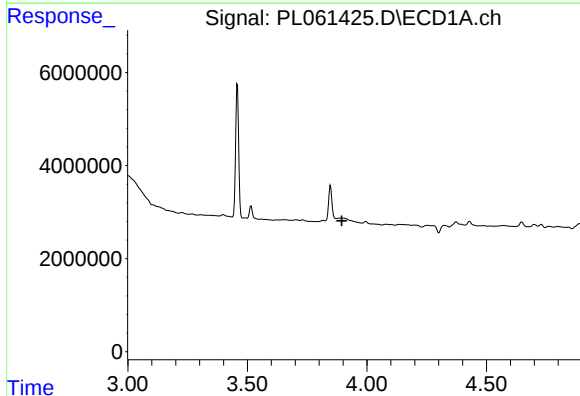


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.895 min
Response: 0
Conc: N.D.

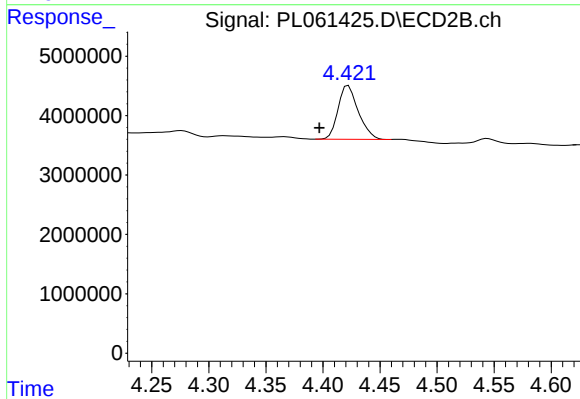

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.025 min
Response: 11179419
Conc: 2.42 ng/ml

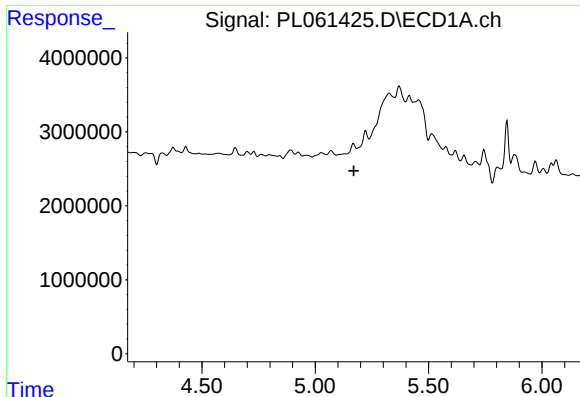

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B20-0-2

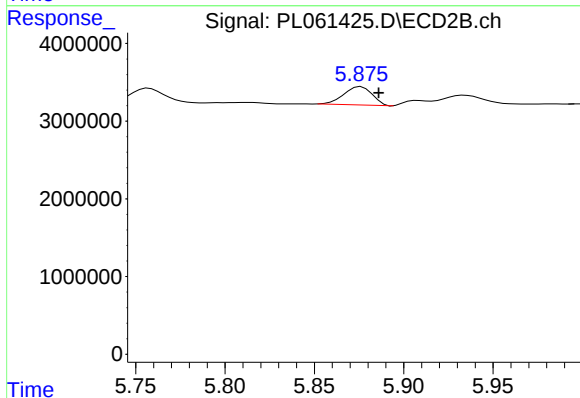


#8 Heptachlor epoxide

R.T.: 5.876 min
Delta R.T.: -0.010 min
Response: 2614263
Conc: 0.88 ng/ml

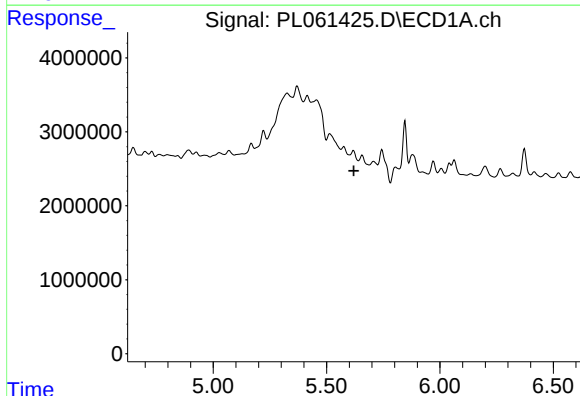


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.621 min
Response: 0
Conc: N.D.

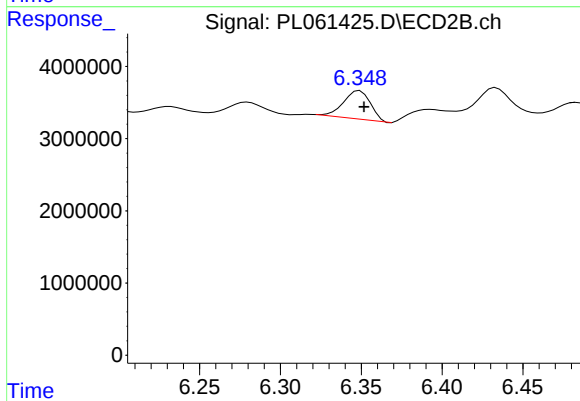

#12 4,4'-DDE


R.T.: 6.349 min
Delta R.T.: -0.003 min
Response: 4570651
Conc: 1.43 ng/ml

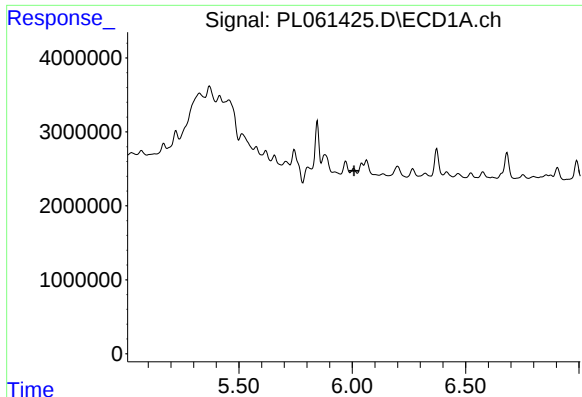

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B20-0-2

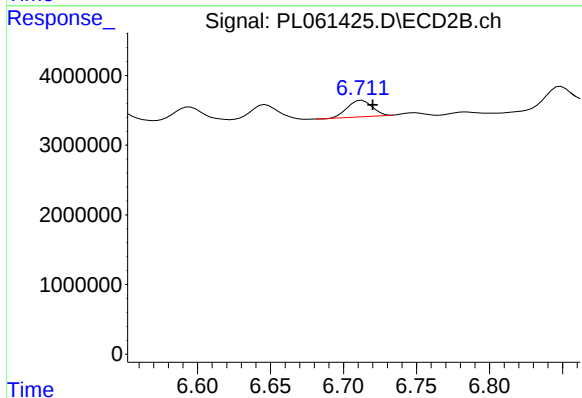


#14 Endrin

R.T.: 6.713 min
Delta R.T.: -0.007 min
Response: 2760710
Conc: 0.99 ng/ml

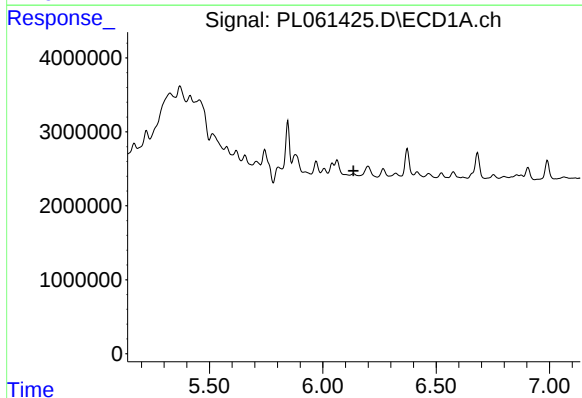


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.136 min
Response: 0
Conc: N.D.

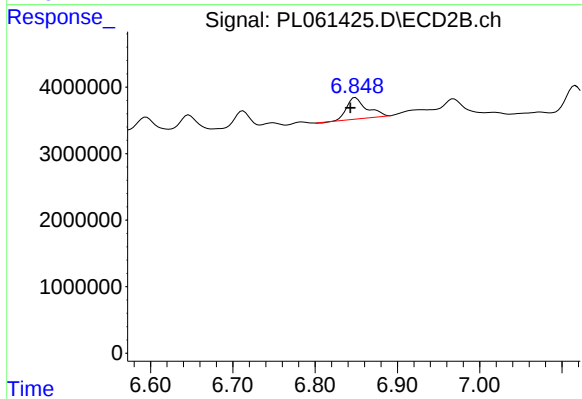

#16 4,4'-DDD


R.T.: 6.849 min
Delta R.T.: 0.006 min
Response: 5429558
Conc: 2.11 ng/ml

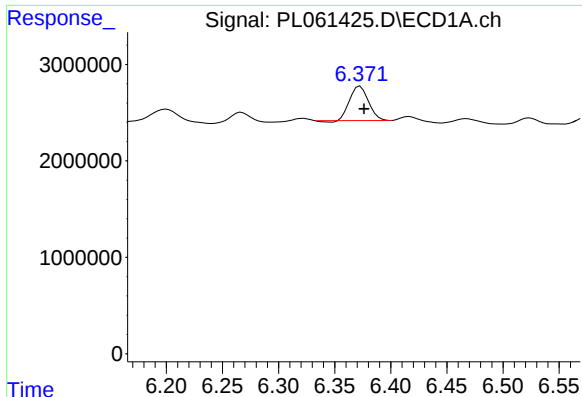

#17 4,4'-DDT


R.T.: 6.373 min
Delta R.T.: -0.004 min
Response: 4116391
Conc: 3.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
B20-0-2

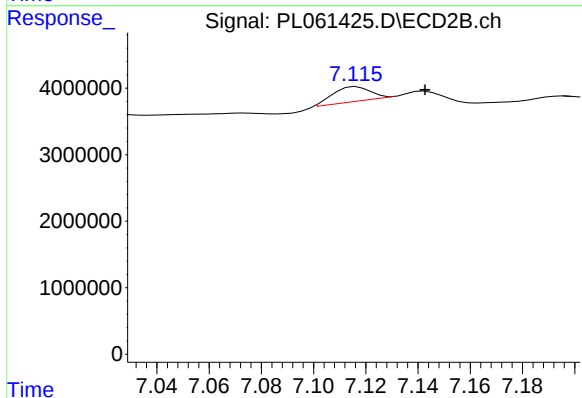


#17 4,4'-DDT

R.T.: 7.117 min
Delta R.T.: -0.026 min
Response: 2133396
Conc: 0.85 ng/ml

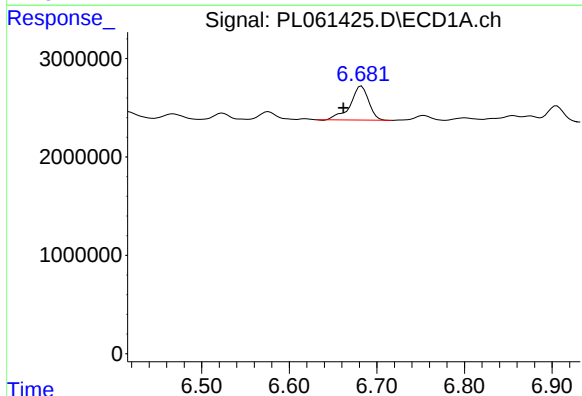


#19 Endosulfan Sulfate

R.T.: 6.683 min
Delta R.T.: 0.021 min
Response: 5063675
Conc: 3.08 ng/ml

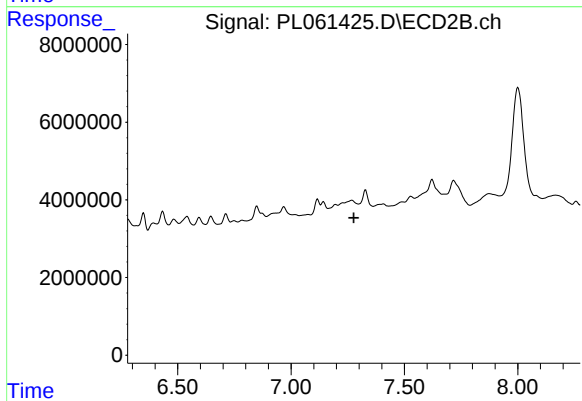

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

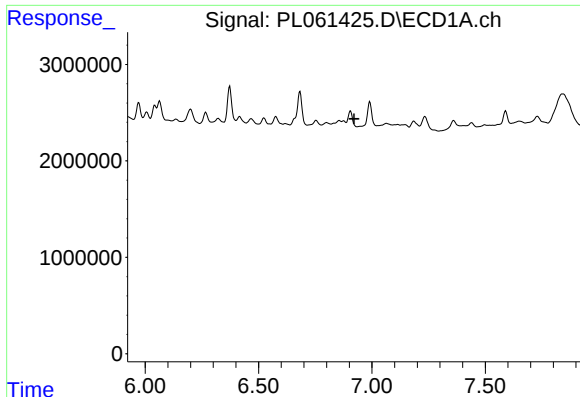

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B20-0-2

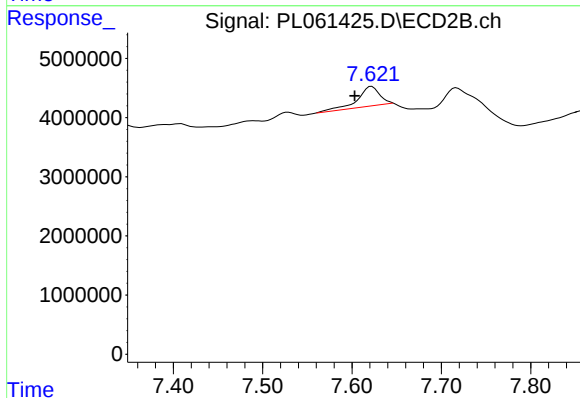


#20 Methoxychlor

R.T.: 7.622 min
Delta R.T.: 0.019 min
Response: 5938385
Conc: 4.13 ng/ml

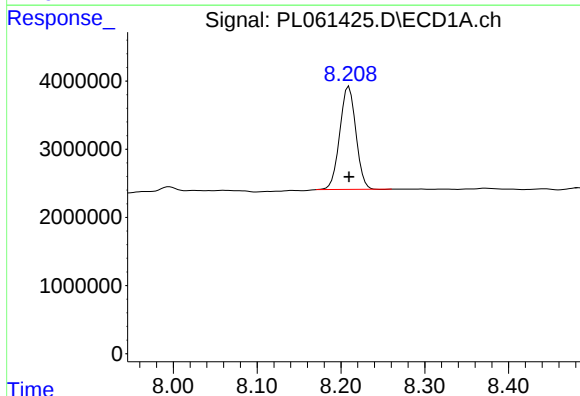

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 20205964
Conc: 12.11 ng/ml

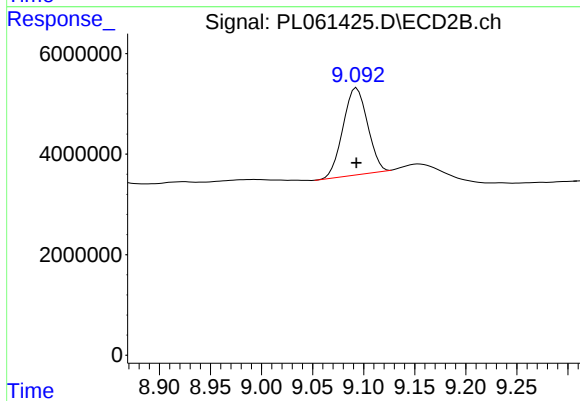

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 28910090
Conc: 12.23 ng/ml