

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
 Data File : PL061430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2020 17:13
 Operator : DD\AJ
 Sample : L3993-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B38-091120-10-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:32:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	39105091	69981753	22.674	22.751
28)	SA Decachlor...	8.210	9.093	30068045	44732021	18.023	18.918
Target Compounds							
3)	MA gamma-BHC...	0.000	4.664f	0	3025023	N.D.	0.705 #
5)	MB Aldrin	4.708f	0.000	2530858	0	1.318	N.D. #
9)	A Endosulfan I	5.529f	6.249	5432649	14261827	3.158	4.446 #
11)	B alpha-Chl...	5.460	0.000	9690306	0	5.231	N.D. #
15)	B Endosulfa...	0.000	6.944	0	4332939	N.D.	1.467 #
23)	Chlordane-1	4.330	0.000	2478431	0	47.247	N.D. #
26)	Chlordane-4	5.460	0.000	9690306	0	70.400	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
Data File : PL061430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2020 17:13
Operator : DD\AJ
Sample : L3993-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:32:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

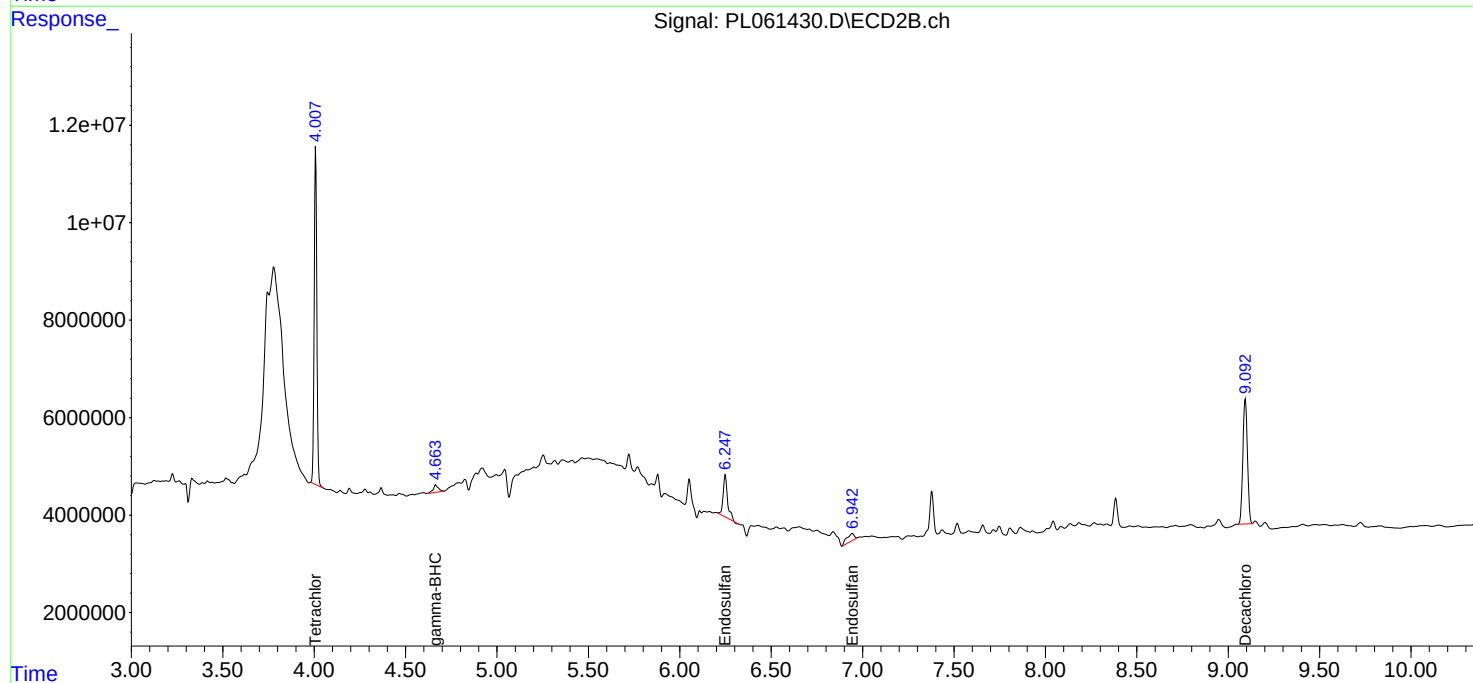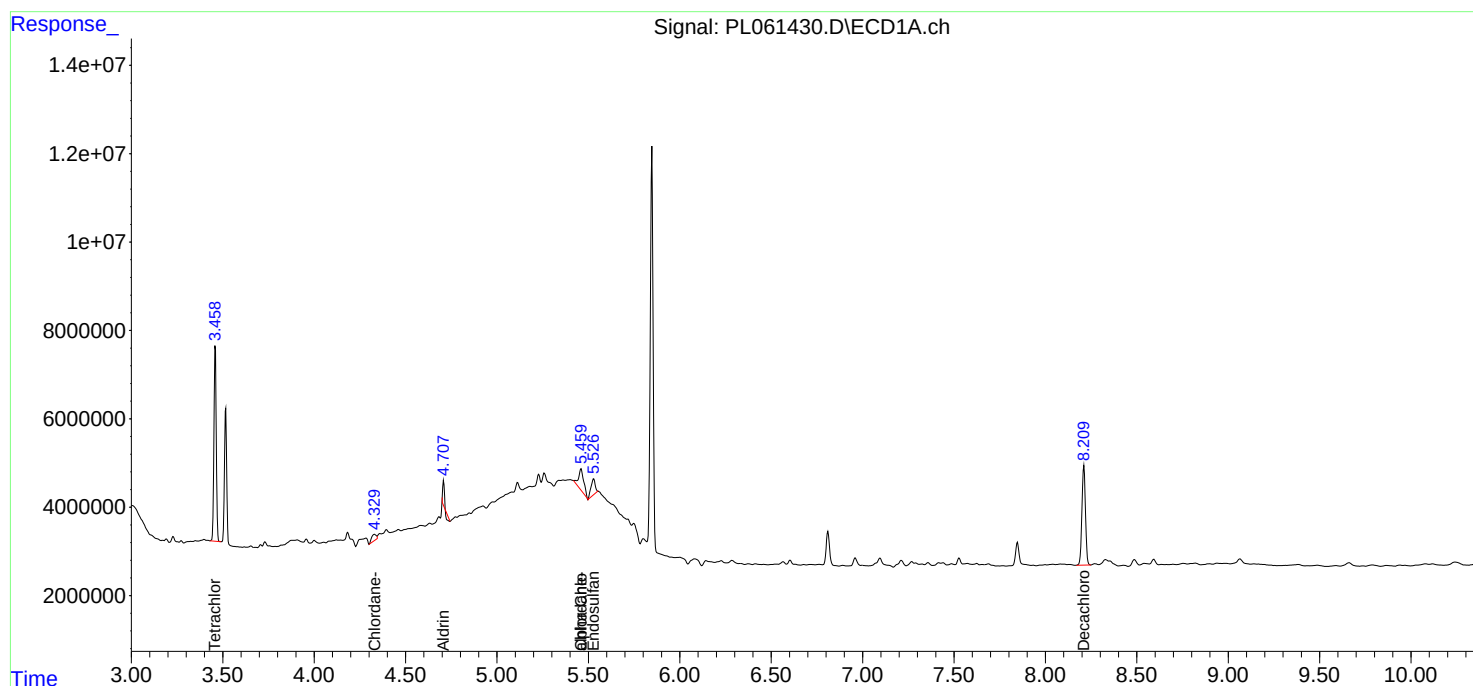


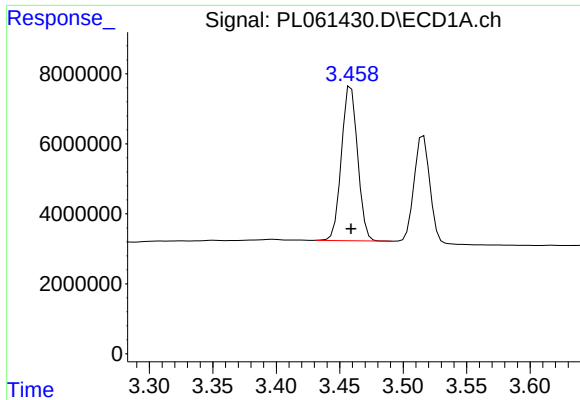

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 39105091
Conc: 22.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

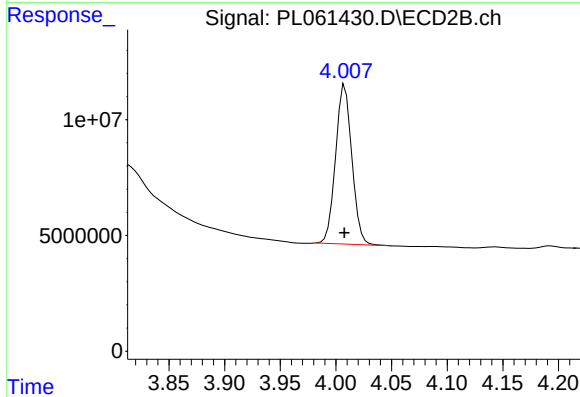


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 69981753
Conc: 22.75 ng/ml

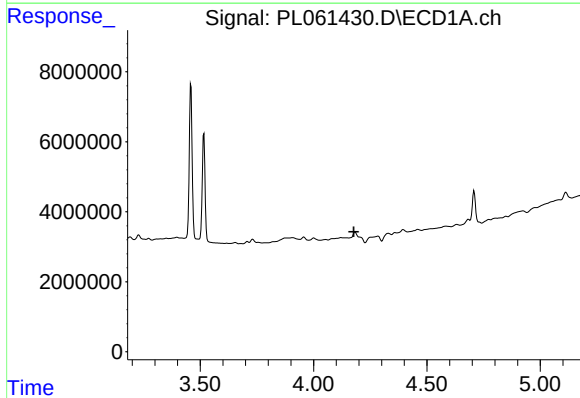


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.178 min
Response: 0
Conc: N.D.

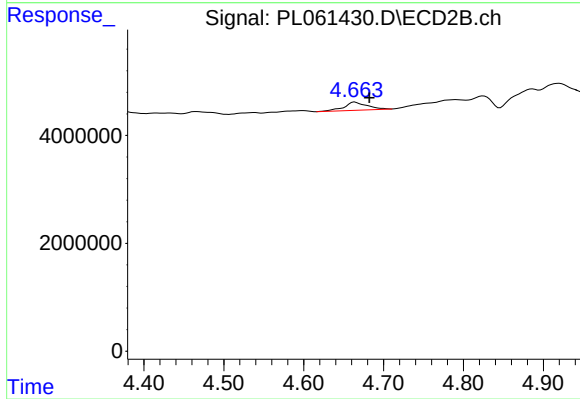

#3 gamma-BHC (Lindane)


R.T.: 4.664 min
Delta R.T.: -0.018 min
Response: 3025023
Conc: 0.71 ng/ml

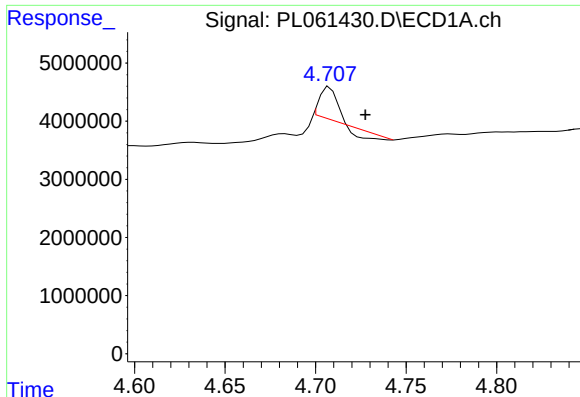

#5 Aldrin


R.T.: 4.708 min
Delta R.T.: -0.019 min
Response: 2530858
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

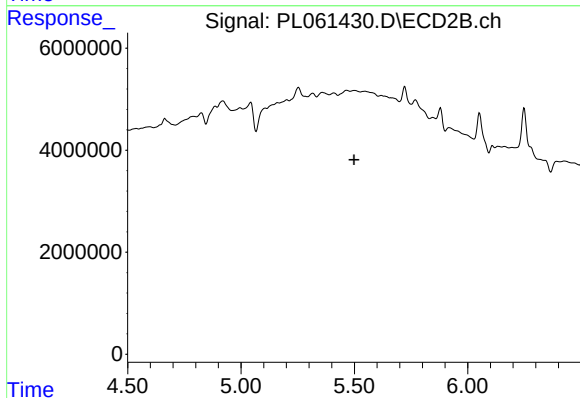


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

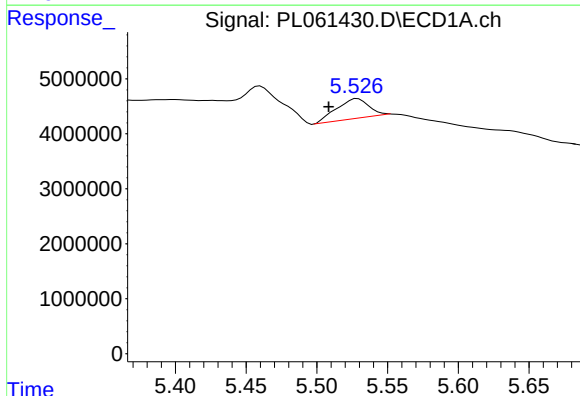


#9 Endosulfan I

R.T.: 5.529 min
Delta R.T.: 0.020 min
Response: 5432649
Conc: 3.16 ng/ml

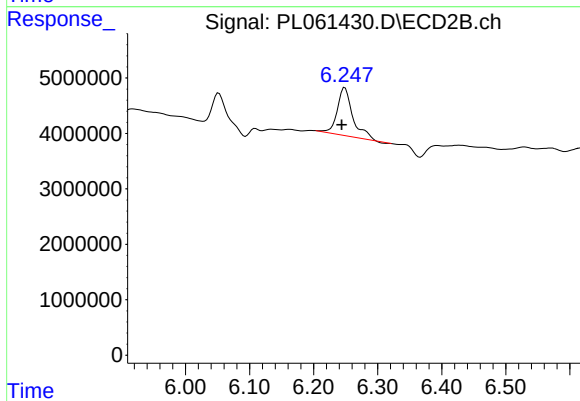

#9 Endosulfan I


R.T.: 6.249 min
Delta R.T.: 0.005 min
Response: 14261827
Conc: 4.45 ng/ml

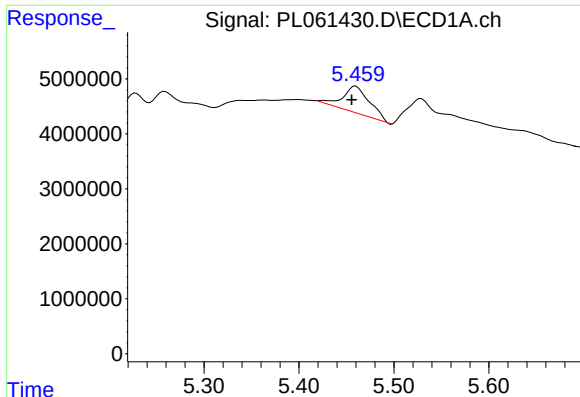

#11 alpha-Chlordane


R.T.: 5.460 min
Delta R.T.: 0.004 min
Response: 9690306
Conc: 5.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

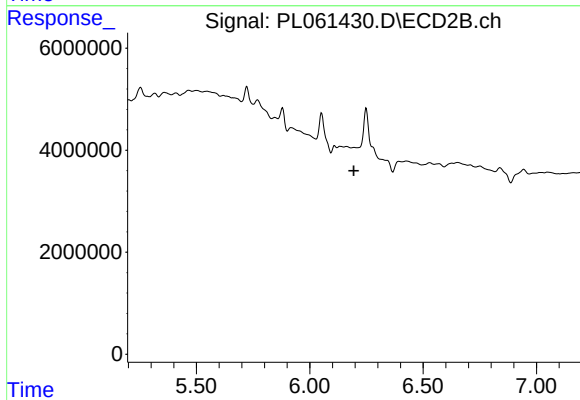


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.194 min
Response: 0
Conc: N.D.

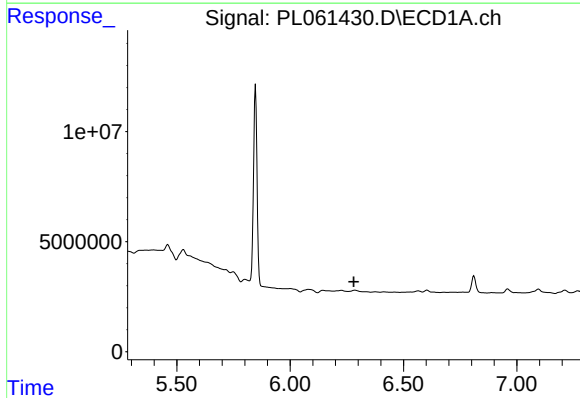


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

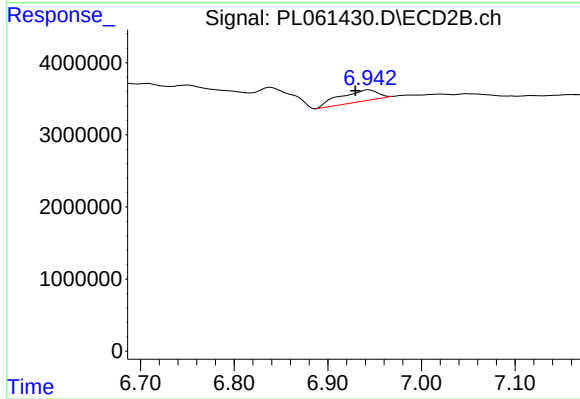

#15 Endosulfan II


R.T.: 6.944 min
Delta R.T.: 0.014 min
Response: 4332939
Conc: 1.47 ng/ml

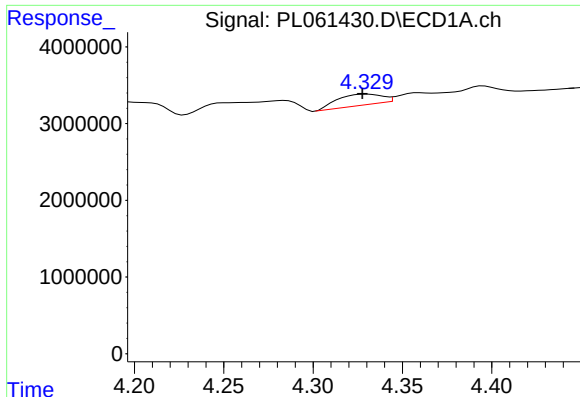

#23 Chlordane-1


R.T.: 4.330 min
Delta R.T.: 0.002 min
Response: 2478431
Conc: 47.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

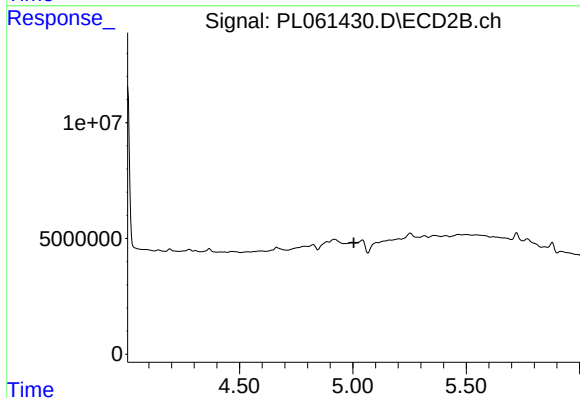


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

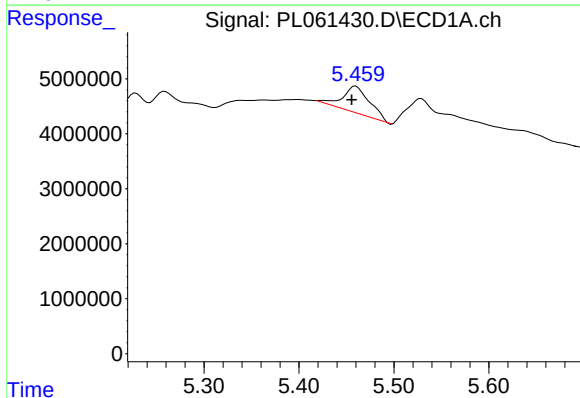


#26 Chlordane-4

R.T.: 5.460 min
Delta R.T.: 0.004 min
Response: 9690306
Conc: 70.40 ng/ml

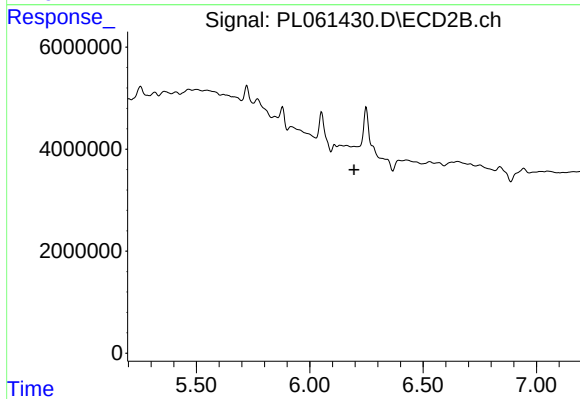

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.196 min
Response: 0
Conc: N.D.

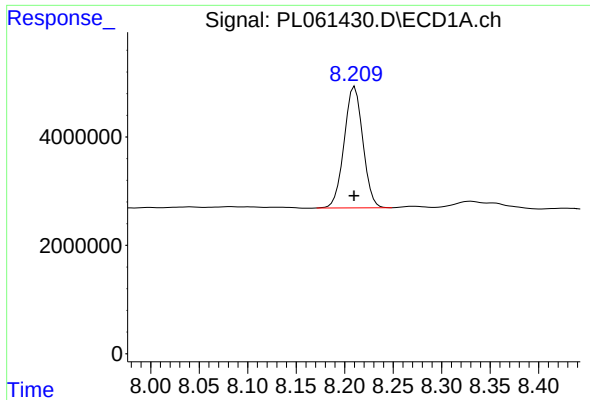

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 30068045
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

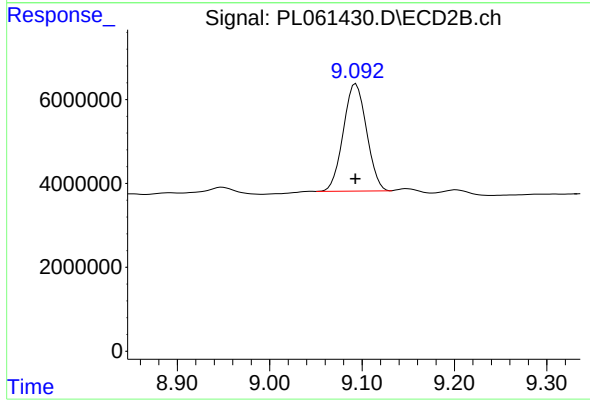

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 44732021
Conc: 18.92 ng/ml