

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
 Data File : PL061434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2020 18:10
 Operator : DD\AJ
 Sample : L3786-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 688-157

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:32:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.009	32609792	54110113	18.908	17.591
28)	SA Decachlor...	8.211	9.095	27793916	43370008	16.660	18.342
Target Compounds							
9)	A Endosulfan I	0.000	6.224f	0	8063441	N.D.	2.514 #
26)	Chlordane-4	0.000	6.224f	0	8063441	N.D.	15.404 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
Data File : PL061434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2020 18:10
Operator : DD\AJ
Sample : L3786-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
688-157

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:32:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

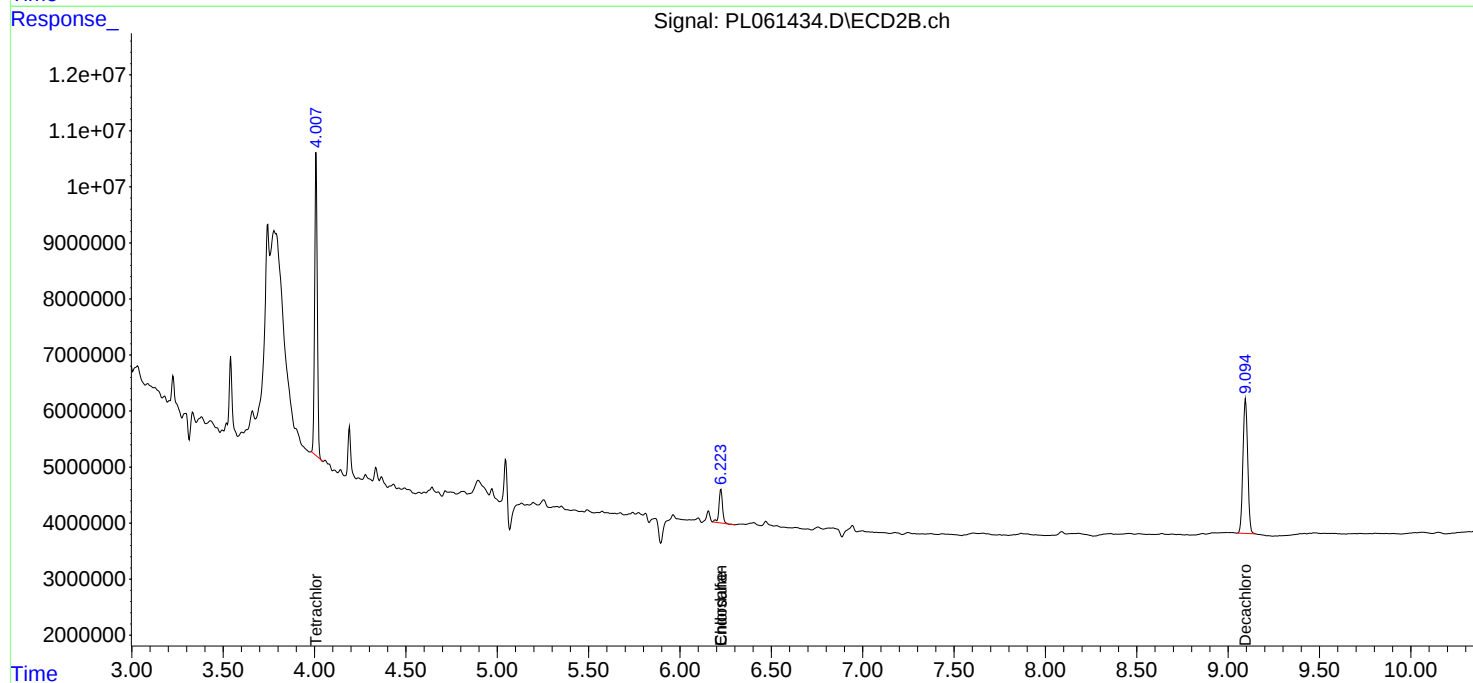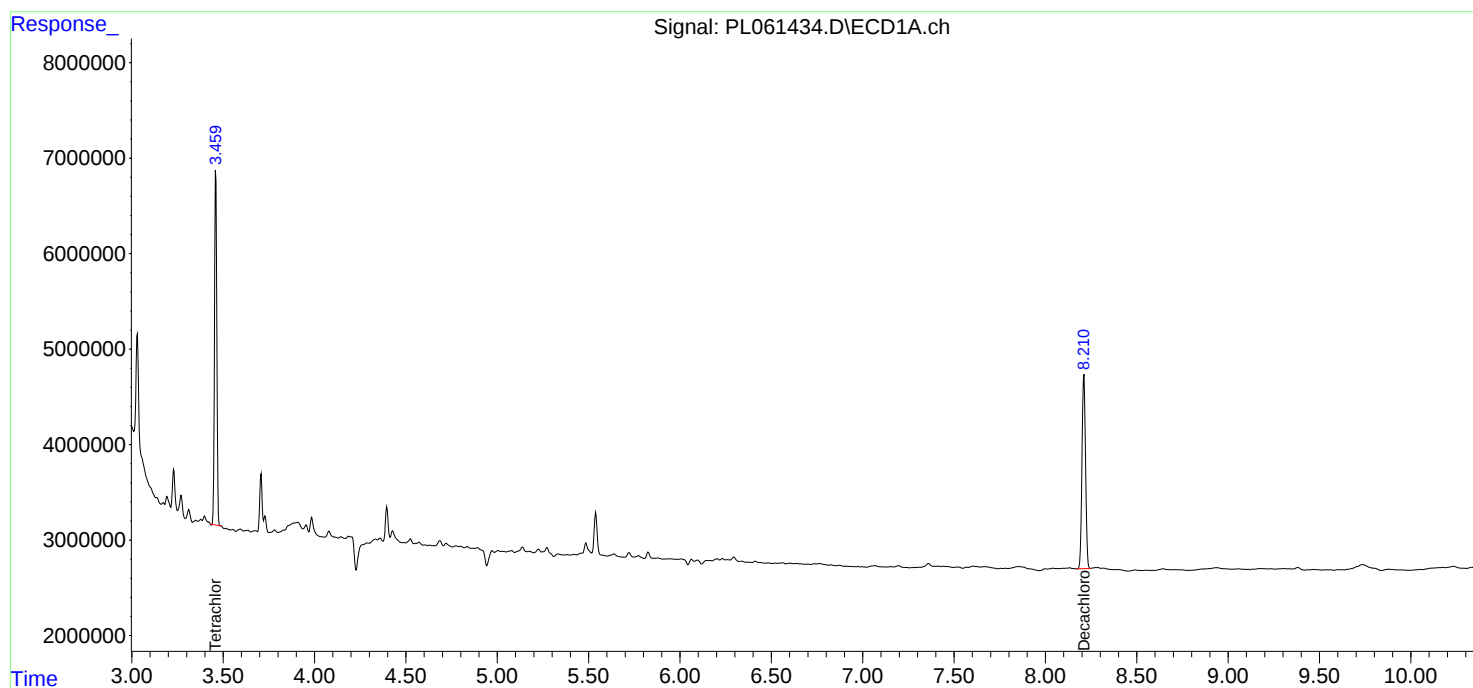


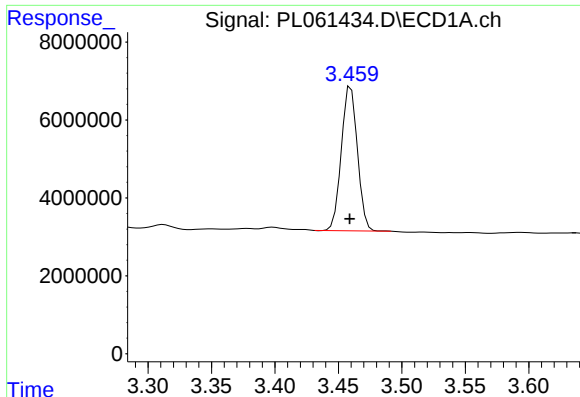

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 32609792
Conc: 18.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
688-157

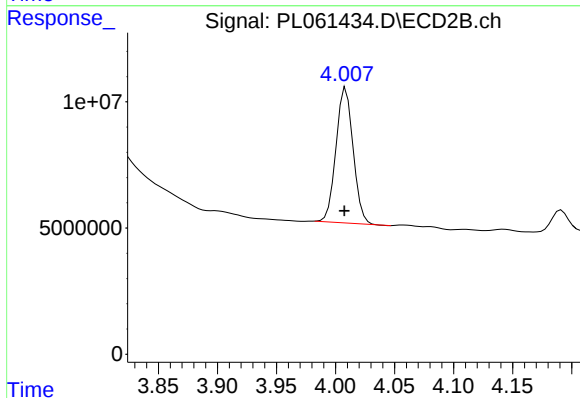


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.001 min
Response: 54110113
Conc: 17.59 ng/ml

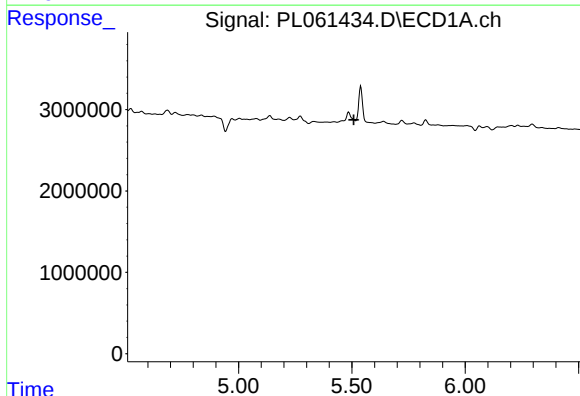


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

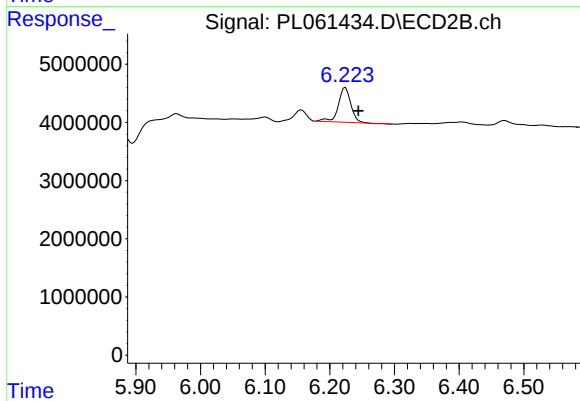

#9 Endosulfan I


R.T.: 6.224 min
Delta R.T.: -0.020 min
Response: 8063441
Conc: 2.51 ng/ml

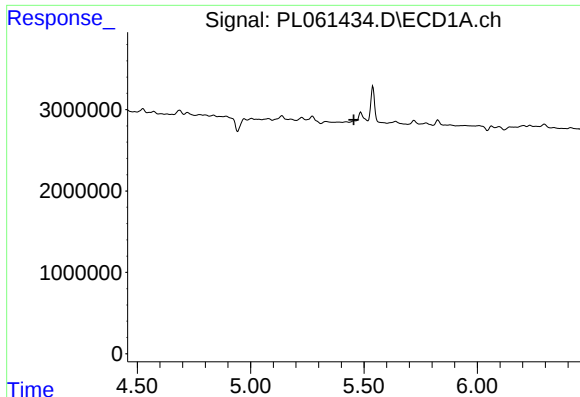

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
688-157

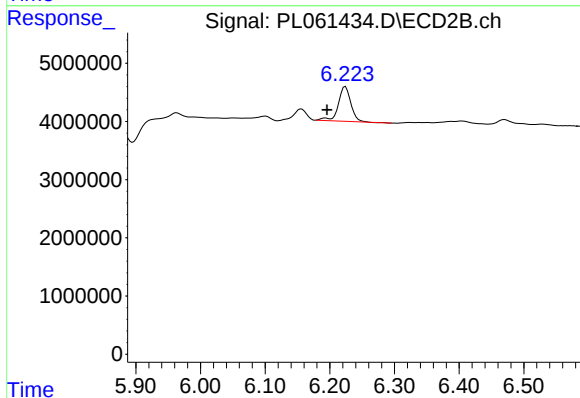


#26 Chlordane-4

R.T.: 6.224 min
Delta R.T.: 0.028 min
Response: 8063441
Conc: 15.40 ng/ml

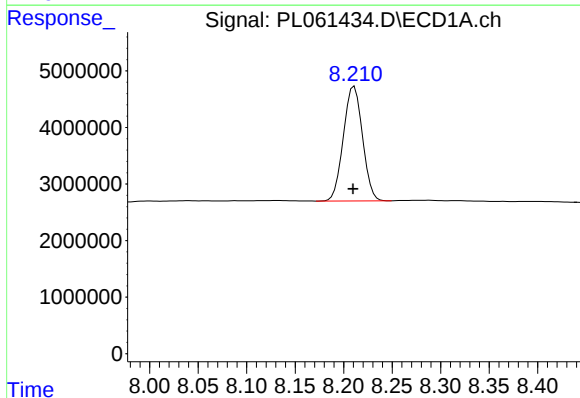

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.001 min
Response: 27793916
Conc: 16.66 ng/ml

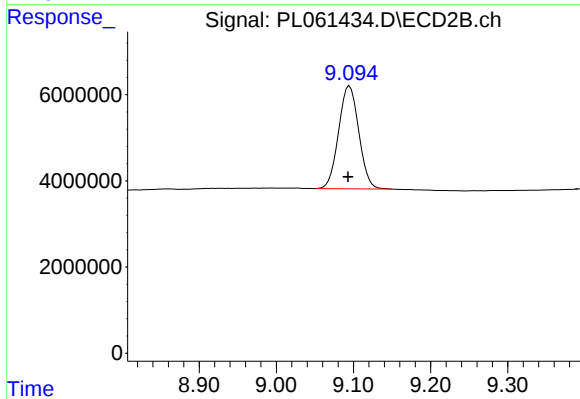

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.002 min
Response: 43370008
Conc: 18.34 ng/ml