

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
 Data File : PL061437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2020 18:52
 Operator : DD\AJ
 Sample : L3786-11
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 129

Manual Integrations
 APPROVED

Ankita
 9/15/2020 10:16:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:33:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	35166733	56002020	20.390	18.206
28)	SA Decachlor...	8.209	9.095	29085477	43974081	17.434m	18.597

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091420\
Data File : PL061437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2020 18:52
Operator : DD\AJ
Sample : L3786-11
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
129


Manual Integrations
APPROVED

Ankita
9/15/2020 10:16:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:33:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

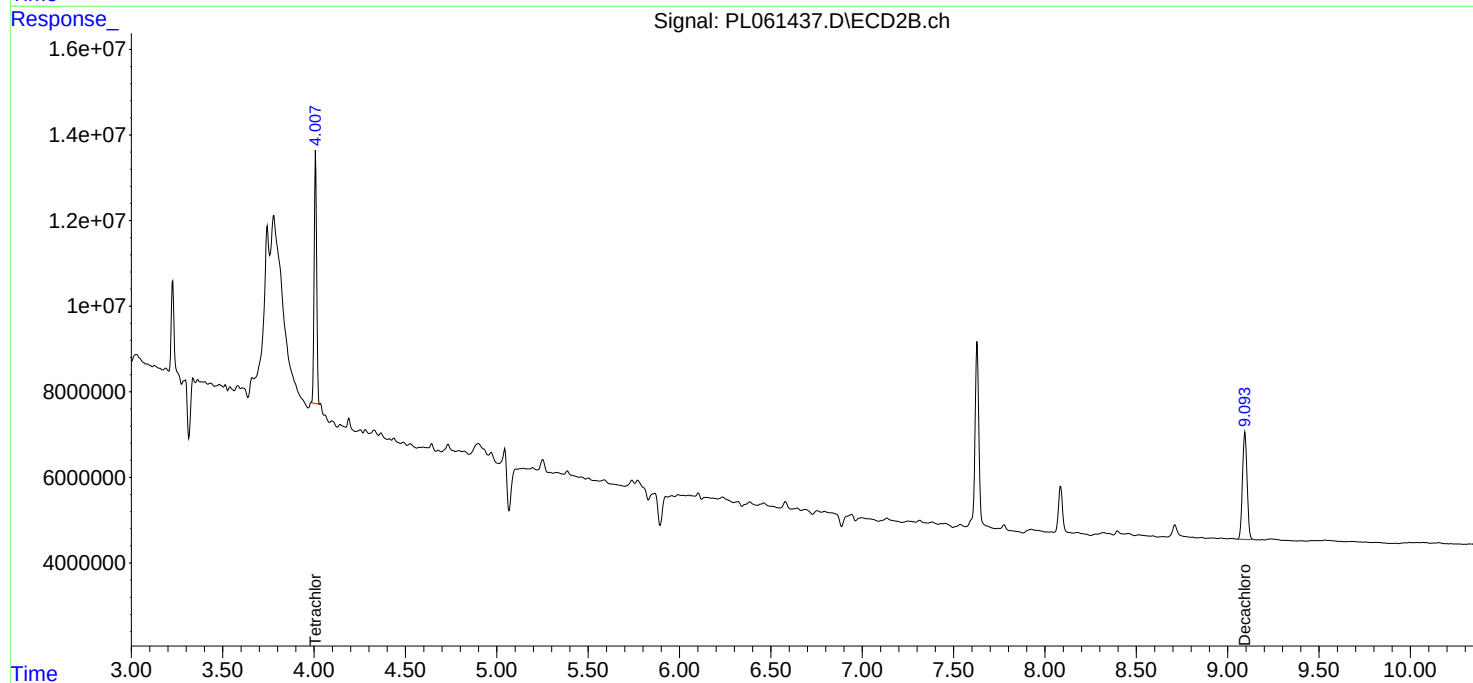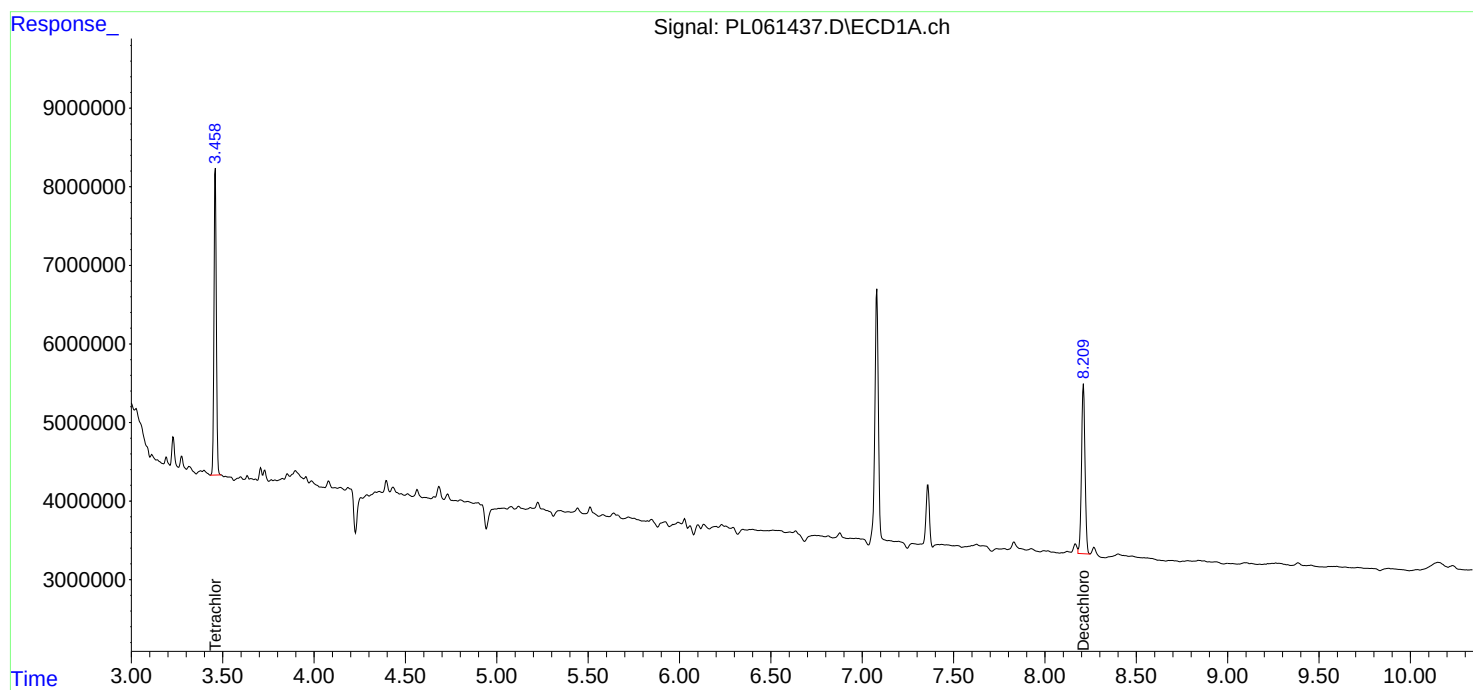

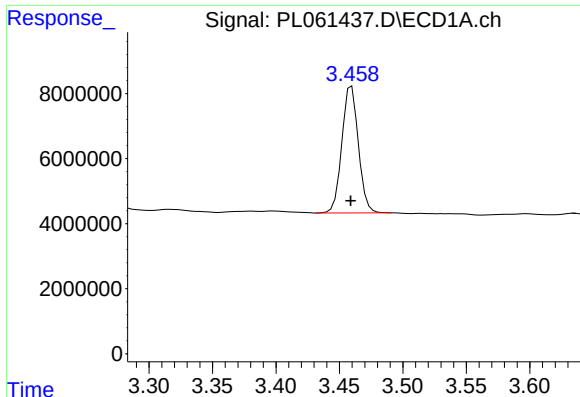


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 35166733
Conc: 20.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
129


Manual Integrations
APPROVED

Ankita
9/15/2020 10:16:12 AM

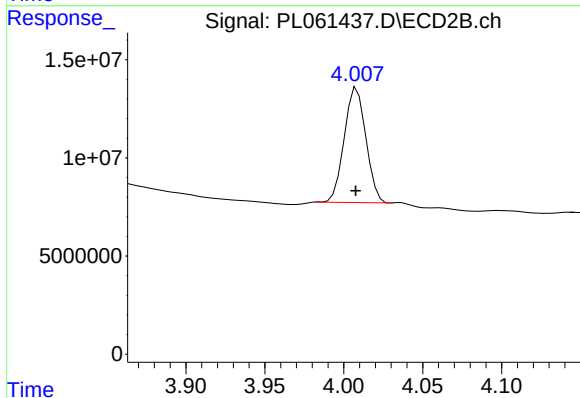


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 56002020
Conc: 18.21 ng/ml

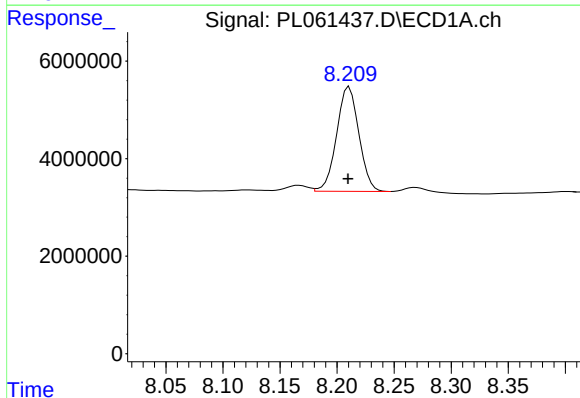

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 29085477
Conc: 17.43 ng/ml m

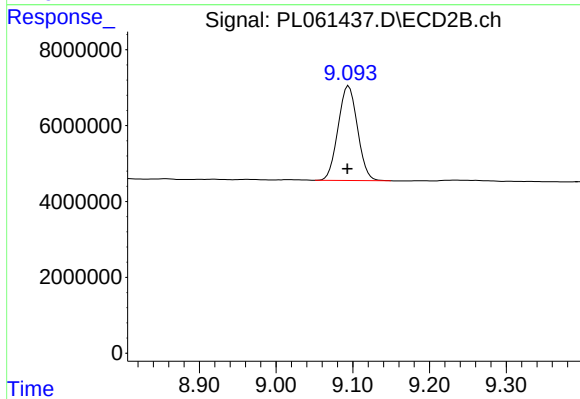

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.002 min
Response: 43974081
Conc: 18.60 ng/ml