

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091421\
 Data File : PL069833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2021 10:51
 Operator : AR\AJ
 Sample : M3686-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MAIN-GUARD-HOUSE-JET-GROUT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 13:07:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.631	5.566	9337790	28040008	22.920	23.036
28) SA Decachlor...	10.399	11.491	11845376	19141637	16.085	16.752

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091421\
Data File : PL069833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2021 10:51
Operator : AR\AJ
Sample : M3686-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MAIN-GUARD-HOUSE-JET-GROUT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 13:07:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

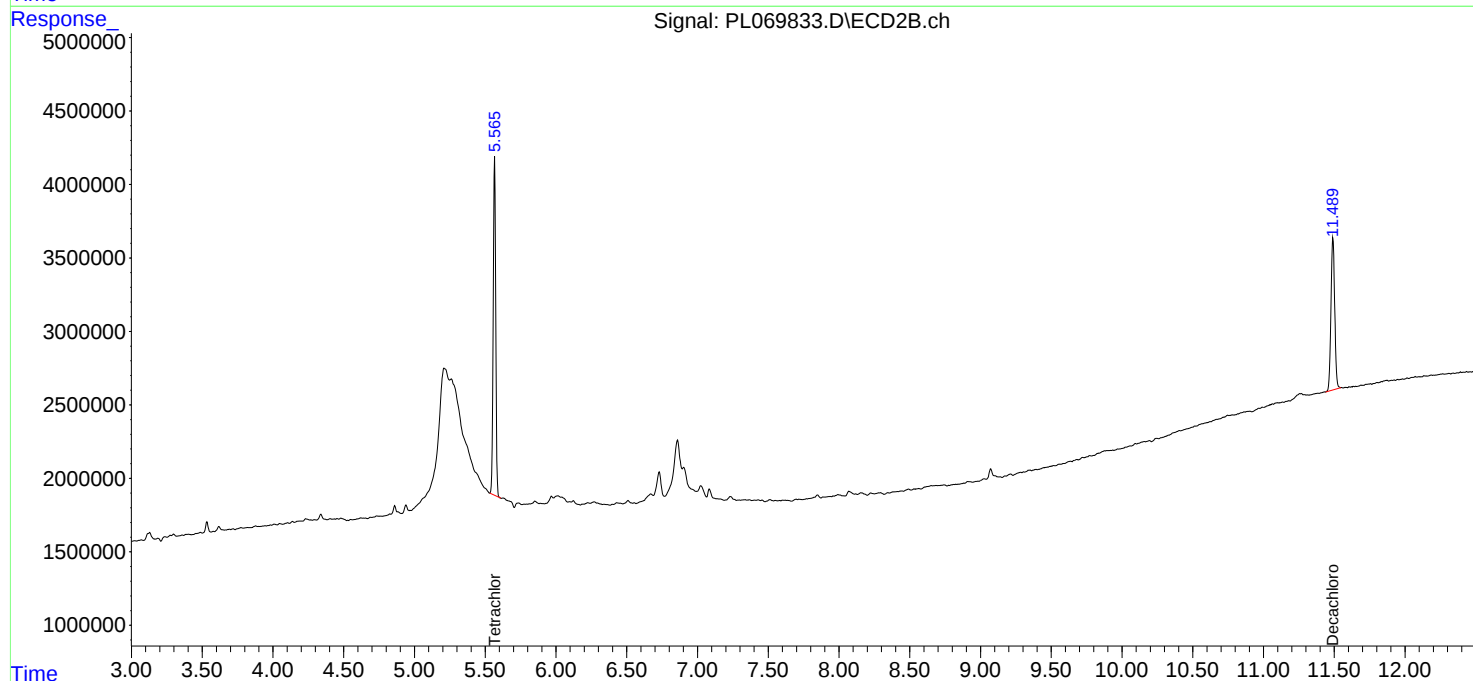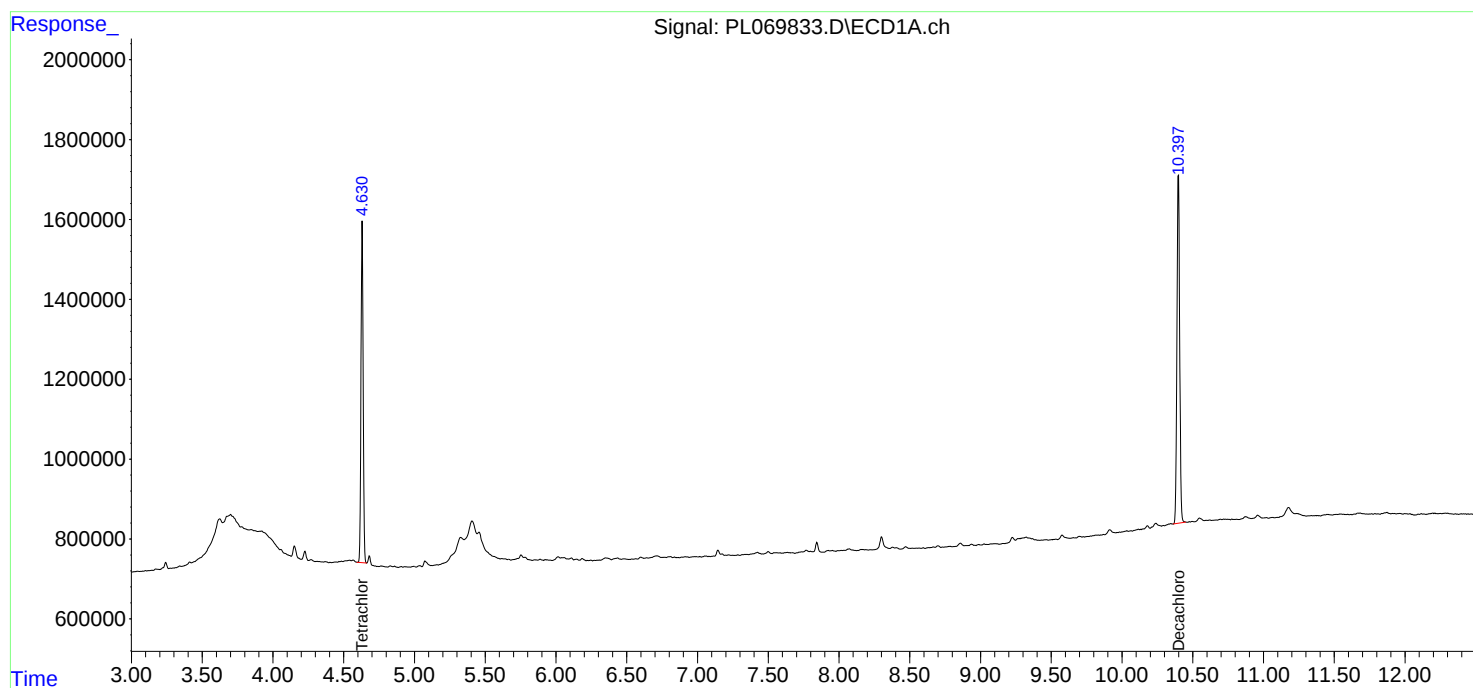


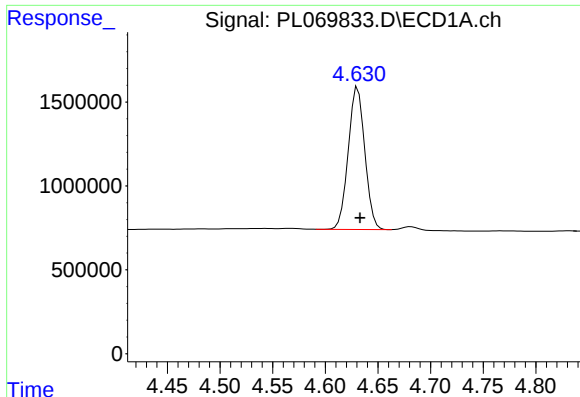

#1 Tetrachloro-m-xylene


R.T.: 4.631 min
Delta R.T.: -0.002 min
Response: 9337790
Conc: 22.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
MAIN-GUARD-HOUSE-JET-GROUT

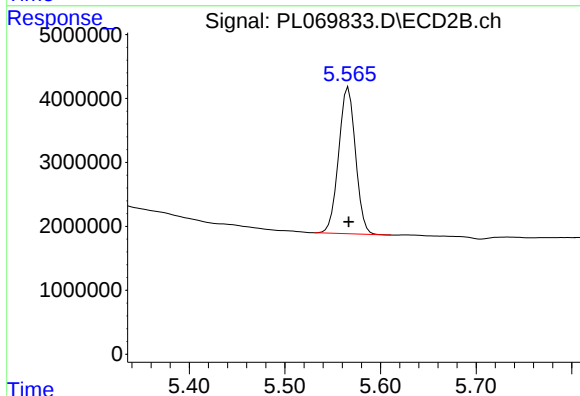


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 28040008
Conc: 23.04 ng/ml

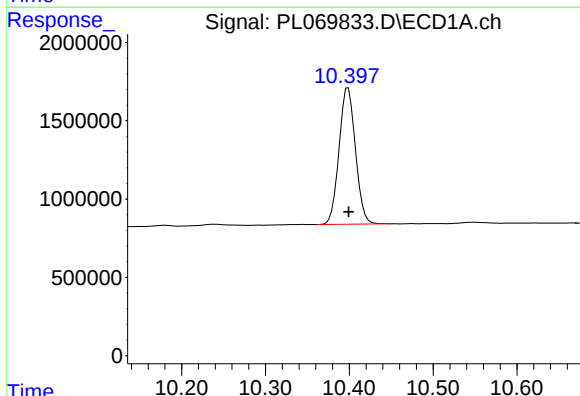

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: 0.000 min
Response: 11845376
Conc: 16.08 ng/ml

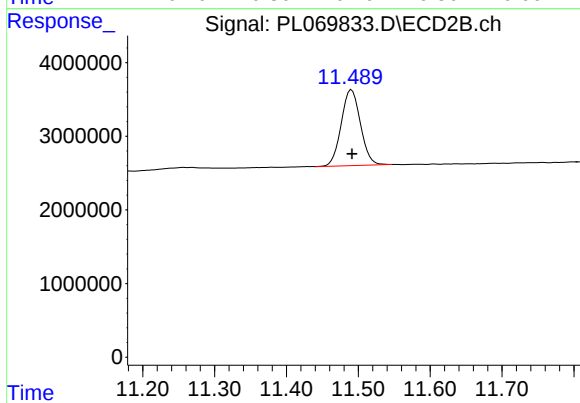

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.000 min
Response: 19141637
Conc: 16.75 ng/ml