

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091422\
 Data File : PL077726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 09:37
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 16:05:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.627	37013231	69050091	23.090	23.259
28)	SA Decachlor...	8.908	7.727	30148434	52121538	23.327	20.764
Target Compounds							
2)	A alpha-BHC	3.882	3.120	25388044	52875345	10.698	11.659
3)	MA gamma-BHC...	4.218	3.443	24461473	46703038	11.056	11.565
6)	B beta-BHC	4.430	3.743	11418161	20234337	11.749	12.154
7)	B delta-BHC	4.673	0.000	101363	0	0.049	N.D. #
8)	B Heptachlo...	5.570	0.000	13414558	0	7.695	N.D. #
10)	B gamma-Chl...	5.806f	0.000	2755056	0	1.574	N.D. #
11)	B alpha-Chl...	5.893	0.000	2766321	0	1.602	N.D. #
13)	MA Dieldrin	0.000	5.178	0	8331271	N.D.	2.513 #
14)	MA Endrin	6.463	5.450	74310108	152.0E6	53.731	53.304
15)	B Endosulfa...	6.708f	5.771f	1406584	147507	1.018	0.056 #
16)	A 4,4'-DDD	6.604	5.608	3297671	8013931	2.816	3.093
17)	MA 4,4'-DDT	6.915	5.856	138.5E6	277.3E6	109.322	105.251
18)	B Endrin al...	6.822	5.927	1813557	4425277	1.715	2.144 #
20)	A Methoxychlor	7.397	6.434	180.6E6	337.7E6	273.490	246.600
21)	B Endrin ke...	7.543	6.648	4247629	19632803	3.074	6.483 #
24)	Chlordane-2	0.000	4.169	0	2081034	N.D.	17.372 #
25)	Chlordane-3	5.806	0.000	2755056	0	11.187	N.D. #
26)	Chlordane-4	5.893	0.000	2766321	0	9.296	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091422\
Data File : PL077726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 09:37
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 16:05:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

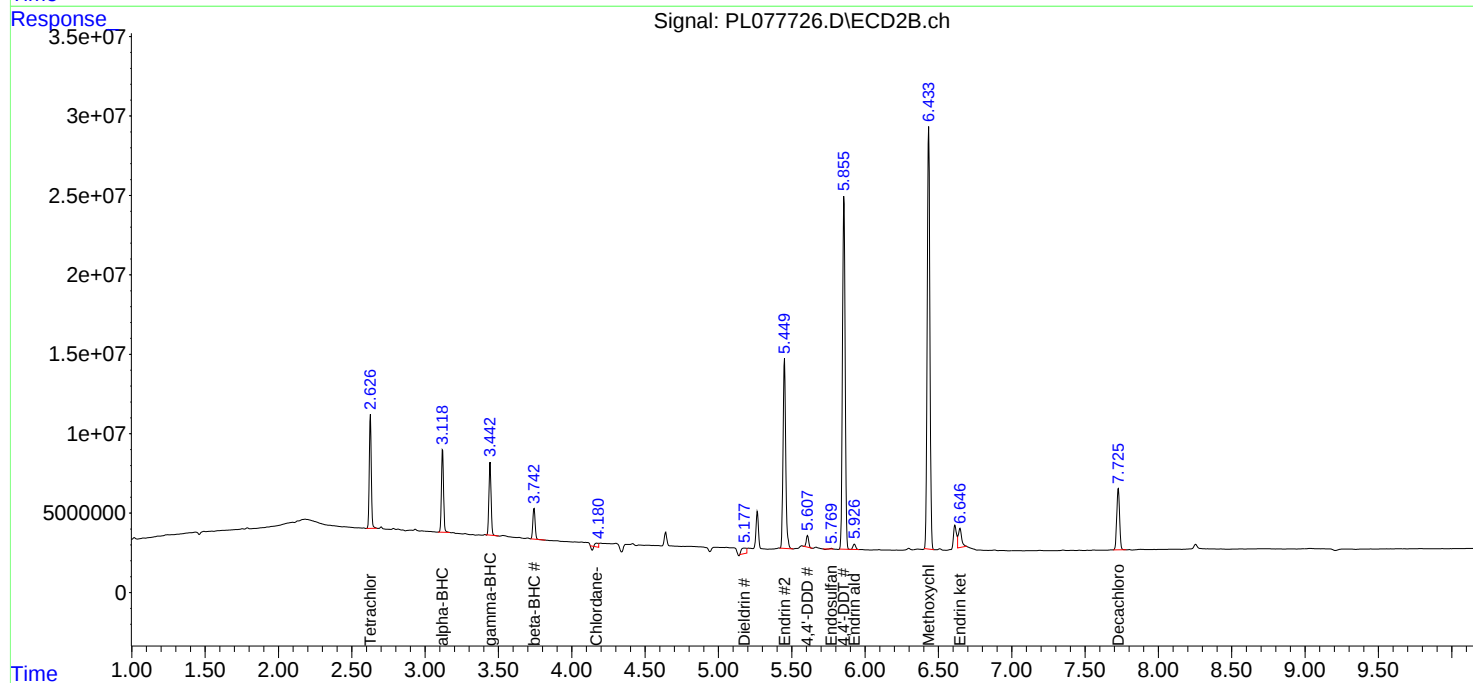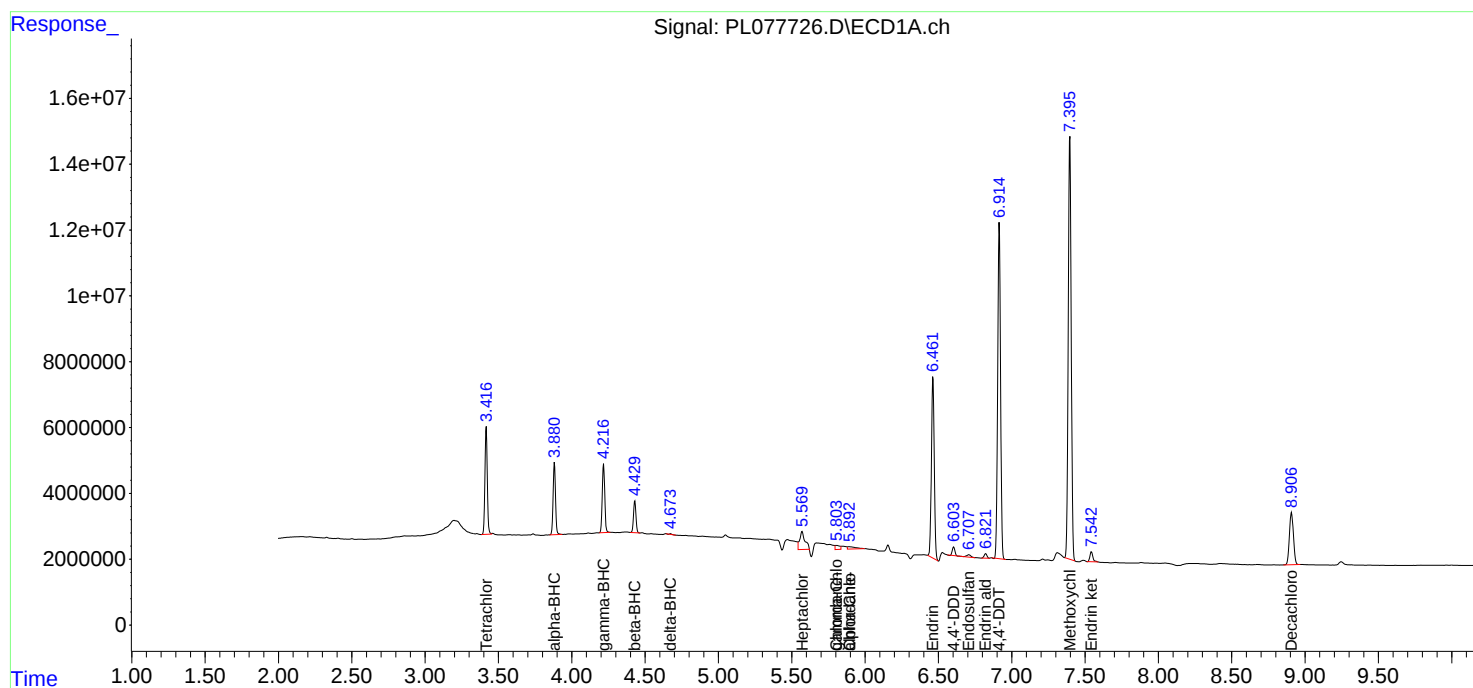


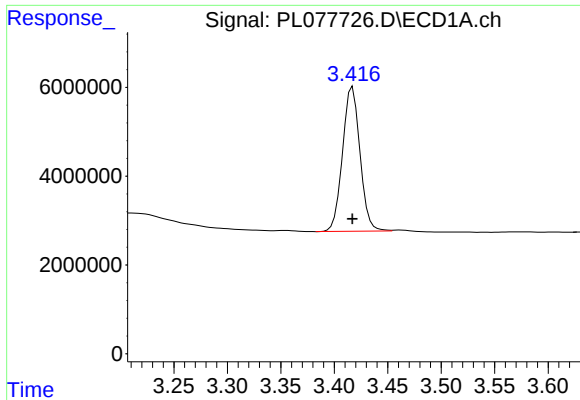

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 37013231
Conc: 23.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

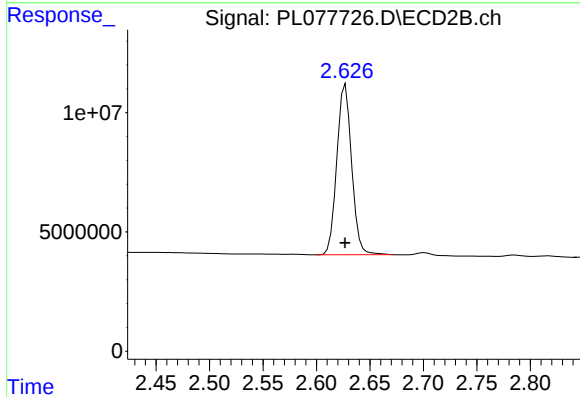


#1 Tetrachloro-m-xylene

R.T.: 2.627 min
Delta R.T.: 0.000 min
Response: 69050091
Conc: 23.26 ng/ml

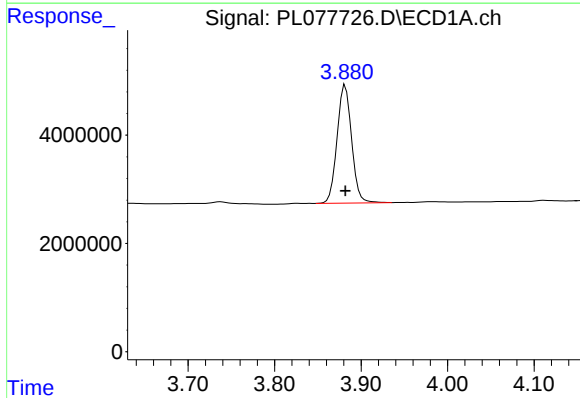


#2 alpha-BHC

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 25388044
Conc: 10.70 ng/ml

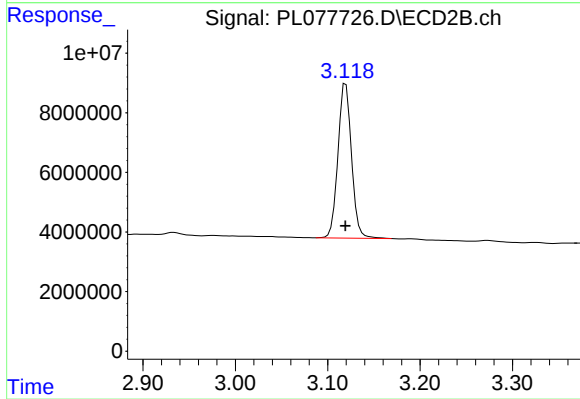

#2 alpha-BHC


R.T.: 3.120 min
Delta R.T.: 0.000 min
Response: 52875345
Conc: 11.66 ng/ml

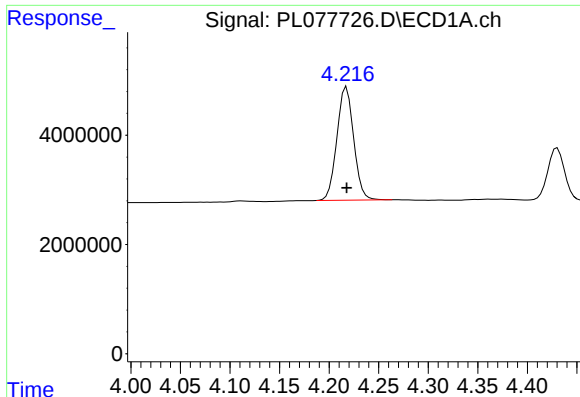

#3 gamma-BHC (Lindane)


R.T.: 4.218 min
Delta R.T.: 0.000 min
Response: 24461473
Conc: 11.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

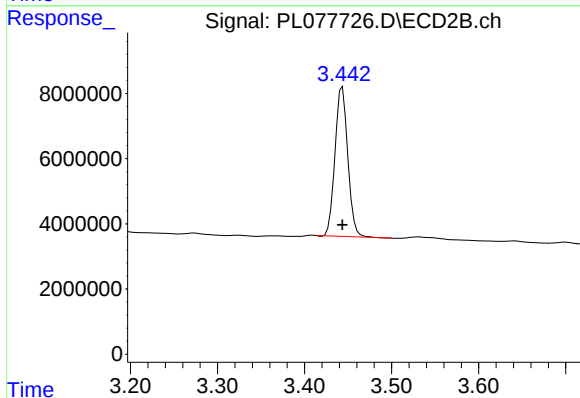


#3 gamma-BHC (Lindane)

R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 46703038
Conc: 11.57 ng/ml

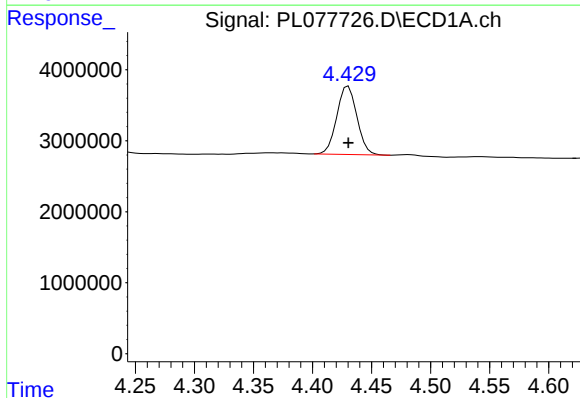


#6 beta-BHC

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 11418161
Conc: 11.75 ng/ml

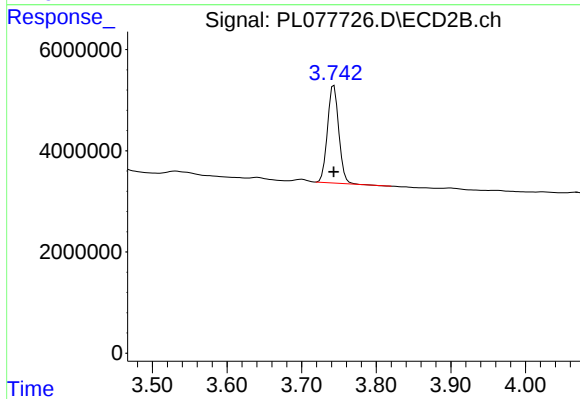

#6 beta-BHC


R.T.: 3.743 min
Delta R.T.: 0.000 min
Response: 20234337
Conc: 12.15 ng/ml

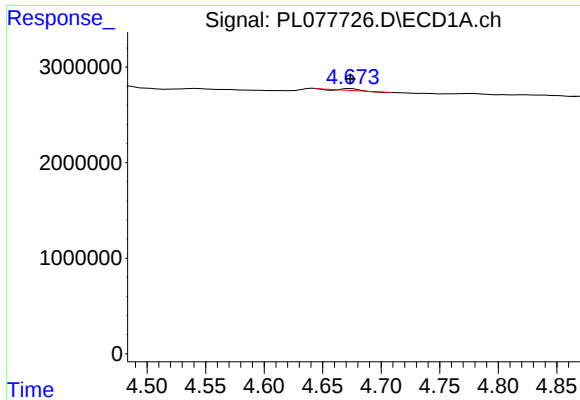

#7 delta-BHC


R.T.: 4.673 min
Delta R.T.: 0.000 min
Response: 101363
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

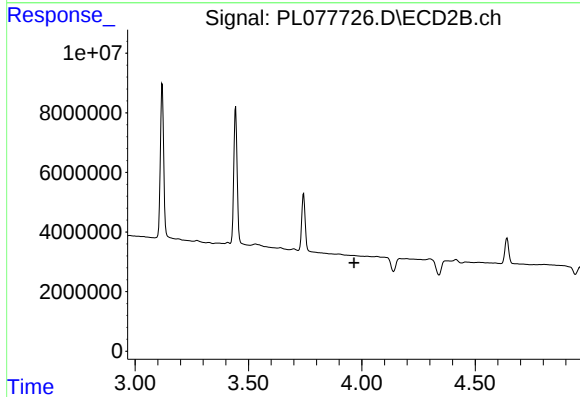


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

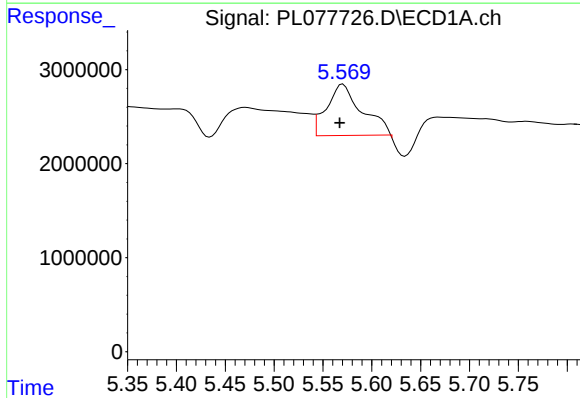


#8 Heptachlor epoxide

R.T.: 5.570 min
Delta R.T.: 0.003 min
Response: 13414558
Conc: 7.69 ng/ml

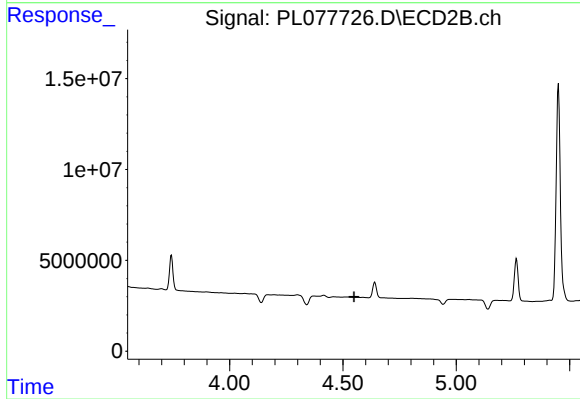

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

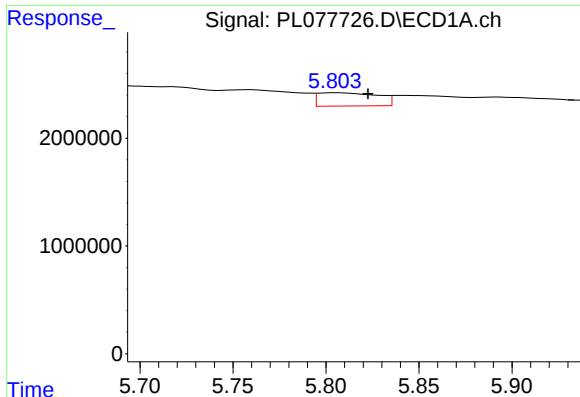

#10 gamma-Chlordane


R.T.: 5.806 min
Delta R.T.: -0.017 min
Response: 2755056
Conc: 1.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

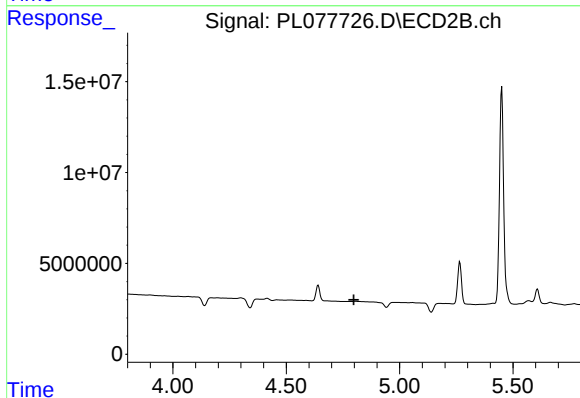


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

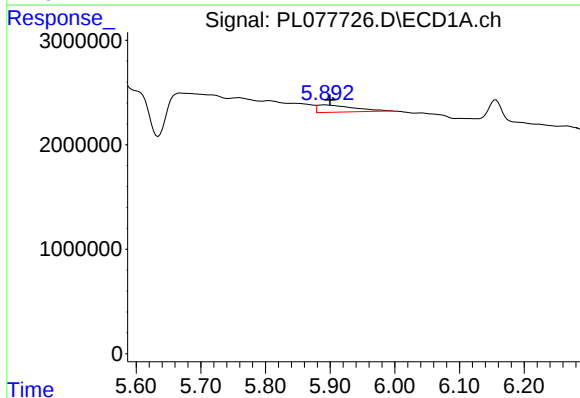


#11 alpha-Chlordane

R.T.: 5.893 min
Delta R.T.: -0.007 min
Response: 2766321
Conc: 1.60 ng/ml

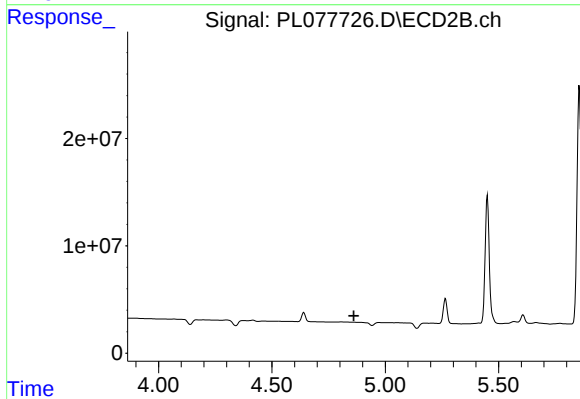

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.861 min
Response: 0
Conc: N.D.

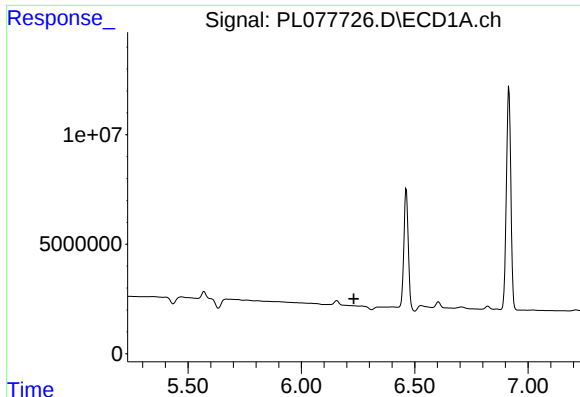

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

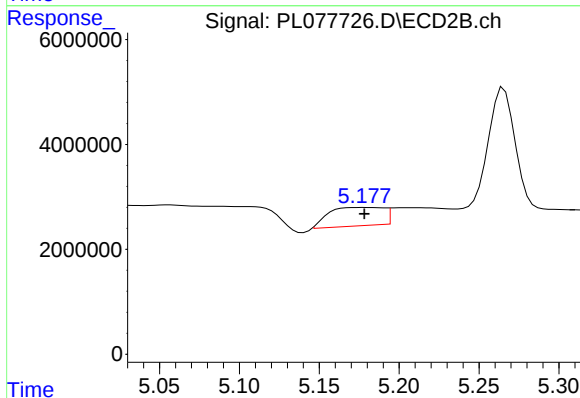


#13 Dieldrin

R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 8331271
Conc: 2.51 ng/ml

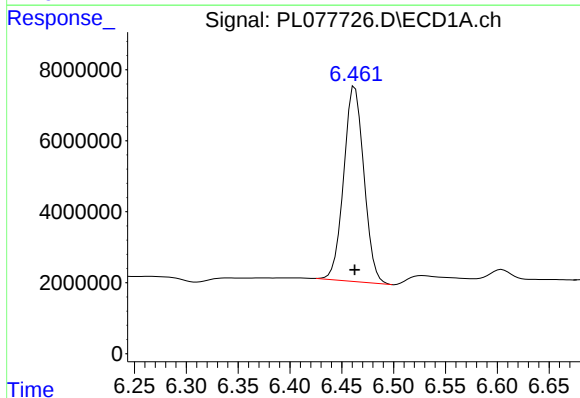


#14 Endrin

R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 74310108
Conc: 53.73 ng/ml

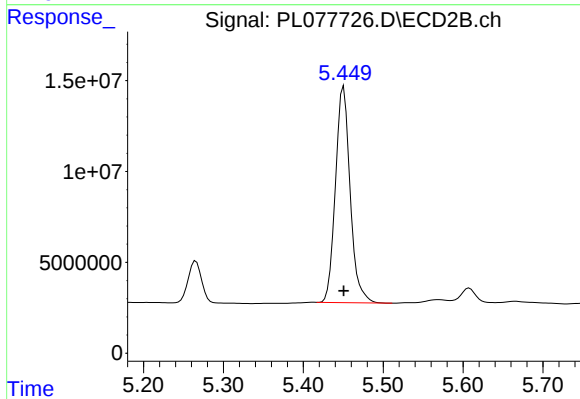

#14 Endrin


R.T.: 5.450 min
Delta R.T.: 0.000 min
Response: 151994433
Conc: 53.30 ng/ml

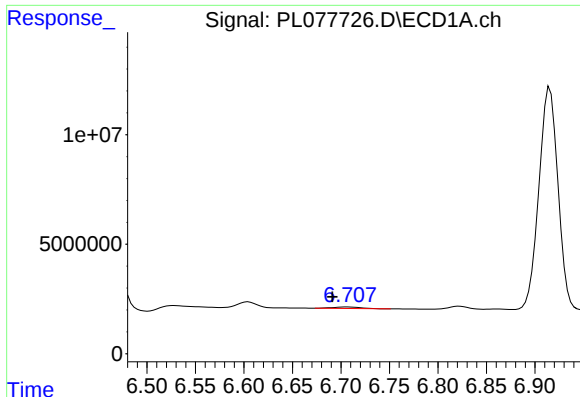

#15 Endosulfan II


R.T.: 6.708 min
Delta R.T.: 0.016 min
Response: 1406584
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

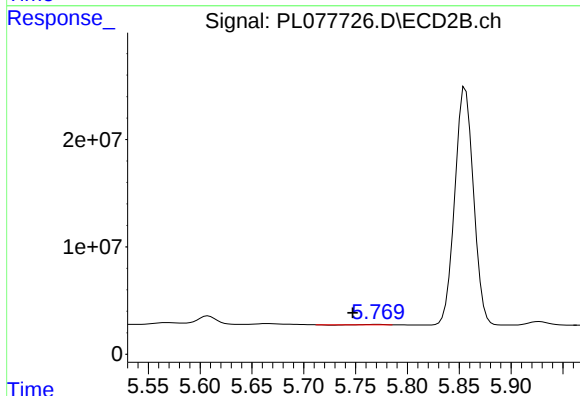


#15 Endosulfan II

R.T.: 5.771 min
Delta R.T.: 0.023 min
Response: 147507
Conc: 0.06 ng/ml

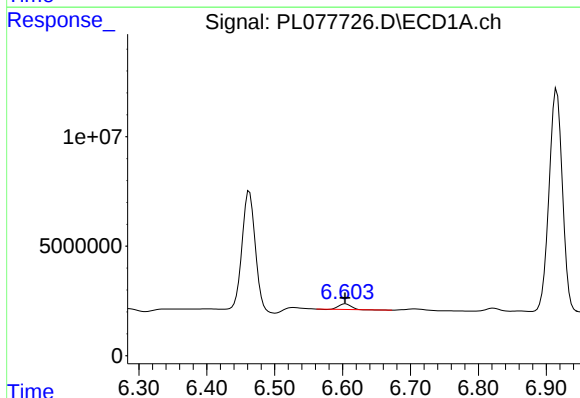


#16 4,4'-DDD

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 3297671
Conc: 2.82 ng/ml

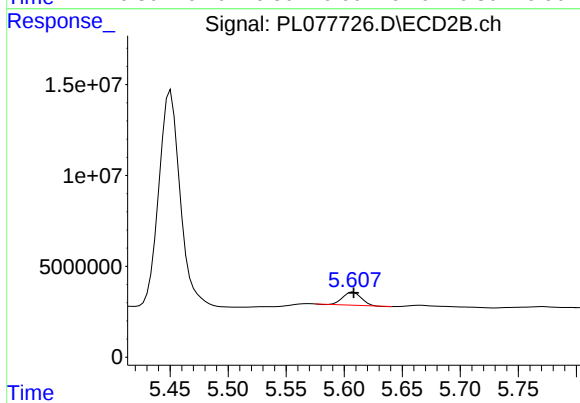

#16 4,4'-DDD


R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 8013931
Conc: 3.09 ng/ml

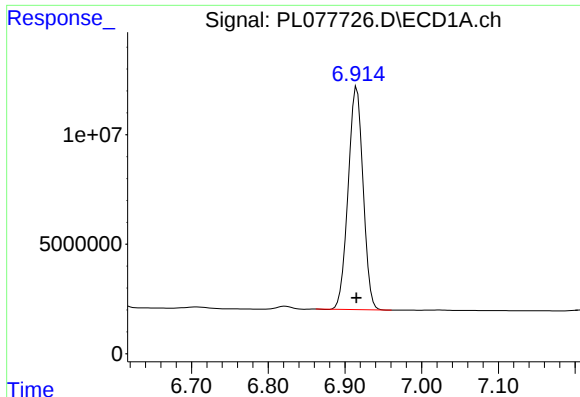

#17 4,4'-DDT


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 138525602
Conc: 109.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

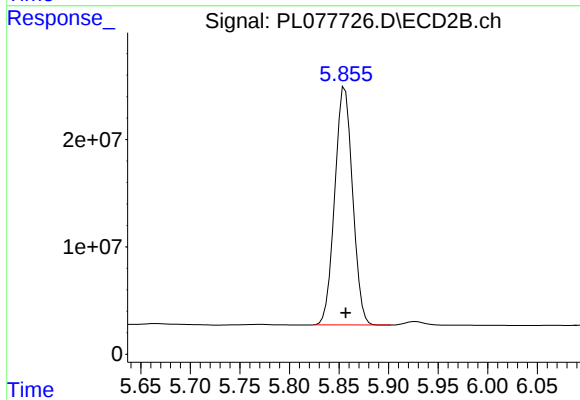


#17 4,4'-DDT

R.T.: 5.856 min
Delta R.T.: 0.000 min
Response: 277315078
Conc: 105.25 ng/ml

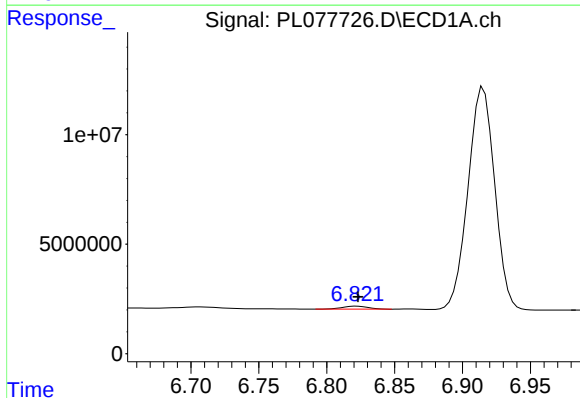


#18 Endrin aldehyde

R.T.: 6.822 min
Delta R.T.: 0.000 min
Response: 1813557
Conc: 1.71 ng/ml

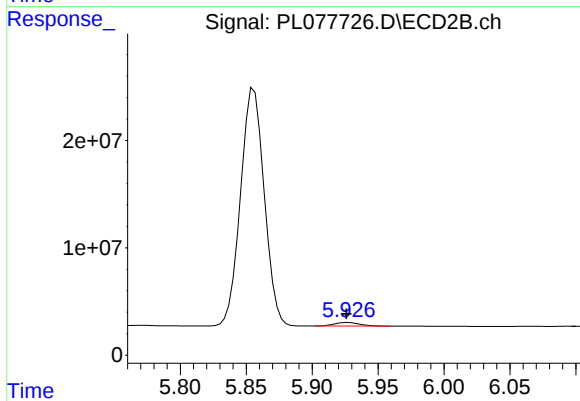

#18 Endrin aldehyde


R.T.: 5.927 min
Delta R.T.: 0.001 min
Response: 4425277
Conc: 2.14 ng/ml

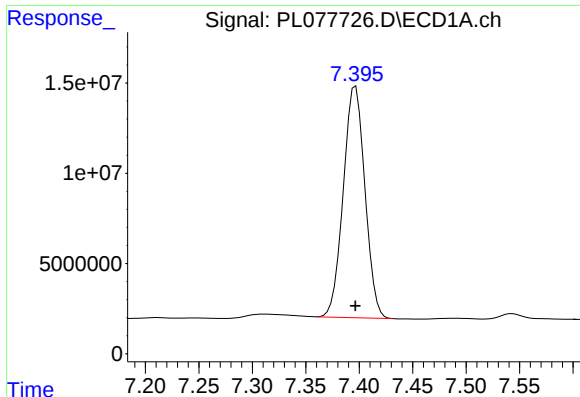

#20 Methoxychlor


R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 180626795
Conc: 273.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

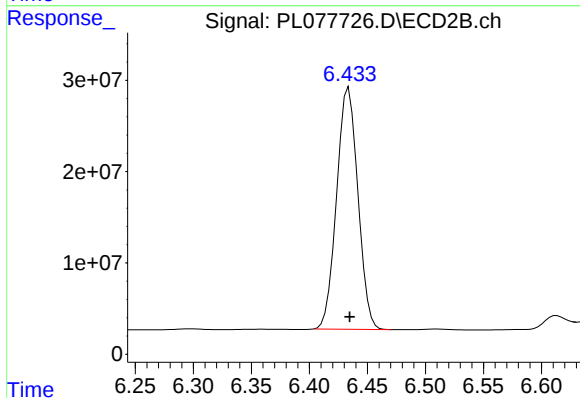


#20 Methoxychlor

R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 337700890
Conc: 246.60 ng/ml

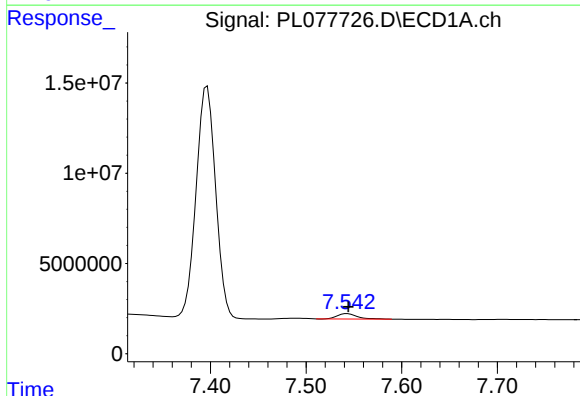


#21 Endrin ketone

R.T.: 7.543 min
Delta R.T.: -0.001 min
Response: 4247629
Conc: 3.07 ng/ml

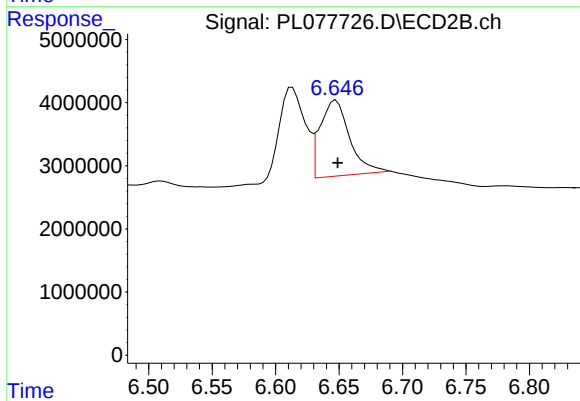

#21 Endrin ketone


R.T.: 6.648 min
Delta R.T.: -0.001 min
Response: 19632803
Conc: 6.48 ng/ml

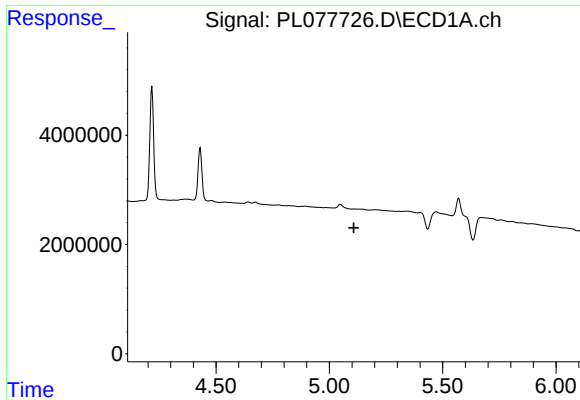

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

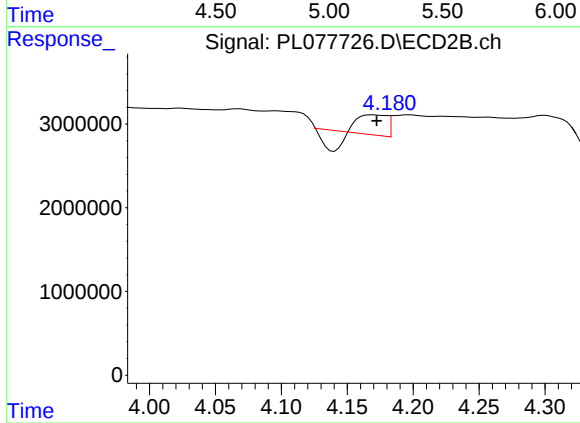


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: -0.003 min
Response: 2081034
Conc: 17.37 ng/ml

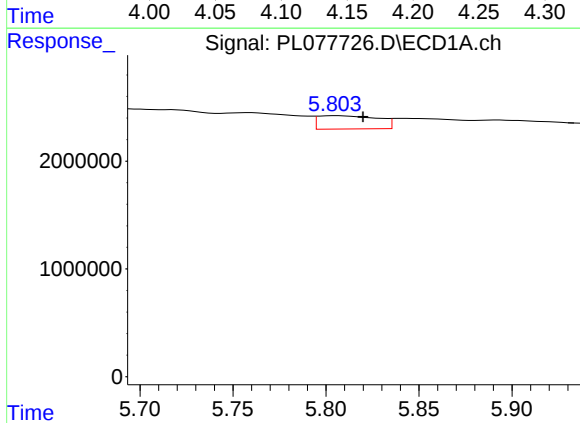


#25 Chlordane-3

R.T.: 5.806 min
Delta R.T.: -0.014 min
Response: 2755056
Conc: 11.19 ng/ml

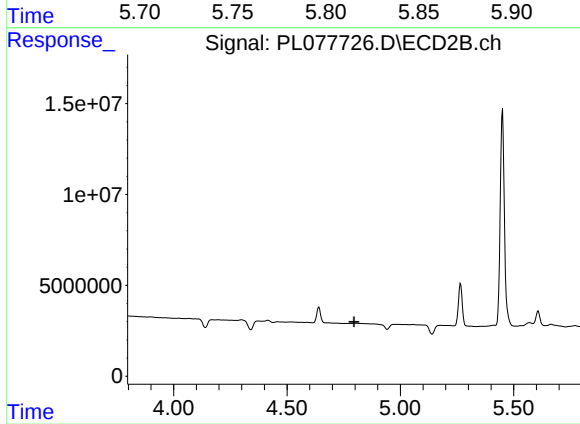

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 4.796 min
Response: 0
Conc: N.D.

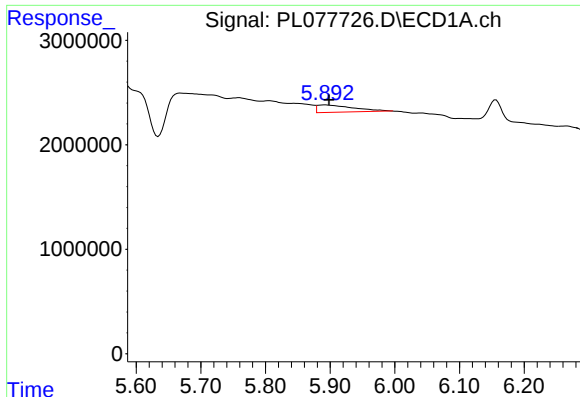

#26 Chlordane-4


R.T.: 5.893 min
Delta R.T.: -0.006 min
Response: 2766321
Conc: 9.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

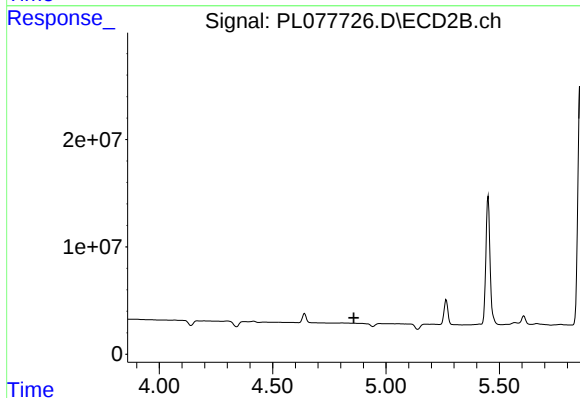


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 4.858 min
Response: 0
Conc: N.D.

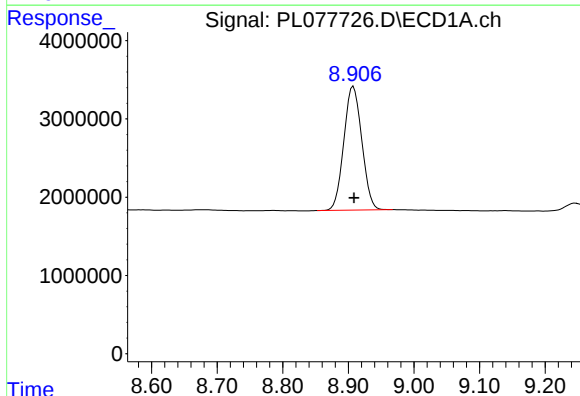

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: -0.001 min
Response: 30148434
Conc: 23.33 ng/ml

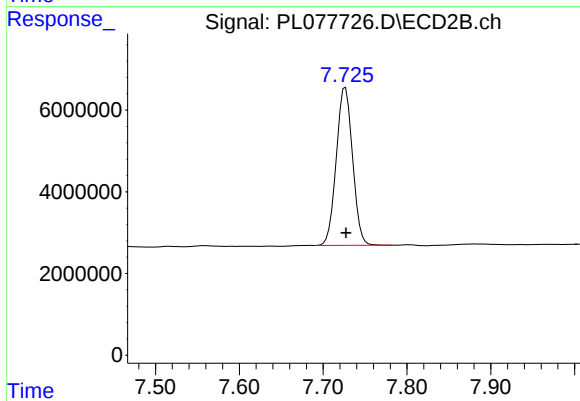

#28 Decachlorobiphenyl

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 52121538
Conc: 20.76 ng/ml