

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091422\
 Data File : PL077745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 14:42
 Operator : AR\AJ
 Sample : PB147632BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 16:08:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.627	27262199	50622064	17.007	17.052
28)	SA Decachlor...	8.910	7.727	25660365	43935407	19.854	17.503
Target Compounds							
7)	B delta-BHC	4.675	0.000	655387	0	0.319	N.D. #
8)	B Heptachlo...	5.573	0.000	2796689	0	1.604	N.D. #
11)	B alpha-Chl...	5.920f	0.000	559211	0	0.324	N.D. #
13)	MA Dieldrin	0.000	5.181	0	8998659	N.D.	2.714 #
14)	MA Endrin	0.000	5.474f	0	4148483	N.D.	1.455 #
15)	B Endosulfa...	6.708f	5.757	1361462	-53443	0.986	N.D. #
21)	B Endrin ke...	7.571f	0.000	635801	0	0.460	N.D. #
26)	Chlordane-4	5.920f	0.000	559211	0	1.879	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091422\
Data File : PL077745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 14:42
Operator : AR\AJ
Sample : PB147632BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 16:08:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

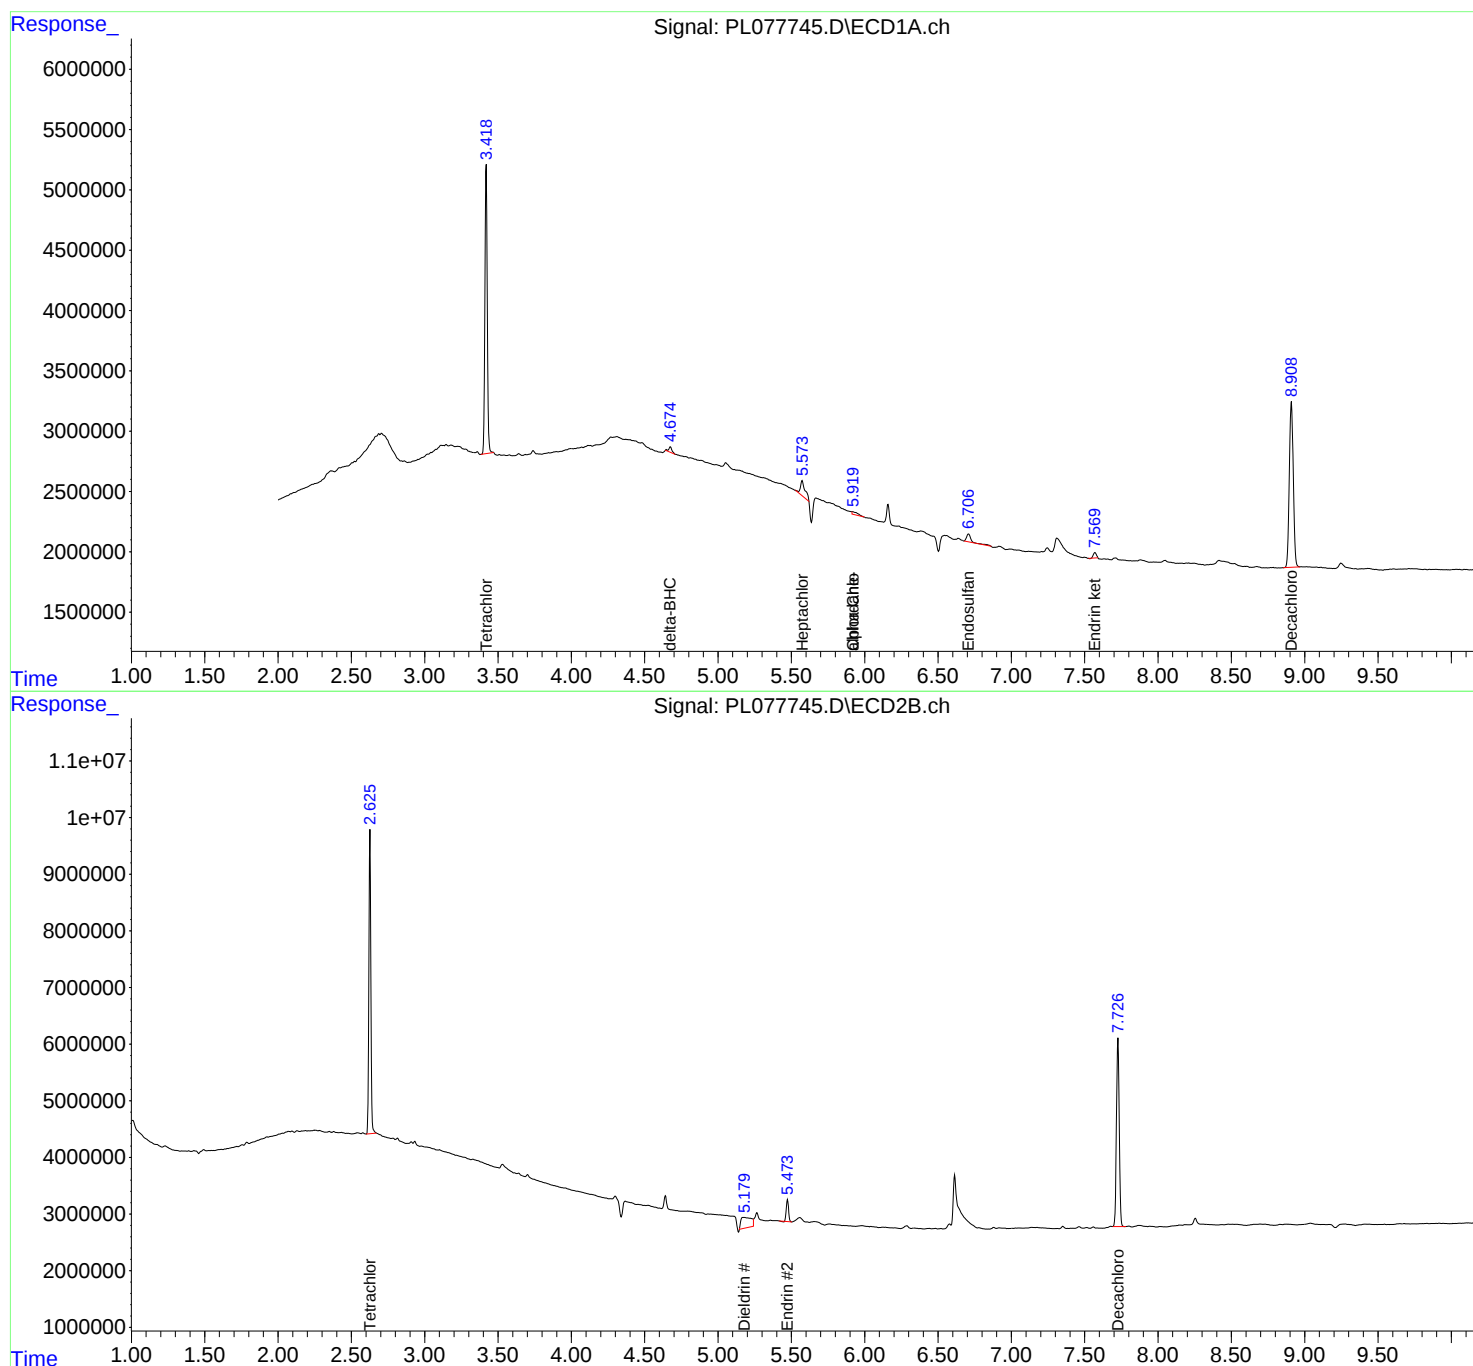


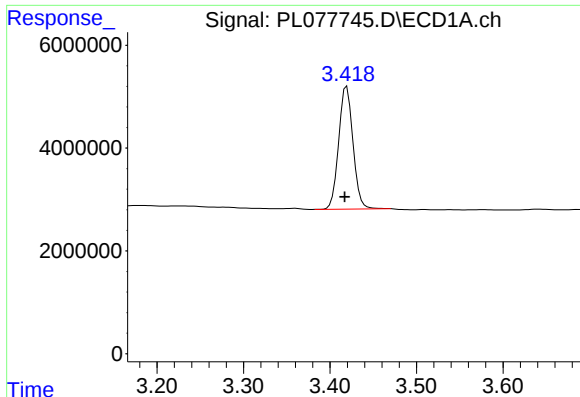

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.002 min
Response: 27262199
Conc: 17.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

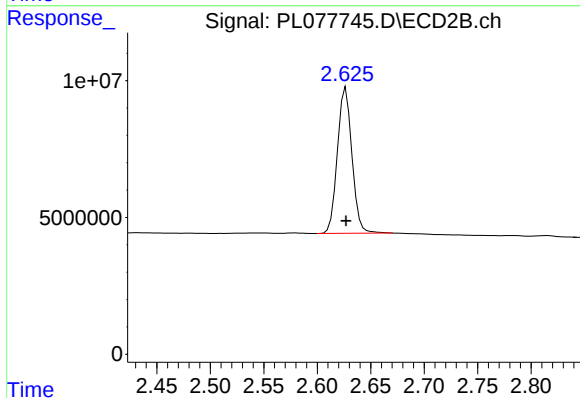


#1 Tetrachloro-m-xylene

R.T.: 2.627 min
Delta R.T.: 0.000 min
Response: 50622064
Conc: 17.05 ng/ml

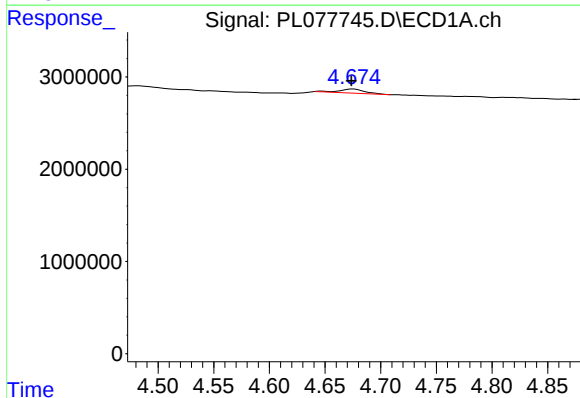


#7 delta-BHC

R.T.: 4.675 min
Delta R.T.: 0.002 min
Response: 655387
Conc: 0.32 ng/ml

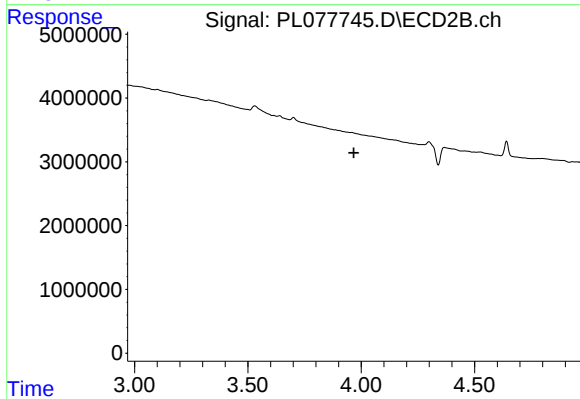

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

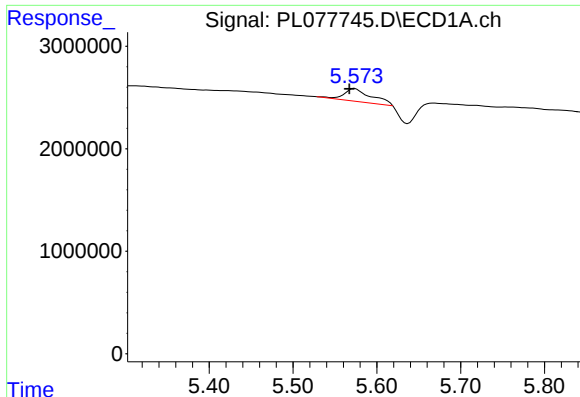

#8 Heptachlor epoxide


R.T.: 5.573 min
Delta R.T.: 0.006 min
Response: 2796689
Conc: 1.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

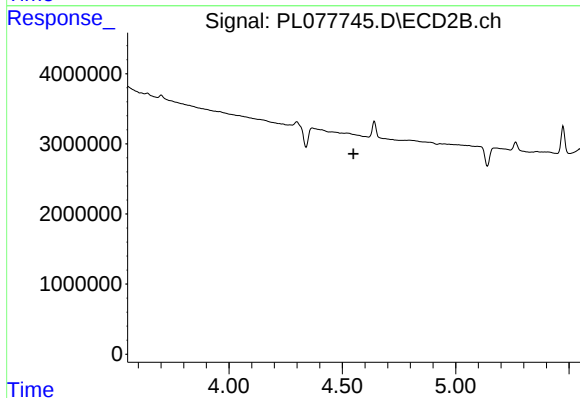


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

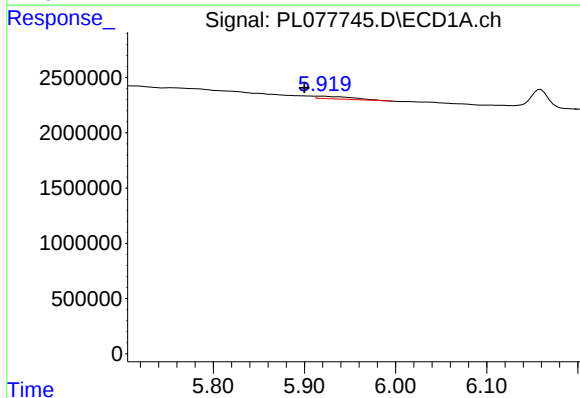


#11 alpha-Chlordane

R.T.: 5.920 min
Delta R.T.: 0.020 min
Response: 559211
Conc: 0.32 ng/ml

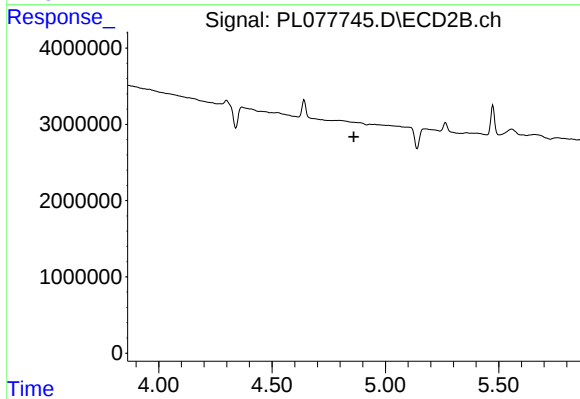

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.861 min
Response: 0
Conc: N.D.

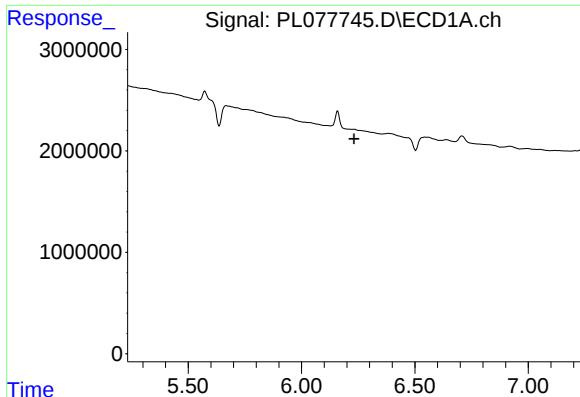

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

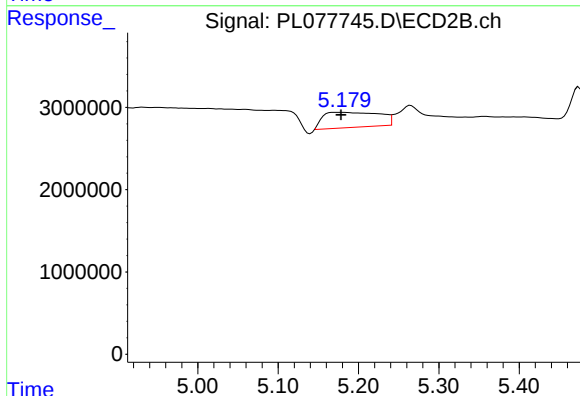


#13 Dieldrin

R.T.: 5.181 min
Delta R.T.: 0.003 min
Response: 8998659
Conc: 2.71 ng/ml

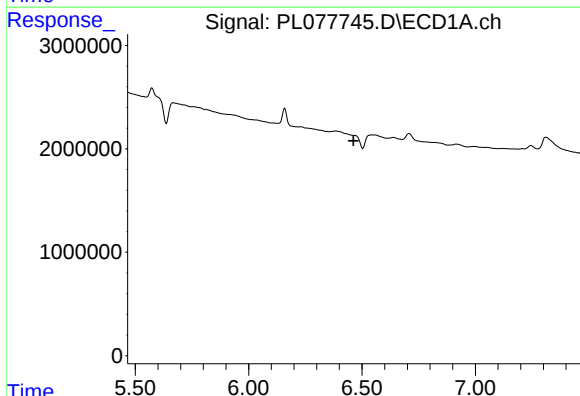


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

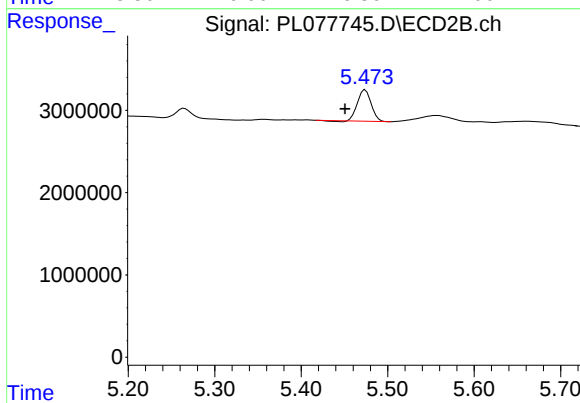

#14 Endrin


R.T.: 5.474 min
Delta R.T.: 0.024 min
Response: 4148483
Conc: 1.45 ng/ml

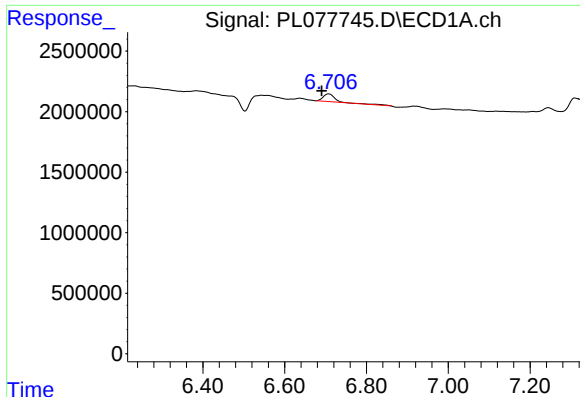

#15 Endosulfan II


R.T.: 6.708 min
Delta R.T.: 0.017 min
Response: 1361462
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

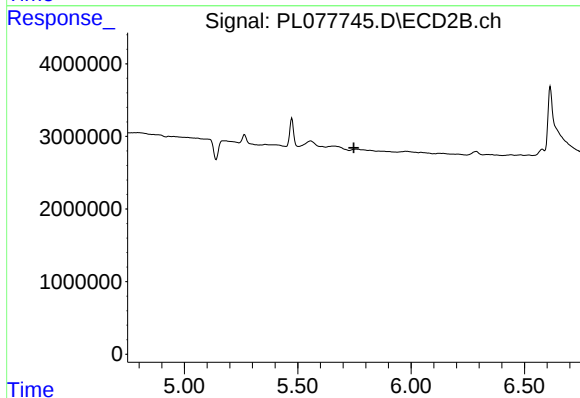


#15 Endosulfan II

R.T.: 5.757 min
Delta R.T.: 0.010 min
Response: -53443
Conc: N.D.

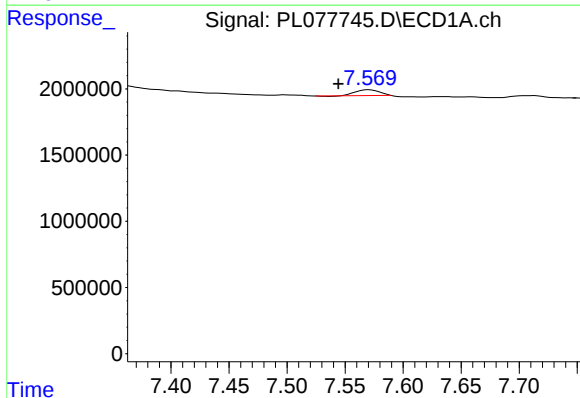


#21 Endrin ketone

R.T.: 7.571 min
Delta R.T.: 0.027 min
Response: 635801
Conc: 0.46 ng/ml

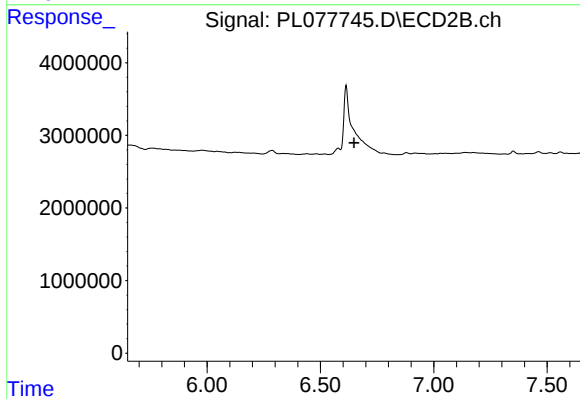

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

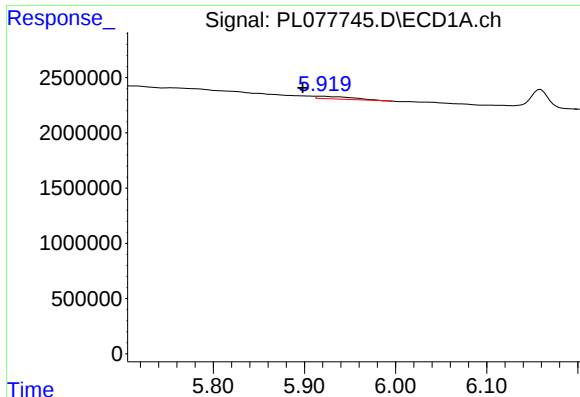

#26 Chlordane-4


R.T.: 5.920 min
Delta R.T.: 0.022 min
Response: 559211
Conc: 1.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

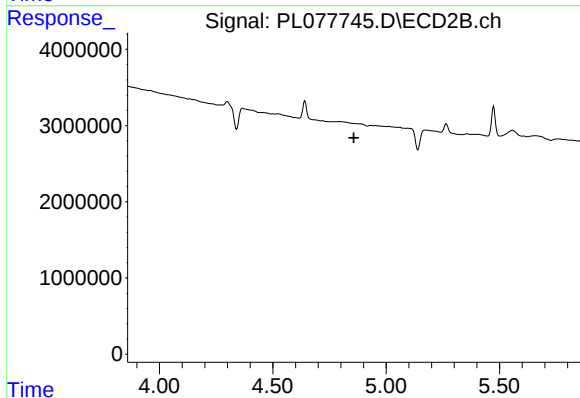


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 4.858 min
Response: 0
Conc: N.D.

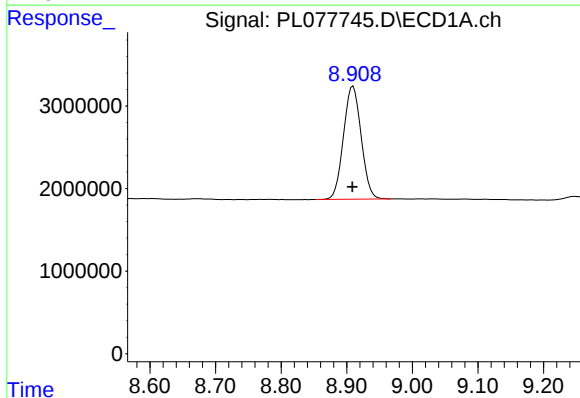

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: 0.001 min
Response: 25660365
Conc: 19.85 ng/ml

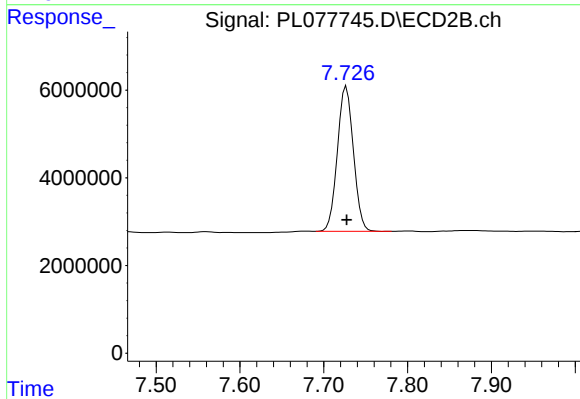

#28 Decachlorobiphenyl

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 43935407
Conc: 17.50 ng/ml