

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091422\
 Data File : PL077747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 15:35
 Operator : AR\AJ
 Sample : N4581-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRUSHED-MASONRY-PILE-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 18:09:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.424	2.626	31997950	59993988	19.961	20.209
28) SA Decachlor...	8.916	7.730	28408199	48168683	21.981	19.189

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091422\
Data File : PL077747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 15:35
Operator : AR\AJ
Sample : N4581-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CRUSHED-MASONRY-PILE-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 18:09:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

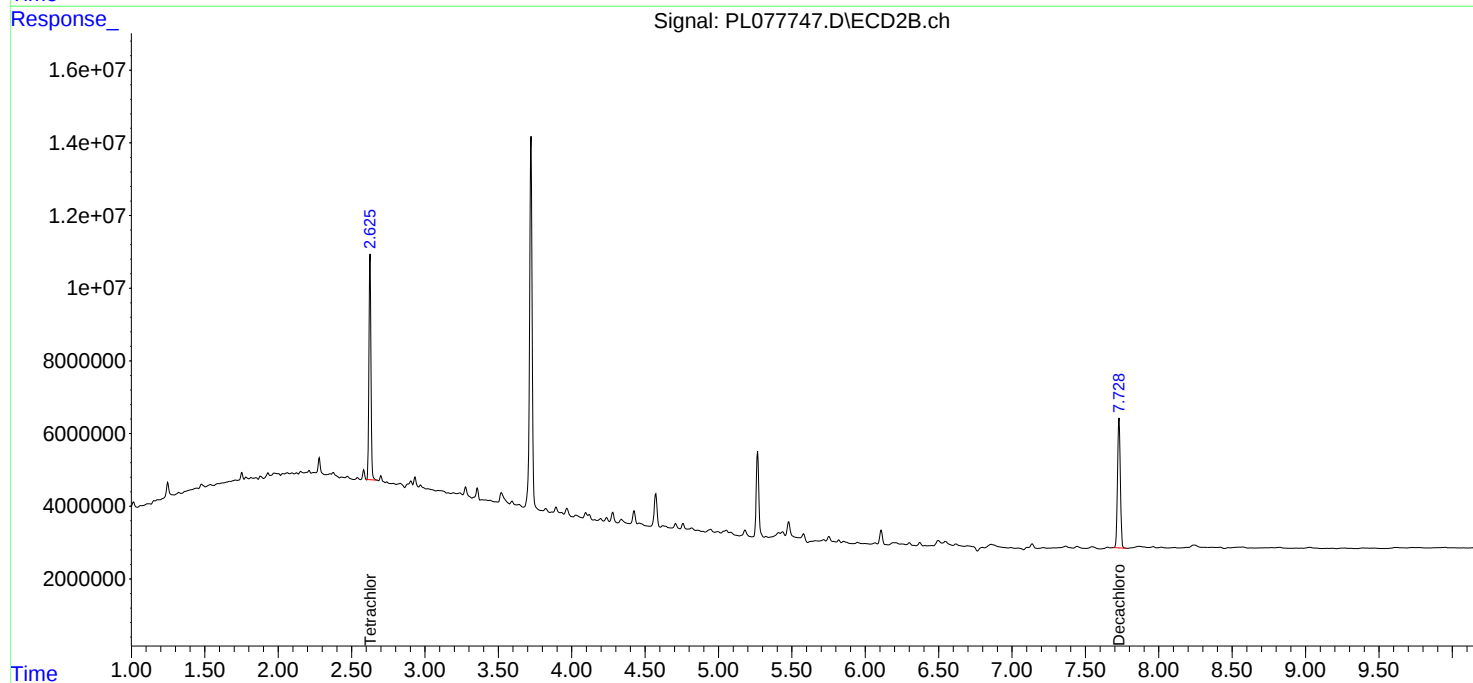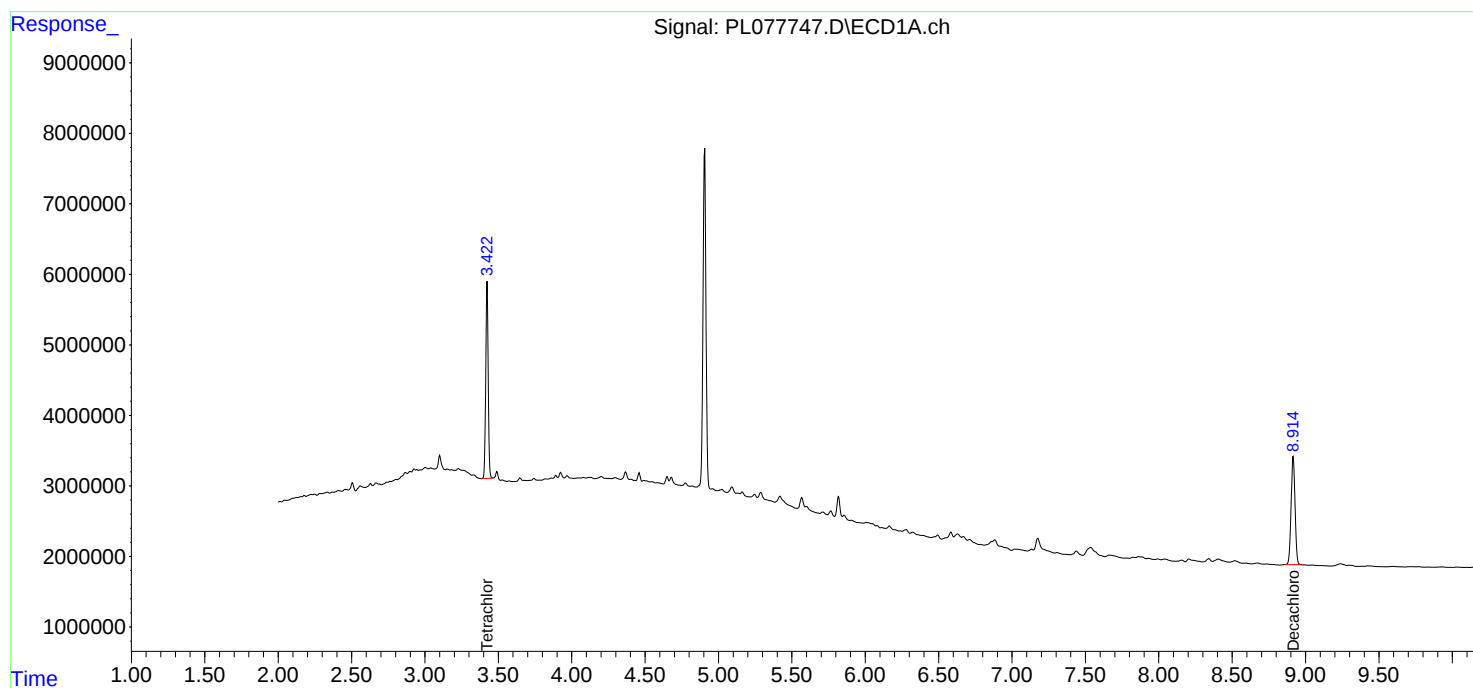


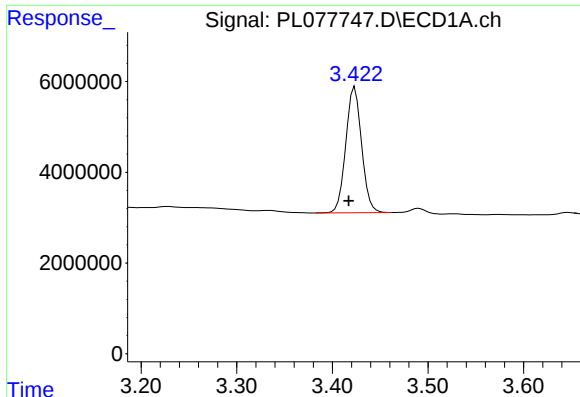

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: 0.007 min
Response: 31997950
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRUSHED-MASONRY-PILE-6

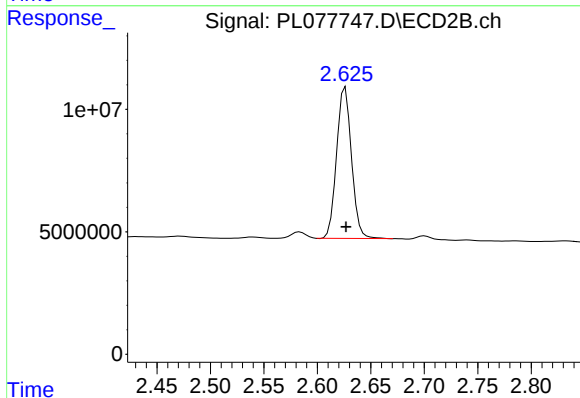


#1 Tetrachloro-m-xylene

R.T.: 2.626 min
Delta R.T.: 0.000 min
Response: 59993988
Conc: 20.21 ng/ml

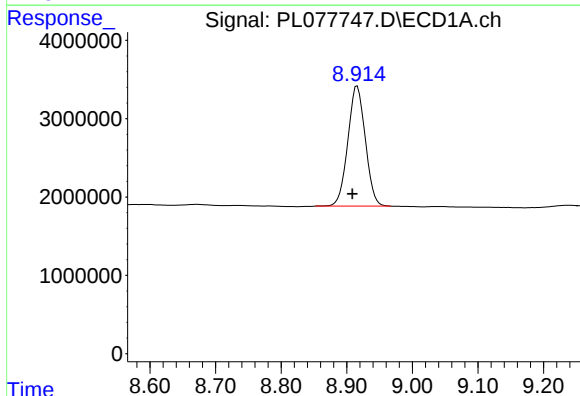

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.007 min
Response: 28408199
Conc: 21.98 ng/ml

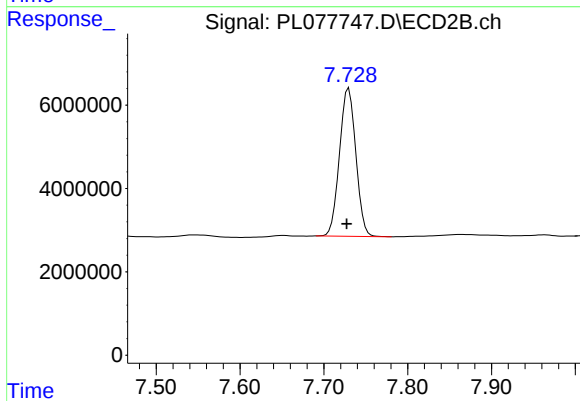

#28 Decachlorobiphenyl

R.T.: 7.730 min
Delta R.T.: 0.002 min
Response: 48168683
Conc: 19.19 ng/ml