

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091423\
 Data File : PL085318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2023 17:14
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 22:38:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.682	113.0E6	66926578	46.218	58.904 #
28)	SA Decachlor...	9.024	7.861	80272390	63499108	49.917	47.704
Target Compounds							
23)	Chlordane-1	4.643	3.683	49040300	19198302	492.831	494.026
24)	Chlordane-2	5.176	4.265	51071127	23488627	487.503	487.350
25)	Chlordane-3	5.890	4.897	176.2E6	66428771	487.566	494.710
26)	Chlordane-4	5.972	4.960	210.6E6	69530620	485.526	467.566
27)	Chlordane-5	6.822	5.858	34451998	24895053	493.452	489.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091423\
Data File : PL085318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2023 17:14
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 22:38:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

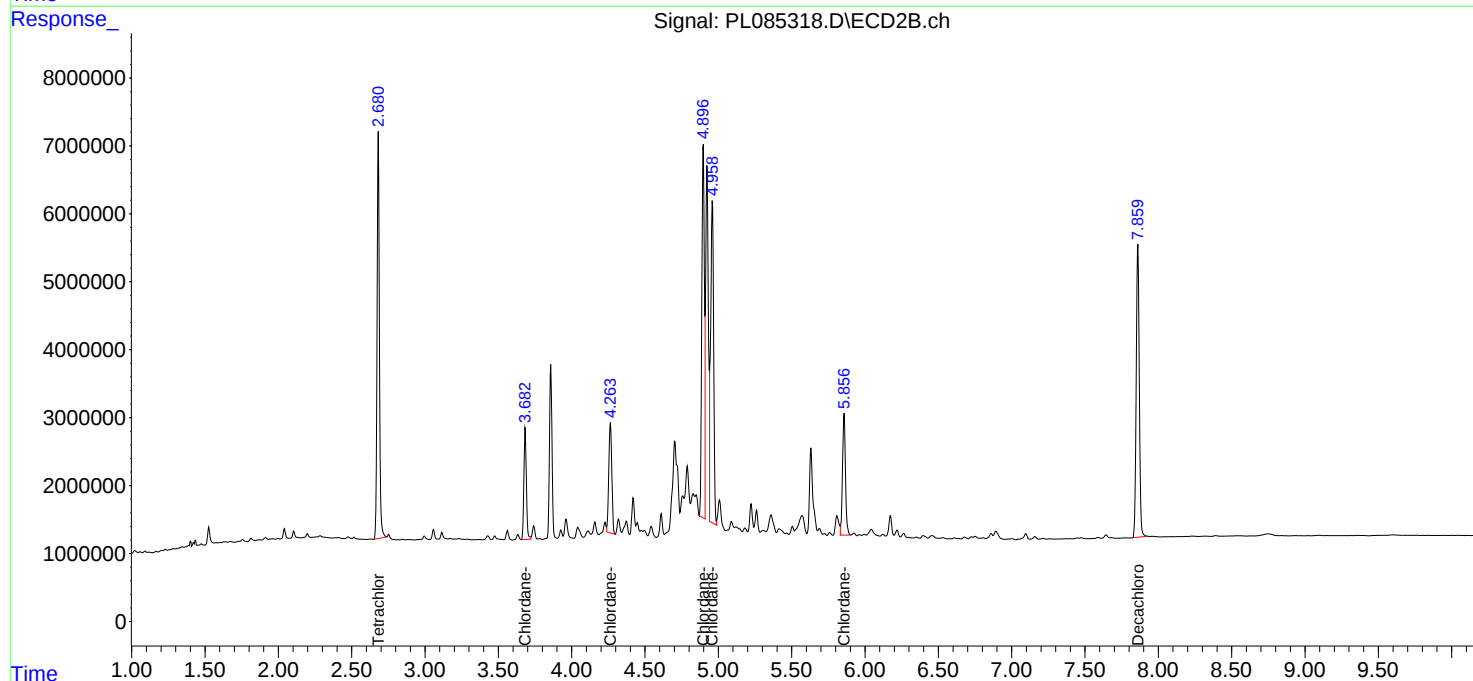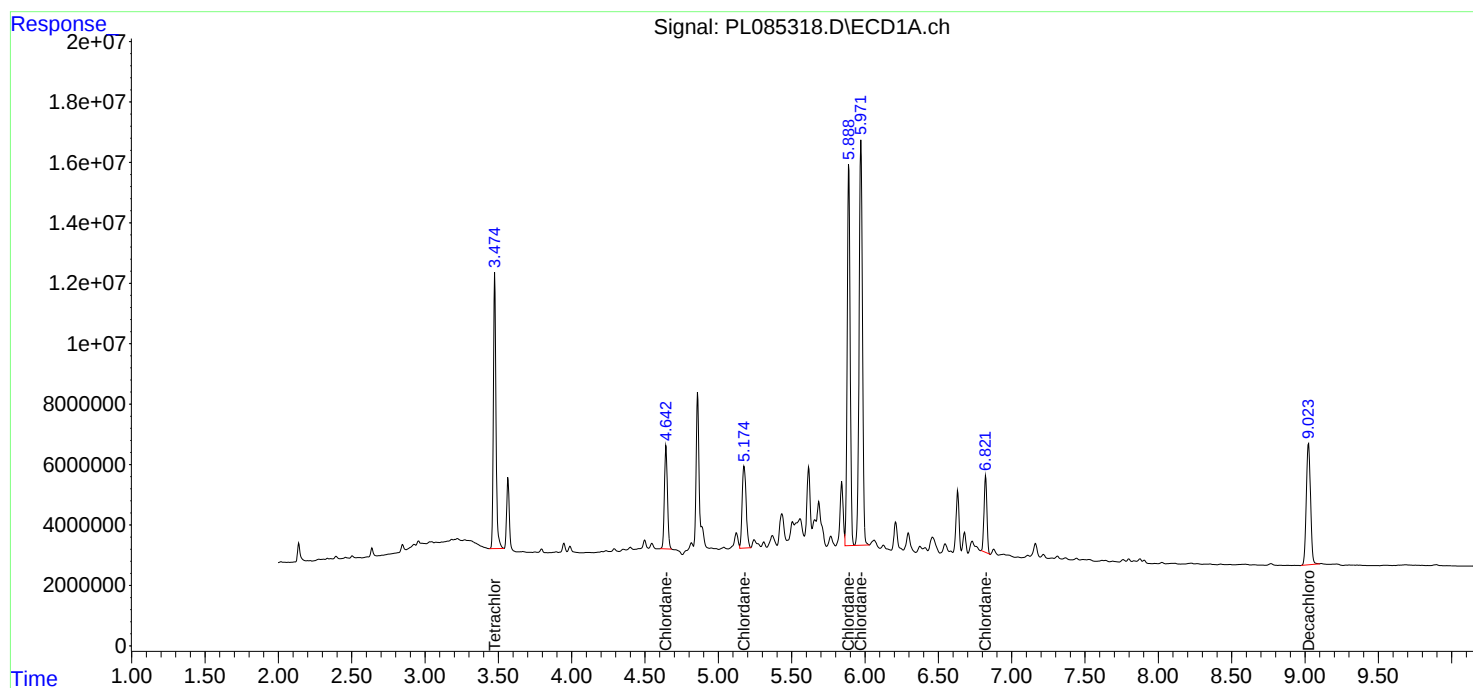


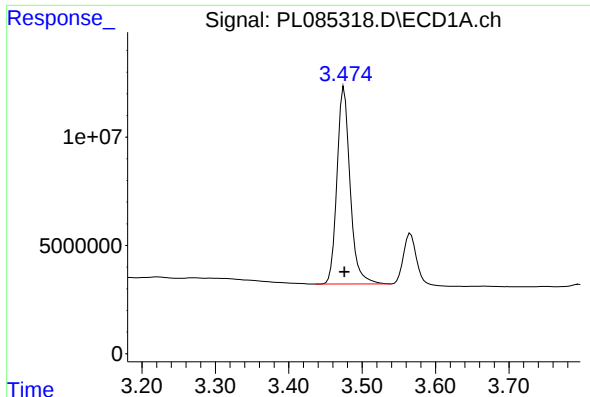

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 113046502
Conc: 46.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

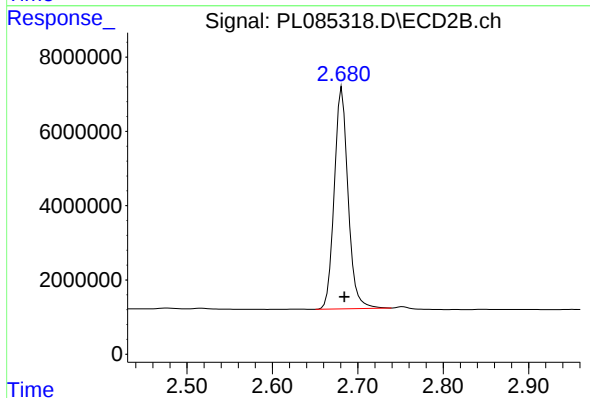


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: -0.003 min
Response: 66926578
Conc: 58.90 ng/ml

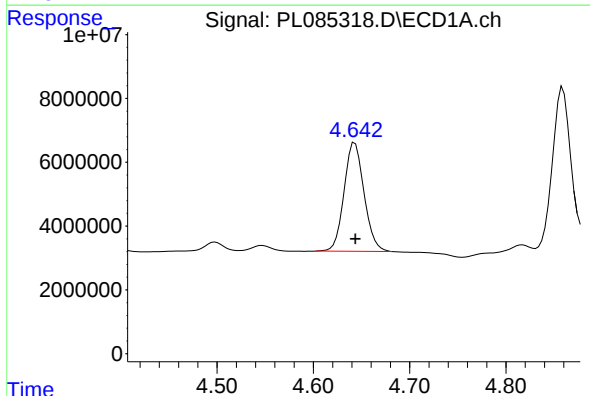


#23 Chlordane-1

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 49040300
Conc: 492.83 ng/ml

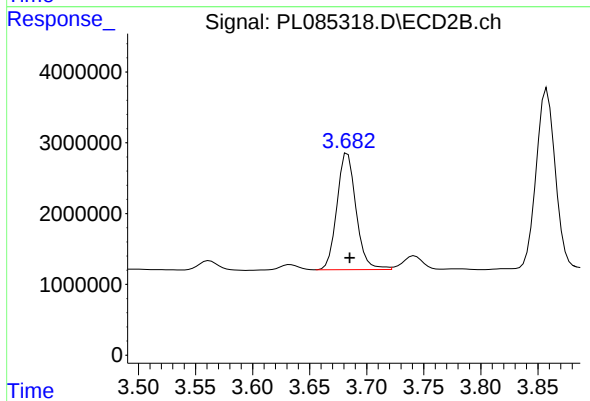

#23 Chlordane-1


R.T.: 3.683 min
Delta R.T.: -0.002 min
Response: 19198302
Conc: 494.03 ng/ml

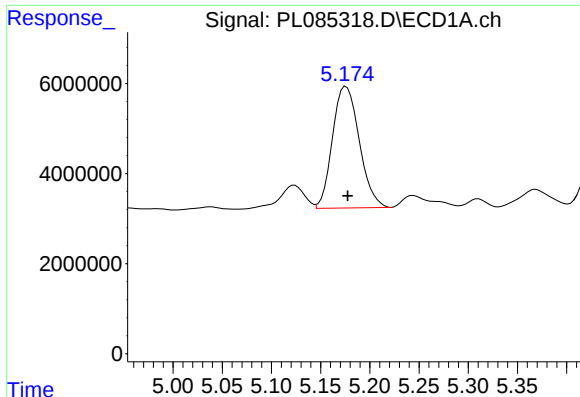

#24 Chlordane-2


R.T.: 5.176 min
Delta R.T.: -0.002 min
Response: 51071127
Conc: 487.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

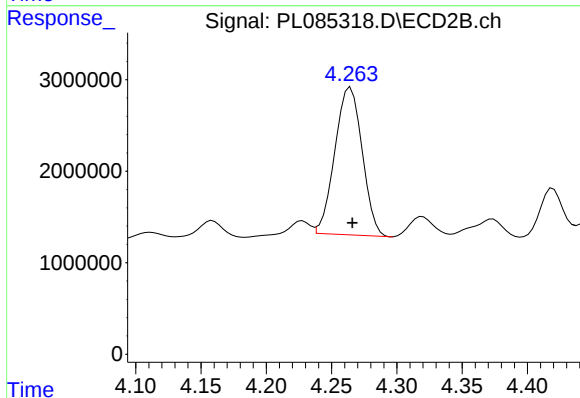


#24 Chlordane-2

R.T.: 4.265 min
Delta R.T.: -0.001 min
Response: 23488627
Conc: 487.35 ng/ml

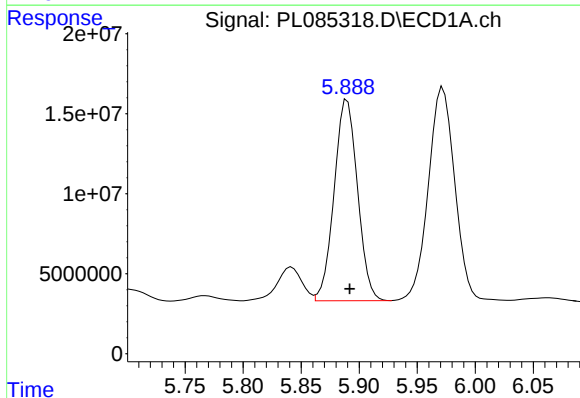


#25 Chlordane-3

R.T.: 5.890 min
Delta R.T.: -0.002 min
Response: 176227380
Conc: 487.57 ng/ml

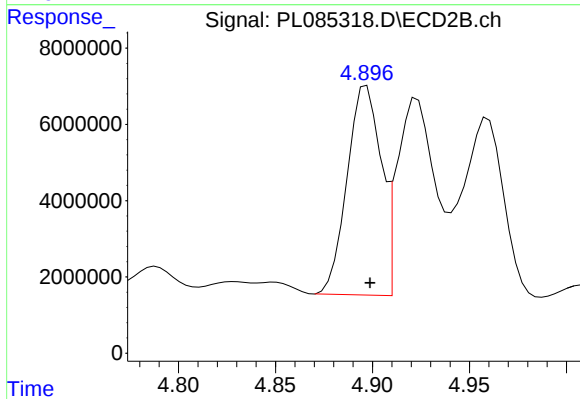

#25 Chlordane-3


R.T.: 4.897 min
Delta R.T.: -0.002 min
Response: 66428771
Conc: 494.71 ng/ml

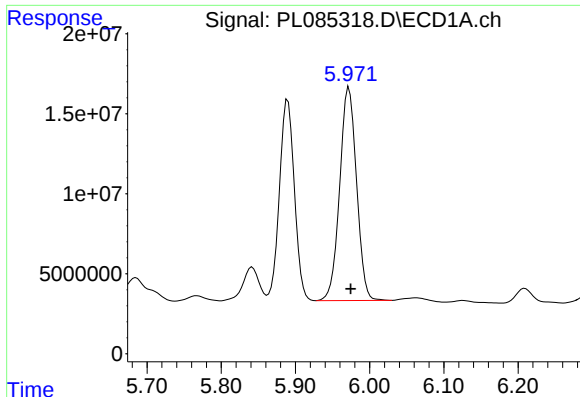

#26 Chlordane-4


R.T.: 5.972 min
Delta R.T.: -0.002 min
Response: 210644131
Conc: 485.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

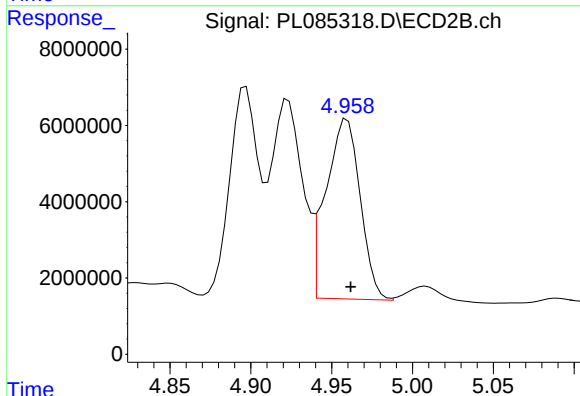


#26 Chlordane-4

R.T.: 4.960 min
Delta R.T.: -0.002 min
Response: 69530620
Conc: 467.57 ng/ml

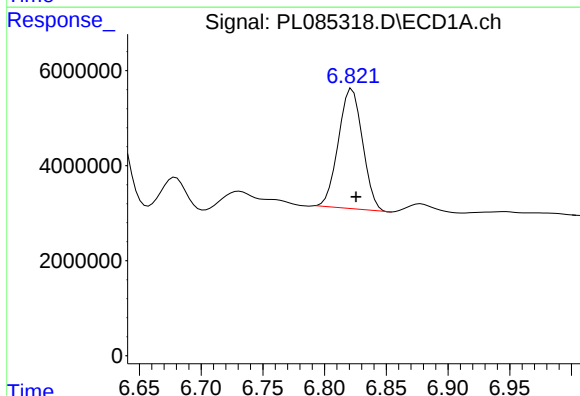


#27 Chlordane-5

R.T.: 6.822 min
Delta R.T.: -0.003 min
Response: 34451998
Conc: 493.45 ng/ml

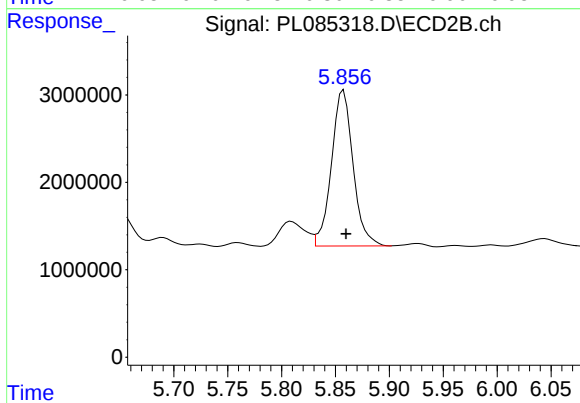

#27 Chlordane-5


R.T.: 5.858 min
Delta R.T.: -0.003 min
Response: 24895053
Conc: 489.05 ng/ml

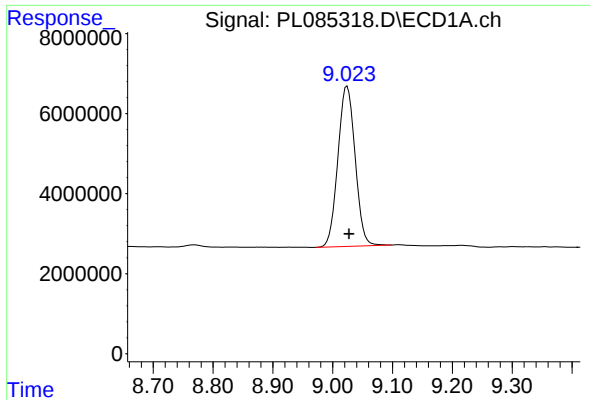

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.003 min
Response: 80272390
Conc: 49.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

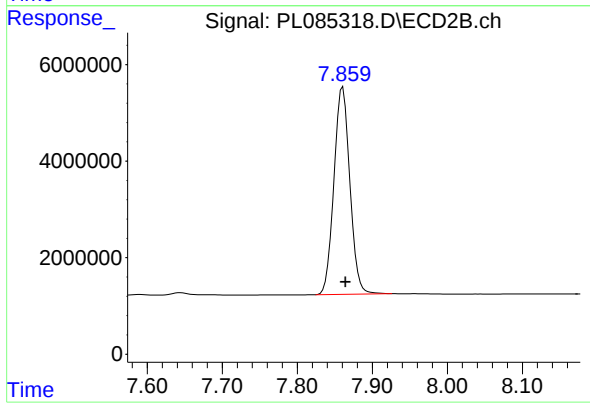

#28 Decachlorobiphenyl

R.T.: 7.861 min
Delta R.T.: -0.004 min
Response: 63499108
Conc: 47.70 ng/ml