

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091424\
 Data File : PL091763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2024 18:17
 Operator : AR\AJ
 Sample : P4002-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/16/2024
 Supervised By :Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 01:46:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.781	29574123	36968112	18.975m	19.766
28) SA Decachlor...	9.047	7.921	39030262	25766774	32.115m	13.954m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091424\
Data File : PL091763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2024 18:17
Operator : AR\AJ
Sample : P4002-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/16/2024
Supervised By : Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 01:46:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

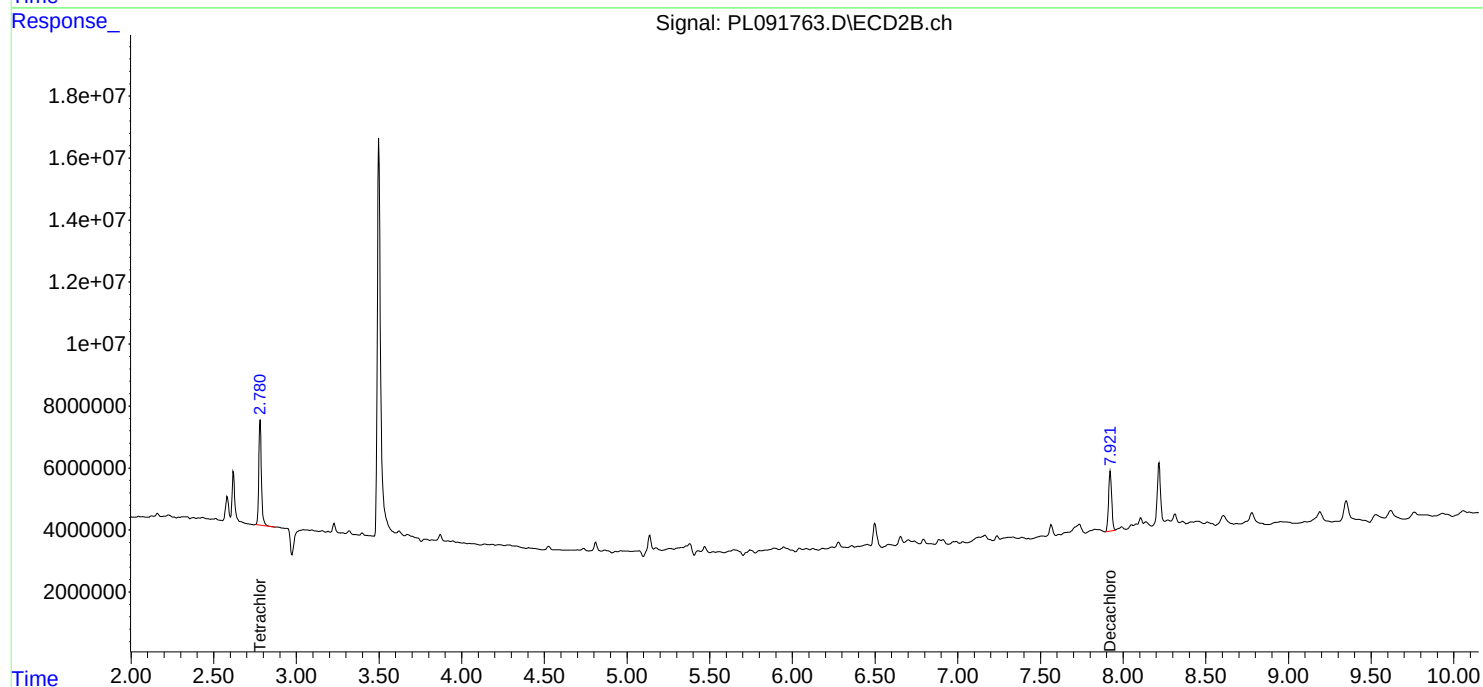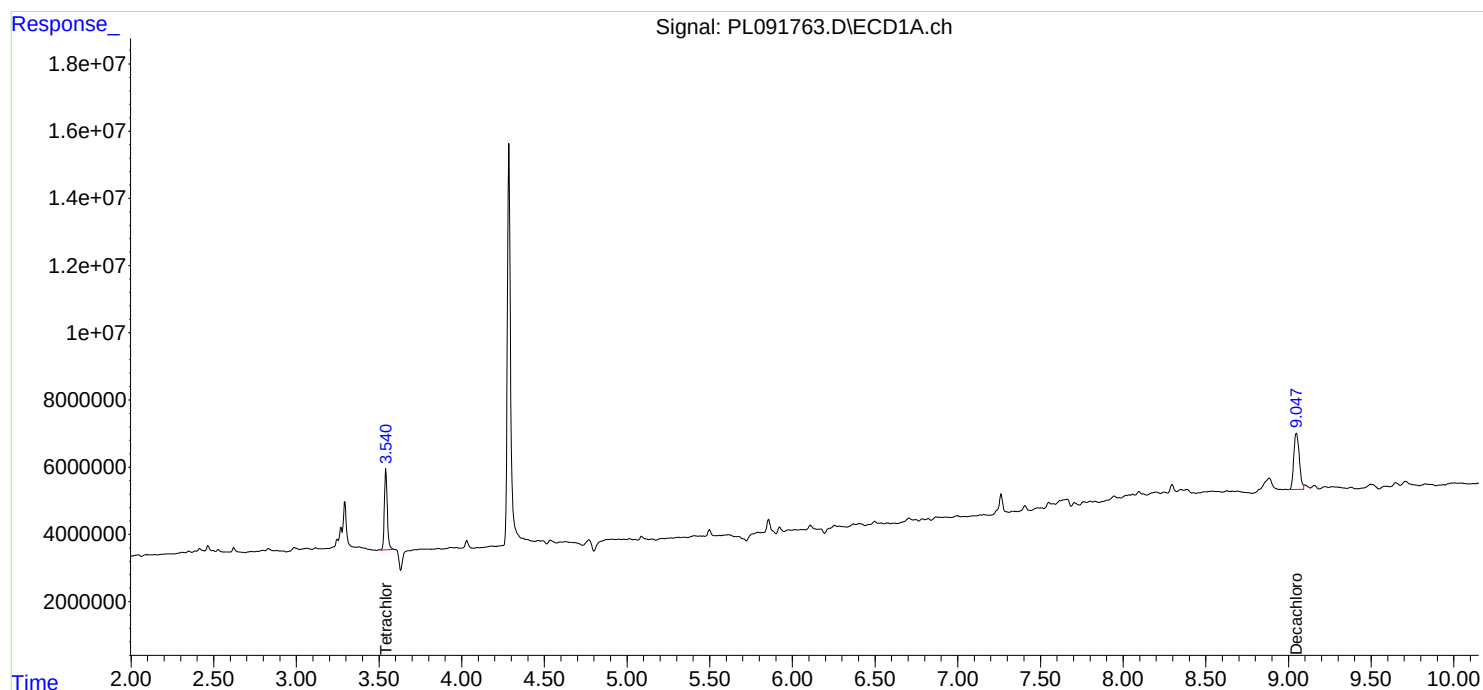

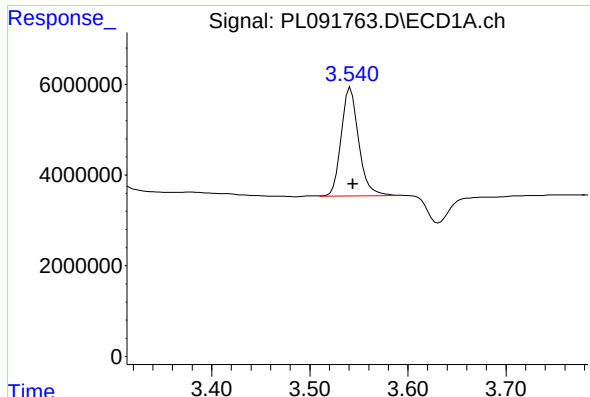


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 29574123
Conc: 18.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/16/2024
Supervised By :Ankita Jodhani 09/16/2024

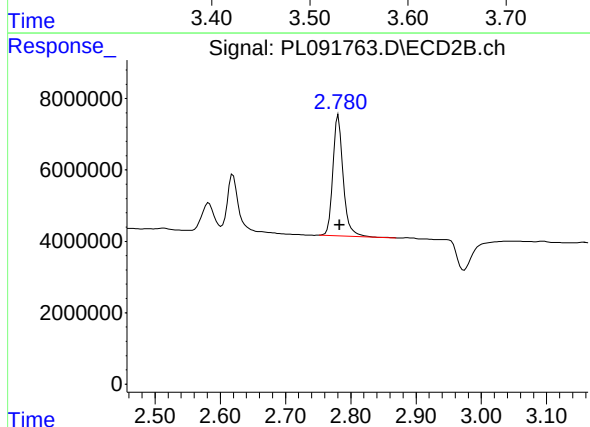


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: -0.002 min
Response: 36968112
Conc: 19.77 ng/ml

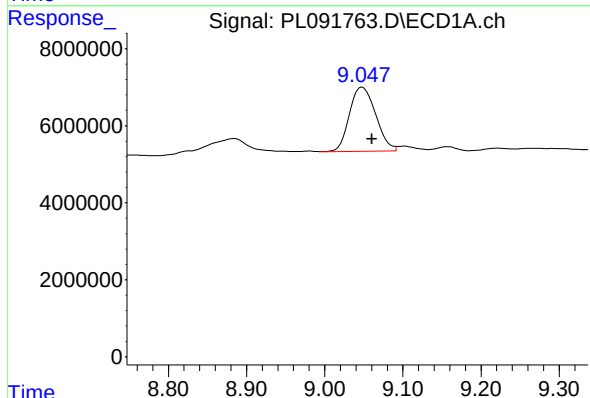

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: -0.014 min
Response: 39030262
Conc: 32.12 ng/ml m

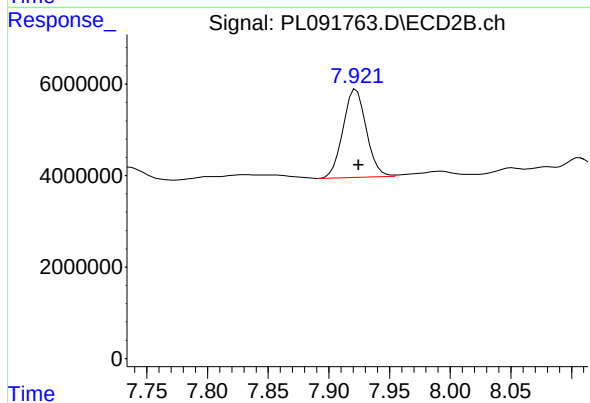

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.004 min
Response: 25766774
Conc: 13.95 ng/ml m