

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091425\
 Data File : PL097190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2025 13:03
 Operator : AR\AJ
 Sample : Q3075-04RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MOO-25-0258RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/16/2025
 Supervised By :mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 02:09:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.525	2.821	12707484	20495431	3.222m	3.636m
28) SA Decachlor...	8.998	7.981	26157112	32855011	8.835	6.851

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091425\
Data File : PL097190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2025 13:03
Operator : AR\AJ
Sample : Q3075-04RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MOO-25-0258RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/16/2025
Supervised By : mohammad ahmed 09/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 02:09:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

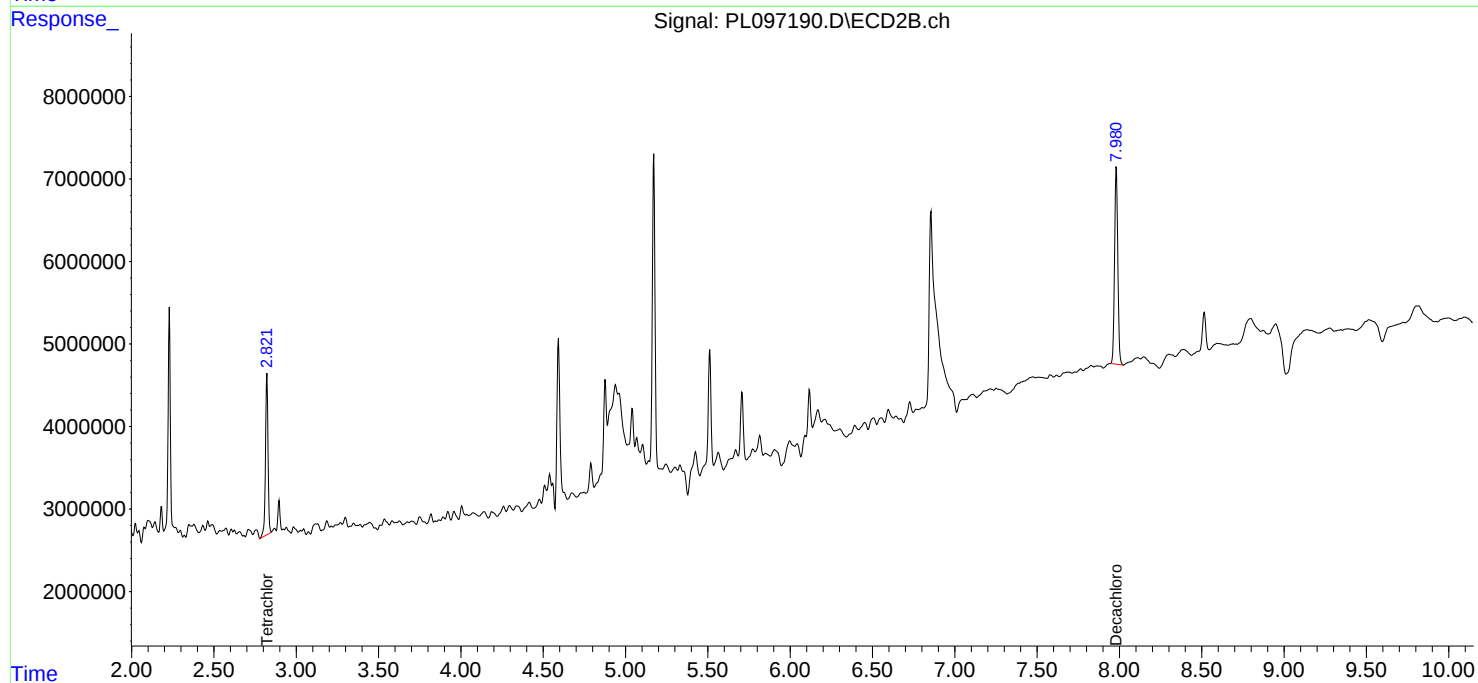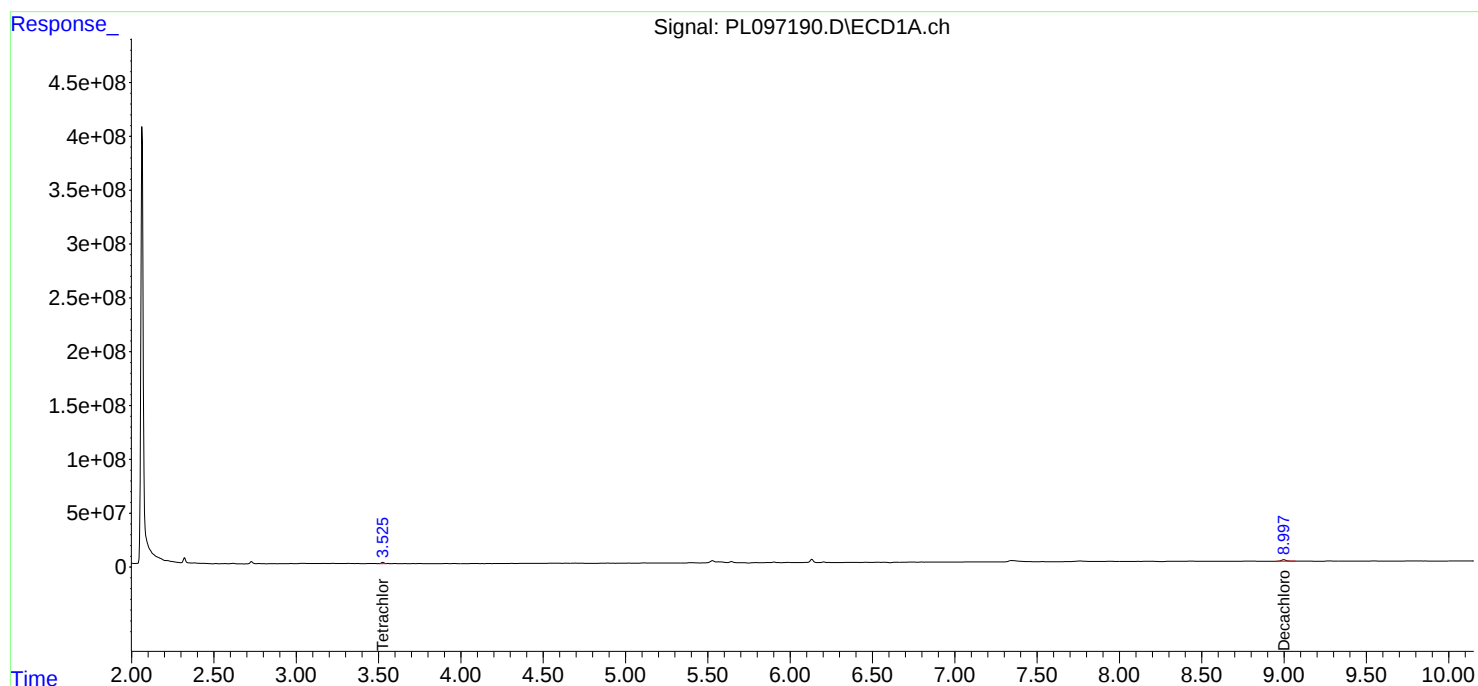

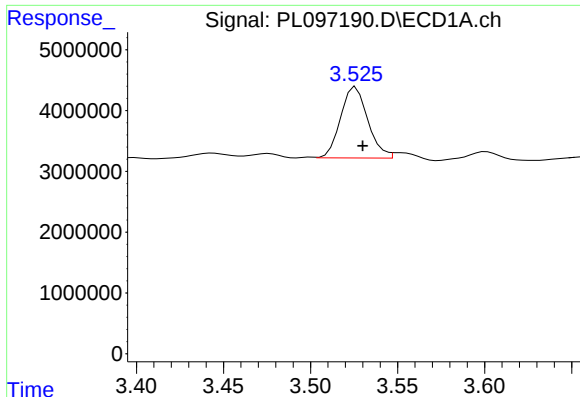


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.005 min
Response: 12707484
Conc: 3.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-25-0258RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/16/2025
Supervised By :mohammad ahmed 09/17/2025

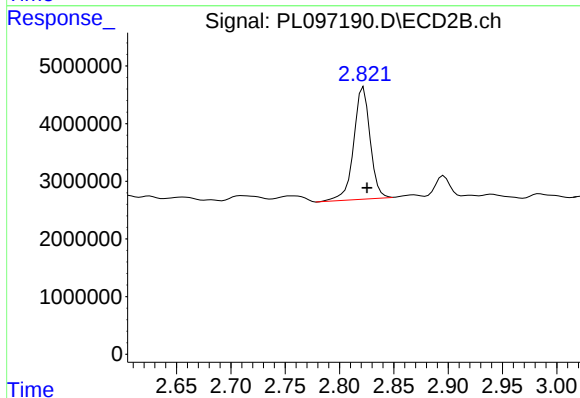


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: -0.005 min
Response: 20495431
Conc: 3.64 ng/ml m

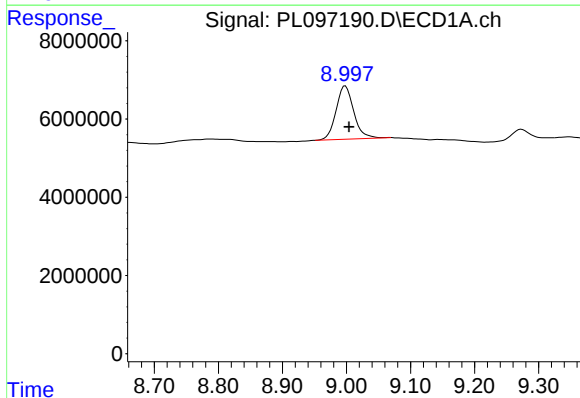

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: -0.006 min
Response: 26157112
Conc: 8.83 ng/ml

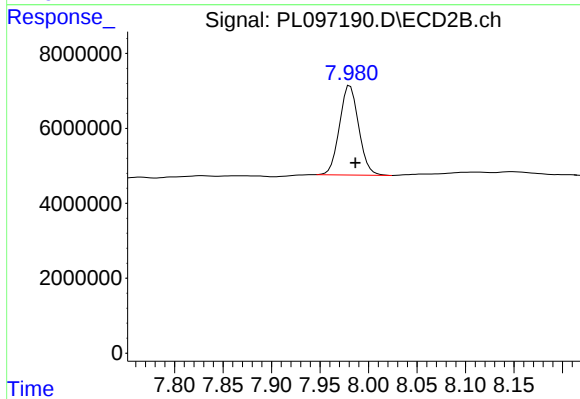

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.006 min
Response: 32855011
Conc: 6.85 ng/ml