

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
 Data File : PL039948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 07:56
 Operator : AJ\SJ
 Sample : J4904-10
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 00:50:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.299	3.903	103.7E6	49112901	13.377	15.392
28)	SA Decachlor...	7.951	8.887	65659508	14809503	7.880	5.453 #
Target Compounds							
3)	MA gamma-BHC...	4.047f	0.000	200.9E6	0	17.558	N.D. #
12)	B 4,4'-DDE	5.401	6.204	40801209	11735643	3.850	3.085
14)	MA Endrin	0.000	6.521f	0	7559760	N.D.	2.322 #
15)	B Endosulfa...	0.000	6.793	0	4446	N.D.	0.001 #
17)	MA 4,4'-DDT	6.210f	0.000	18522973	0	2.046	N.D. #
18)	B Endrin al...	6.210	0.000	18522973	0	2.417	N.D. #
19)	B Endosulfa...	6.458	0.000	3047.7E6	0	332.545	N.D. #
21)	B Endrin ke...	6.928	0.000	26154725	0	2.678	N.D. #
27)	Chlordane-5	0.000	6.793	0	4446	N.D.	0.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
Data File : PL039948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 07:56
Operator : AJ\SJ
Sample : J4904-10
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 00:50:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

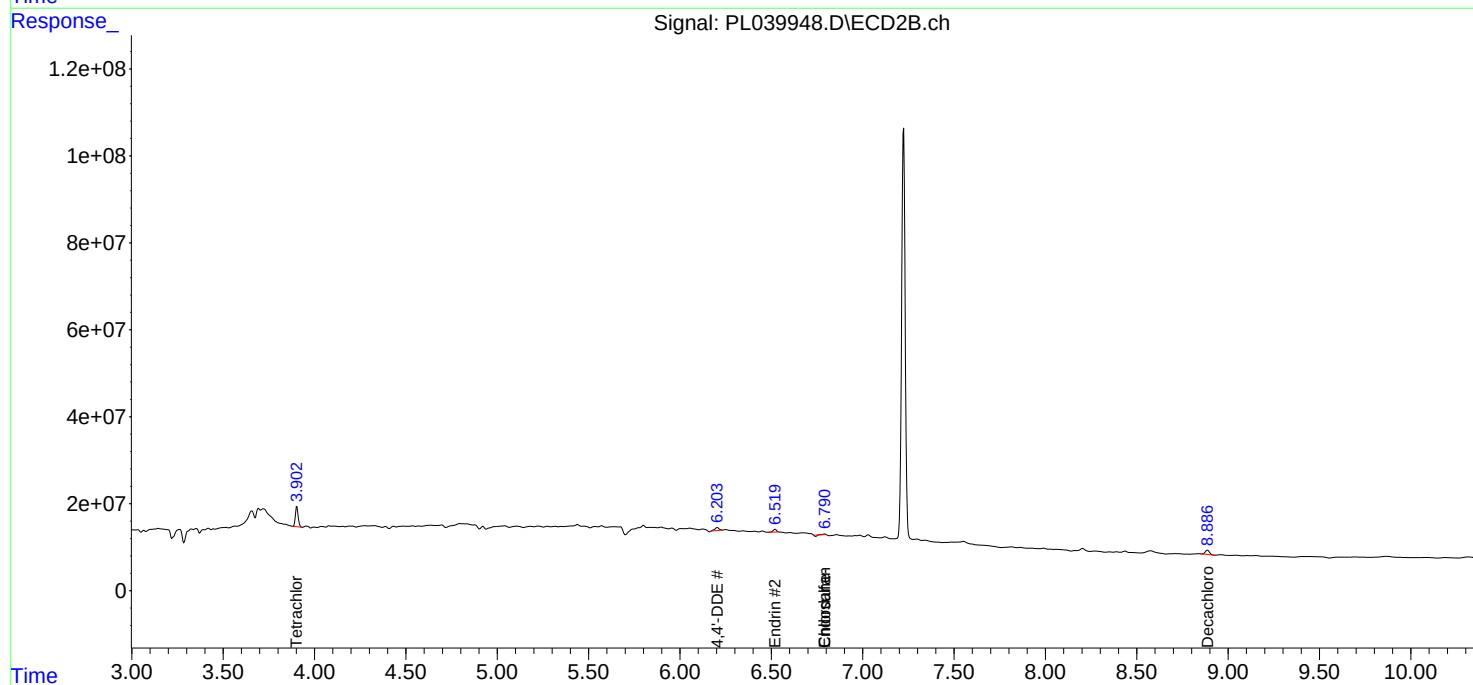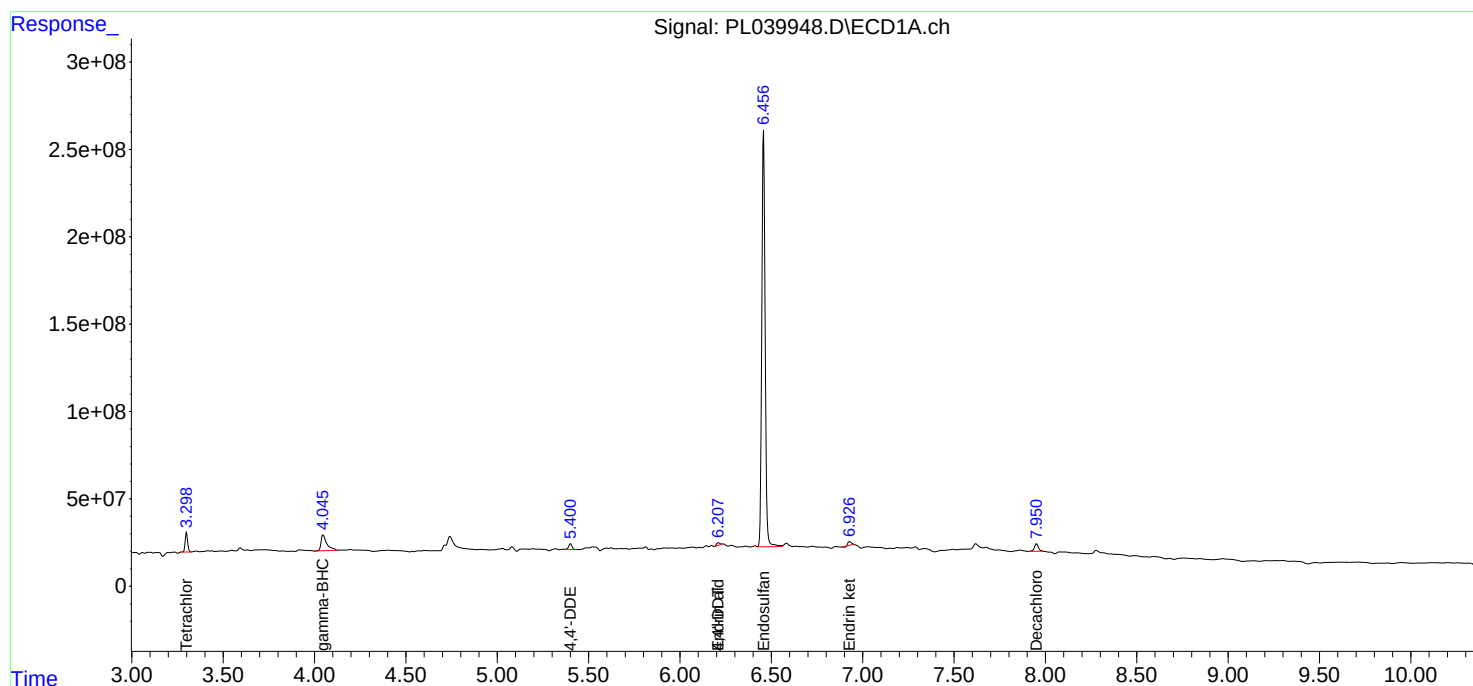


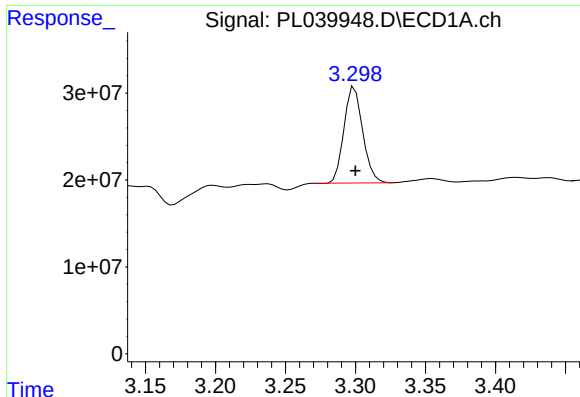

#1 Tetrachloro-m-xylene


R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 103735886
Conc: 13.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

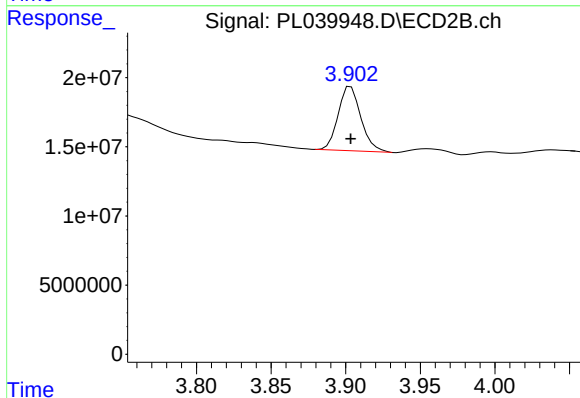


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 49112901
Conc: 15.39 ng/ml

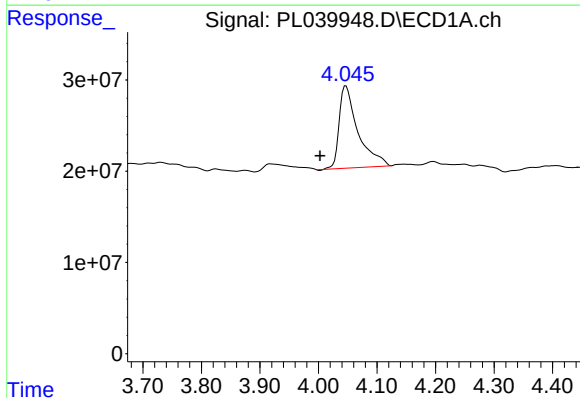


#3 gamma-BHC (Lindane)

R.T.: 4.047 min
Delta R.T.: 0.044 min
Response: 200935967
Conc: 17.56 ng/ml

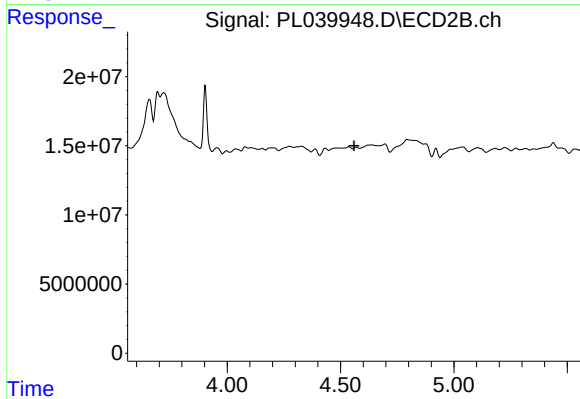

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.559 min
Response: 0
Conc: N.D.

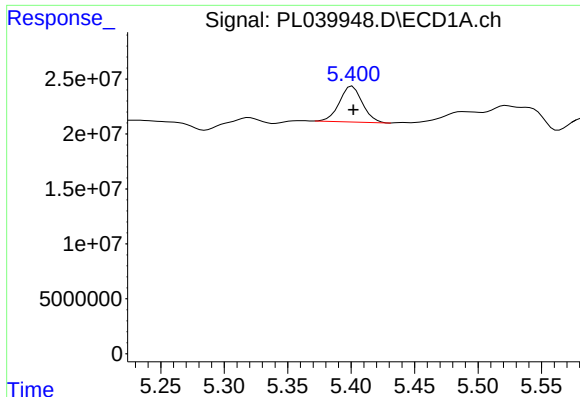

#12 4,4'-DDE


R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 40801209
Conc: 3.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

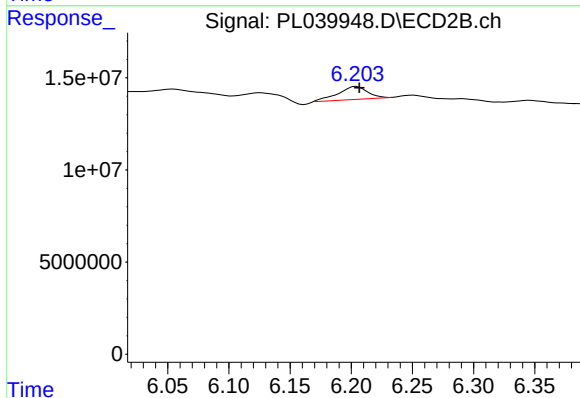


#12 4,4'-DDE

R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 11735643
Conc: 3.09 ng/ml

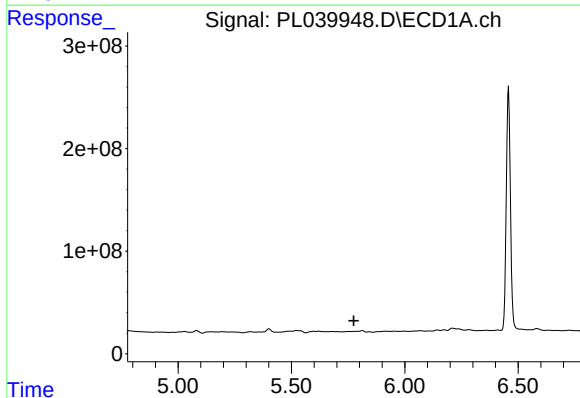


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.776 min
Response: 0
Conc: N.D.

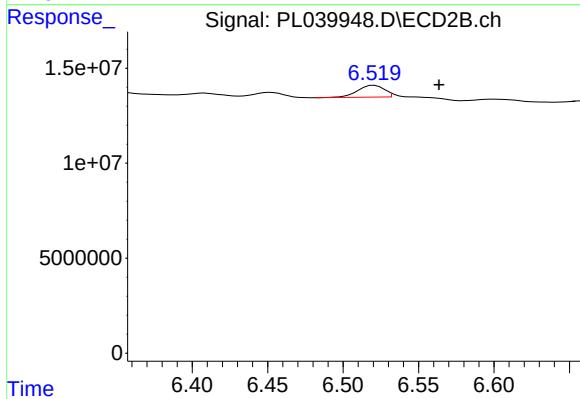

#14 Endrin


R.T.: 6.521 min
Delta R.T.: -0.043 min
Response: 7559760
Conc: 2.32 ng/ml

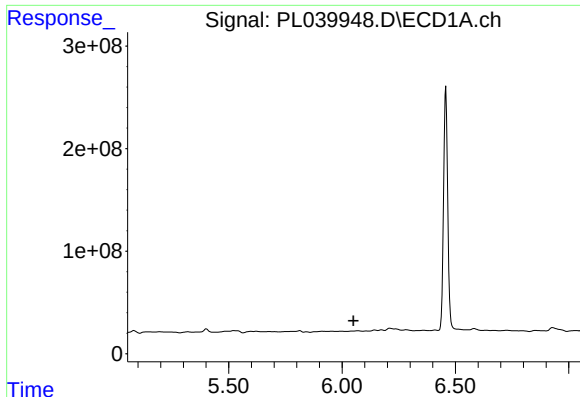

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

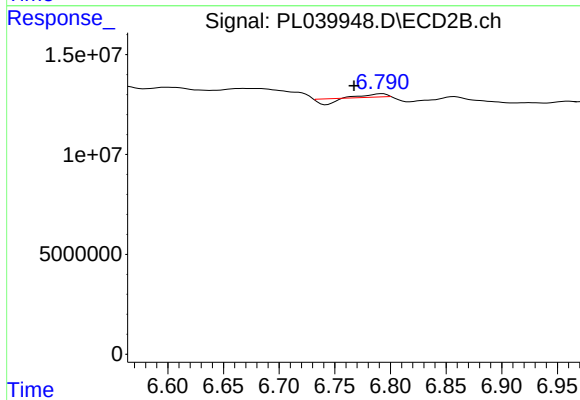


#15 Endosulfan II

R.T.: 6.793 min
Delta R.T.: 0.025 min
Response: 4446
Conc: 0.00 ng/ml

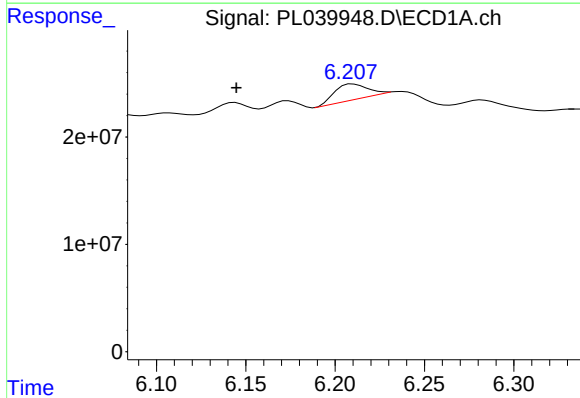


#17 4,4'-DDT

R.T.: 6.210 min
Delta R.T.: 0.065 min
Response: 18522973
Conc: 2.05 ng/ml

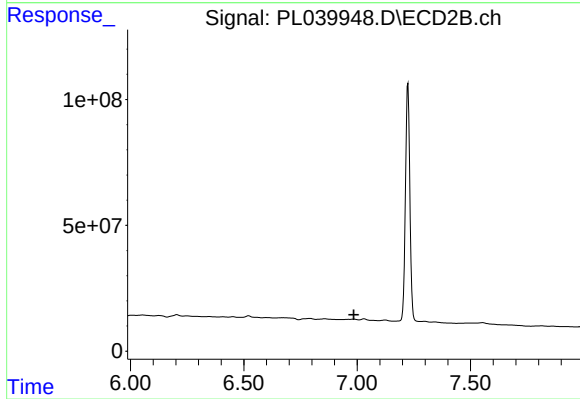

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.986 min
Response: 0
Conc: N.D.

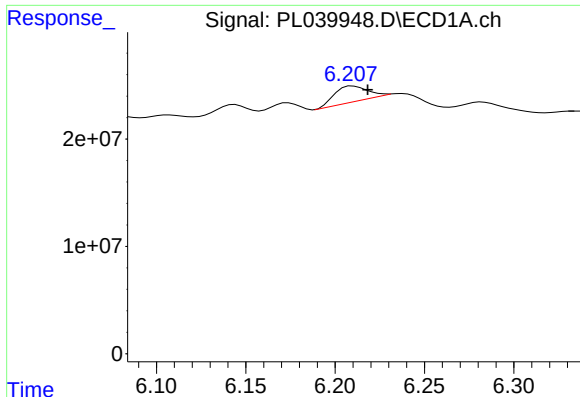

#18 Endrin aldehyde


R.T.: 6.210 min
Delta R.T.: -0.008 min
Response: 18522973
Conc: 2.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

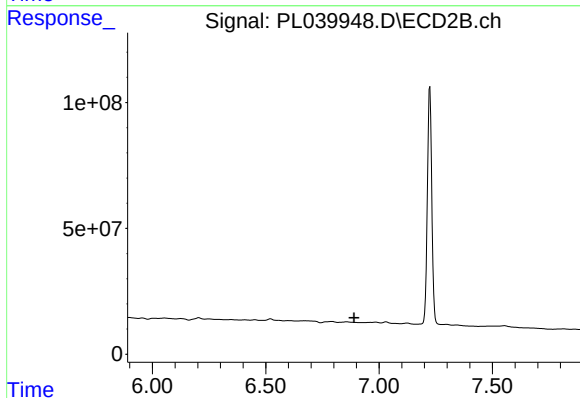


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.890 min
Response: 0
Conc: N.D.

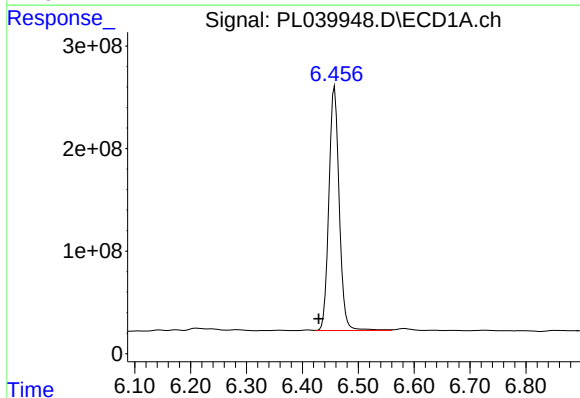


#19 Endosulfan Sulfate

R.T.: 6.458 min
Delta R.T.: 0.029 min
Response: 3047709619
Conc: 332.54 ng/ml

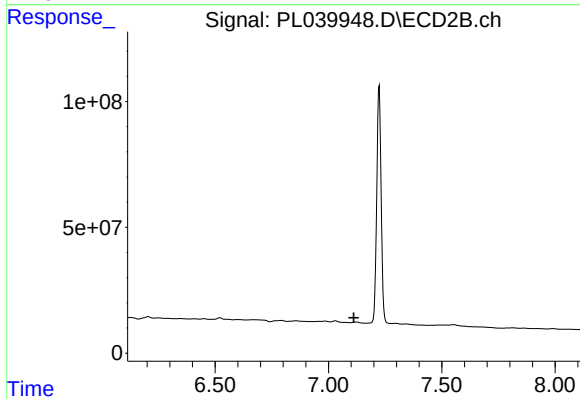

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.112 min
Response: 0
Conc: N.D.

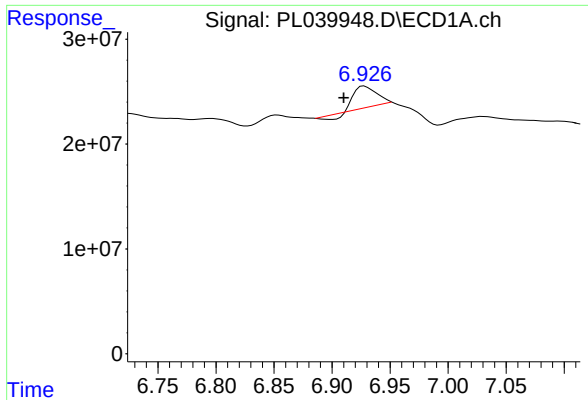

#21 Endrin ketone


R.T.: 6.928 min
Delta R.T.: 0.018 min
Response: 26154725
Conc: 2.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

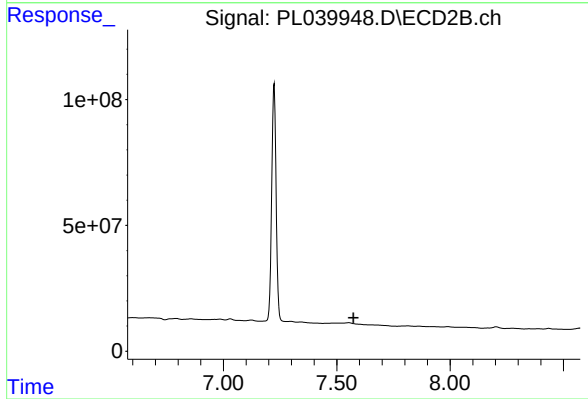


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.574 min
Response: 0
Conc: N.D.

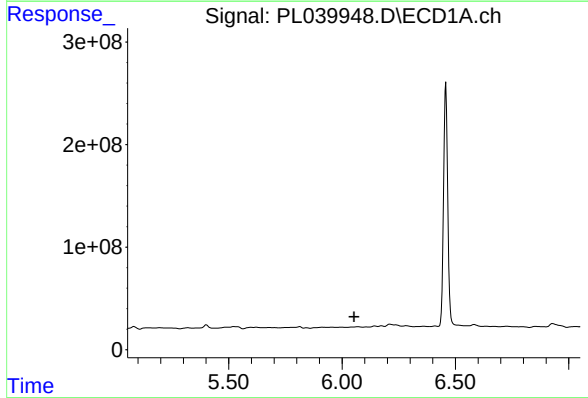


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

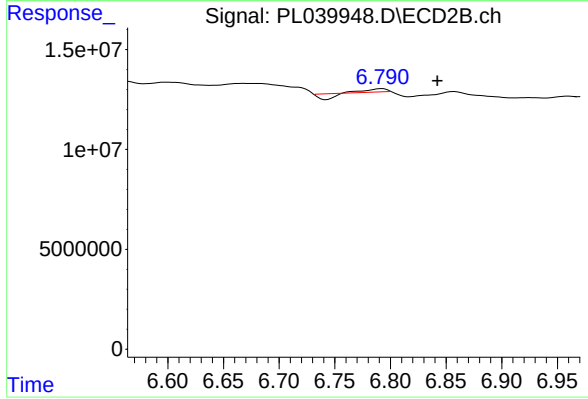

#27 Chlordane-5


R.T.: 6.793 min
Delta R.T.: -0.050 min
Response: 4446
Conc: 0.04 ng/ml

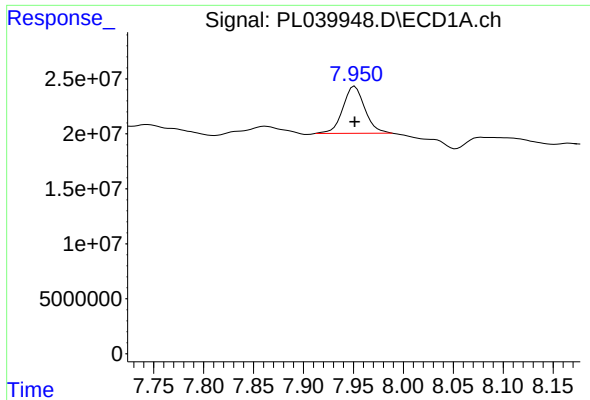

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 65659508
Conc: 7.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

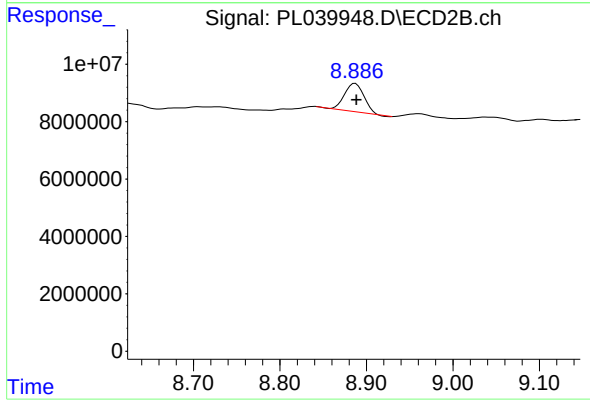

#28 Decachlorobiphenyl

R.T.: 8.887 min
Delta R.T.: -0.001 min
Response: 14809503
Conc: 5.45 ng/ml