

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
 Data File : PL039962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 11:43
 Operator : AJ\SJ
 Sample : J4904-21
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 00:53:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	156.0E6	66859977	20.122	20.954
28)	SA Decachlor...	7.951	8.889	118.6E6	49107477	14.232	18.080 #
Target Compounds							
3)	MA gamma-BHC...	4.049f	0.000	148.8E6	0	13.000	N.D. #
7)	B delta-BHC	0.000	4.926	0	8063631	N.D.	2.027 #
8)	B Heptachlo...	0.000	5.778	0	11480178	N.D.	2.903 #
12)	B 4,4'-DDE	5.401	6.206	358.7E6	131.8E6	33.848	34.652
15)	B Endosulfa...	0.000	6.793	0	1211494	N.D.	0.367 #
17)	MA 4,4'-DDT	6.144	6.986	621.5E6	227.7E6	68.661	76.108
23)	Chlordane-1	0.000	4.926	0	8063631	N.D.	52.075 #
27)	Chlordane-5	0.000	6.793	0	1211494	N.D.	10.440 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
Data File : PL039962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 11:43
Operator : AJ\SJ
Sample : J4904-21
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 00:53:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

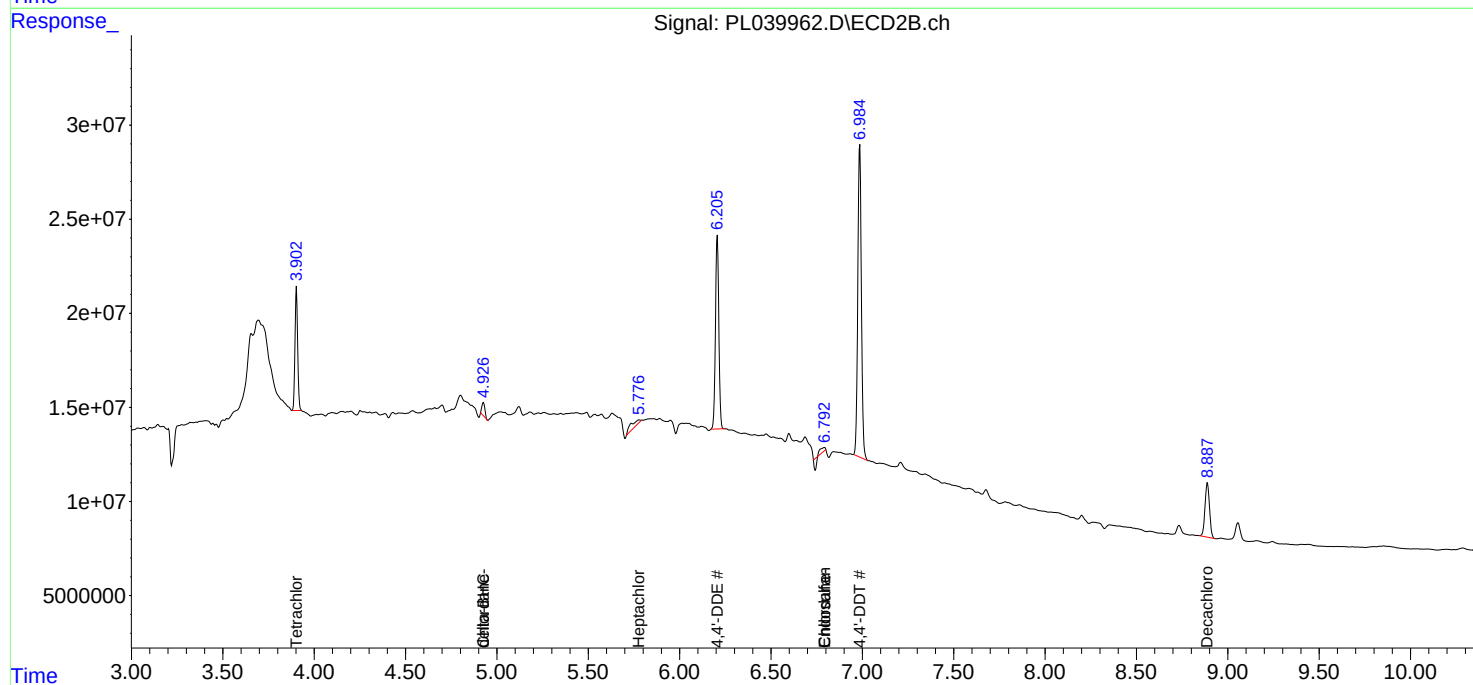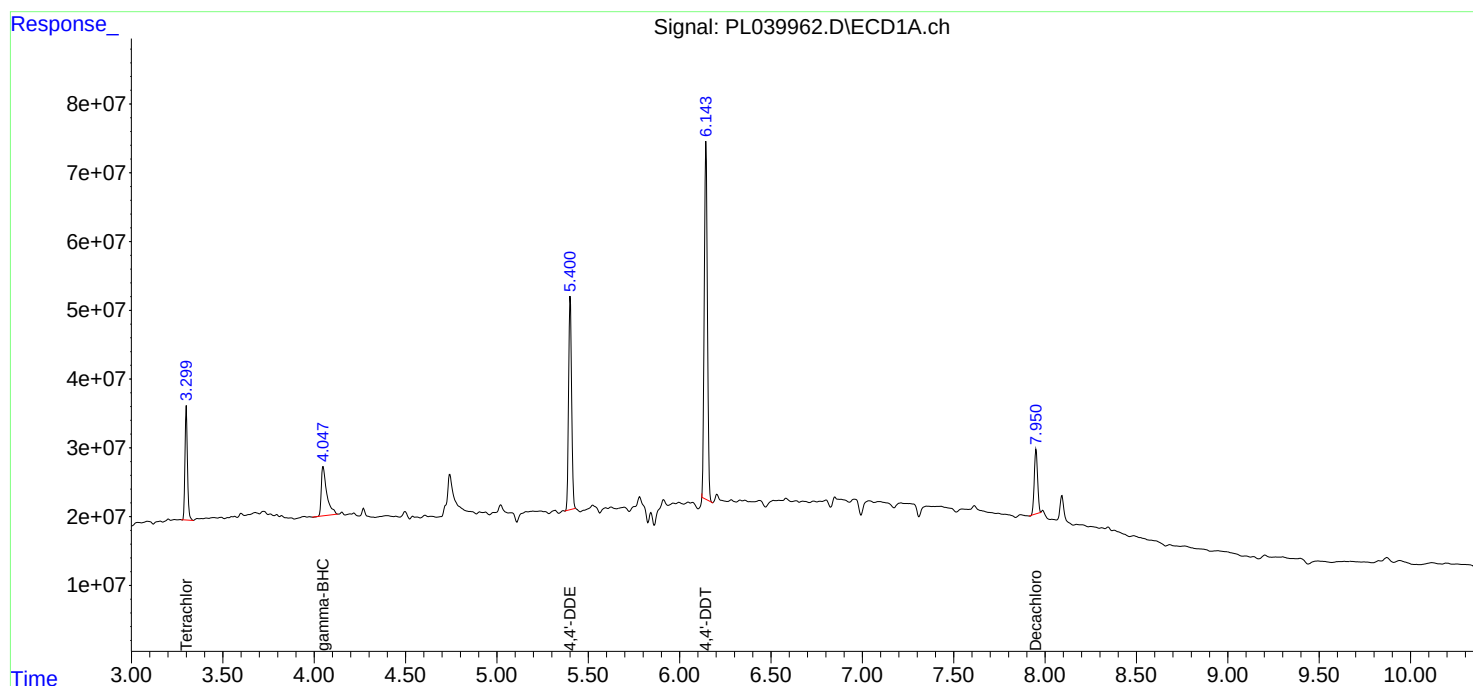


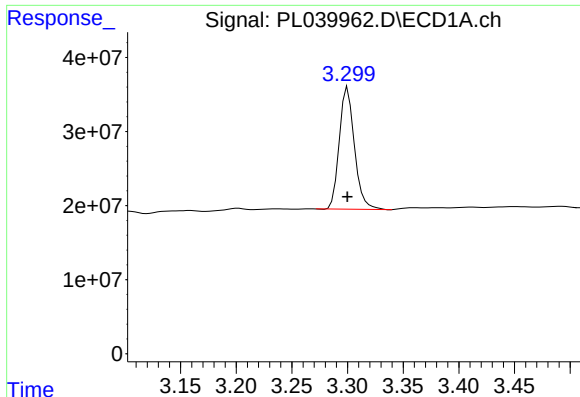

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 156040684
Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

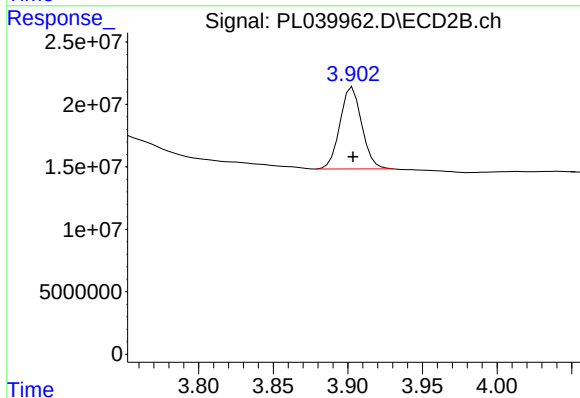


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 66859977
Conc: 20.95 ng/ml

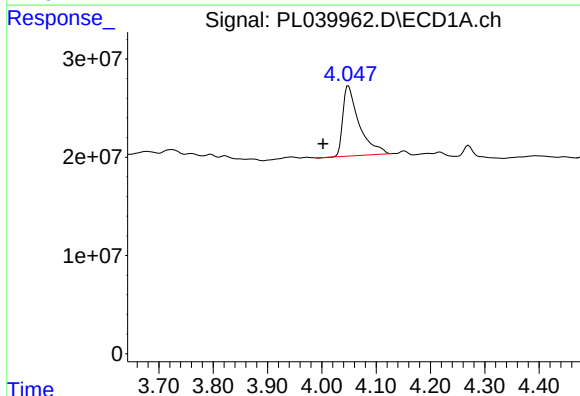


#3 gamma-BHC (Lindane)

R.T.: 4.049 min
Delta R.T.: 0.047 min
Response: 148777673
Conc: 13.00 ng/ml

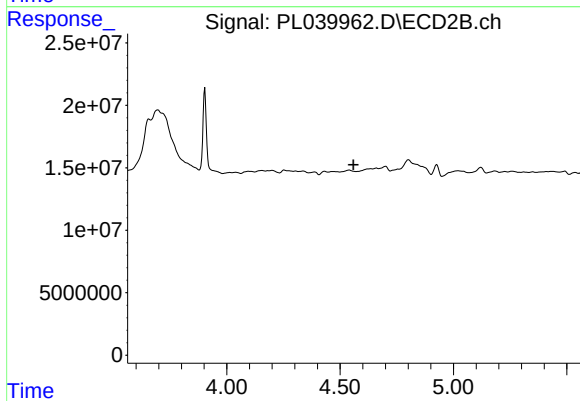

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.559 min
Response: 0
Conc: N.D.

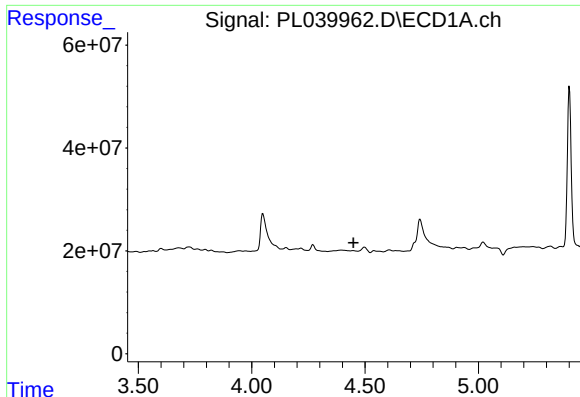

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

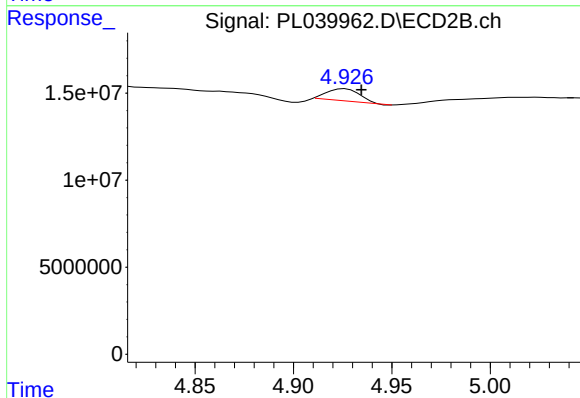


#7 delta-BHC

R.T.: 4.926 min
Delta R.T.: -0.008 min
Response: 8063631
Conc: 2.03 ng/ml

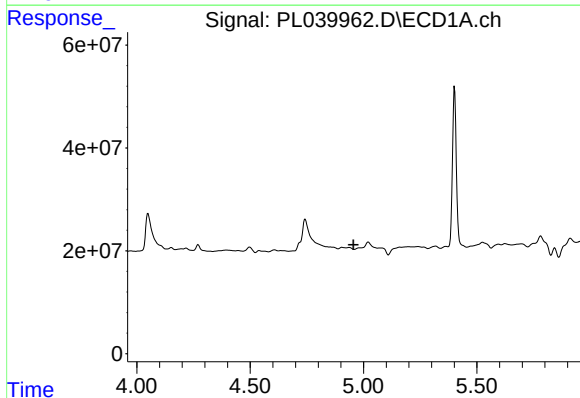


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

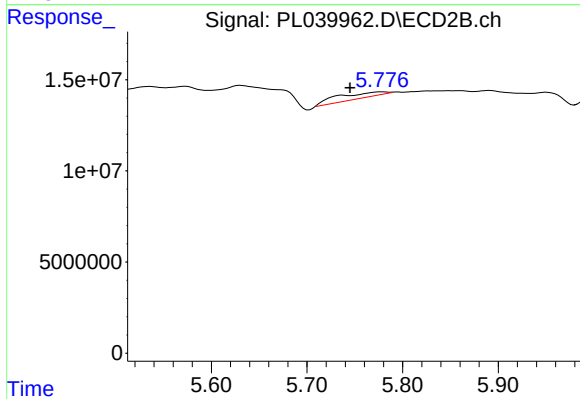

#8 Heptachlor epoxide


R.T.: 5.778 min
Delta R.T.: 0.033 min
Response: 11480178
Conc: 2.90 ng/ml

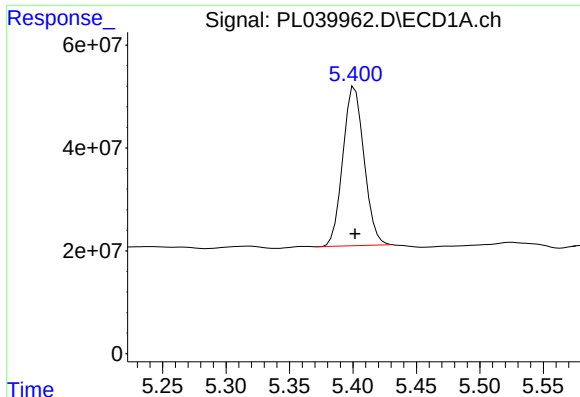

#12 4,4'-DDE


R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 358742751
Conc: 33.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

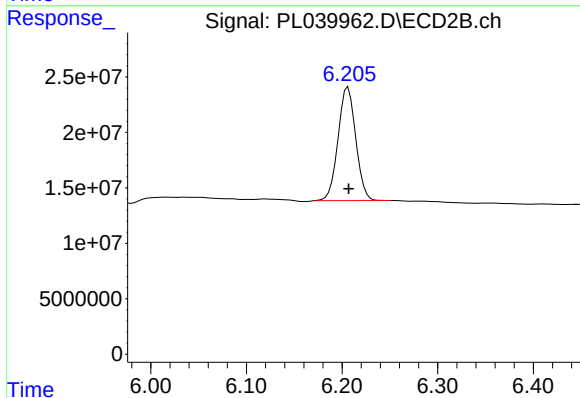


#12 4,4'-DDE

R.T.: 6.206 min
Delta R.T.: 0.000 min
Response: 131803203
Conc: 34.65 ng/ml

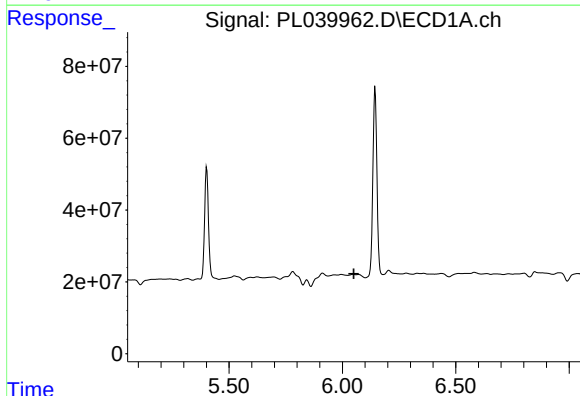


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

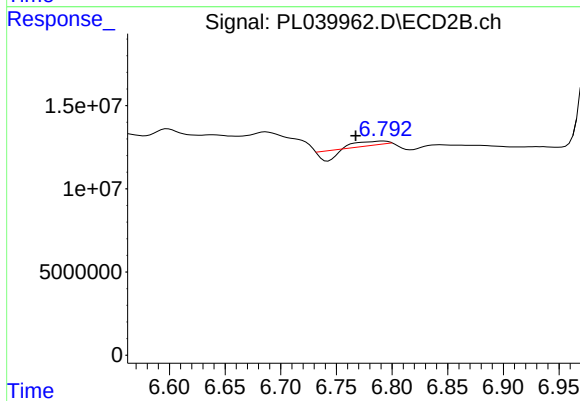

#15 Endosulfan II


R.T.: 6.793 min
Delta R.T.: 0.025 min
Response: 1211494
Conc: 0.37 ng/ml

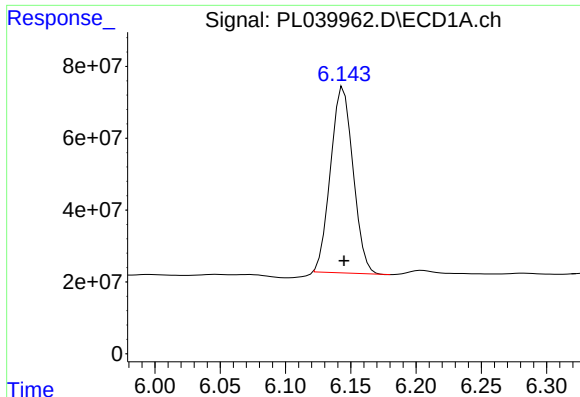

#17 4,4'-DDT


R.T.: 6.144 min
Delta R.T.: 0.000 min
Response: 621471864
Conc: 68.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

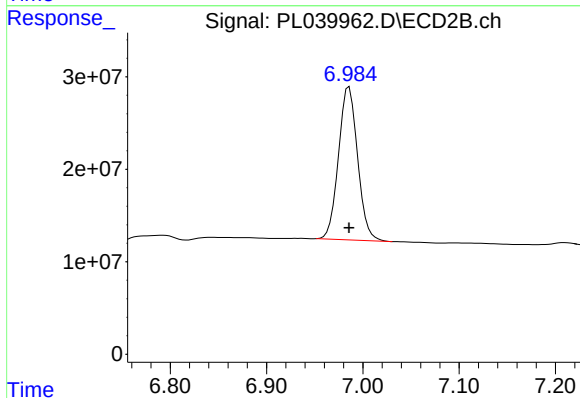


#17 4,4'-DDT

R.T.: 6.986 min
Delta R.T.: 0.000 min
Response: 227694697
Conc: 76.11 ng/ml

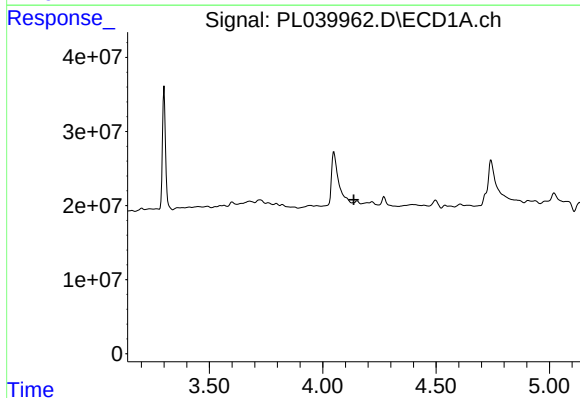


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.136 min
Response: 0
Conc: N.D.

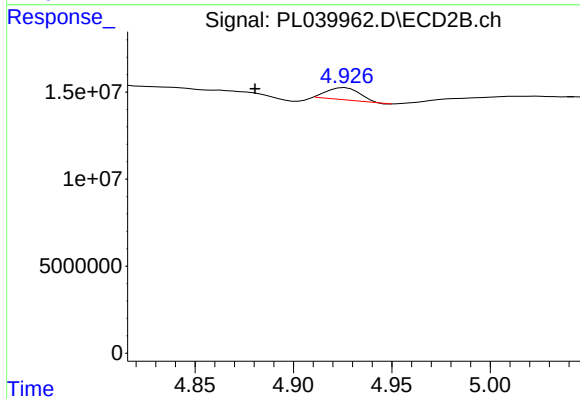

#23 Chlordane-1


R.T.: 4.926 min
Delta R.T.: 0.046 min
Response: 8063631
Conc: 52.08 ng/ml

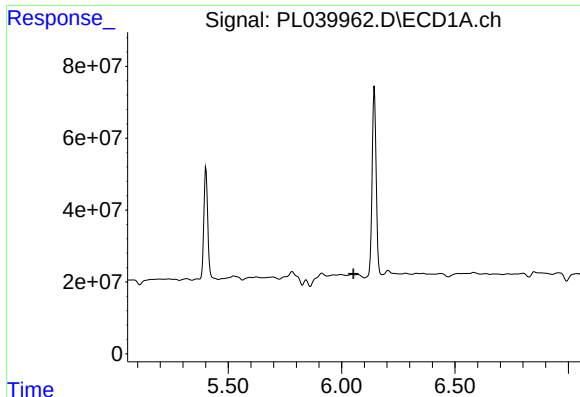

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

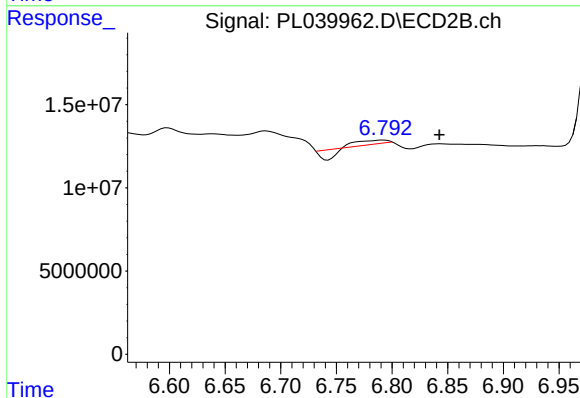


#27 Chlordane-5

R.T.: 6.793 min
Delta R.T.: -0.050 min
Response: 1211494
Conc: 10.44 ng/ml

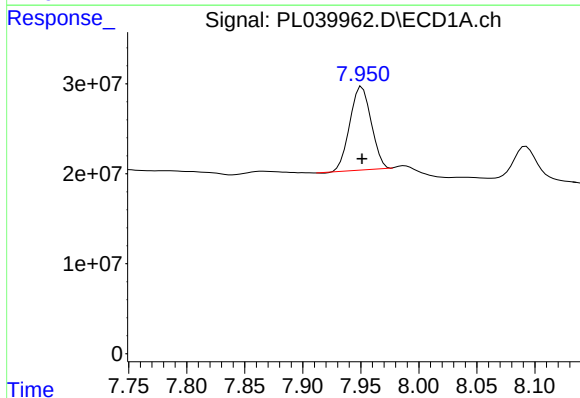

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 118591464
Conc: 14.23 ng/ml

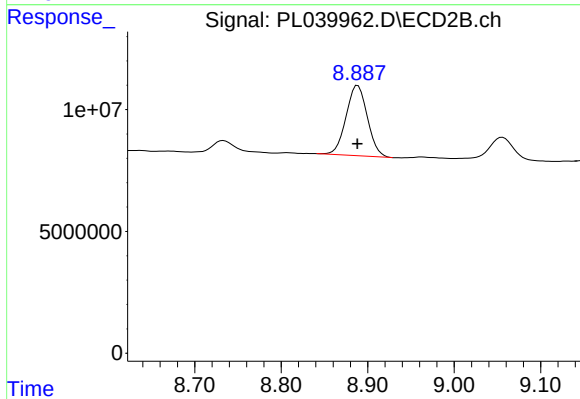

#28 Decachlorobiphenyl

R.T.: 8.889 min
Delta R.T.: 0.000 min
Response: 49107477
Conc: 18.08 ng/ml