

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
 Data File : PL039971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 13:51
 Operator : AJ\SJ
 Sample : J4906-24
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 00:54:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	116.5E6	52886420	15.021	16.575
28)	SA Decachlor...	7.951	8.888	148.1E6	51604146	17.772	19.000
Target Compounds							
2)	A alpha-BHC	3.742	4.287	76963422	11661738	6.067	2.254 #
3)	MA gamma-BHC...	4.008	0.000	12191055	0	1.065	N.D. #
19)	B Endosulfa...	6.446	0.000	30359728	0	3.313	N.D. #
20)	A Methoxychlor	6.628f	0.000	41909630	0	9.042	N.D. #
23)	Chlordane-1	4.180	4.879	29682242	3155537	81.895	20.379 #
24)	Chlordane-2	4.597	0.000	17078567	0	45.347	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
Data File : PL039971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 13:51
Operator : AJ\SJ
Sample : J4906-24
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 00:54:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

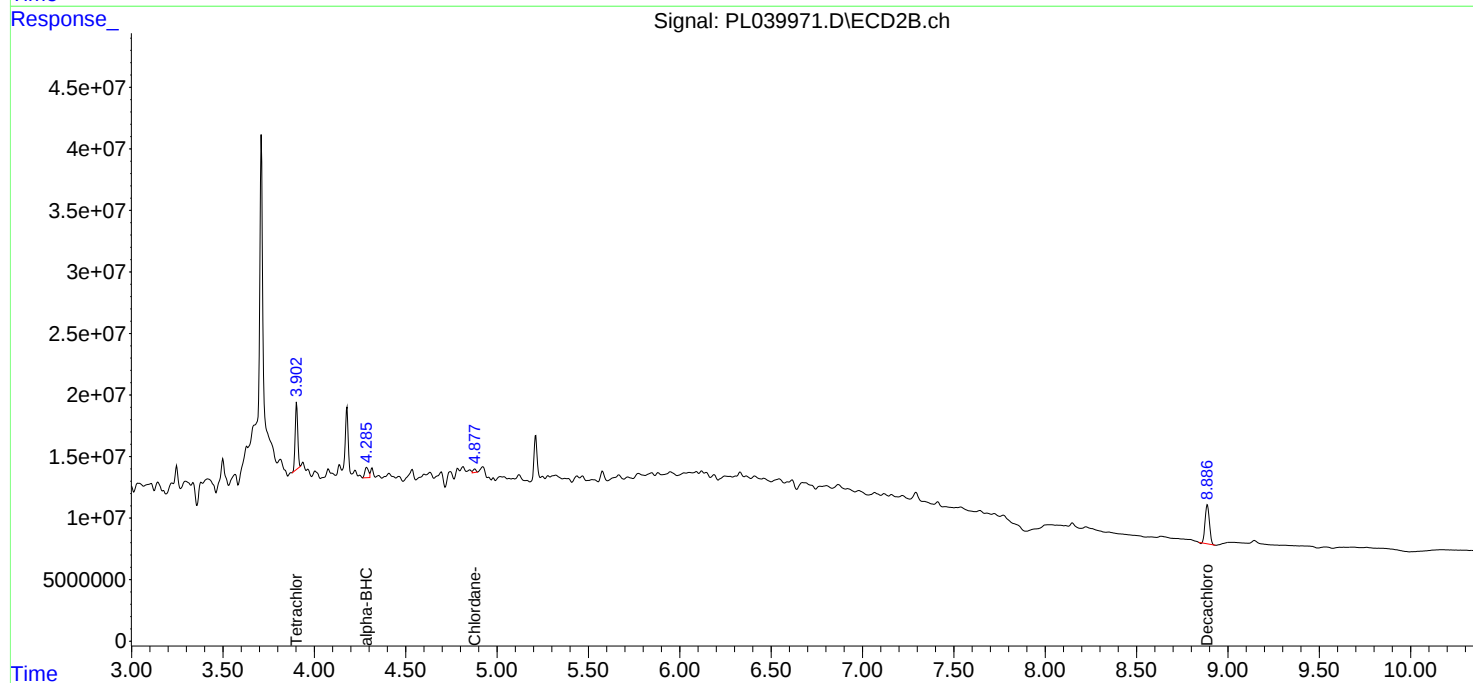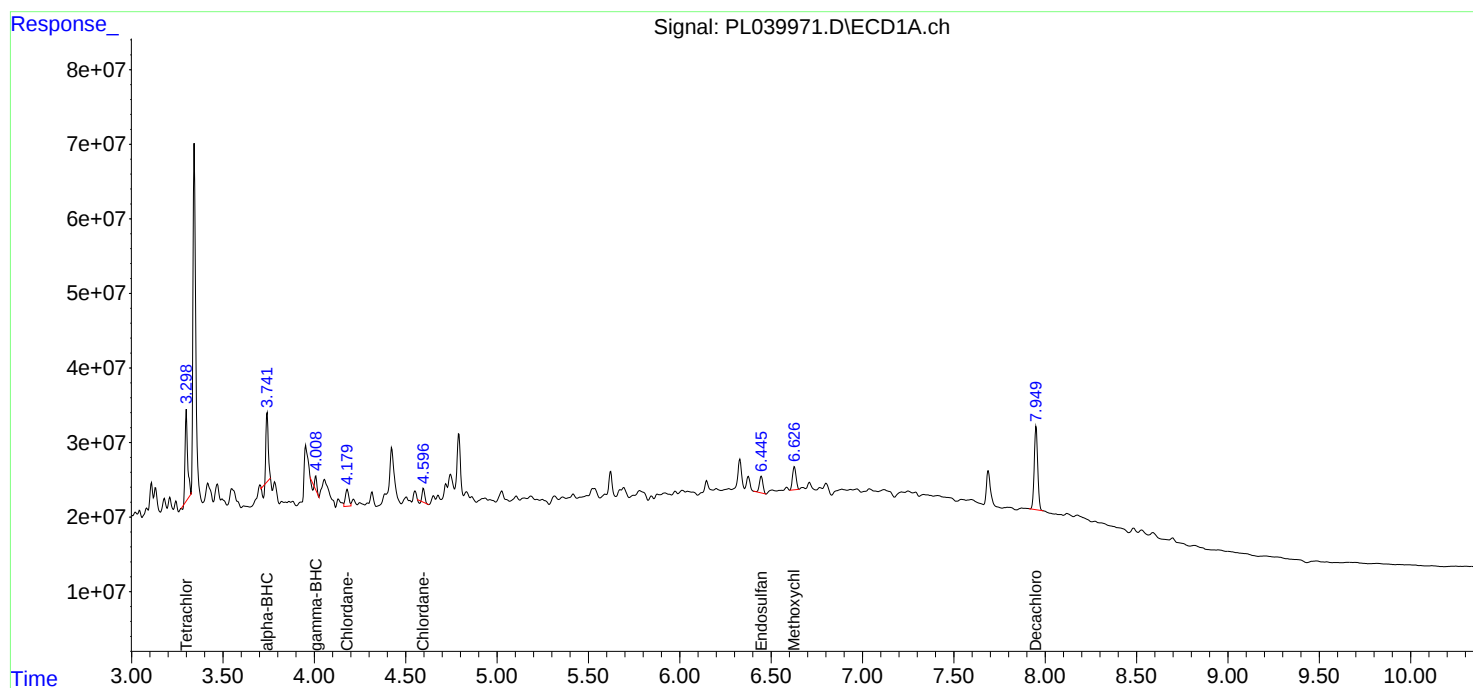


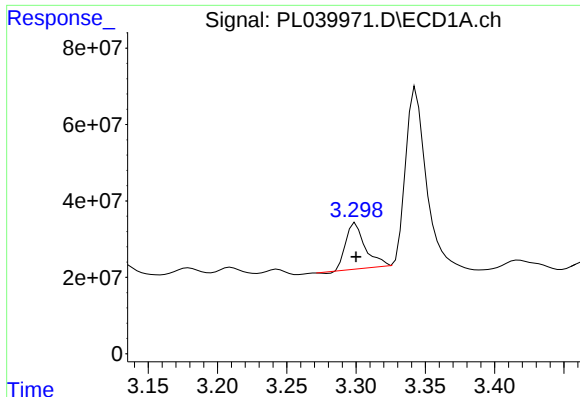

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 116489580
Conc: 15.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

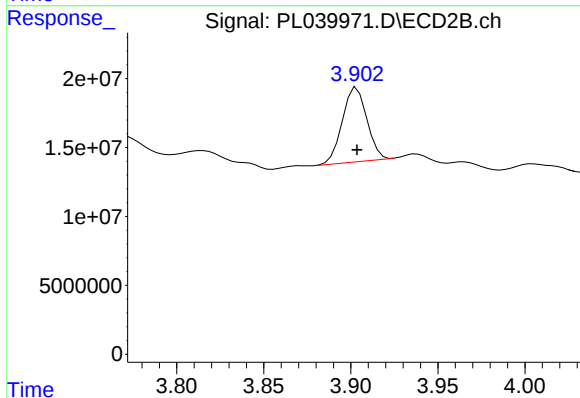


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 52886420
Conc: 16.57 ng/ml

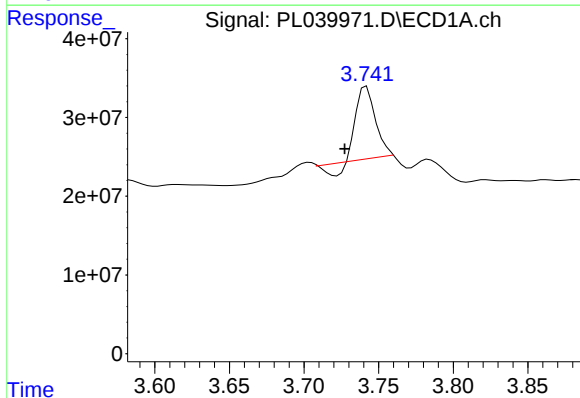


#2 alpha-BHC

R.T.: 3.742 min
Delta R.T.: 0.015 min
Response: 76963422
Conc: 6.07 ng/ml

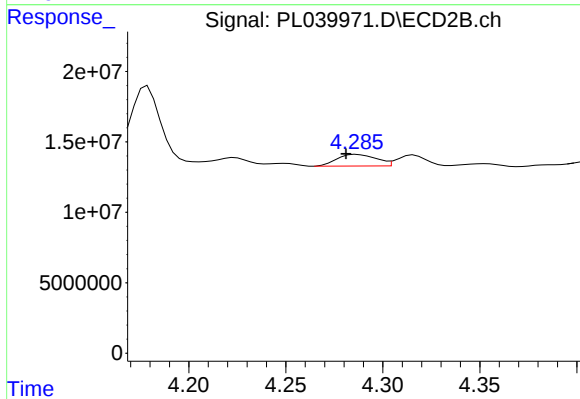

#2 alpha-BHC


R.T.: 4.287 min
Delta R.T.: 0.006 min
Response: 11661738
Conc: 2.25 ng/ml

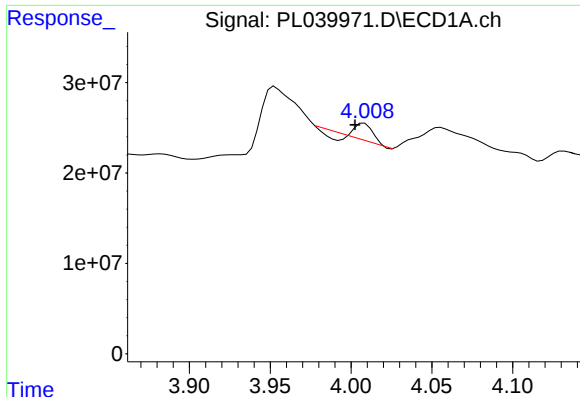

#3 gamma-BHC (Lindane)


R.T.: 4.008 min
Delta R.T.: 0.006 min
Response: 12191055
Conc: 1.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

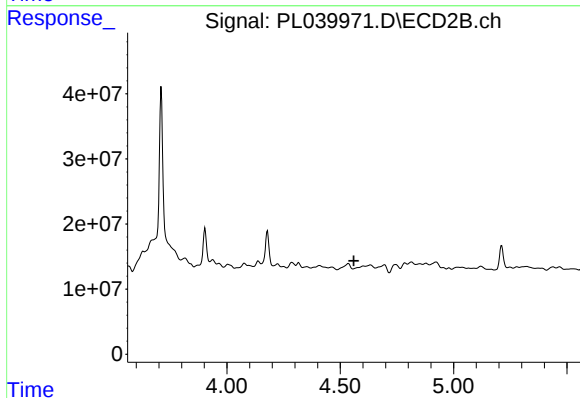


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

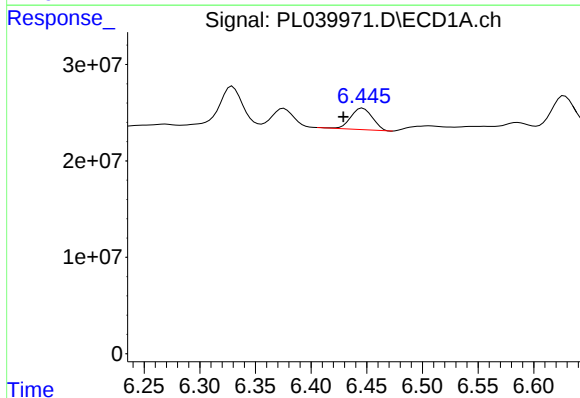


#19 Endosulfan Sulfate

R.T.: 6.446 min
Delta R.T.: 0.017 min
Response: 30359728
Conc: 3.31 ng/ml

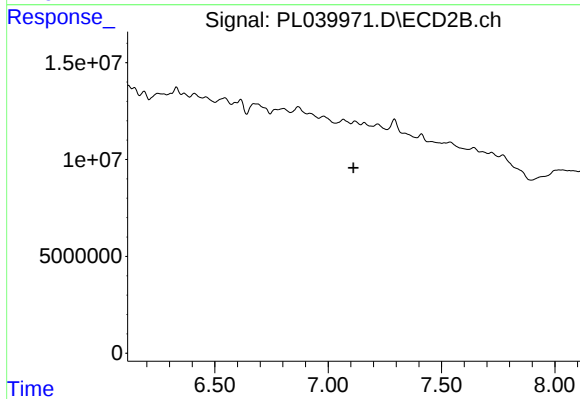

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.112 min
Response: 0
Conc: N.D.

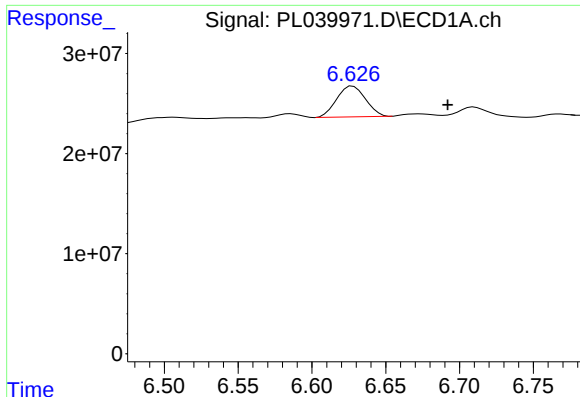

#20 Methoxychlor


R.T.: 6.628 min
Delta R.T.: -0.064 min
Response: 41909630
Conc: 9.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

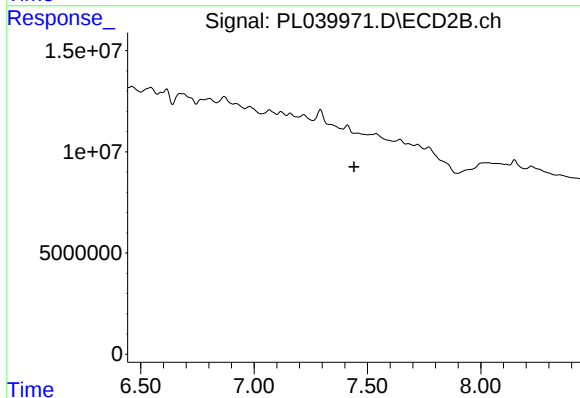


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.441 min
Response: 0
Conc: N.D.

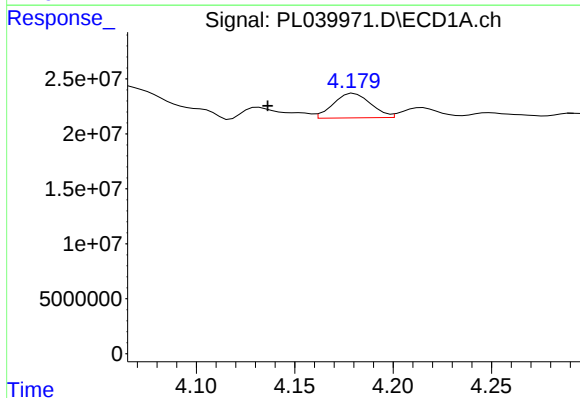


#23 Chlordane-1

R.T.: 4.180 min
Delta R.T.: 0.044 min
Response: 29682242
Conc: 81.90 ng/ml

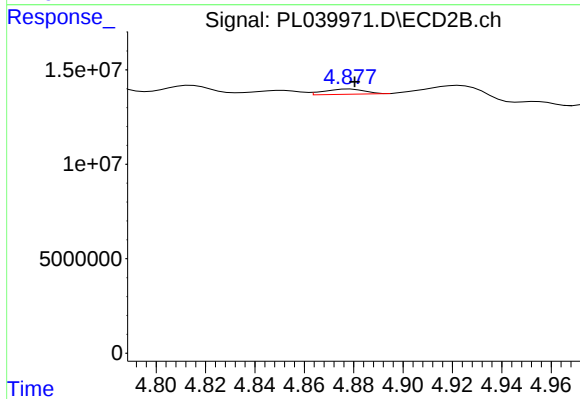

#23 Chlordane-1


R.T.: 4.879 min
Delta R.T.: -0.002 min
Response: 3155537
Conc: 20.38 ng/ml

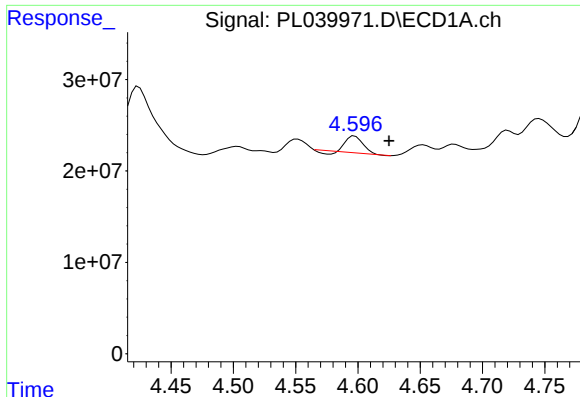

#24 Chlordane-2


R.T.: 4.597 min
Delta R.T.: -0.028 min
Response: 17078567
Conc: 45.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

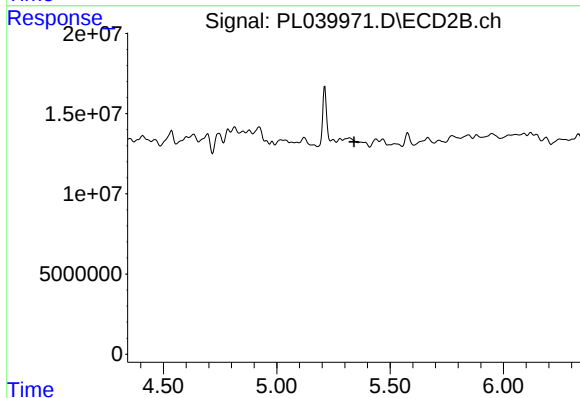


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.341 min
Response: 0
Conc: N.D.

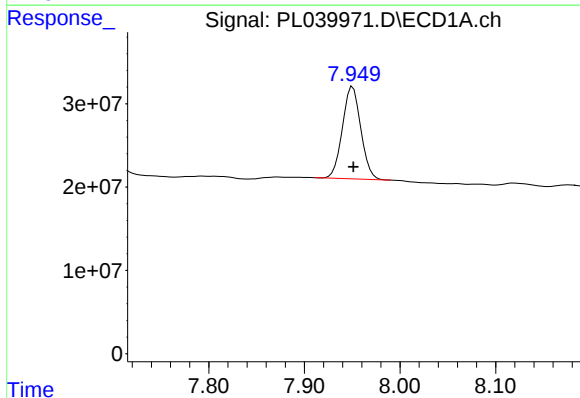

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 148086608
Conc: 17.77 ng/ml

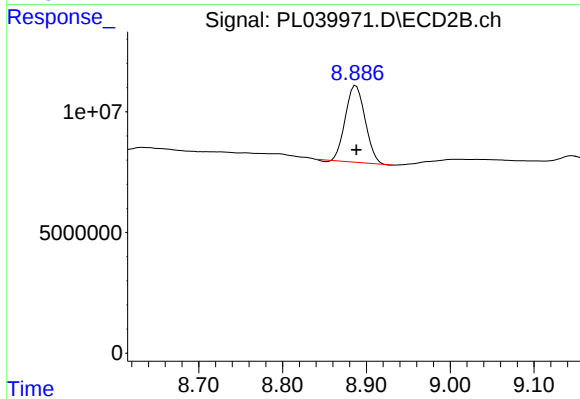

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 51604146
Conc: 19.00 ng/ml