

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
 Data File : PL039975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 15:02
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 00:55:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.299	3.904	135.4E6	58924457	17.455	18.467
28)	SA Decachlor...	7.951	8.888	156.4E6	58585837	18.765	21.570
Target Compounds							
10)	B gamma-Chl...	0.000	5.925f	0	940570	N.D.	0.249 #
25)	Chlordane-3	0.000	5.925	0	940570	N.D.	1.837 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091518\
Data File : PL039975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 15:02
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 00:55:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

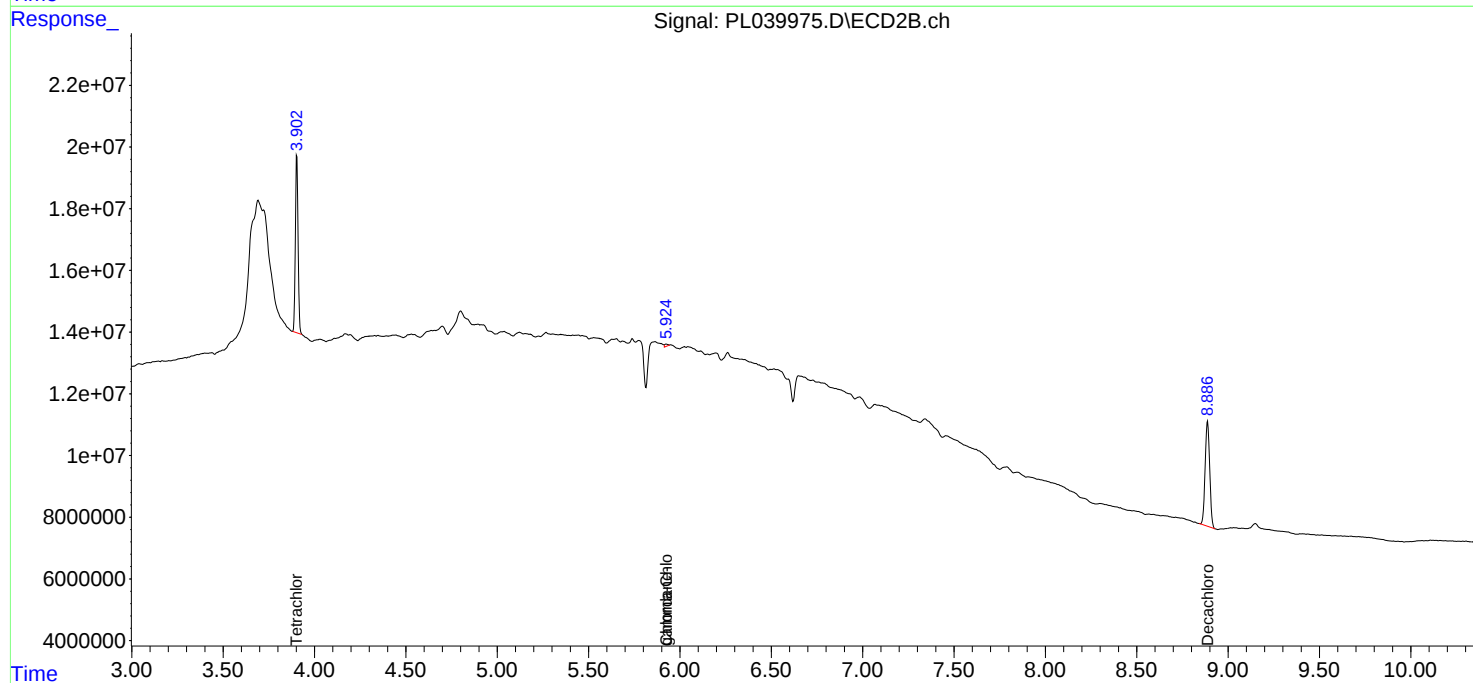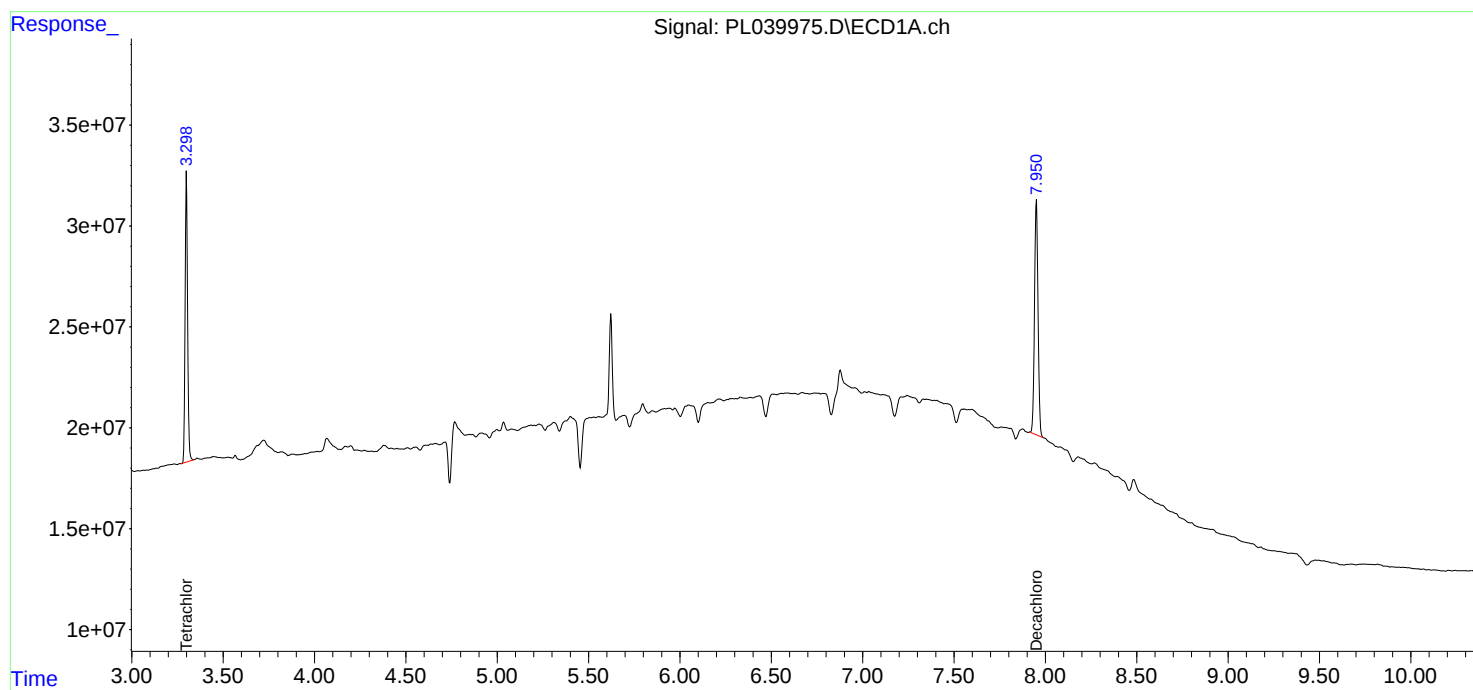


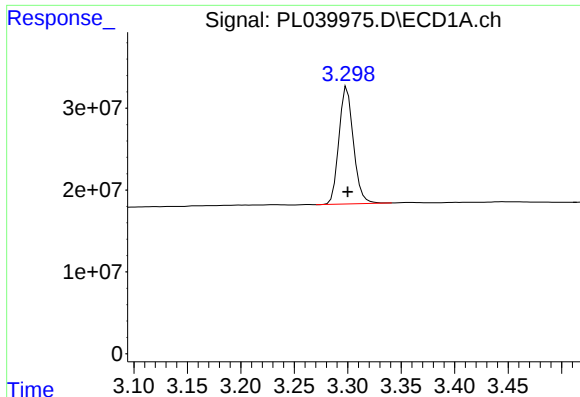

#1 Tetrachloro-m-xylene


R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 135362432
Conc: 17.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

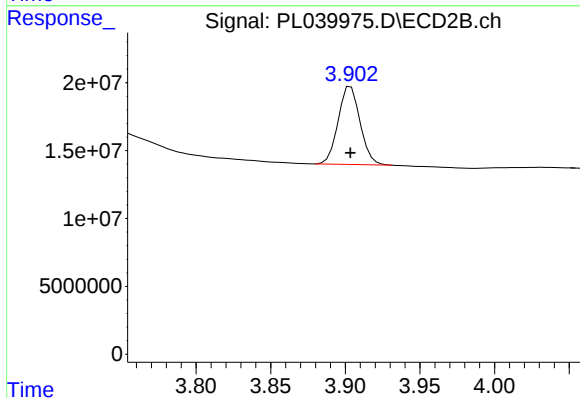


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 58924457
Conc: 18.47 ng/ml

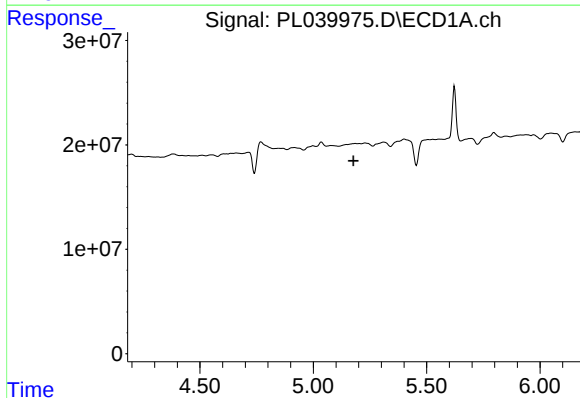


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

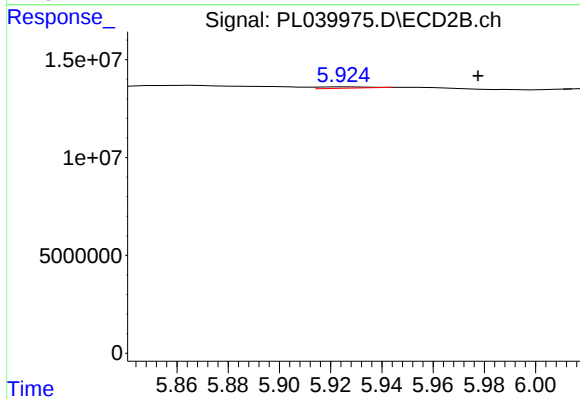

#10 gamma-Chlordane


R.T.: 5.925 min
Delta R.T.: -0.052 min
Response: 940570
Conc: 0.25 ng/ml

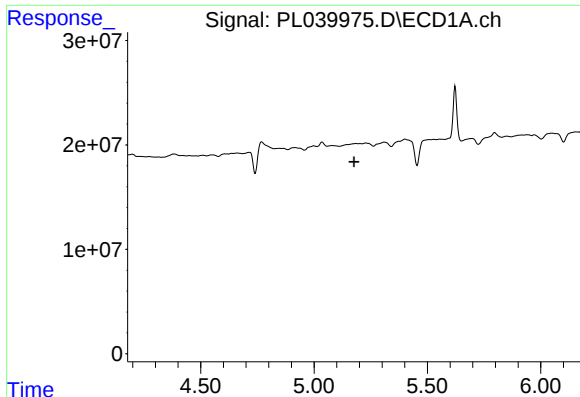

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

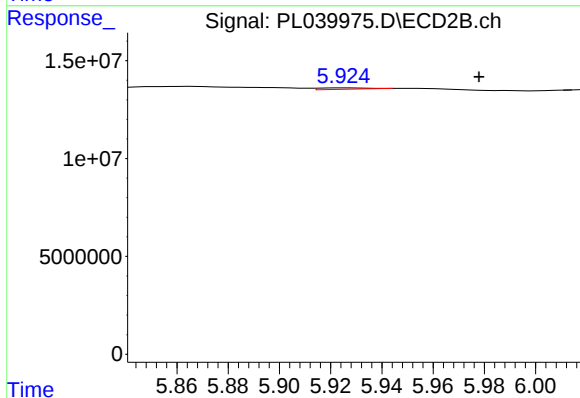


#25 Chlordane-3

R.T.: 5.925 min
Delta R.T.: -0.053 min
Response: 940570
Conc: 1.84 ng/ml

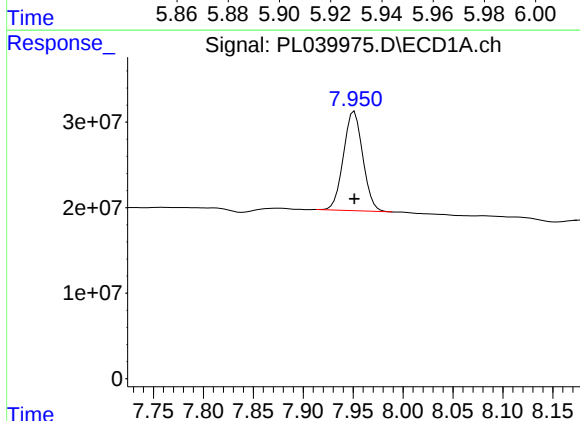

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 156361094
Conc: 18.76 ng/ml

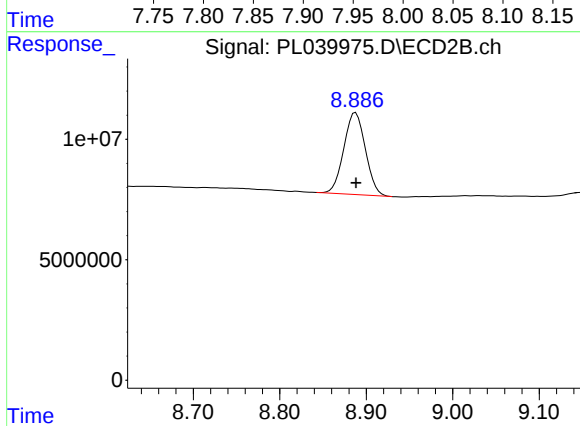

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 58585837
Conc: 21.57 ng/ml