

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
 Data File : PL061452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 10:02
 Operator : DD\AJ
 Sample : L3993-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B38-091120-10-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:32:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	37697007	64695246	21.857	21.032
28)	SA Decachlor...	8.209	9.092	29326395	42648276	17.578	18.036
Target Compounds							
8)	B Heptachlo...	0.000	5.880	0	19049086	N.D.	6.380 #
9)	A Endosulfan I	5.528f	6.247	4490449	14887576	2.610	4.641 #
11)	B alpha-Chl...	5.458	0.000	7543727	0	4.072	N.D. #
14)	MA Endrin	6.009	0.000	12223986	0	7.274	N.D. #
15)	B Endosulfa...	0.000	6.943	0	3849960	N.D.	1.303 #
21)	B Endrin ke...	0.000	7.742	0	6004173	N.D.	2.212 #
26)	Chlordane-4	5.458	0.000	7543727	0	54.805	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
Data File : PL061452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 10:02
Operator : DD\AJ
Sample : L3993-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:32:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

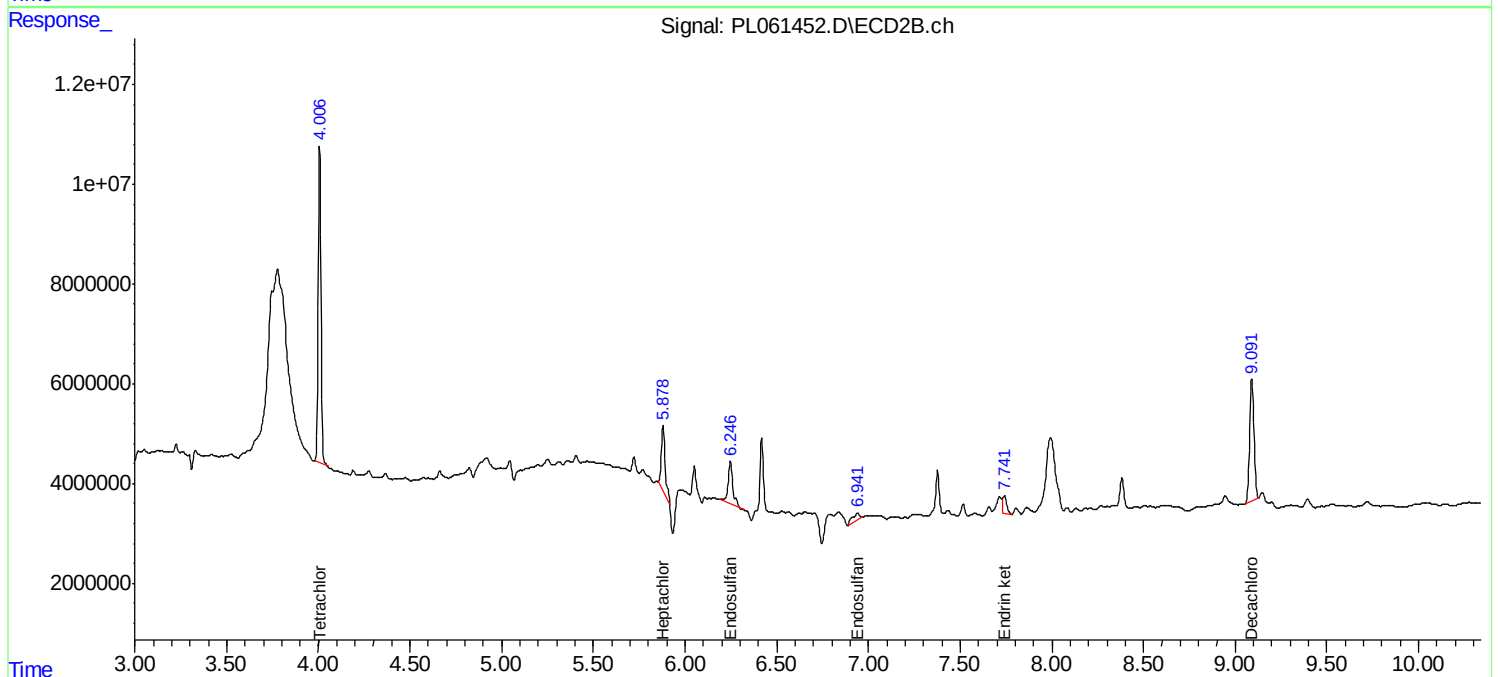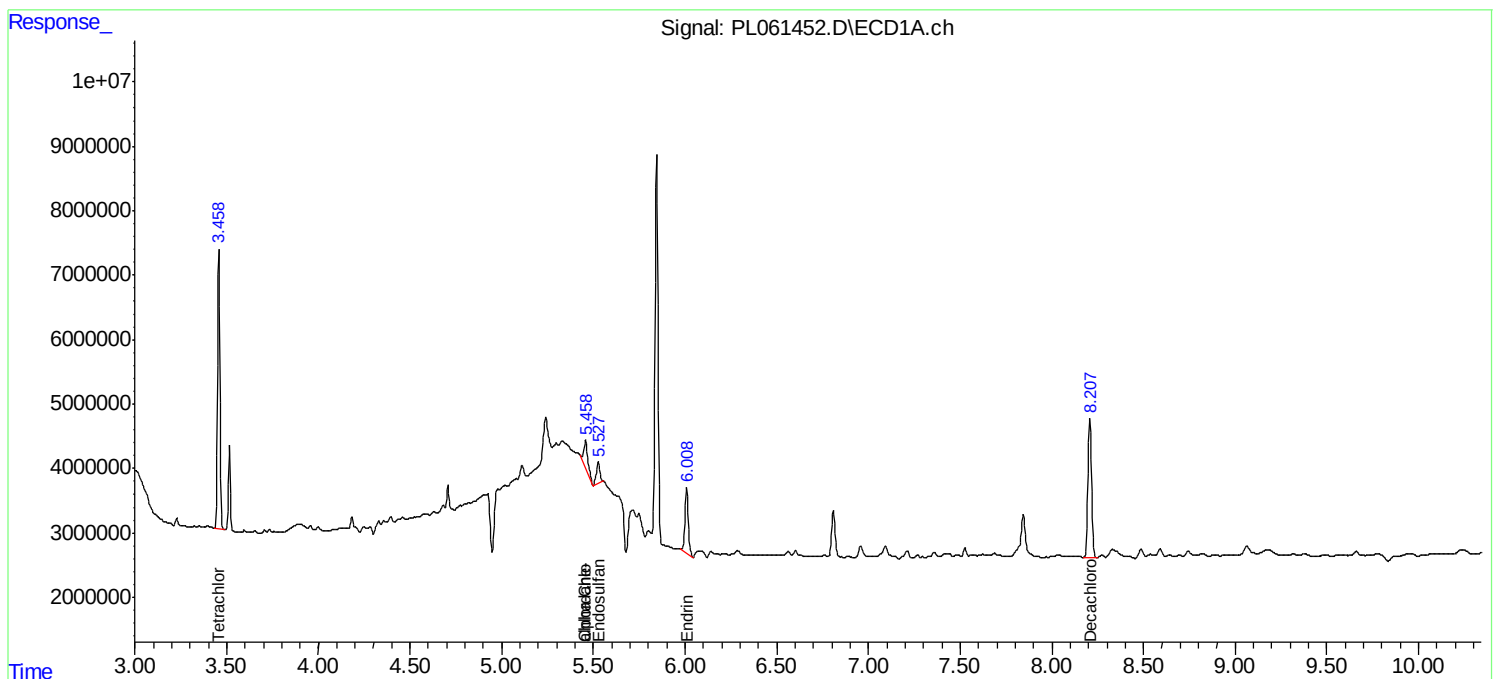


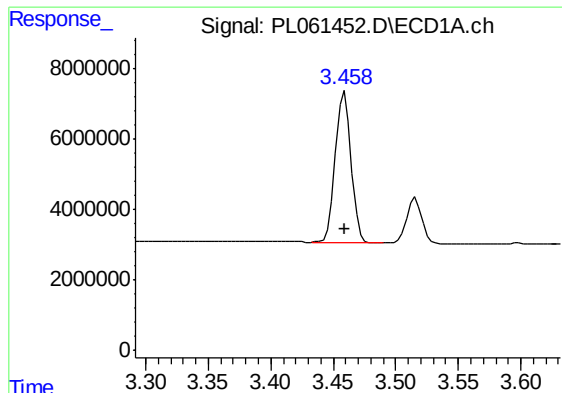

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 37697007
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

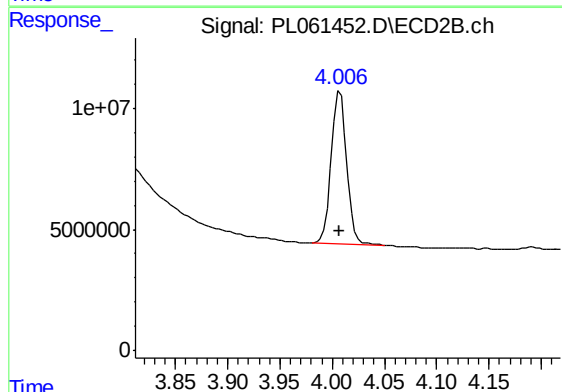


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 64695246
Conc: 21.03 ng/ml

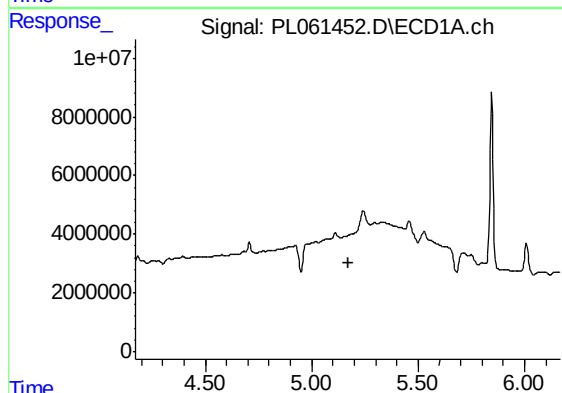


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.170 min
Response: 0
Conc: N.D.

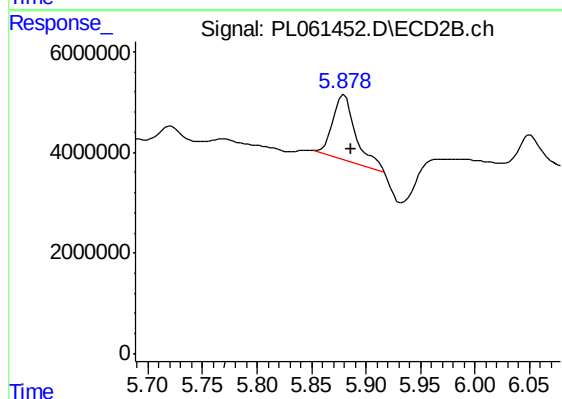

#8 Heptachlor epoxide


R.T.: 5.880 min
Delta R.T.: -0.006 min
Response: 19049086
Conc: 6.38 ng/ml

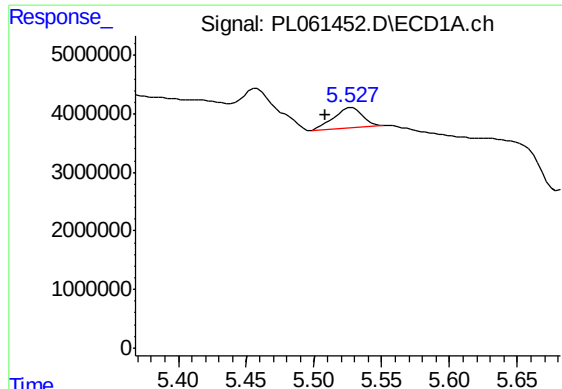

#9 Endosulfan I


R.T.: 5.528 min
Delta R.T.: 0.020 min
Response: 4490449
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

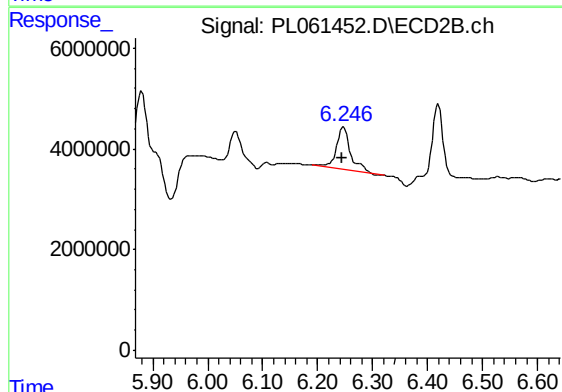


#9 Endosulfan I

R.T.: 6.247 min
Delta R.T.: 0.003 min
Response: 14887576
Conc: 4.64 ng/ml

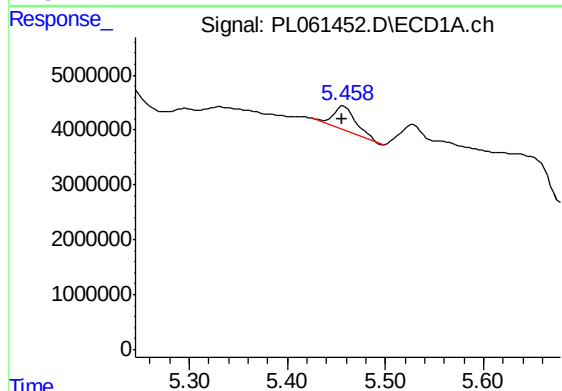


#11 alpha-Chlordane

R.T.: 5.458 min
Delta R.T.: 0.002 min
Response: 7543727
Conc: 4.07 ng/ml

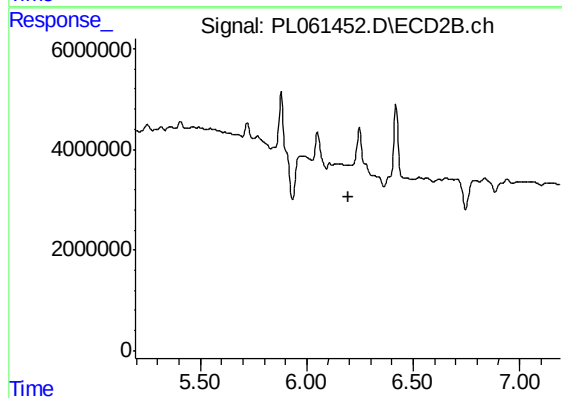

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.194 min
Response: 0
Conc: N.D.

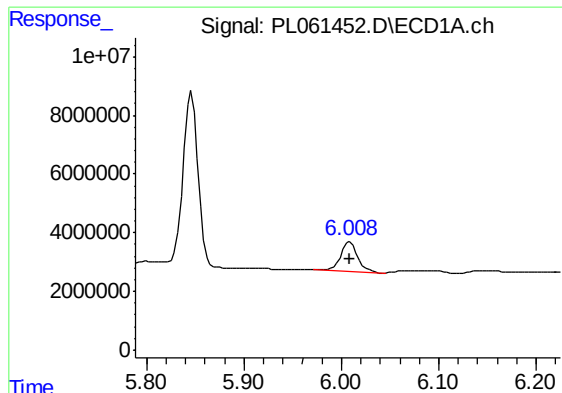

#14 Endrin


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 12223986
Conc: 7.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

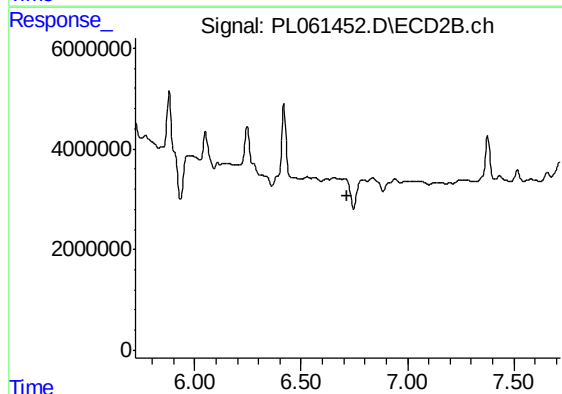


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.720 min
Response: 0
Conc: N.D.

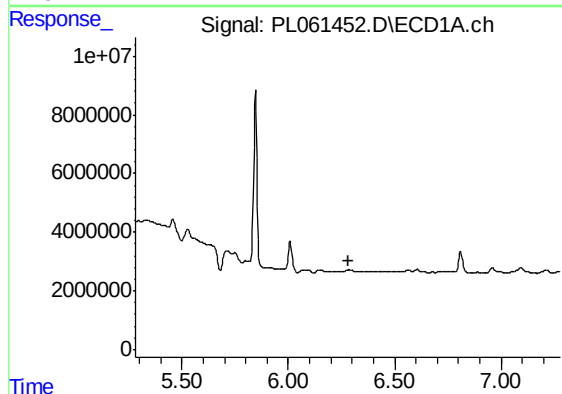


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

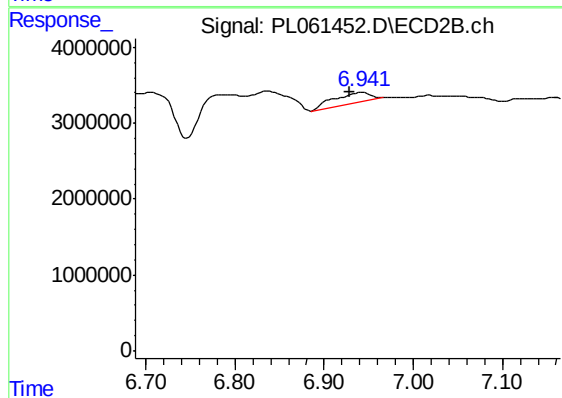

#15 Endosulfan II


R.T.: 6.943 min
Delta R.T.: 0.013 min
Response: 3849960
Conc: 1.30 ng/ml

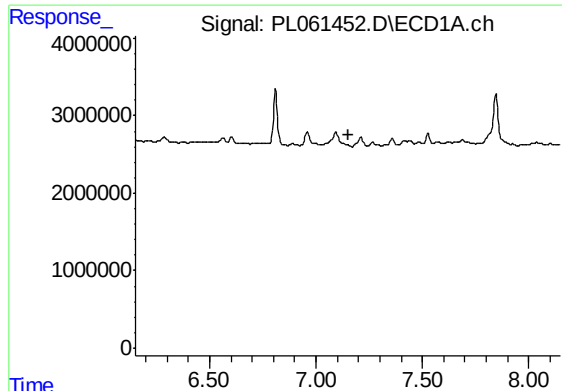

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

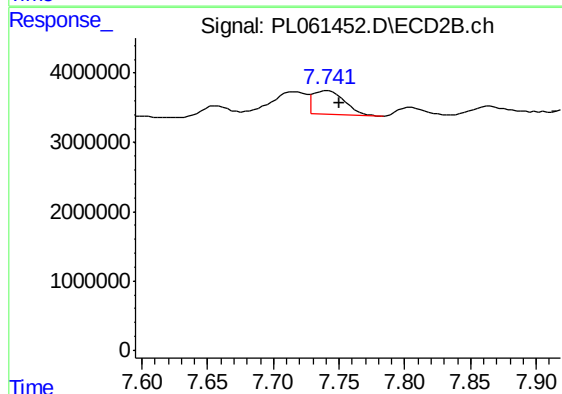


#21 Endrin ketone

R.T.: 7.742 min
Delta R.T.: -0.007 min
Response: 6004173
Conc: 2.21 ng/ml

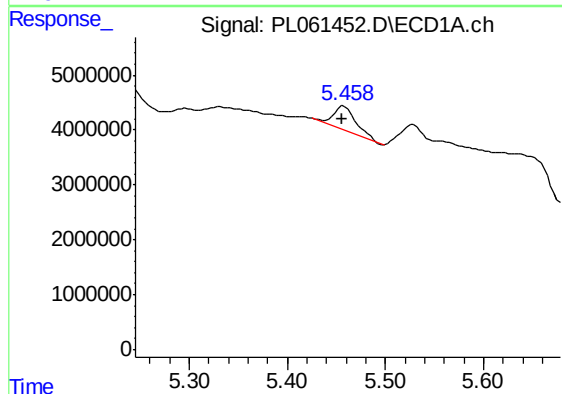


#26 Chlordane-4

R.T.: 5.458 min
Delta R.T.: 0.002 min
Response: 7543727
Conc: 54.81 ng/ml

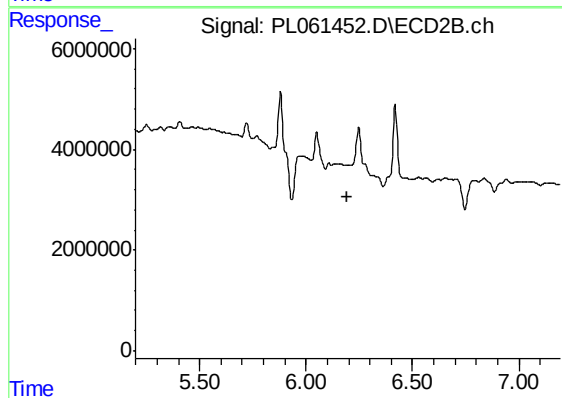

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.196 min
Response: 0
Conc: N.D.

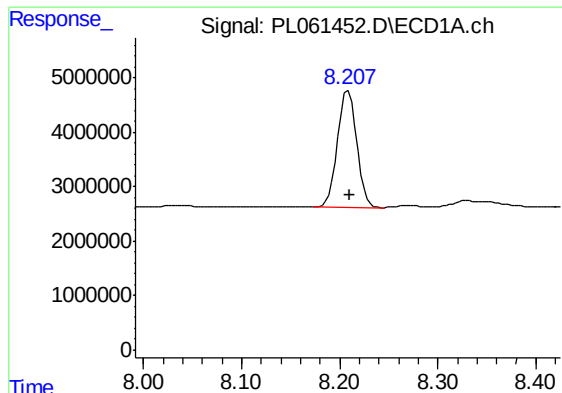

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 29326395
Conc: 17.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B38-091120-10-17

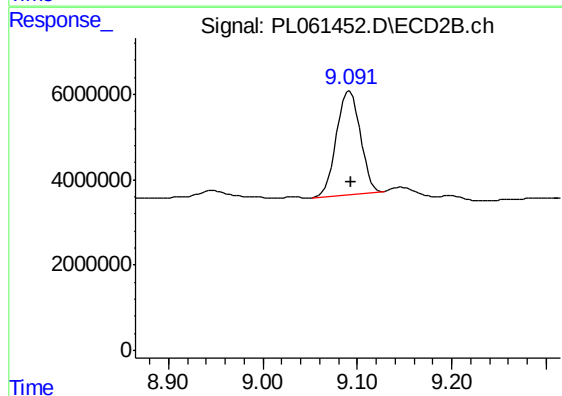

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.000 min
Response: 42648276
Conc: 18.04 ng/ml