

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
 Data File : PL061461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 13:29
 Operator : DD\AJ
 Sample : L3998-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-EF-01-TEST1-ABCD-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:34:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	24486744	40591083	14.198	13.196
28)	SA Decachlor...	8.210	9.092	19188082	30622895	11.501	12.951

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
Data File : PL061461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 13:29
Operator : DD\AJ
Sample : L3998-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-TEST1-ABCD-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:34:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

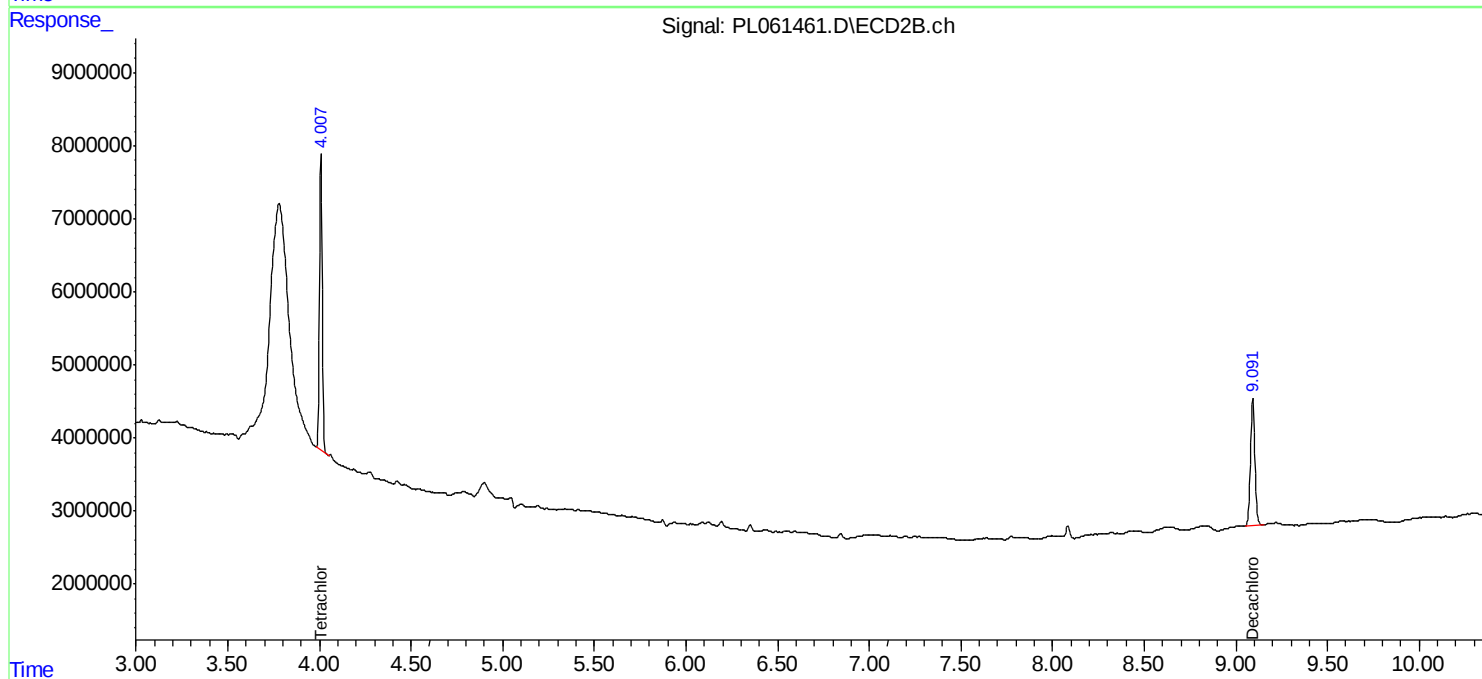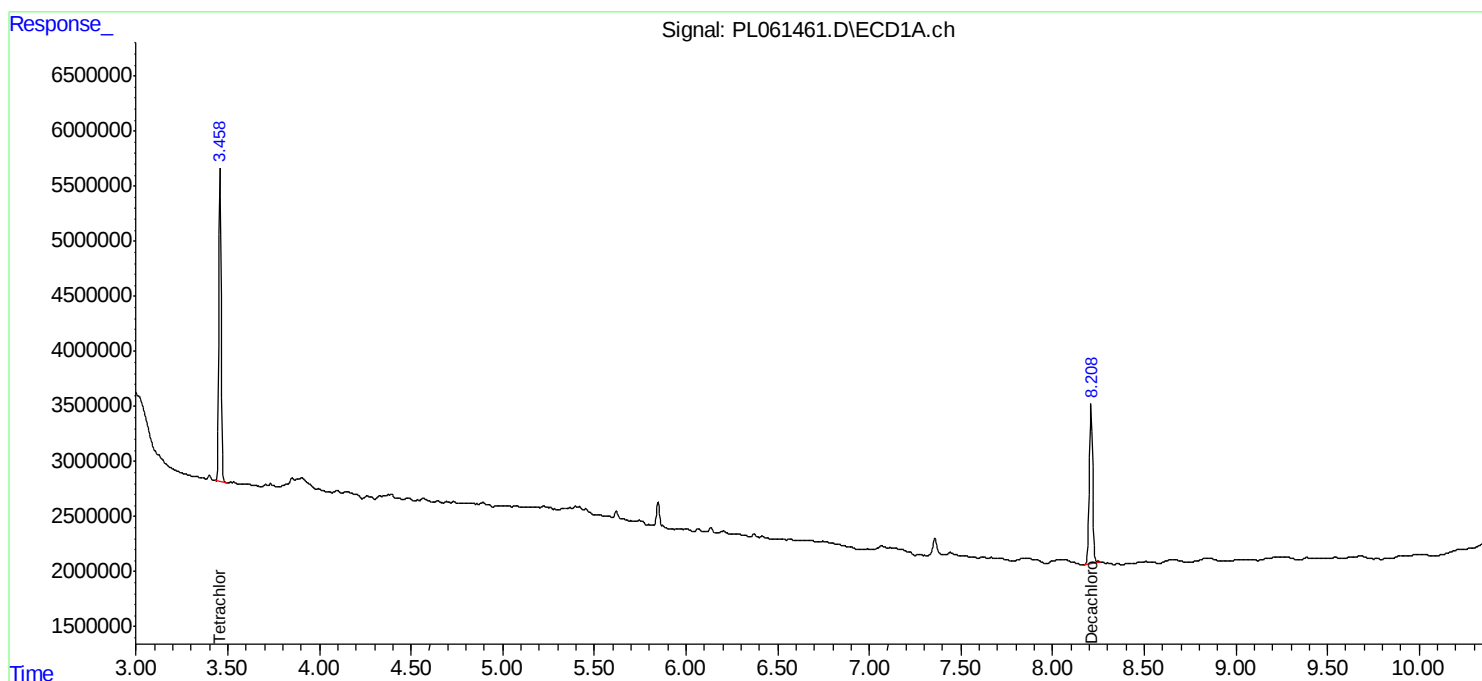


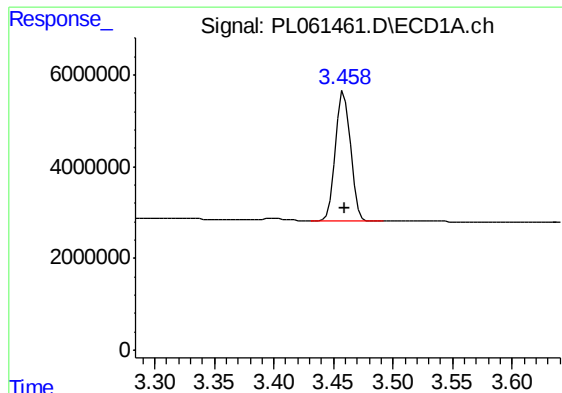

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 24486744
Conc: 14.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-TEST1-ABCD-A

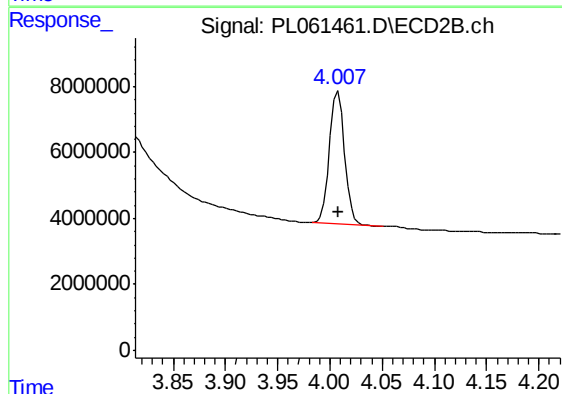


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 40591083
Conc: 13.20 ng/ml

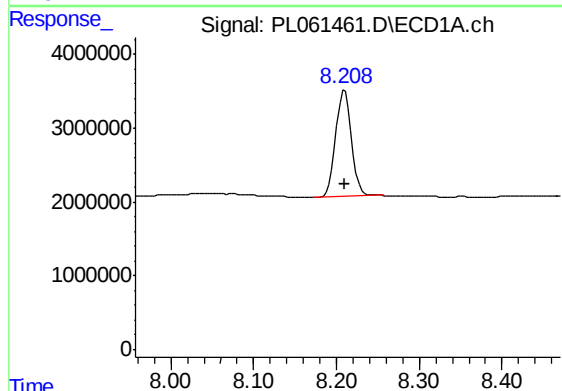

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 19188082
Conc: 11.50 ng/ml

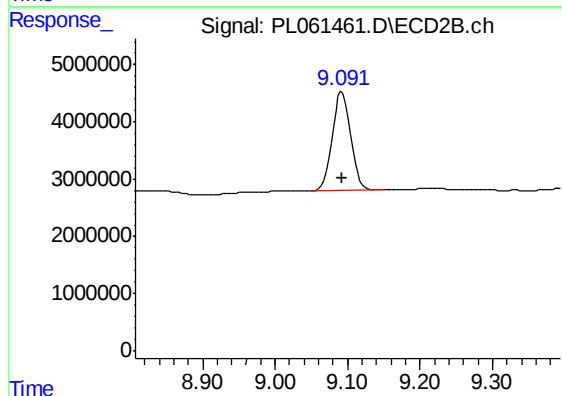

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.000 min
Response: 30622895
Conc: 12.95 ng/ml