

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
 Data File : PL061463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 13:57
 Operator : DD\AJ
 Sample : L3998-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-EF-01-TEST1-ABCD-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:35:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	39817180	69848281	23.087	22.708
28)	SA Decachlor...	8.210	9.094	25835419	41001618	15.486	17.340
Target Compounds							
12)	B 4,4'-DDE	0.000	6.351	0	2535208	N.D.	0.791 #
15)	B Endosulfa...	0.000	6.945f	0	3646516	N.D.	1.235 #
16)	A 4,4'-DDD	6.136	6.843	1859234	5631479	1.287	2.193 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
Data File : PL061463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 13:57
Operator : DD\AJ
Sample : L3998-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-TEST1-ABCD-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:35:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

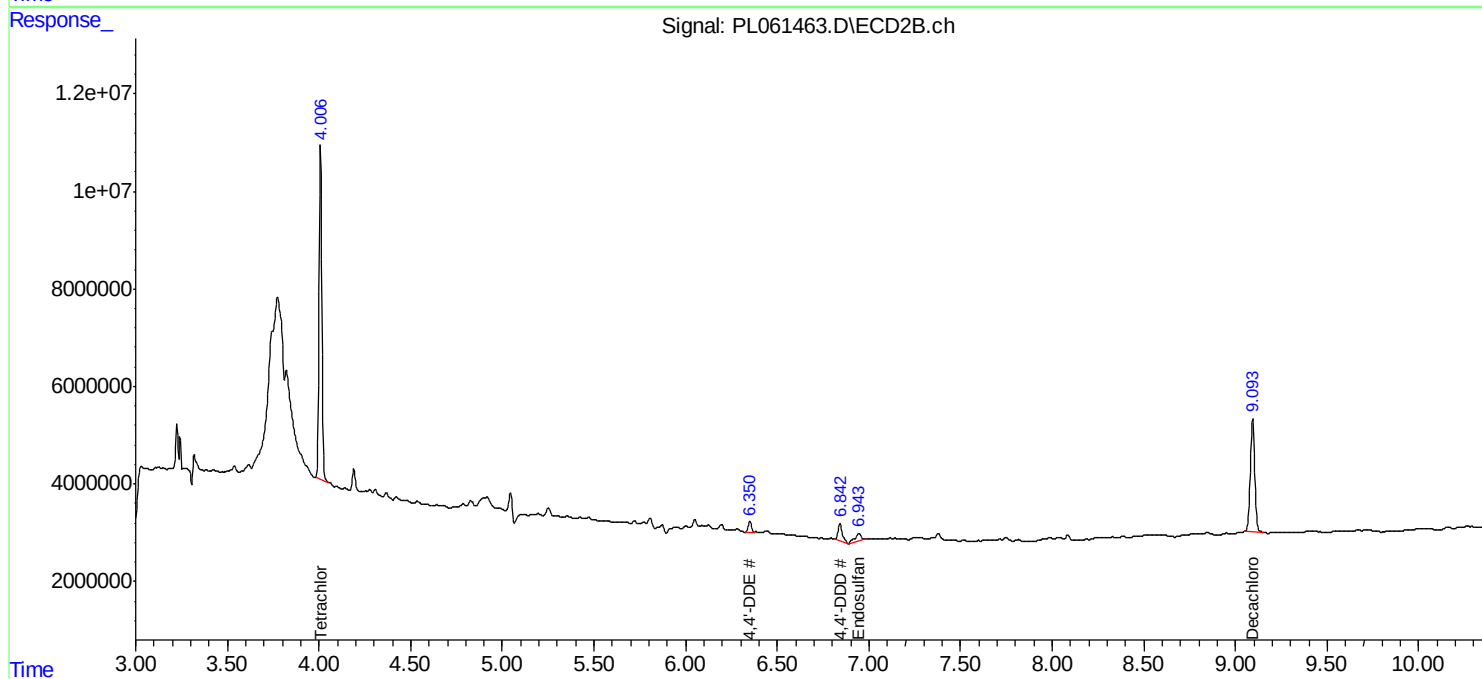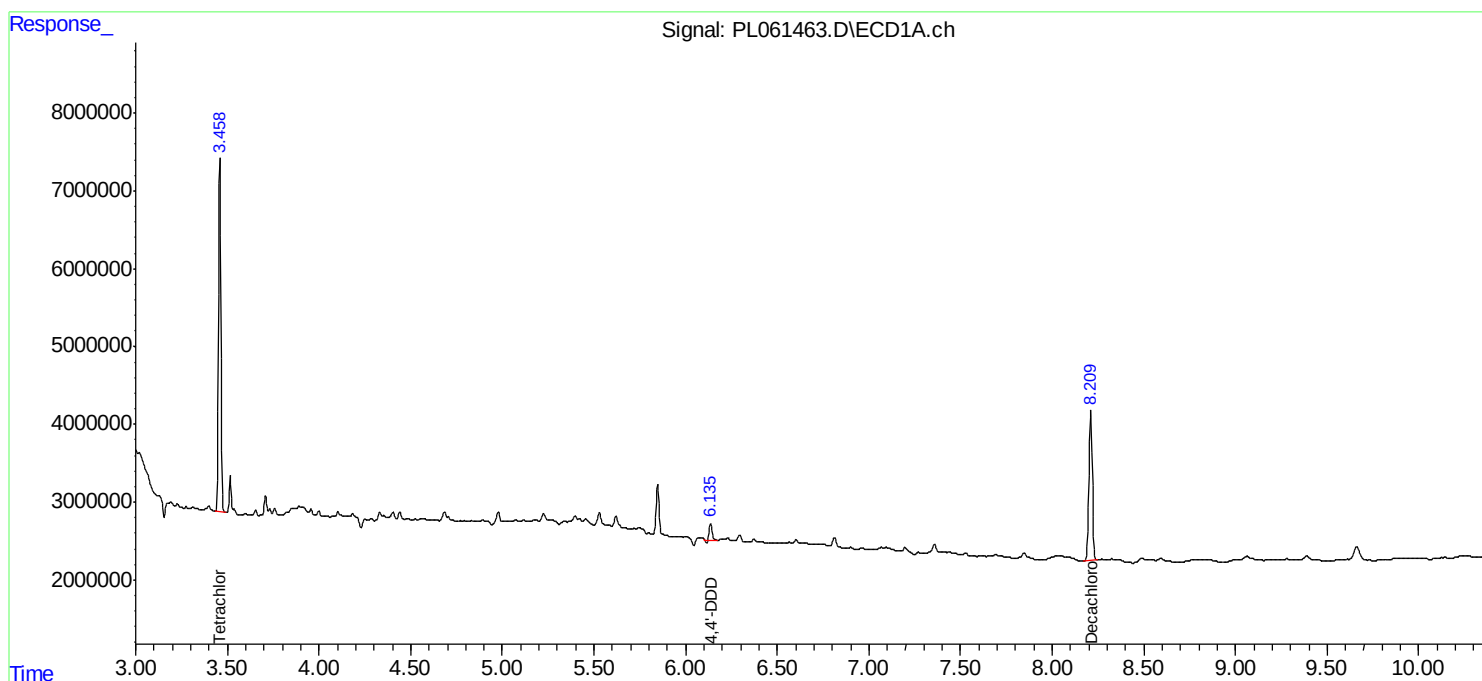


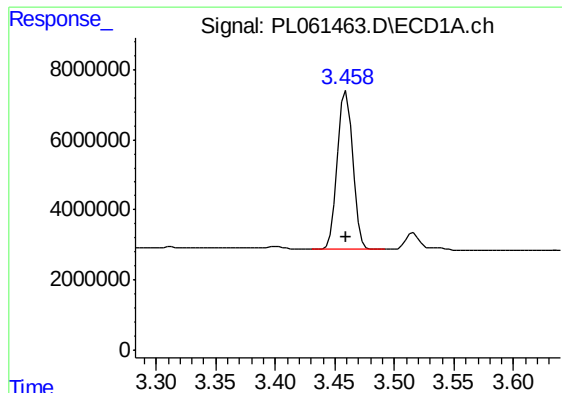

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 39817180
Conc: 23.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-TEST1-ABCD-B

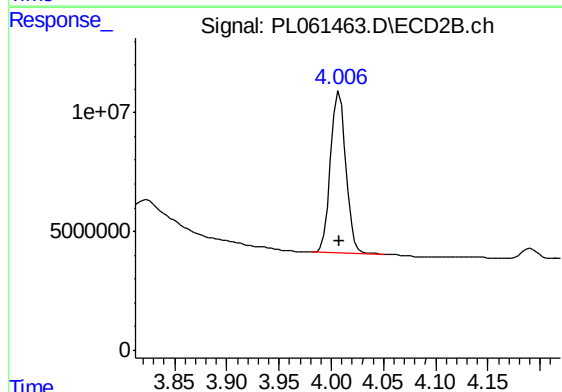


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 69848281
Conc: 22.71 ng/ml

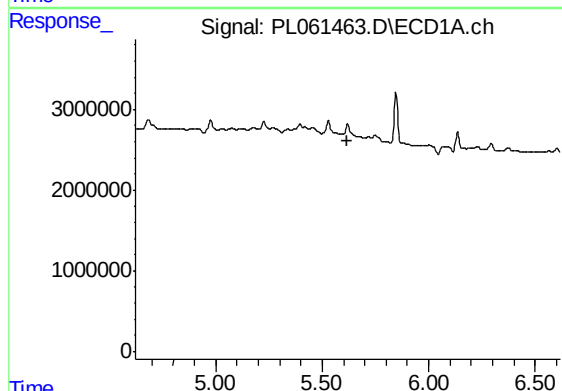


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.621 min
Response: 0
Conc: N.D.

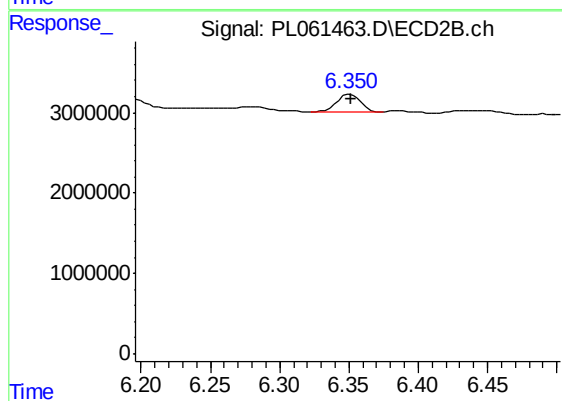

#12 4,4'-DDE


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 2535208
Conc: 0.79 ng/ml

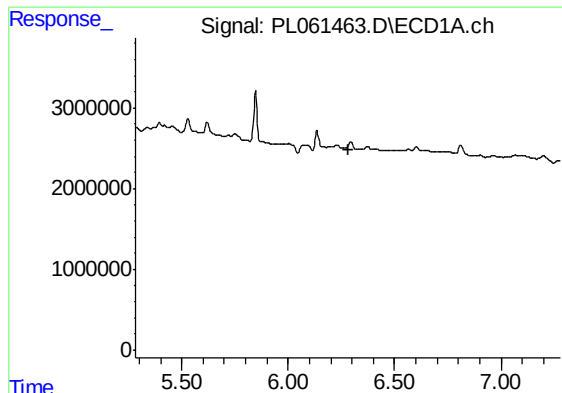

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-TEST1-ABCD-B

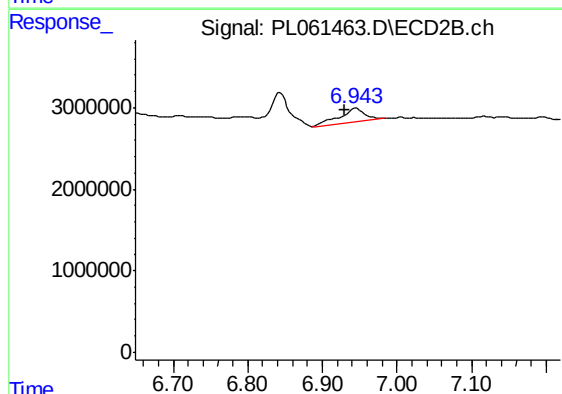


#15 Endosulfan II

R.T.: 6.945 min
Delta R.T.: 0.016 min
Response: 3646516
Conc: 1.23 ng/ml

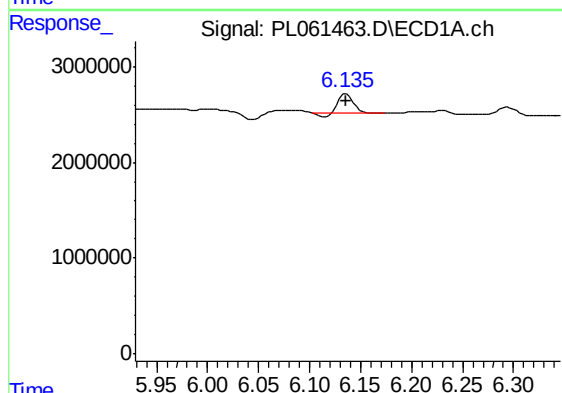


#16 4,4'-DDD

R.T.: 6.136 min
Delta R.T.: 0.000 min
Response: 1859234
Conc: 1.29 ng/ml

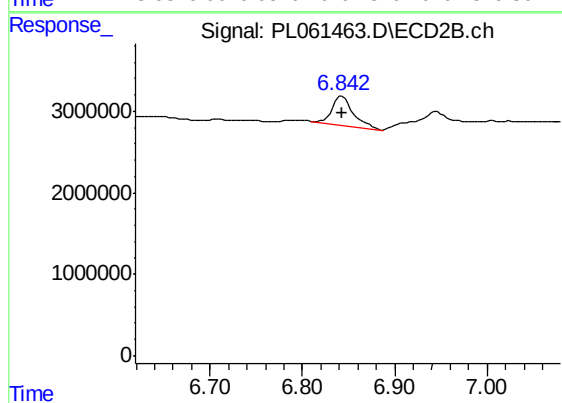

#16 4,4'-DDD


R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 5631479
Conc: 2.19 ng/ml

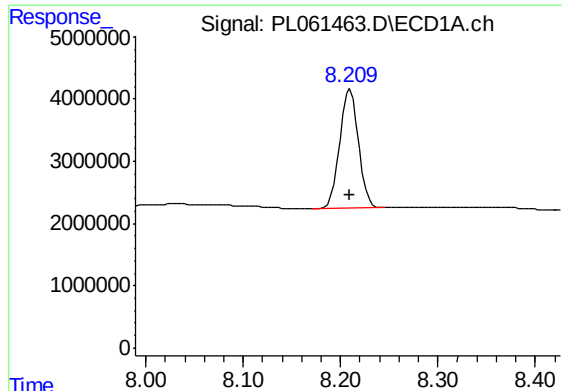

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 25835419
Conc: 15.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-TEST1-ABCD-B

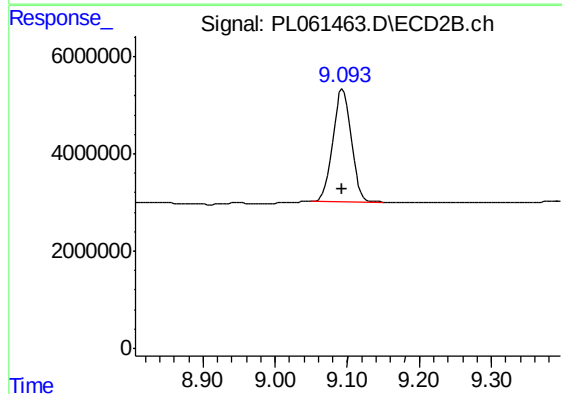

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.001 min
Response: 41001618
Conc: 17.34 ng/ml