

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
 Data File : PL061460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 13:15
 Operator : DD\AJ
 Sample : L3871-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-091420

Manual Integrations
 APPROVED

Ankita
 9/16/2020 1:54:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:34:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	4.007	25155495	39248783	14.586	12.760
28) SA Decachlor...	8.209	9.093	19990071	29360148	11.982	12.417
Target Compounds						
12) B 4,4'-DDE	5.620	6.351	3760190	6280346	2.211	1.959
17) MA 4,4'-DDT	6.372	7.141	1659314	1787874	1.208m	0.714m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
Data File : PL061460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 13:15
Operator : DD\AJ
Sample : L3871-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-04-091420


Manual Integrations
APPROVED

Ankita
9/16/2020 1:54:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:34:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

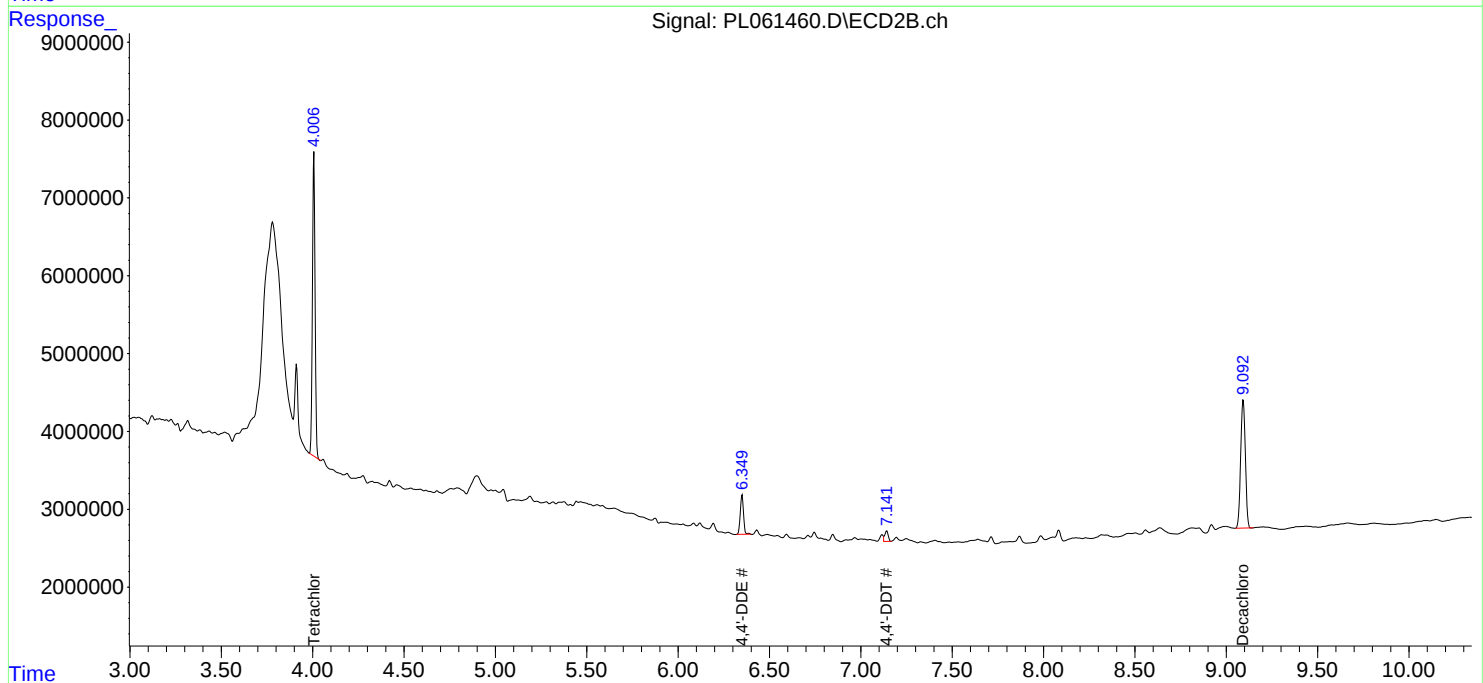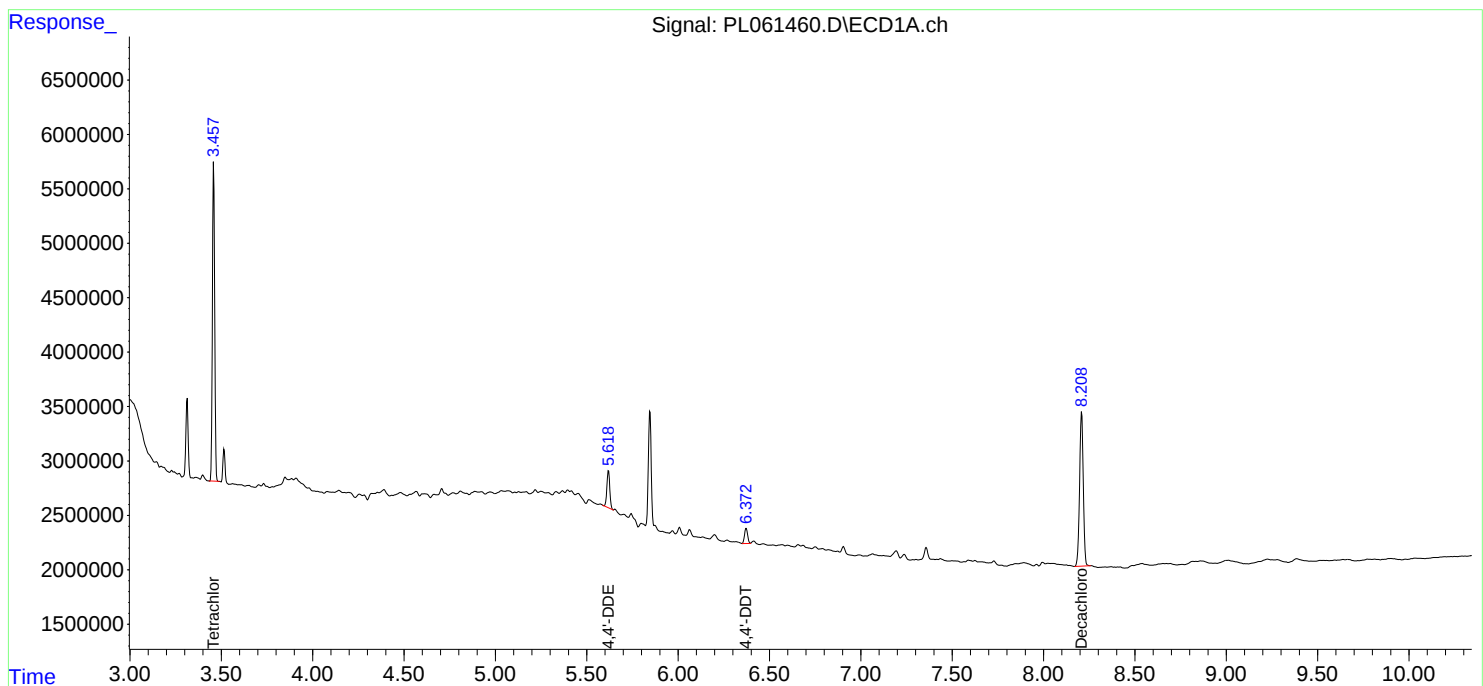

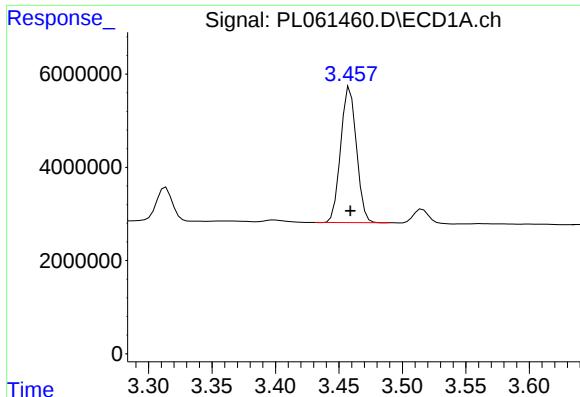


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 25155495
Conc: 14.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-091420


Manual Integrations
APPROVED

Ankita
9/16/2020 1:54:18 PM

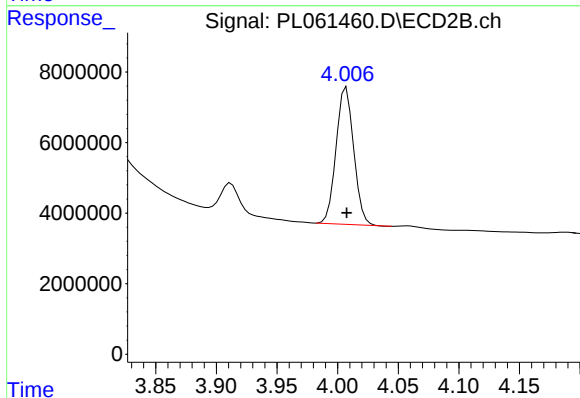


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 39248783
Conc: 12.76 ng/ml

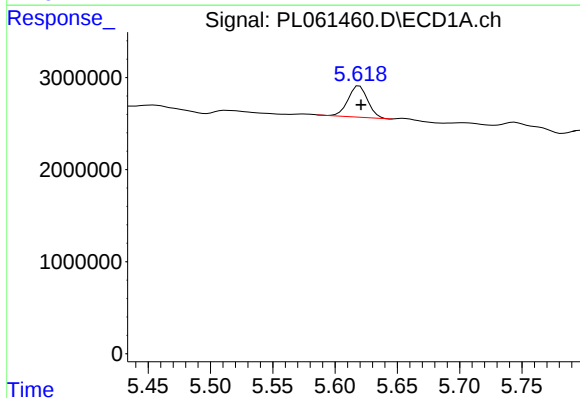


#12 4,4'-DDE

R.T.: 5.620 min
Delta R.T.: -0.001 min
Response: 3760190
Conc: 2.21 ng/ml

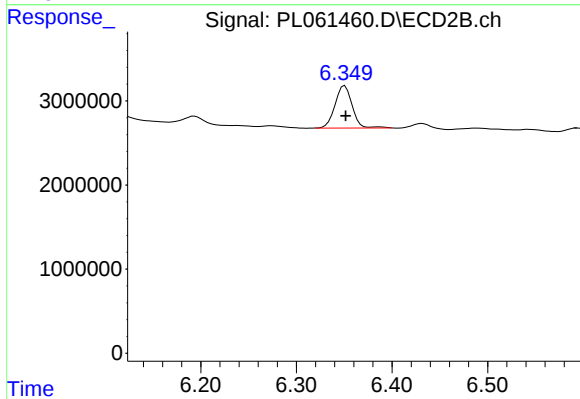

#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: -0.001 min
Response: 6280346
Conc: 1.96 ng/ml

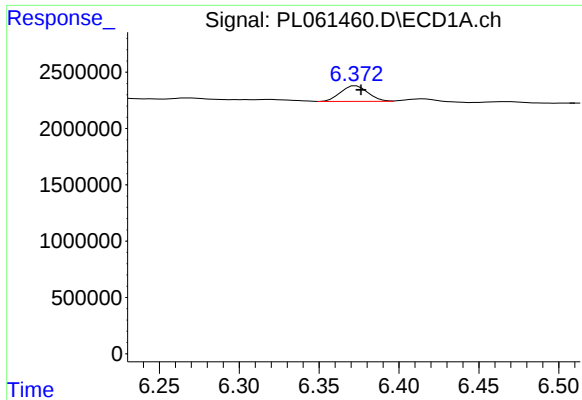


#17 4,4'-DDT

R.T.: 6.372 min
Delta R.T.: -0.004 min
Response: 1659314
Conc: 1.21 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-04-091420


Manual Integrations
APPROVED

Ankita
9/16/2020 1:54:18 PM

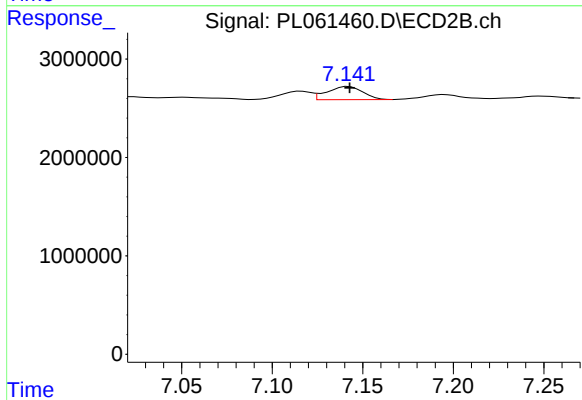


#17 4,4'-DDT

R.T.: 7.141 min
Delta R.T.: -0.002 min
Response: 1787874
Conc: 0.71 ng/ml m

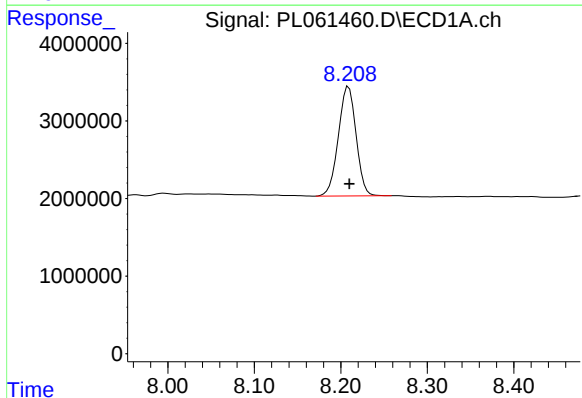

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 19990071
Conc: 11.98 ng/ml

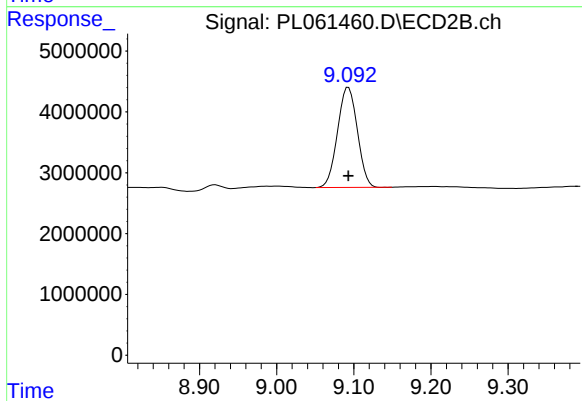

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 29360148
Conc: 12.42 ng/ml