

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
 Data File : PL061485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 19:22
 Operator : DD\AJ
 Sample : L3871-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-091420

Manual Integrations
 APPROVED

Ankita
 9/16/2020 1:54:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:42:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.030f	35779670	63057669	20.746	20.500m
28)	SA Decachlor...	8.210	9.116f	31173232	47553798	18.685	20.111m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091520\
Data File : PL061485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 19:22
Operator : DD\AJ
Sample : L3871-10
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-04-091420


Manual Integrations
APPROVED

Ankita
9/16/2020 1:54:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:42:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

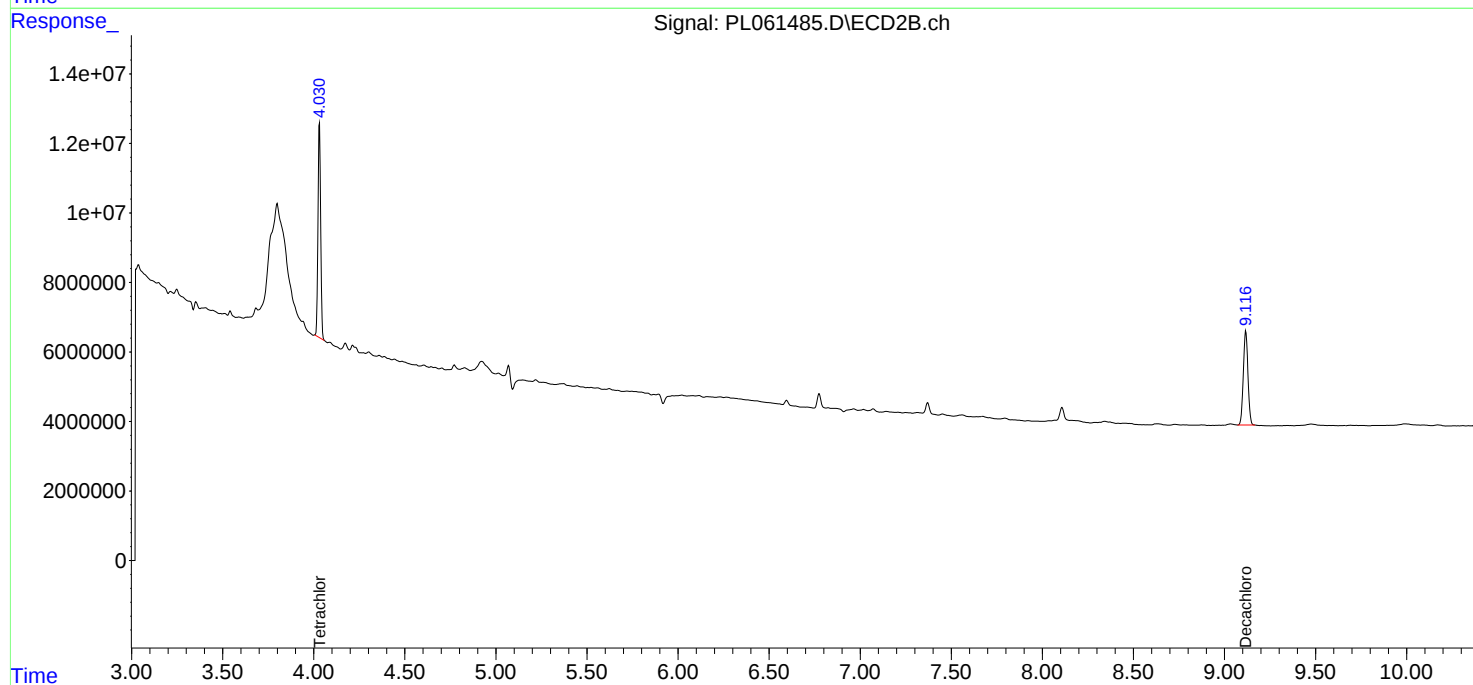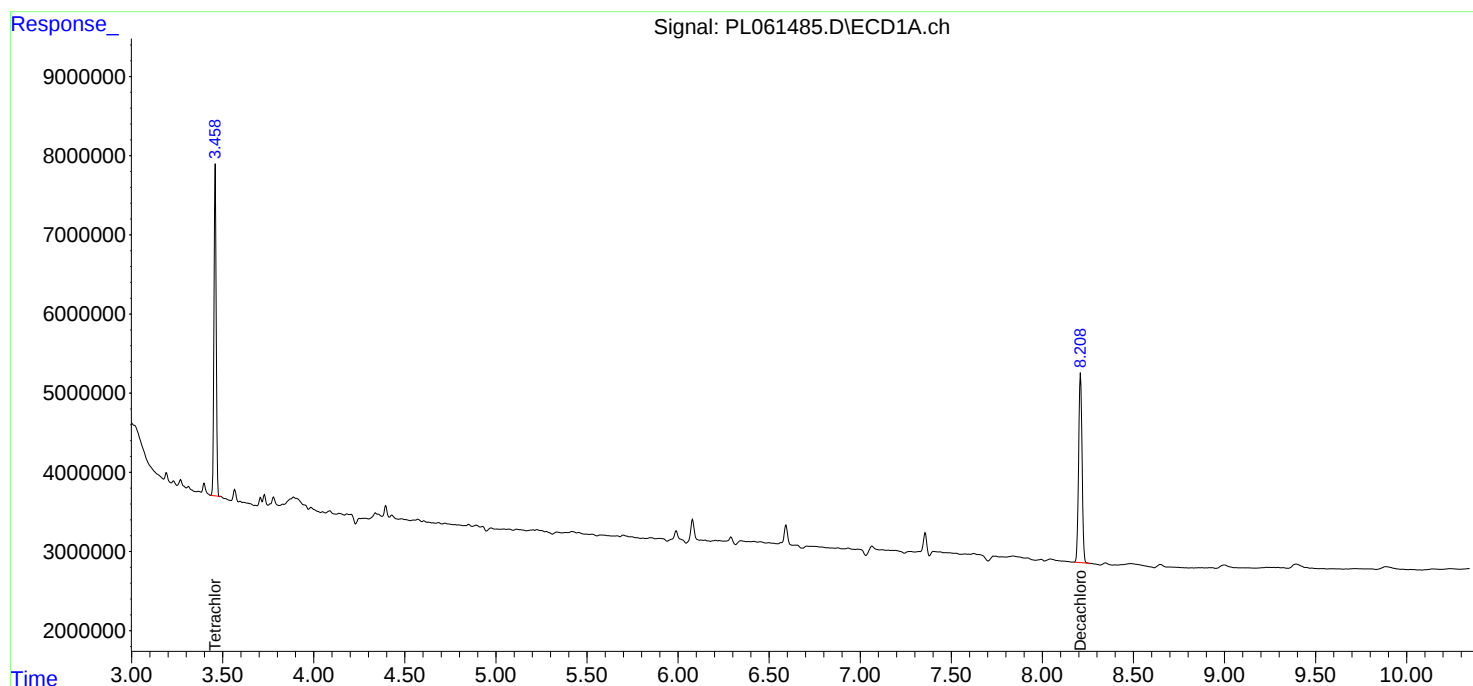

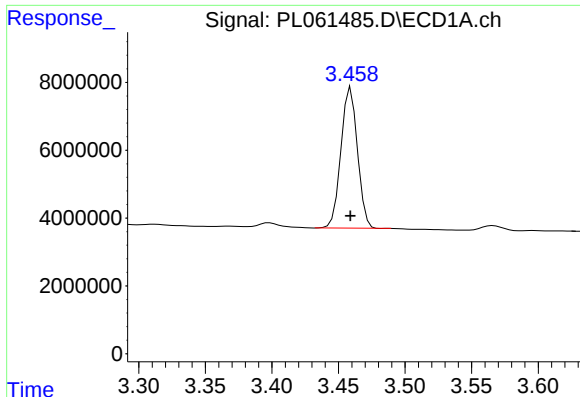


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 35779670
Conc: 20.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-091420


Manual Integrations
APPROVED

Ankita
9/16/2020 1:54:27 PM

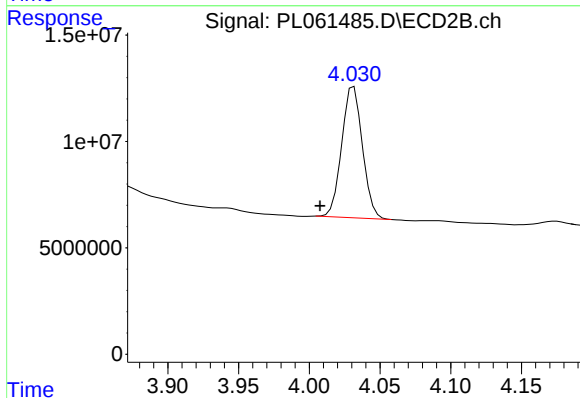


#1 Tetrachloro-m-xylene

R.T.: 4.030 min
Delta R.T.: 0.023 min
Response: 63057669
Conc: 20.50 ng/ml m

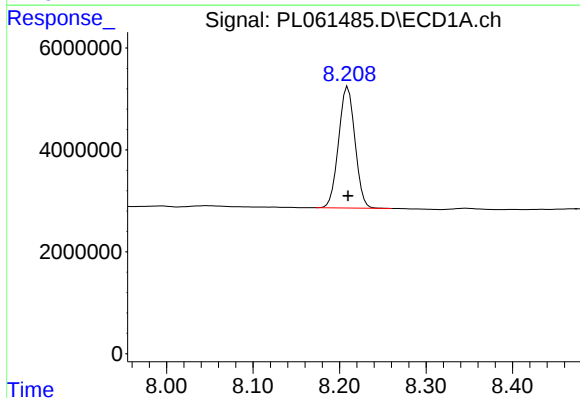

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 31173232
Conc: 18.69 ng/ml

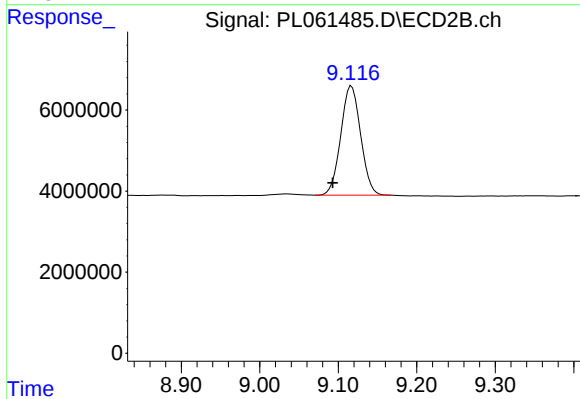

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.023 min
Response: 47553798
Conc: 20.11 ng/ml m