

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091521\
 Data File : PL069853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 09:26
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 04:45:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	8.038	0	695376	N.D. 0.542 #
9) A	Endosulfan I	0.000	8.425	0	22439	N.D. 0.017 #
11) B	alpha-Chl...	0.000	8.397f	0	131559	N.D. 0.097 #
23)	Chlordane-1	0.000	6.976f	0	372373	N.D. 9.072 #
26)	Chlordane-4	0.000	8.397	0	131559	N.D. 0.565 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091521\
Data File : PL069853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 09:26
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 04:45:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

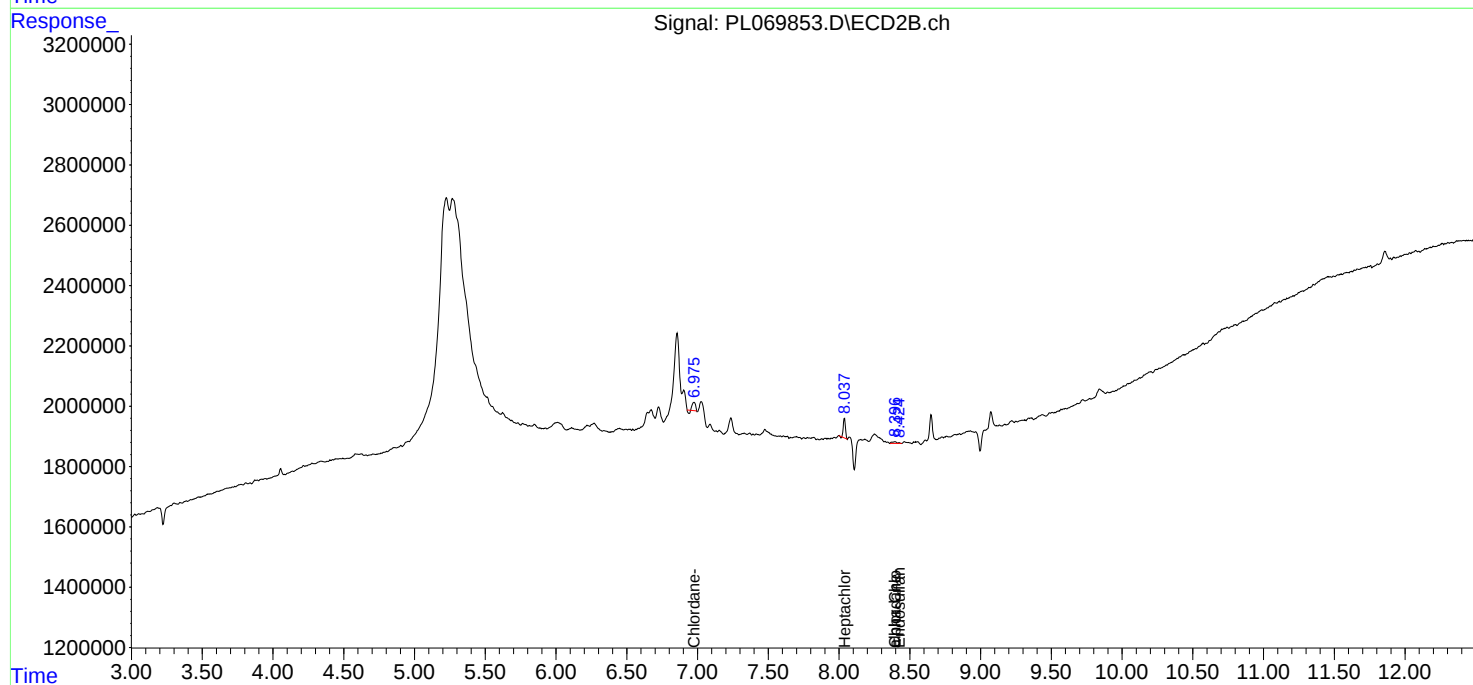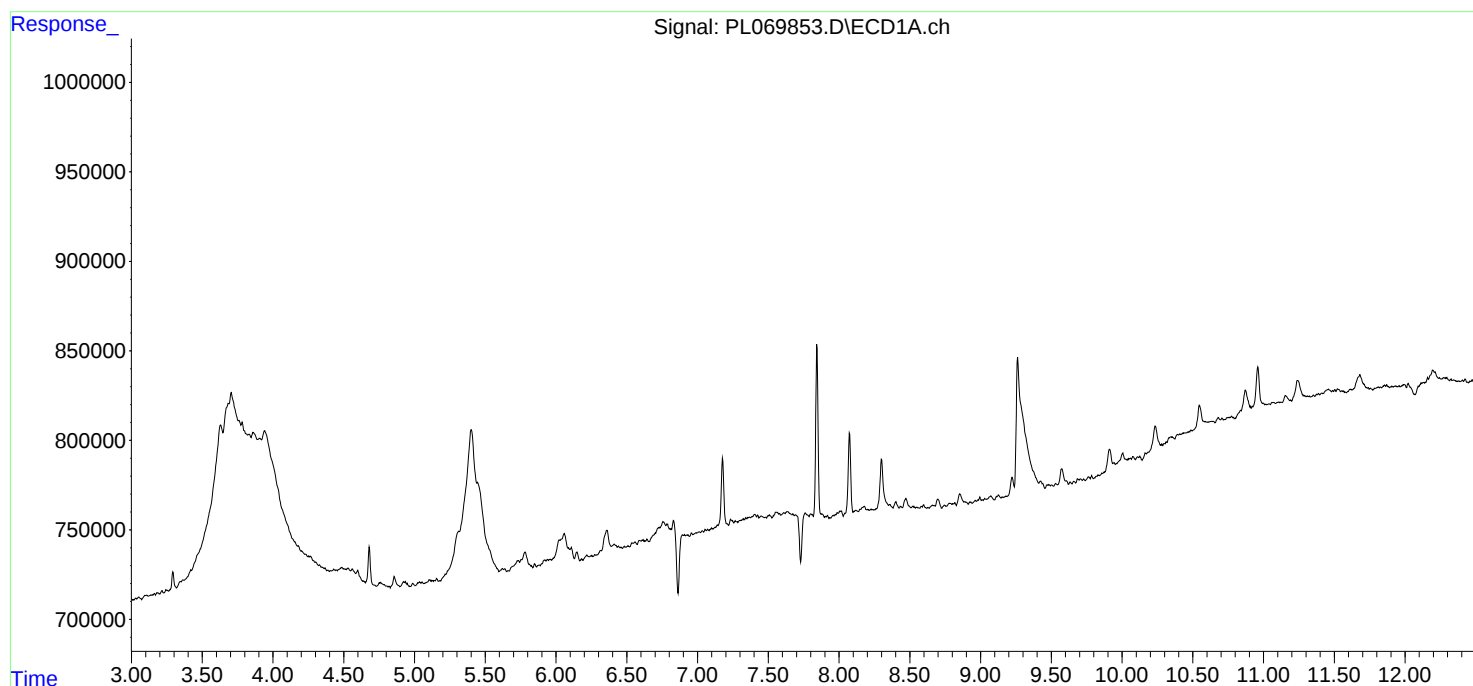


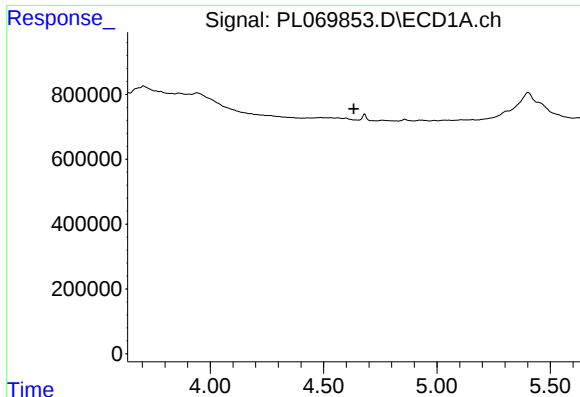

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.633 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

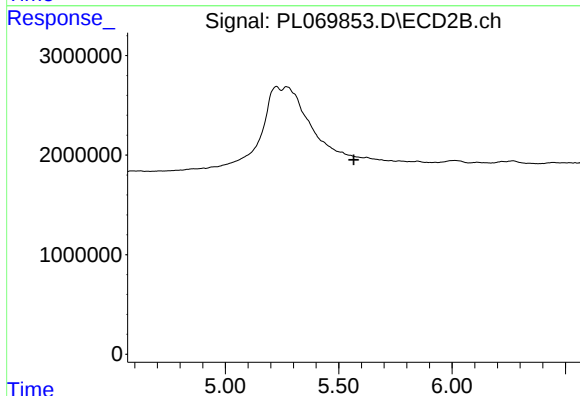


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.567 min
Response: 0
Conc: N.D.

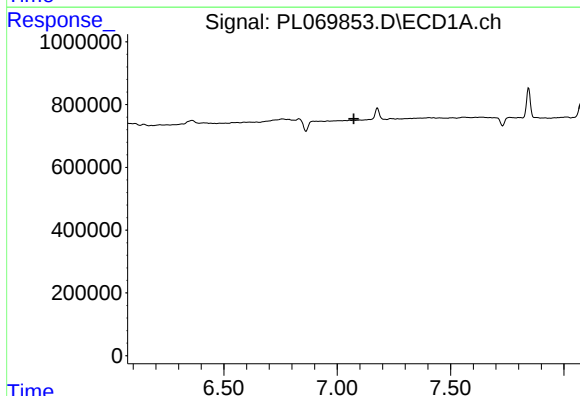


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

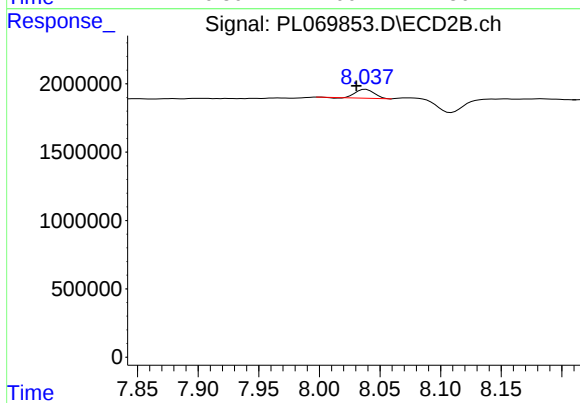

#8 Heptachlor epoxide


R.T.: 8.038 min
Delta R.T.: 0.008 min
Response: 695376
Conc: 0.54 ng/ml

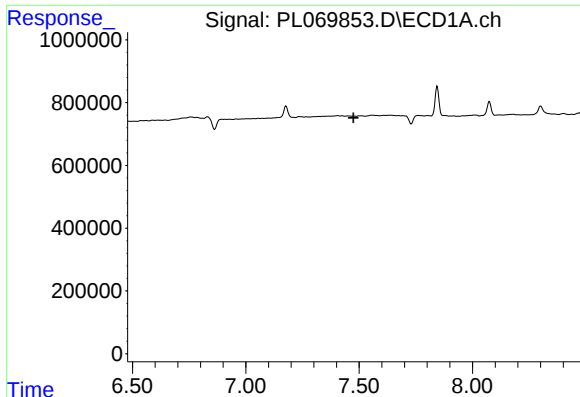

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

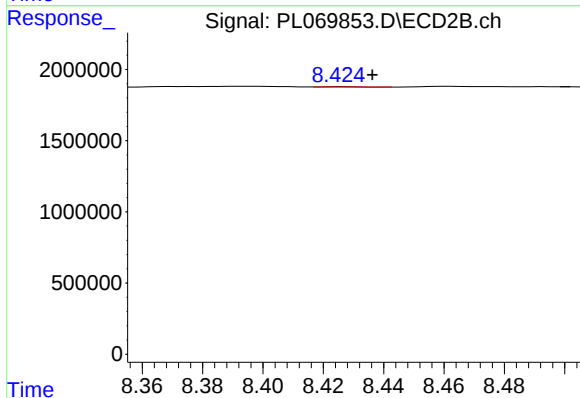


#9 Endosulfan I

R.T.: 8.425 min
Delta R.T.: -0.011 min
Response: 22439
Conc: 0.02 ng/ml

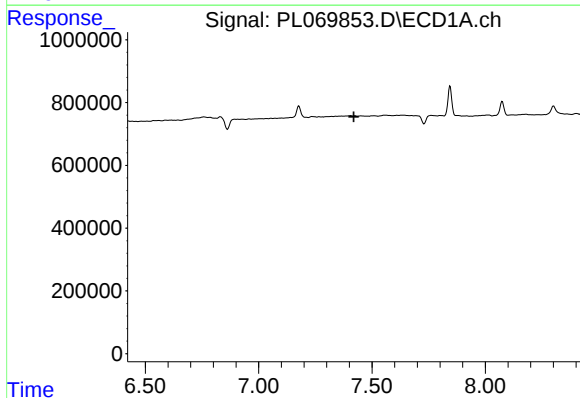


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

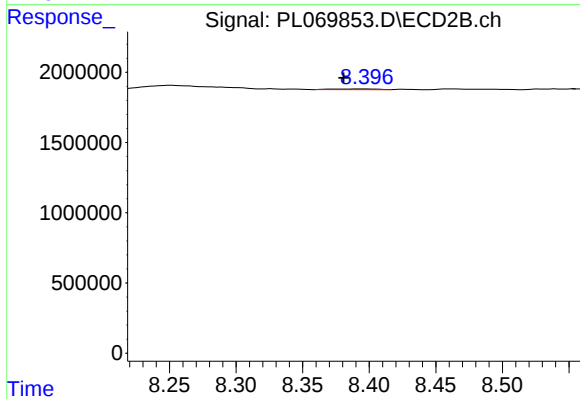

#11 alpha-Chlordane


R.T.: 8.397 min
Delta R.T.: 0.016 min
Response: 131559
Conc: 0.10 ng/ml

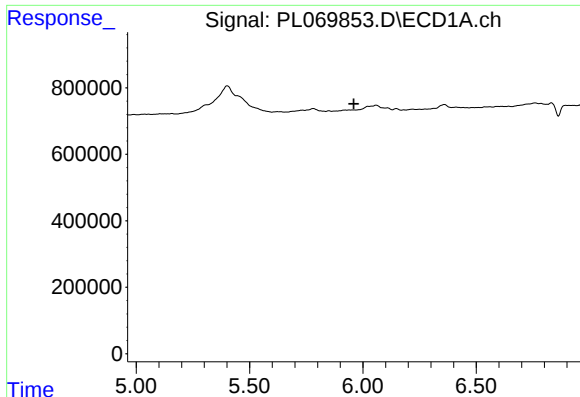

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

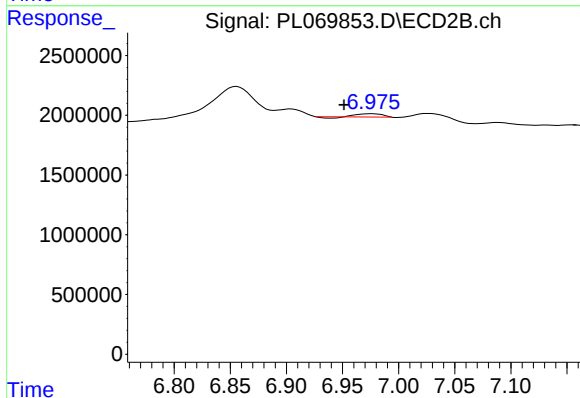


#23 Chlordane-1

R.T.: 6.976 min
Delta R.T.: 0.025 min
Response: 372373
Conc: 9.07 ng/ml

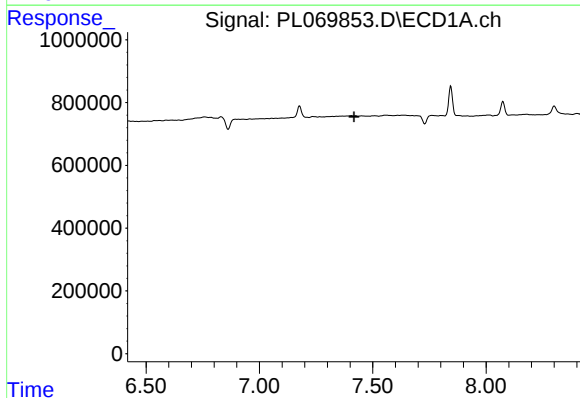


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

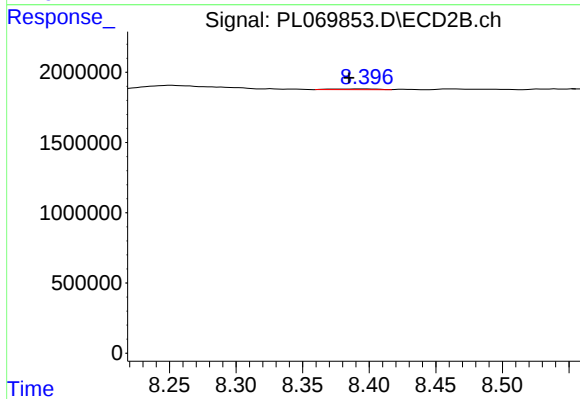

#26 Chlordane-4


R.T.: 8.397 min
Delta R.T.: 0.012 min
Response: 131559
Conc: 0.56 ng/ml

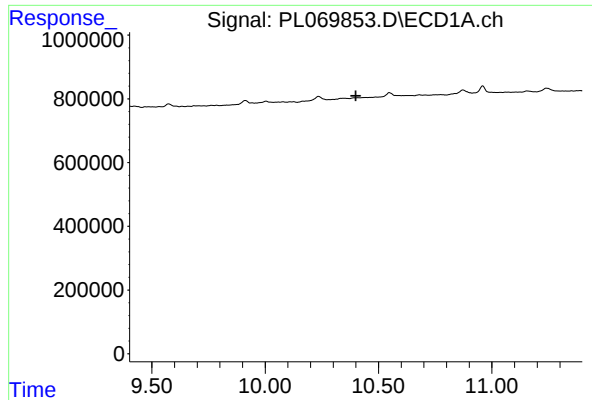

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

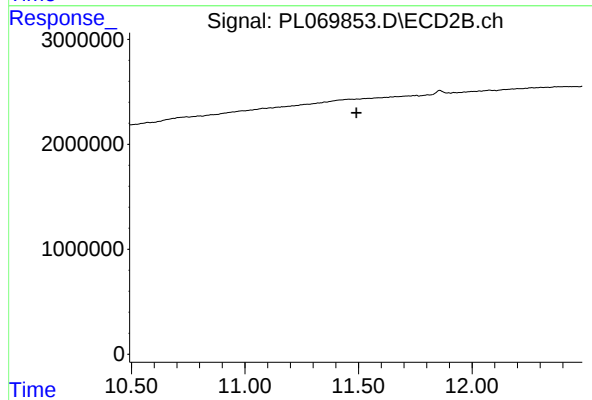

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.491 min
Response: 0
Conc: N.D.