

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091521\
 Data File : PL069868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 17:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 04:50:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	5.563	9970308	32665925	24.472	26.836
28)	SA Decachlor...	10.394	11.484	16394162	30139028	22.262	26.377
Target Compounds							
2)	A alpha-BHC	5.353	0.000	1687515	0	3.078	N.D. #
4)	MA Heptachlor	6.145f	0.000	703074	0	1.037	N.D. #
7)	B delta-BHC	0.000	7.080f	0	2574264	N.D.	1.545 #
10)	B gamma-Chl...	0.000	8.291	0	1222191	N.D.	0.915 #
17)	MA 4,4'-DDT	0.000	9.440	0	287300	N.D.	0.257 #
21)	B Endrin ke...	0.000	10.088f	0	231662	N.D.	0.188 #
23)	Chlordane-1	0.000	6.965	0	1467899	N.D.	35.762 #
25)	Chlordane-3	0.000	8.291	0	1222191	N.D.	6.443 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091521\
Data File : PL069868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 17:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 04:50:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

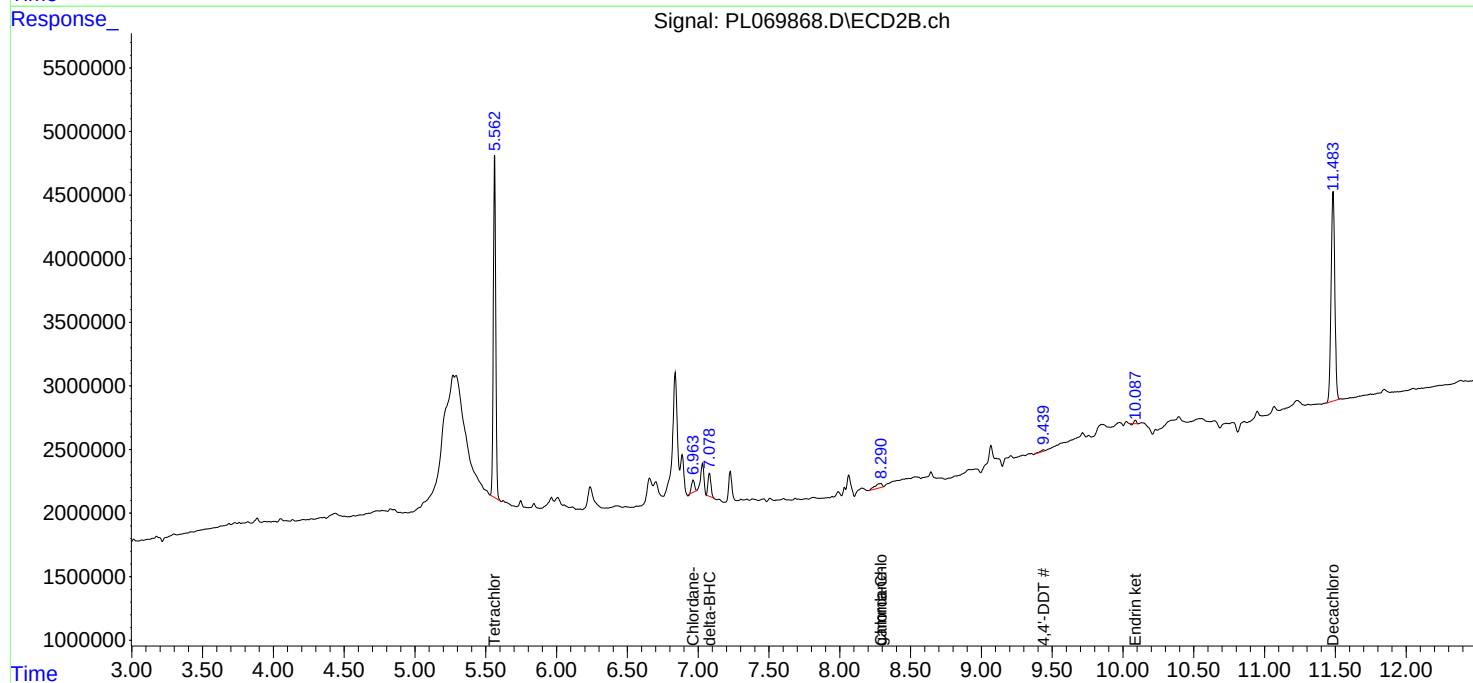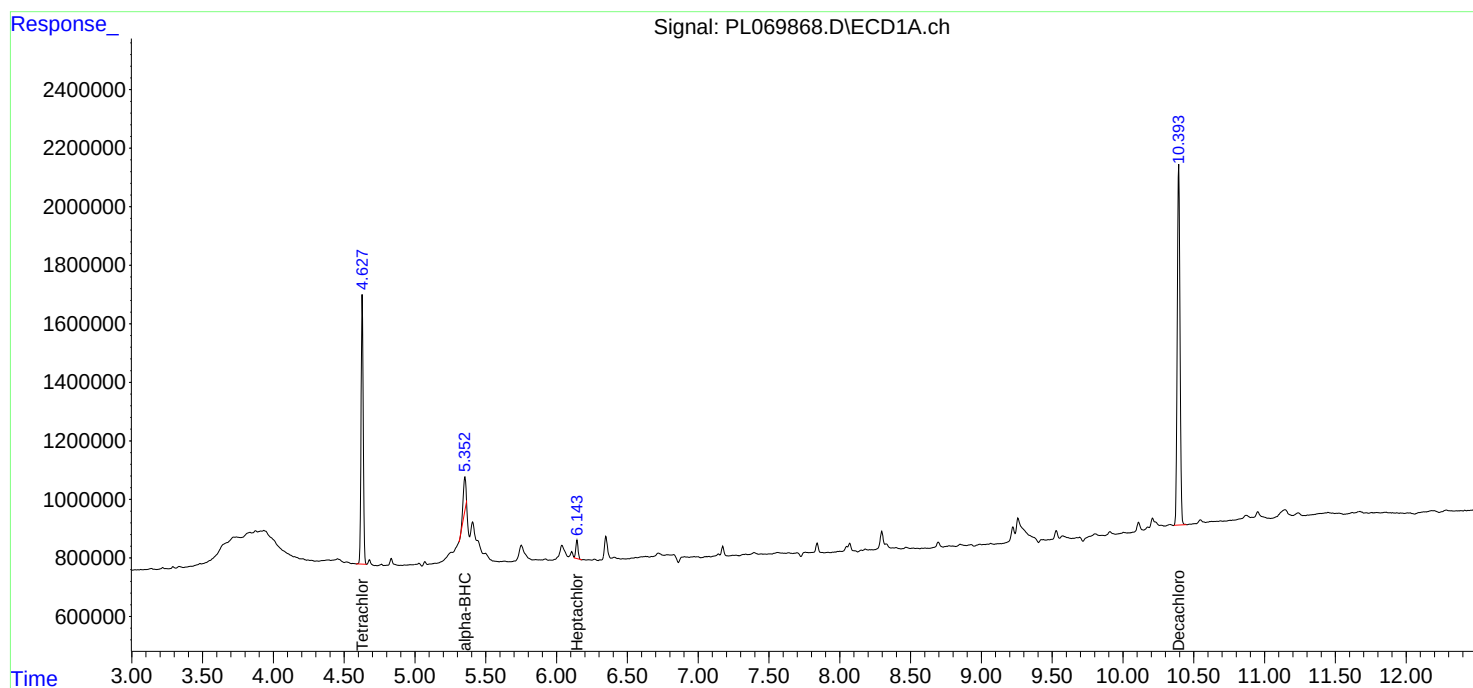


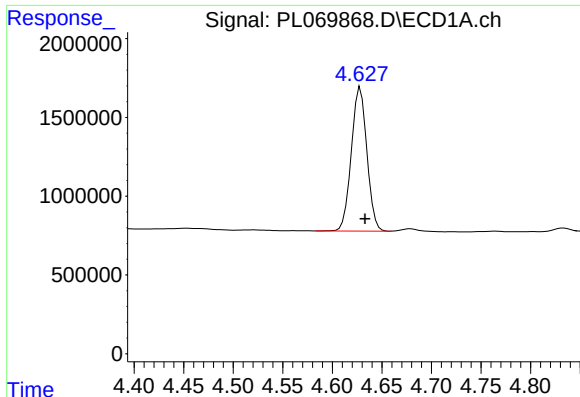

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.005 min
Response: 9970308
Conc: 24.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

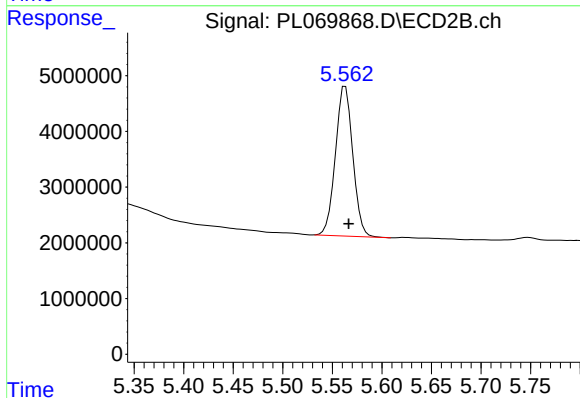


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.003 min
Response: 32665925
Conc: 26.84 ng/ml

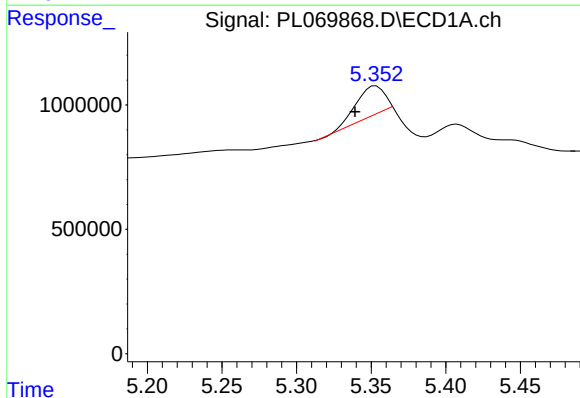


#2 alpha-BHC

R.T.: 5.353 min
Delta R.T.: 0.014 min
Response: 1687515
Conc: 3.08 ng/ml

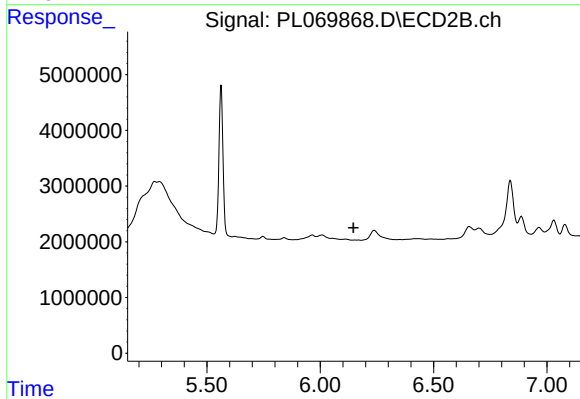

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.147 min
Response: 0
Conc: N.D.

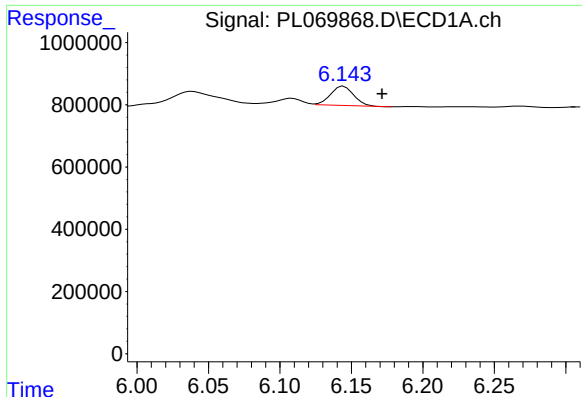

#4 Heptachlor


R.T.: 6.145 min
Delta R.T.: -0.027 min
Response: 703074
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

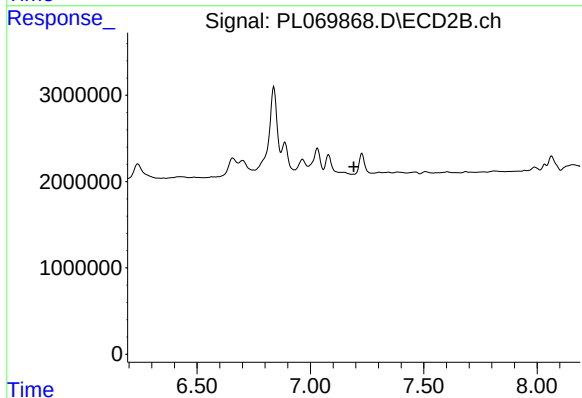


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

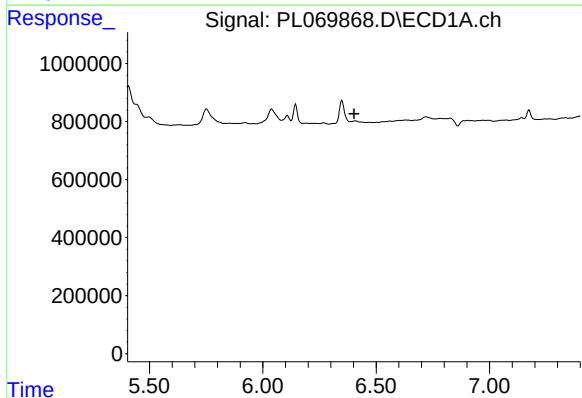


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

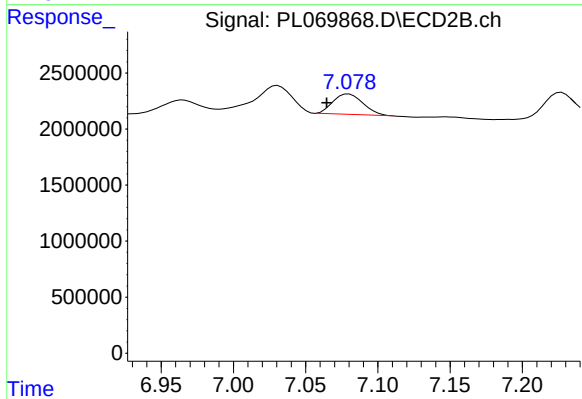

#7 delta-BHC


R.T.: 7.080 min
Delta R.T.: 0.015 min
Response: 2574264
Conc: 1.55 ng/ml

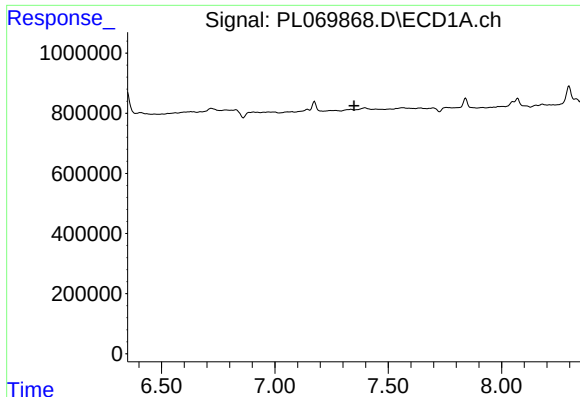

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

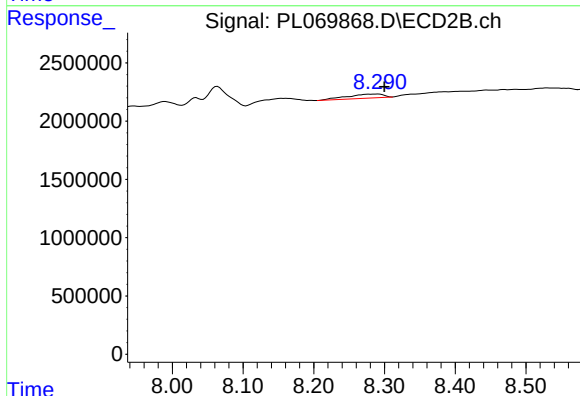


#10 gamma-Chlordane

R.T.: 8.291 min
Delta R.T.: -0.009 min
Response: 1222191
Conc: 0.91 ng/ml

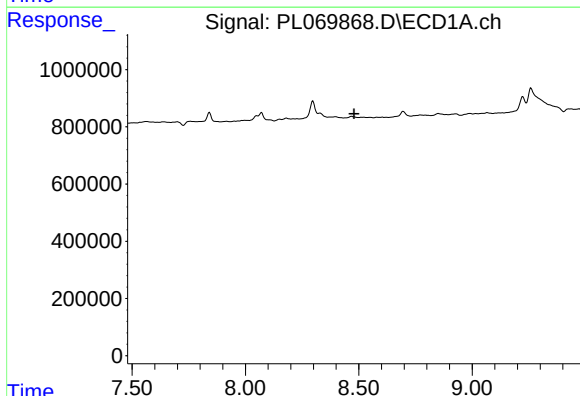


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

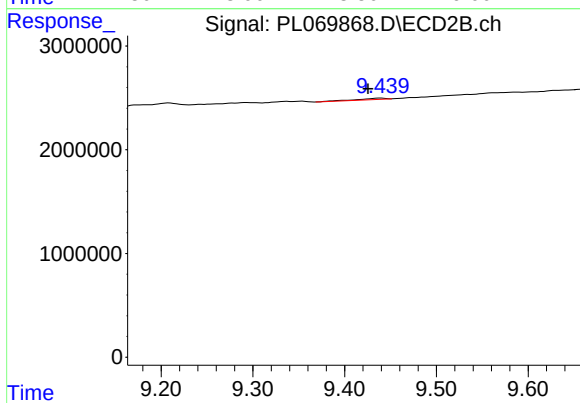

#17 4,4'-DDT


R.T.: 9.440 min
Delta R.T.: 0.014 min
Response: 287300
Conc: 0.26 ng/ml

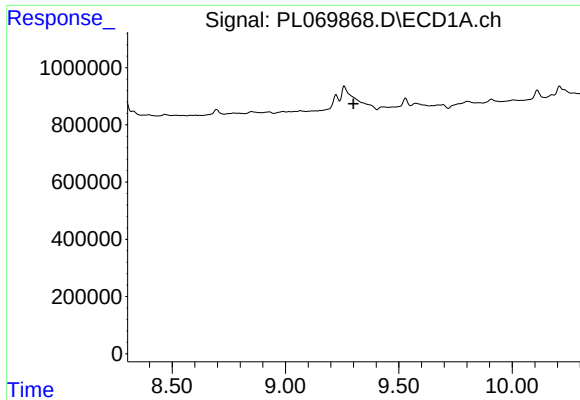

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.301 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

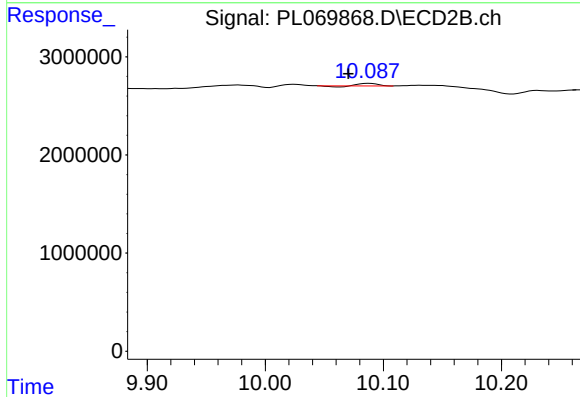


#21 Endrin ketone

R.T.: 10.088 min
Delta R.T.: 0.018 min
Response: 231662
Conc: 0.19 ng/ml

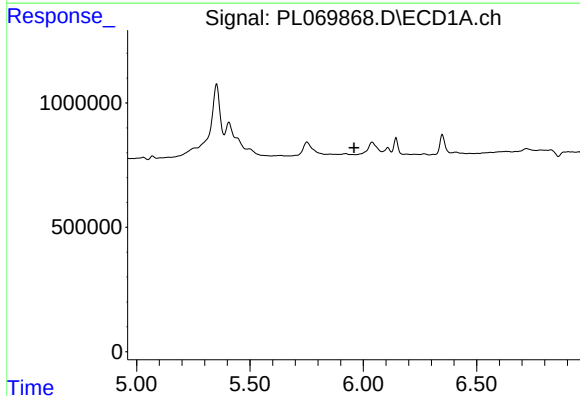


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

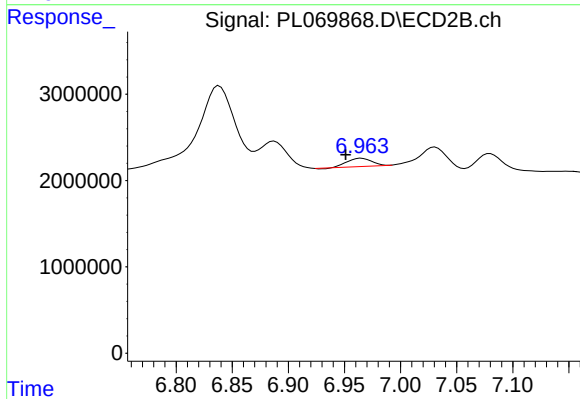

#23 Chlordane-1


R.T.: 6.965 min
Delta R.T.: 0.014 min
Response: 1467899
Conc: 35.76 ng/ml

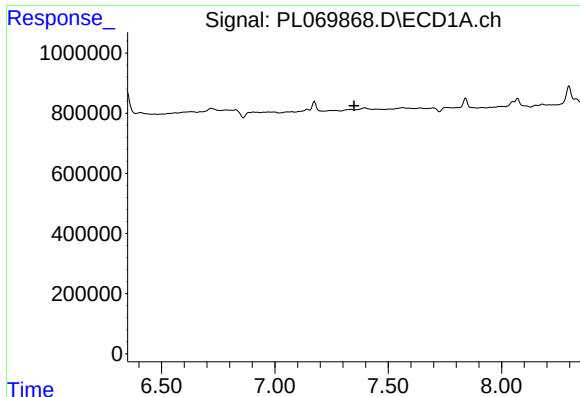

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

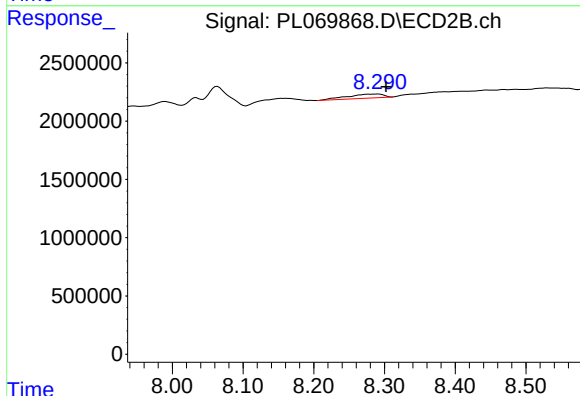


#25 Chlordane-3

R.T.: 8.291 min
Delta R.T.: -0.011 min
Response: 1222191
Conc: 6.44 ng/ml

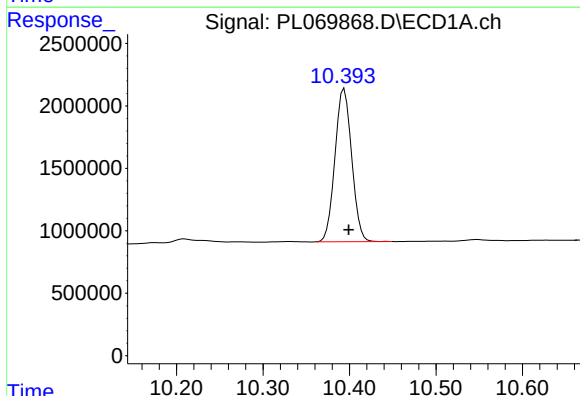

#28 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: -0.005 min
Response: 16394162
Conc: 22.26 ng/ml

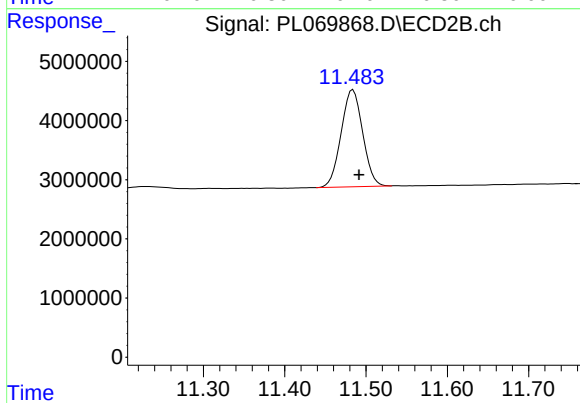

#28 Decachlorobiphenyl

R.T.: 11.484 min
Delta R.T.: -0.007 min
Response: 30139028
Conc: 26.38 ng/ml