

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091521\
 Data File : PL069872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2021 19:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 04:52:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	5.564	10113547	33086362	24.824	27.182
28)	SA Decachlor...	10.394	11.483	16260277	30618151	22.080	26.796
Target Compounds							
4)	MA Heptachlor	6.144f	0.000	707772	0	1.044	N.D. #
7)	B delta-BHC	0.000	7.080f	0	2316369	N.D.	1.391 #
10)	B gamma-Chl...	0.000	8.286	0	1503887	N.D.	1.126 #
11)	B alpha-Chl...	0.000	8.383	0	240317	N.D.	0.177 #
15)	B Endosulfa...	0.000	9.210	0	322561	N.D.	0.286 #
21)	B Endrin ke...	0.000	10.088f	0	868203	N.D.	0.704 #
23)	Chlordane-1	0.000	6.968f	0	1081344	N.D.	26.344 #
25)	Chlordane-3	0.000	8.286f	0	1503887	N.D.	7.928 #
26)	Chlordane-4	0.000	8.383	0	240317	N.D.	1.032 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091521\
Data File : PL069872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2021 19:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 04:52:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

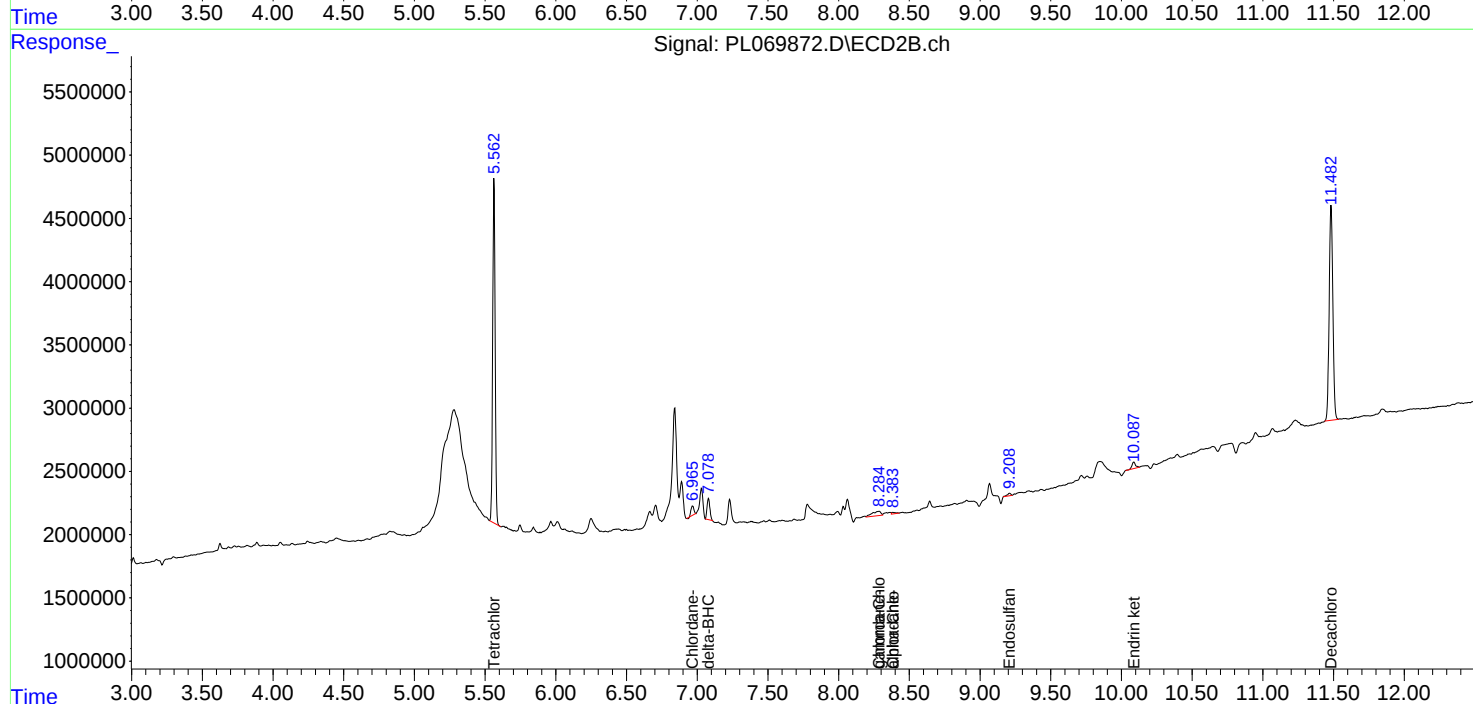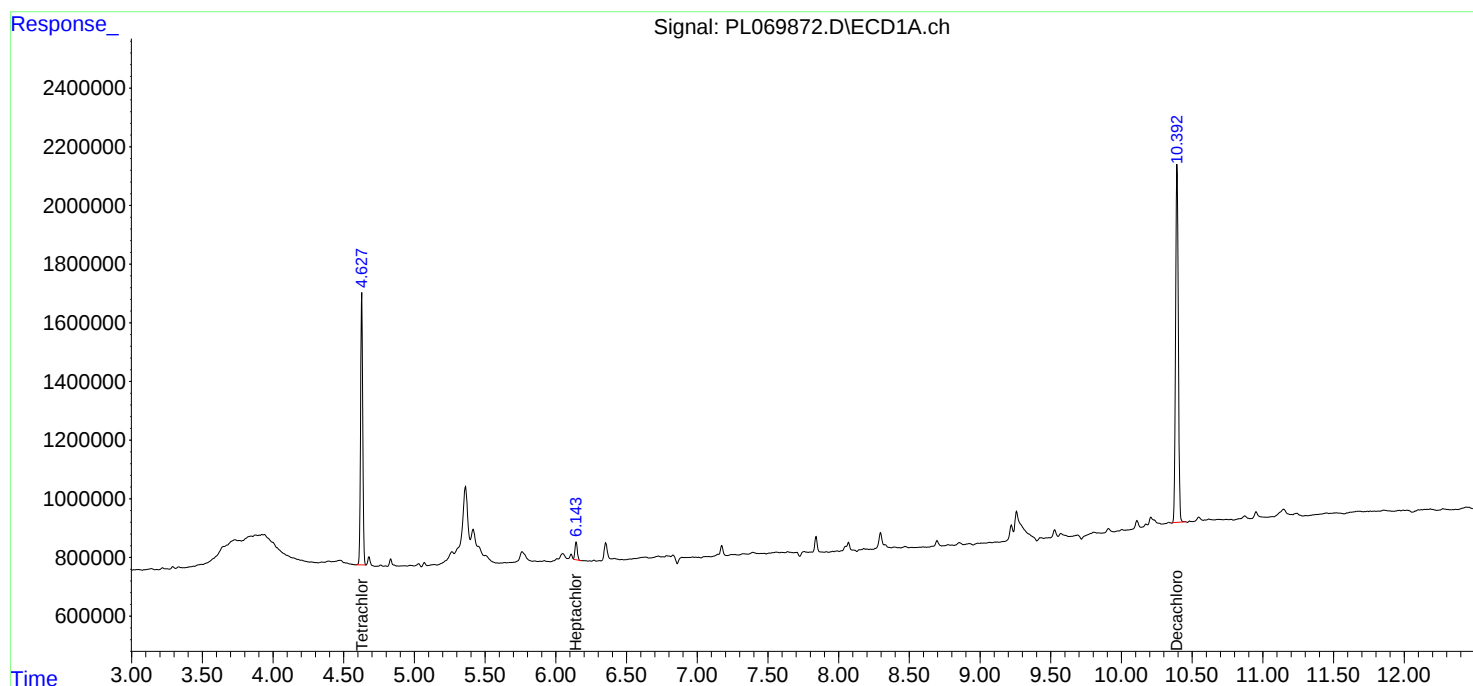


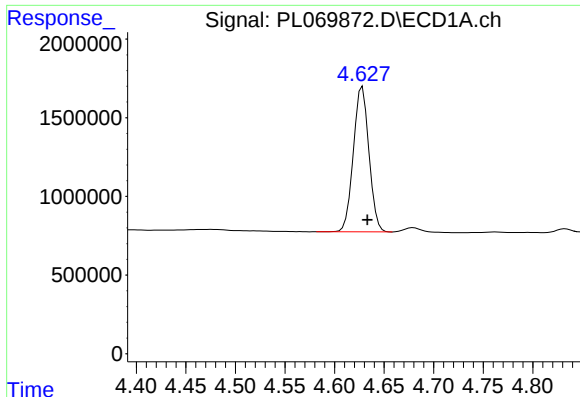

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.005 min
Response: 10113547
Conc: 24.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

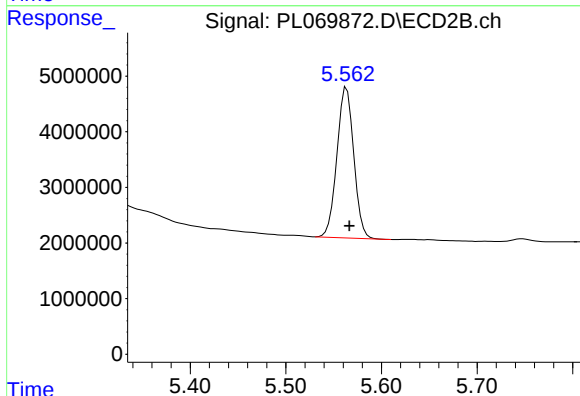


#1 Tetrachloro-m-xylene

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 33086362
Conc: 27.18 ng/ml

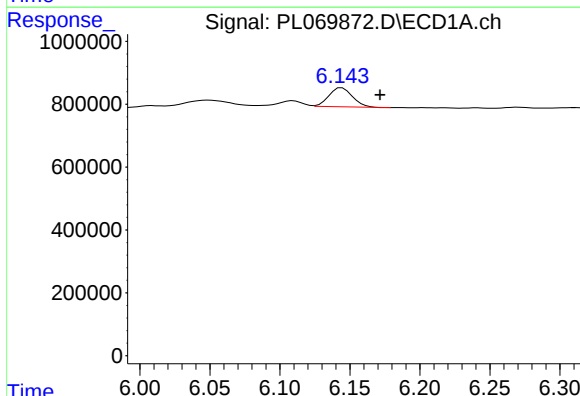


#4 Heptachlor

R.T.: 6.144 min
Delta R.T.: -0.027 min
Response: 707772
Conc: 1.04 ng/ml

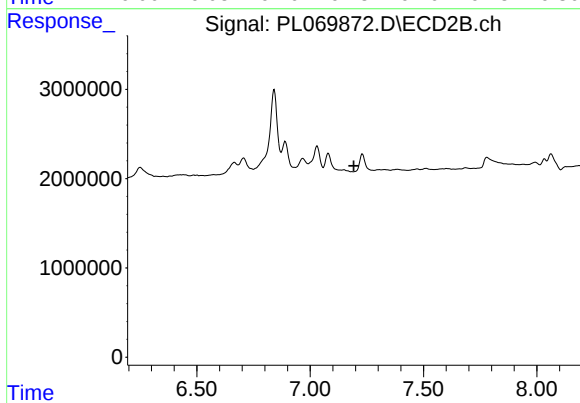

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

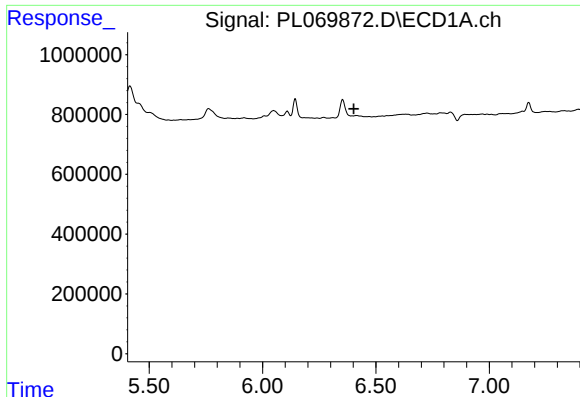

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

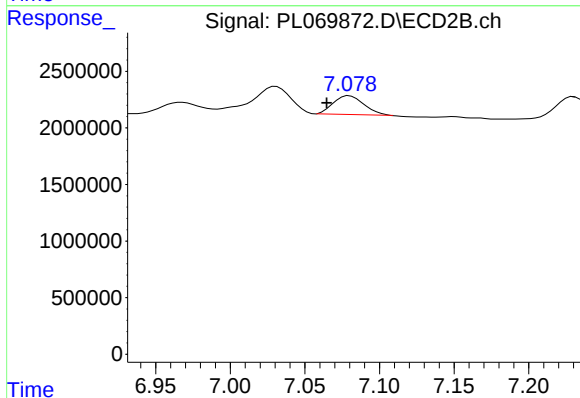


#7 delta-BHC

R.T.: 7.080 min
Delta R.T.: 0.015 min
Response: 2316369
Conc: 1.39 ng/ml

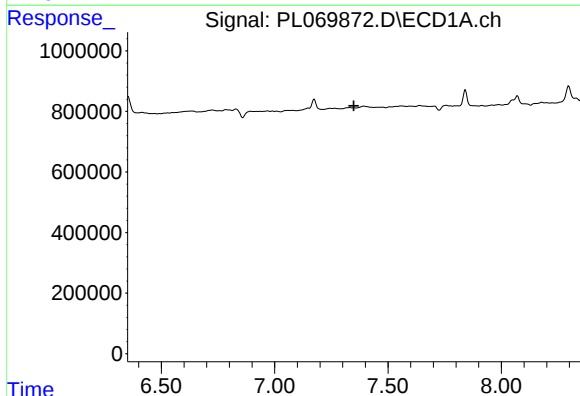


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

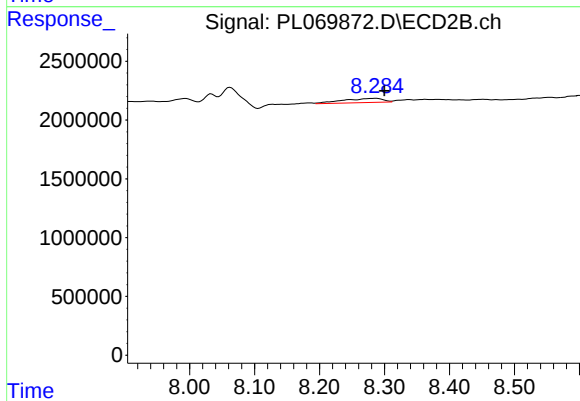

#10 gamma-Chlordane


R.T.: 8.286 min
Delta R.T.: -0.014 min
Response: 1503887
Conc: 1.13 ng/ml

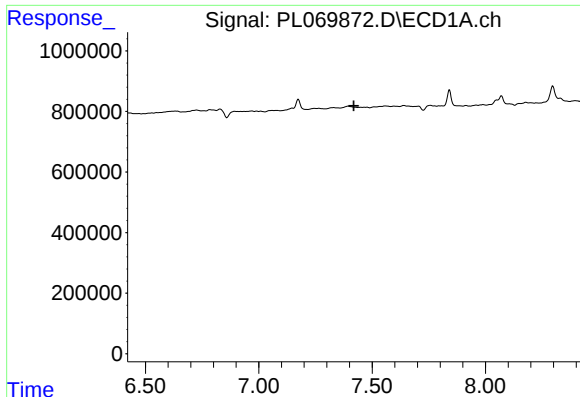

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

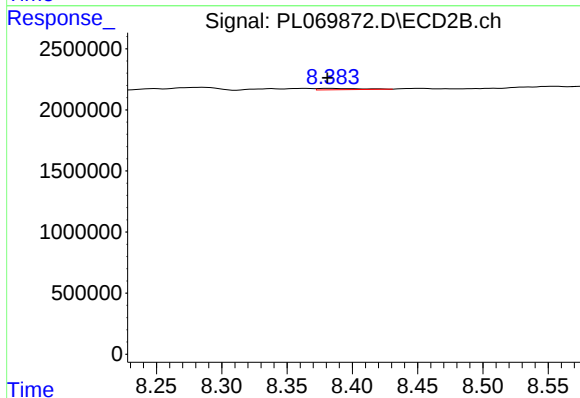


#11 alpha-Chlordane

R.T.: 8.383 min
Delta R.T.: 0.002 min
Response: 240317
Conc: 0.18 ng/ml

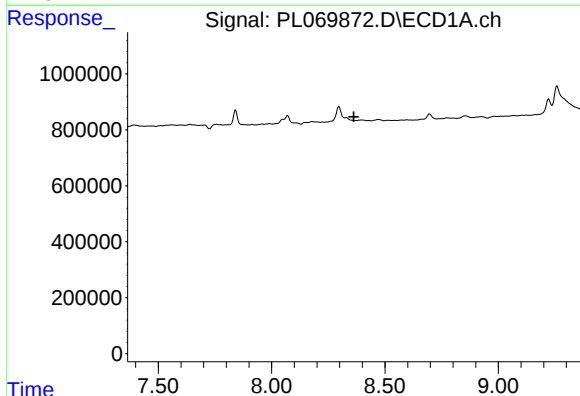


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

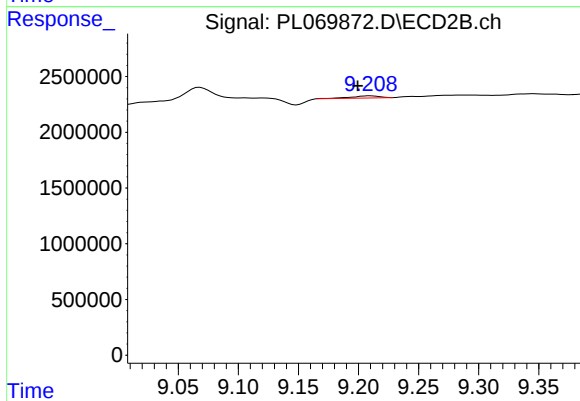

#15 Endosulfan II


R.T.: 9.210 min
Delta R.T.: 0.010 min
Response: 322561
Conc: 0.29 ng/ml

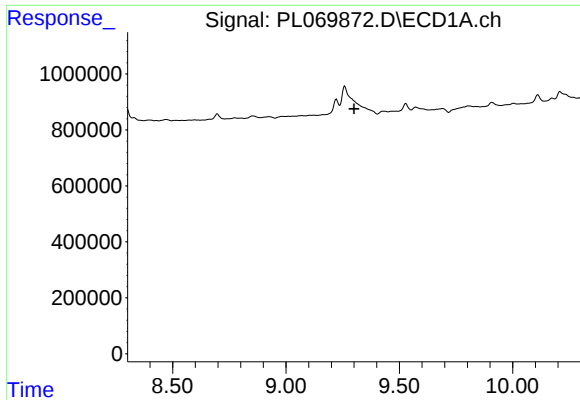

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.301 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

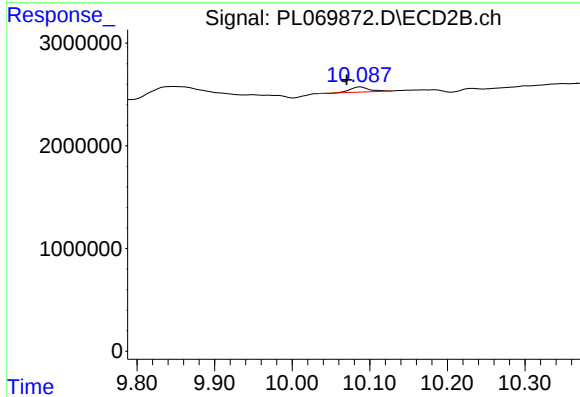


#21 Endrin ketone

R.T.: 10.088 min
Delta R.T.: 0.018 min
Response: 868203
Conc: 0.70 ng/ml

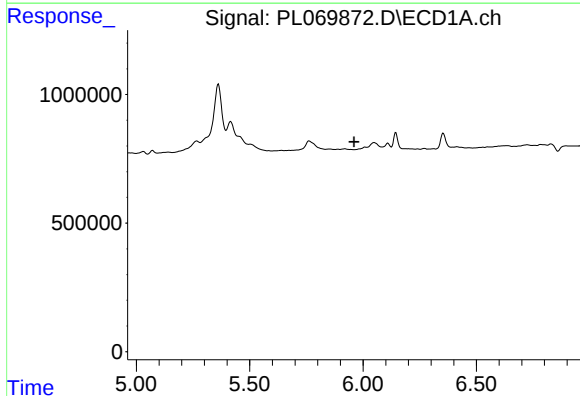


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

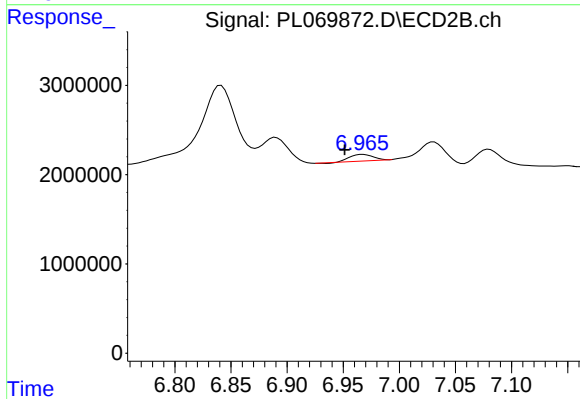

#23 Chlordane-1


R.T.: 6.968 min
Delta R.T.: 0.016 min
Response: 1081344
Conc: 26.34 ng/ml

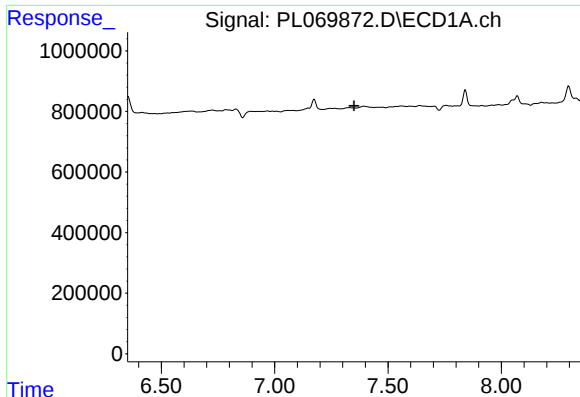

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

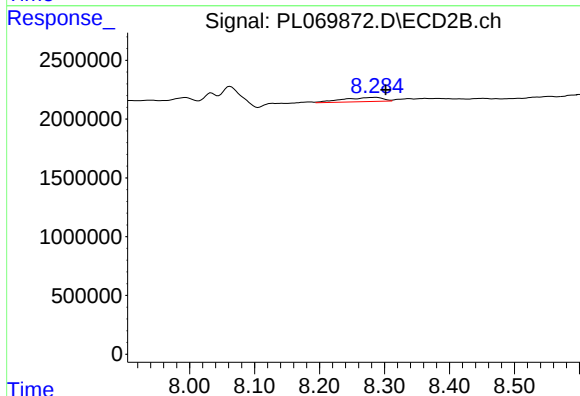


#25 Chlordane-3

R.T.: 8.286 min
Delta R.T.: -0.016 min
Response: 1503887
Conc: 7.93 ng/ml

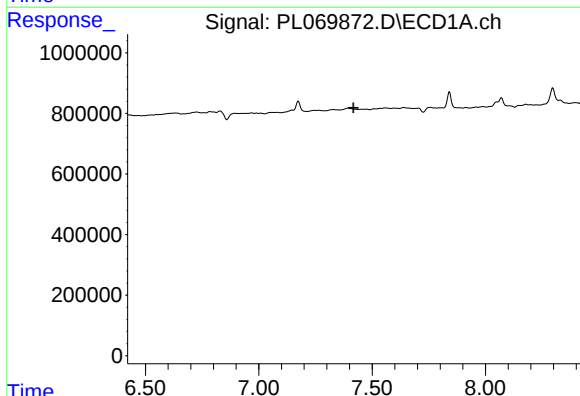


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

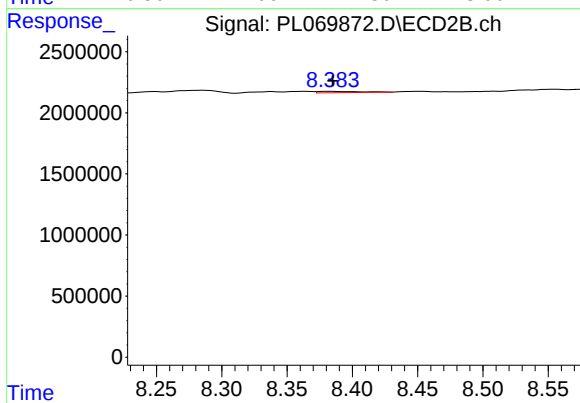

#26 Chlordane-4


R.T.: 8.383 min
Delta R.T.: -0.002 min
Response: 240317
Conc: 1.03 ng/ml

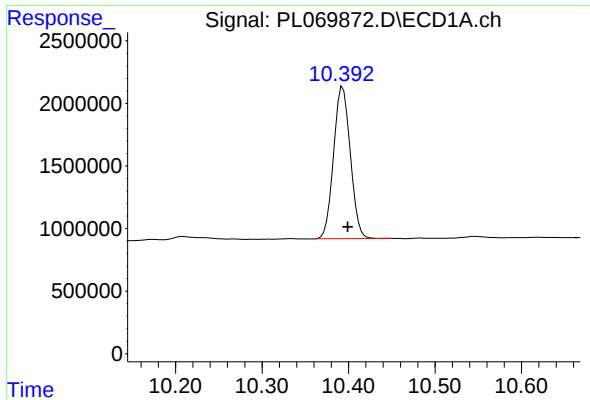

#28 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: -0.006 min
Response: 16260277
Conc: 22.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

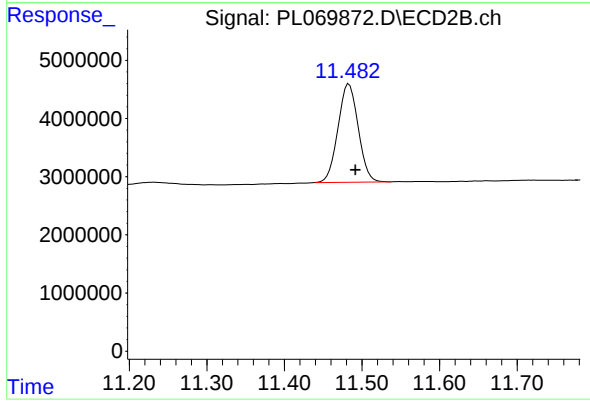

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.008 min
Response: 30618151
Conc: 26.80 ng/ml