

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091522\
 Data File : PL077768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2022 13:21
 Operator : AR\AJ
 Sample : PB147485TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 14:44:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.624	28871276	52040372	18.011	17.529
28)	SA Decachlor...	8.904	7.724	26503346	47128313	20.507	18.775
Target Compounds							
8)	B Heptachlo...	5.587f	0.000	2318770	0	1.330	N.D. #
10)	B gamma-Chl...	0.000	4.791	0	979378	N.D.	0.287 #
13)	MA Dieldrin	0.000	5.157f	0	76774	N.D.	0.023 #
14)	MA Endrin	0.000	5.470f	0	1044088	N.D.	0.366 #
15)	B Endosulfa...	6.707f	0.000	581181	0	0.421	N.D. #
21)	B Endrin ke...	7.568f	0.000	521850	0	0.378	N.D. #
24)	Chlordane-2	0.000	4.155f	0	71931	N.D.	0.600 #
25)	Chlordane-3	0.000	4.791	0	979378	N.D.	2.847 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091522\
Data File : PL077768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2022 13:21
Operator : AR\AJ
Sample : PB147485TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 14:44:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

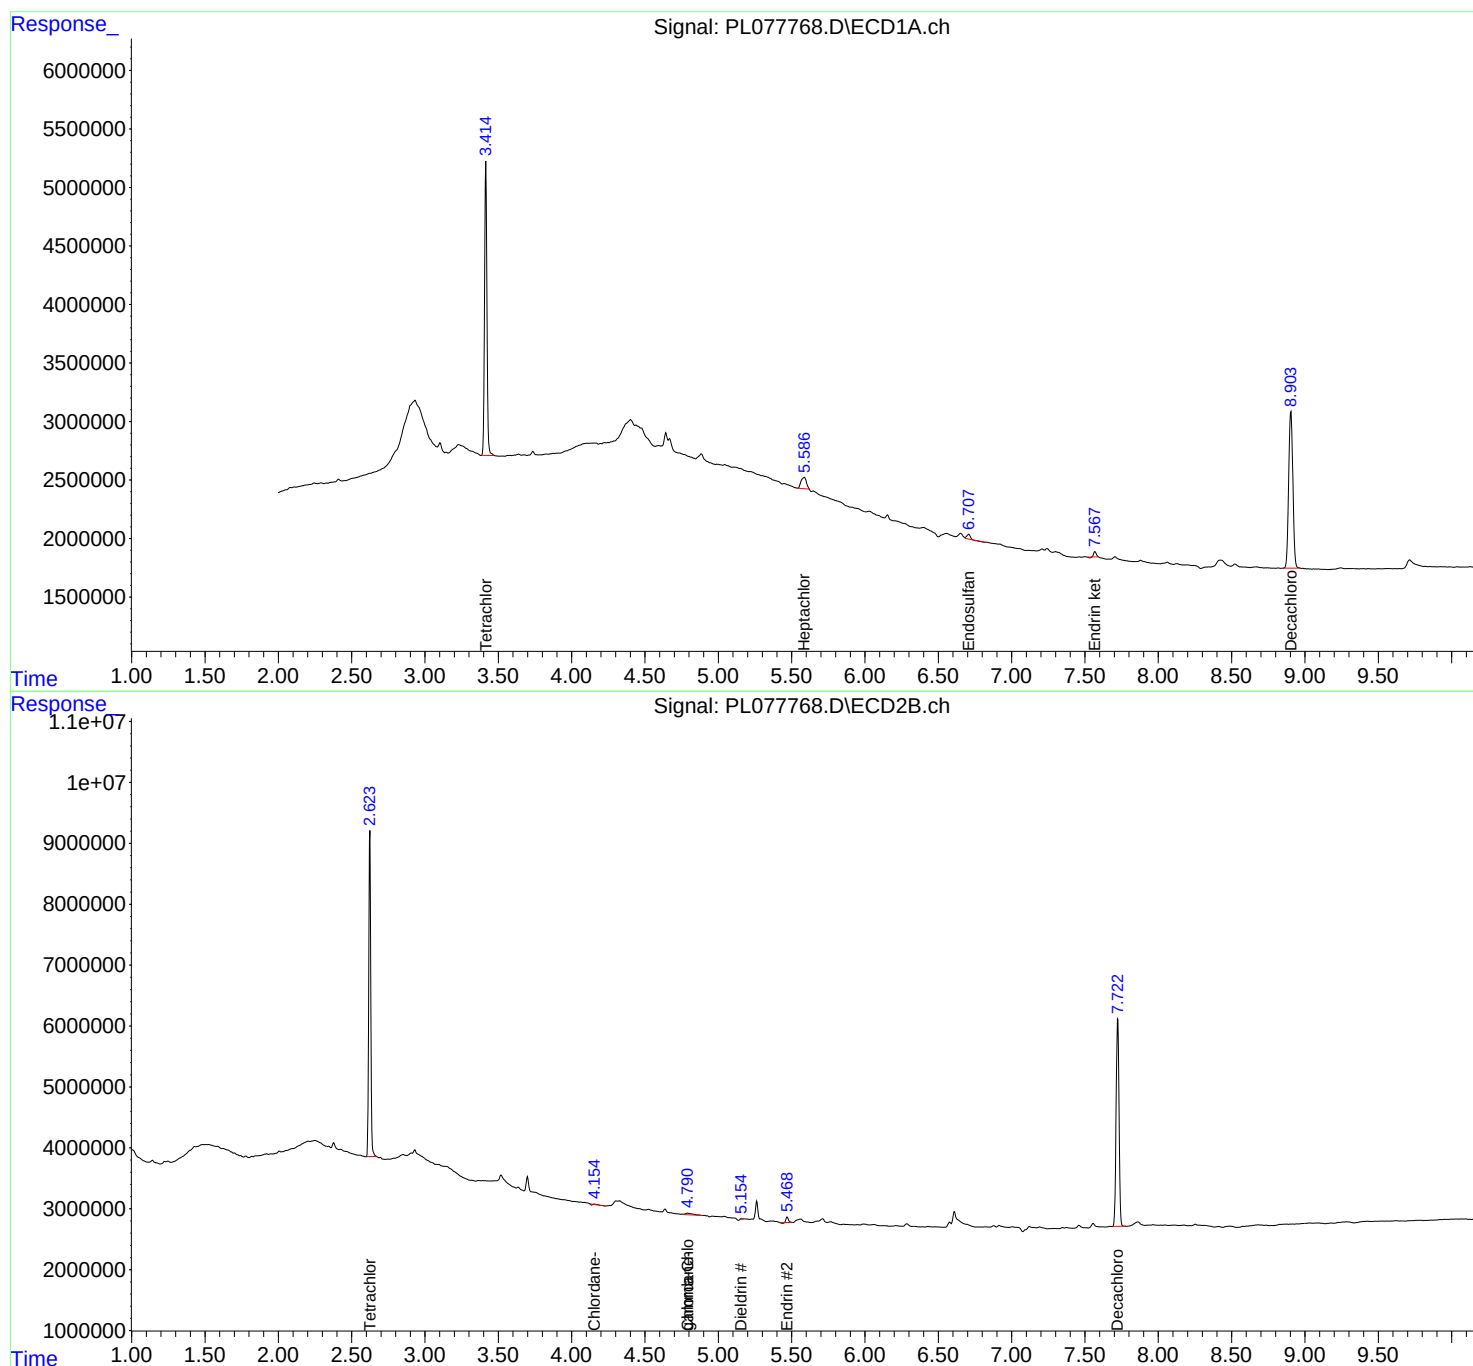


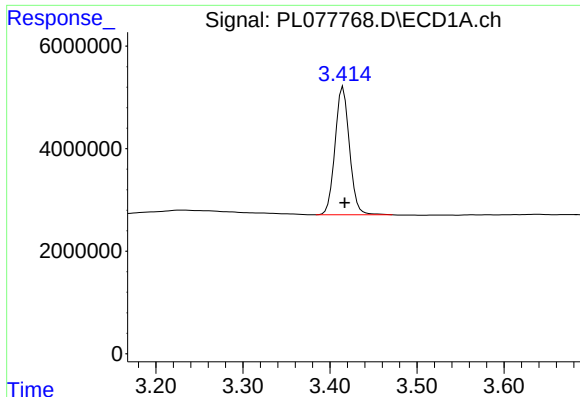

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: -0.002 min
Response: 28871276
Conc: 18.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

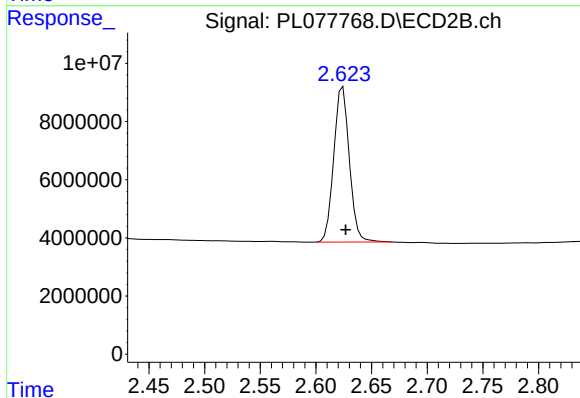


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 52040372
Conc: 17.53 ng/ml

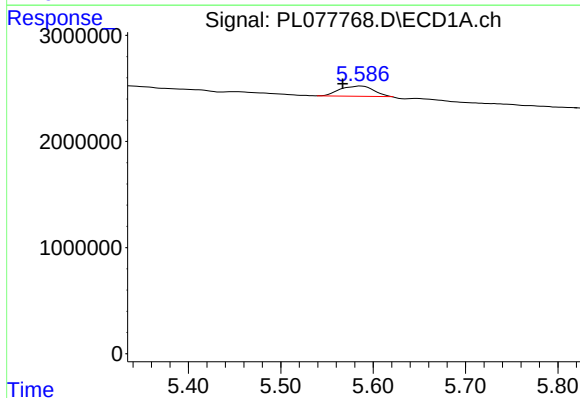


#8 Heptachlor epoxide

R.T.: 5.587 min
Delta R.T.: 0.020 min
Response: 2318770
Conc: 1.33 ng/ml

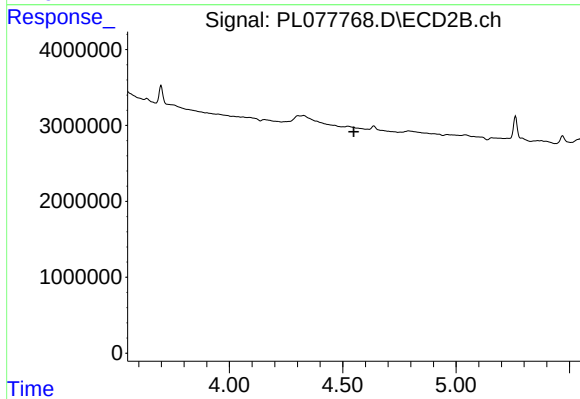

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.549 min
Response: 0
Conc: N.D.

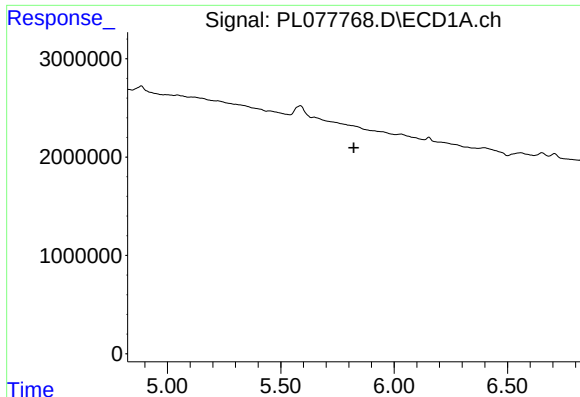

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

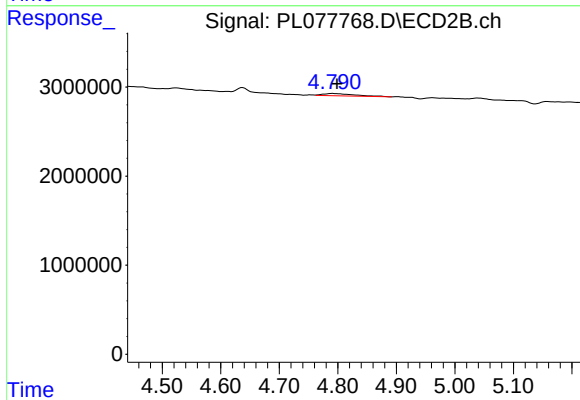


#10 gamma-Chlordane

R.T.: 4.791 min
Delta R.T.: -0.008 min
Response: 979378
Conc: 0.29 ng/ml

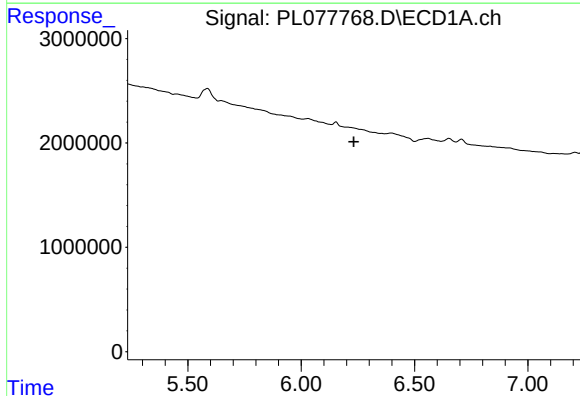


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.232 min
Response: 0
Conc: N.D.

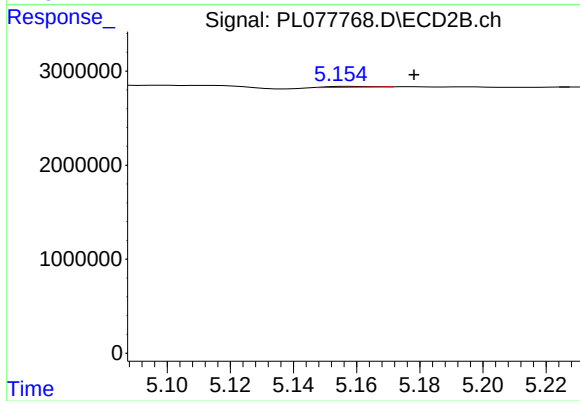

#13 Dieldrin


R.T.: 5.157 min
Delta R.T.: -0.021 min
Response: 76774
Conc: 0.02 ng/ml

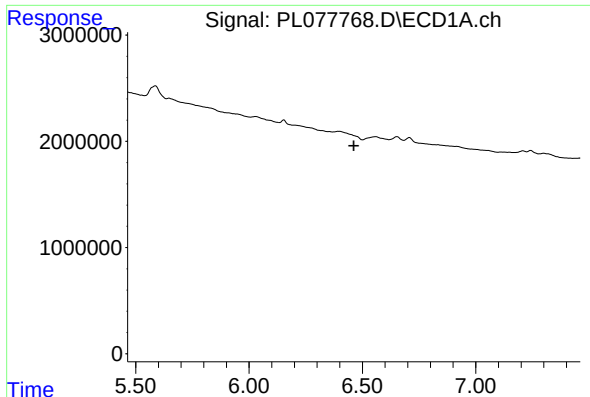

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

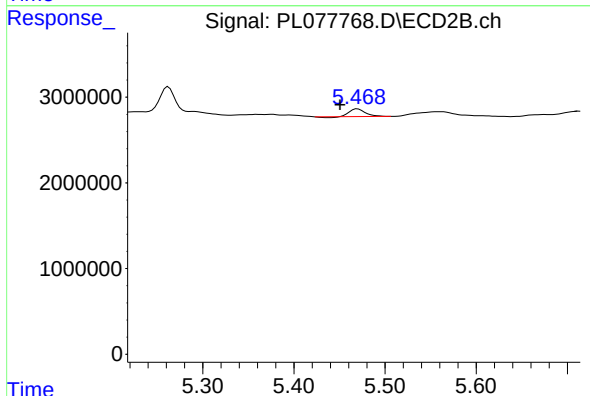


#14 Endrin

R.T.: 5.470 min
Delta R.T.: 0.019 min
Response: 1044088
Conc: 0.37 ng/ml

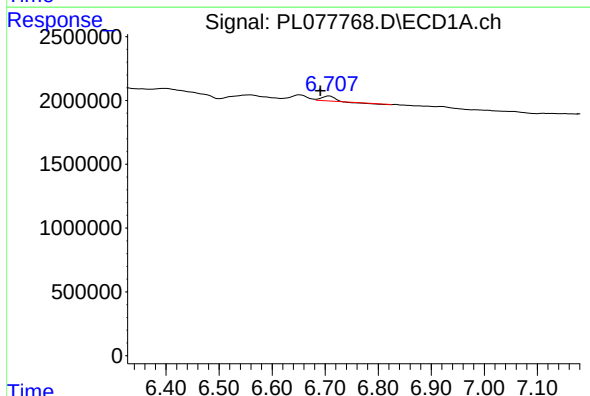


#15 Endosulfan II

R.T.: 6.707 min
Delta R.T.: 0.016 min
Response: 581181
Conc: 0.42 ng/ml

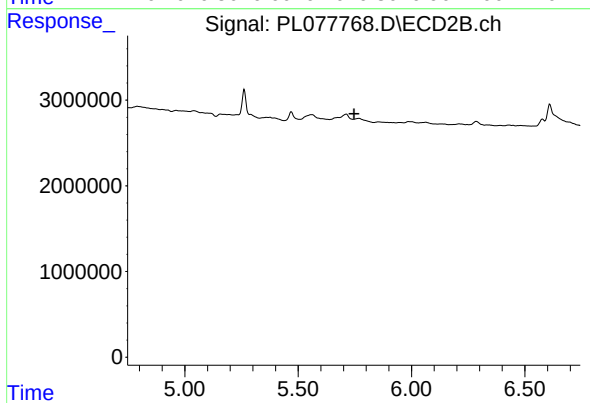

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.747 min
Response: 0
Conc: N.D.

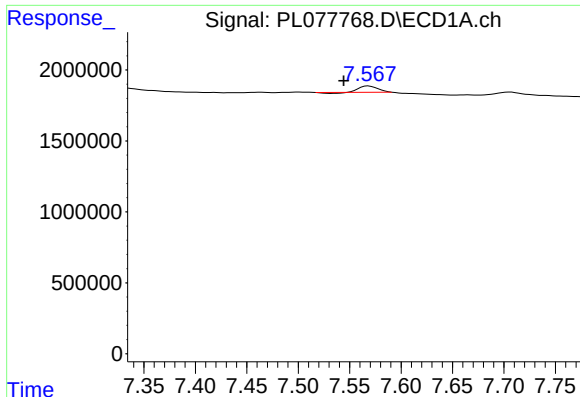

#21 Endrin ketone


R.T.: 7.568 min
Delta R.T.: 0.024 min
Response: 521850
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

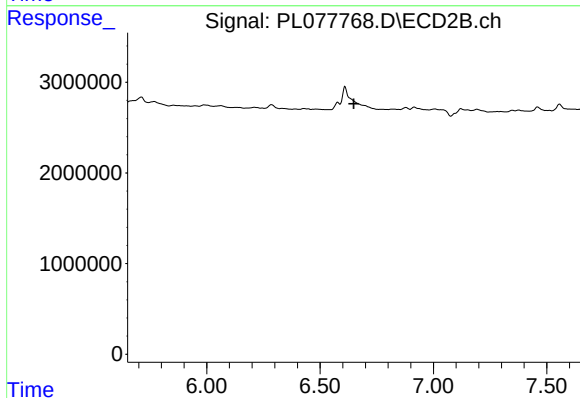


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

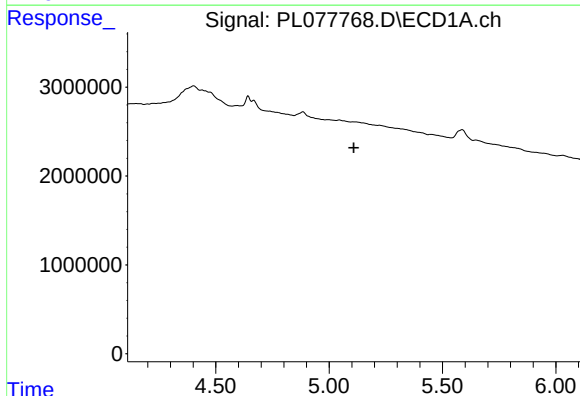


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

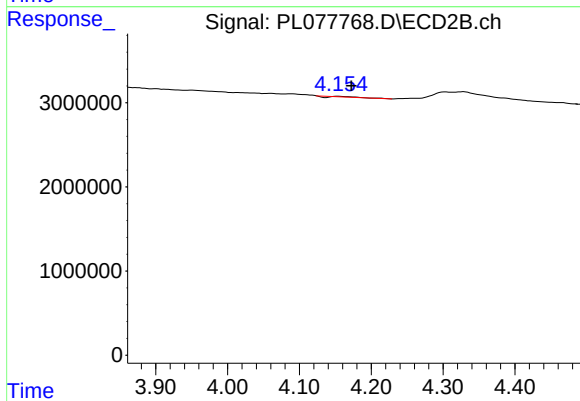

#24 Chlordane-2


R.T.: 4.155 min
Delta R.T.: -0.018 min
Response: 71931
Conc: 0.60 ng/ml

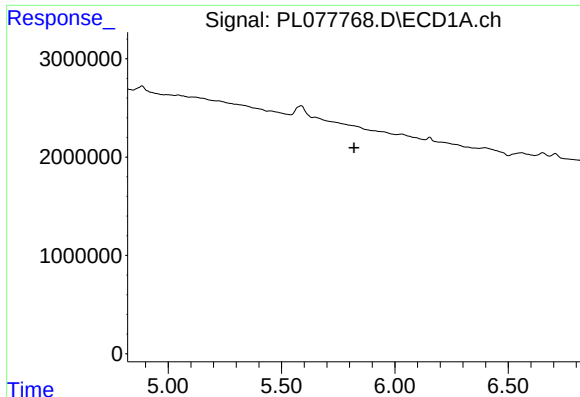

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

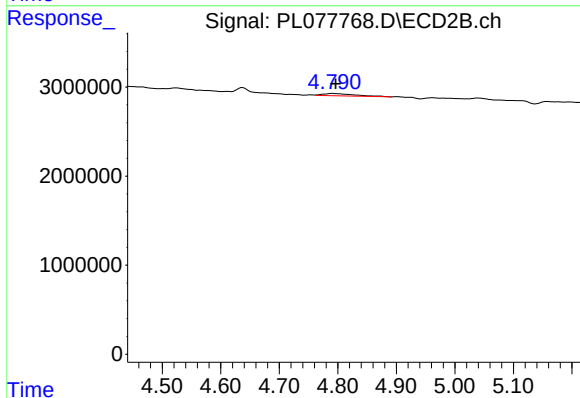


#25 Chlordane-3

R.T.: 4.791 min
Delta R.T.: -0.006 min
Response: 979378
Conc: 2.85 ng/ml

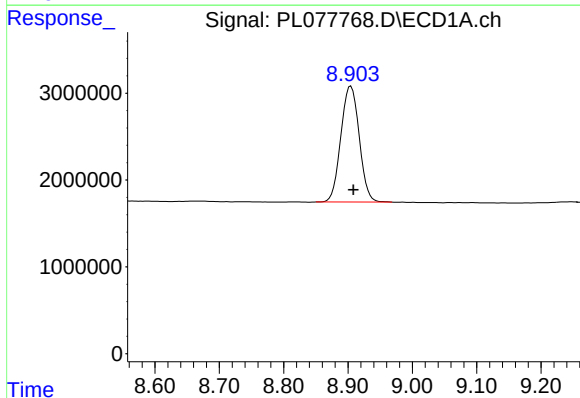

#28 Decachlorobiphenyl

R.T.: 8.904 min
Delta R.T.: -0.004 min
Response: 26503346
Conc: 20.51 ng/ml

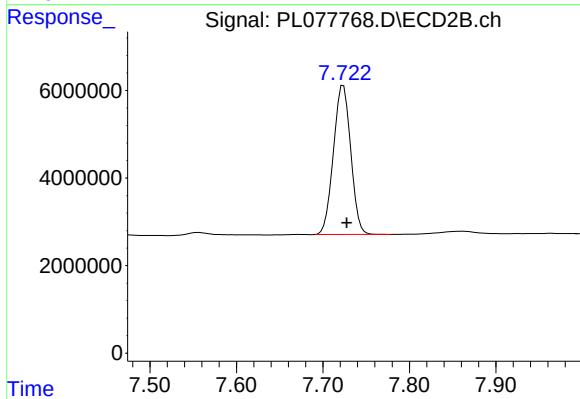

#28 Decachlorobiphenyl

R.T.: 7.724 min
Delta R.T.: -0.004 min
Response: 47128313
Conc: 18.77 ng/ml